
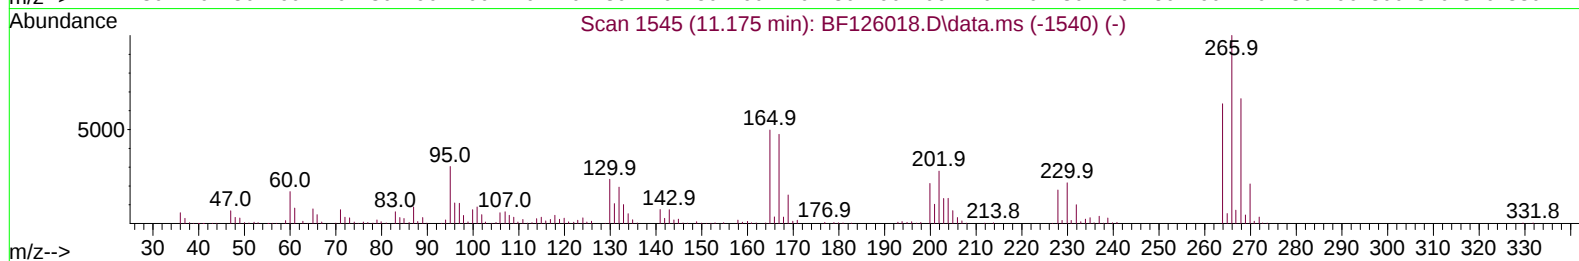
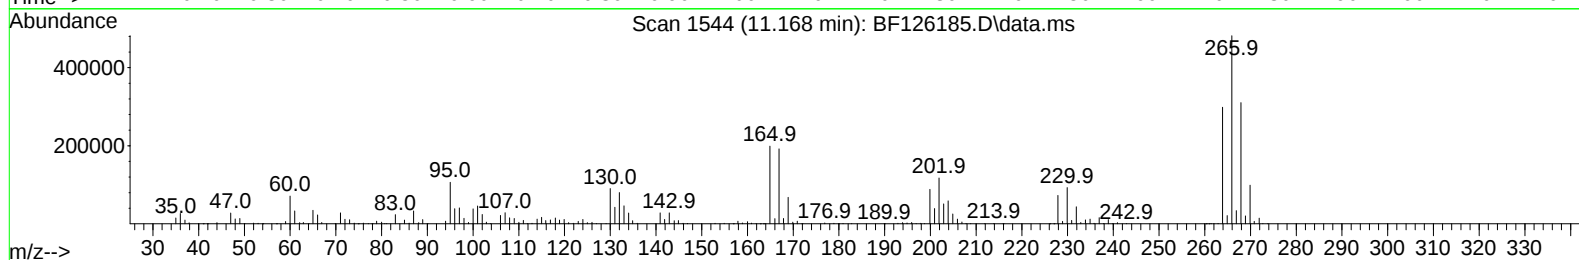


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120321\
 Data File : BF126185.D
 Acq On : 3 Dec 2021 10:32
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 16:49:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 03 16:45:52 2021
 Response via : Initial Calibration

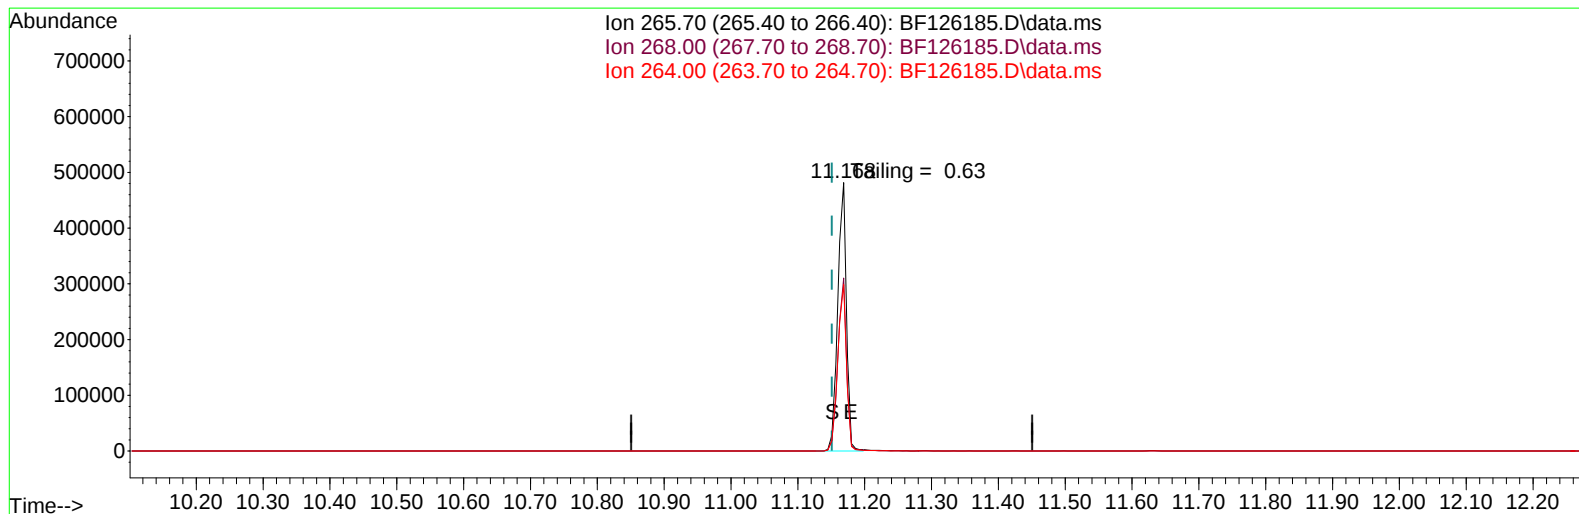

TIC: BF126185.D\data.ms

(70) Pentachlorophenol (C)

11.168min (+ 0.018) 0.00 ng

response 439771

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.46
264.00	69.90	62.00
0.00	0.00	0.00