
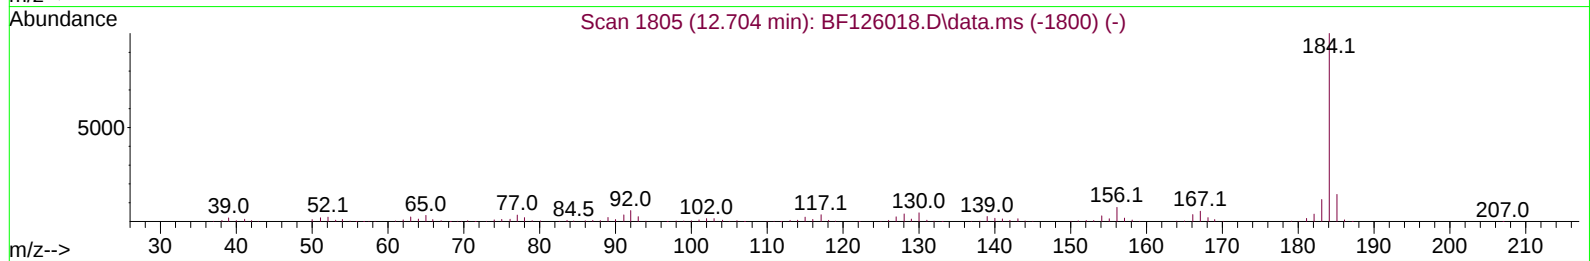
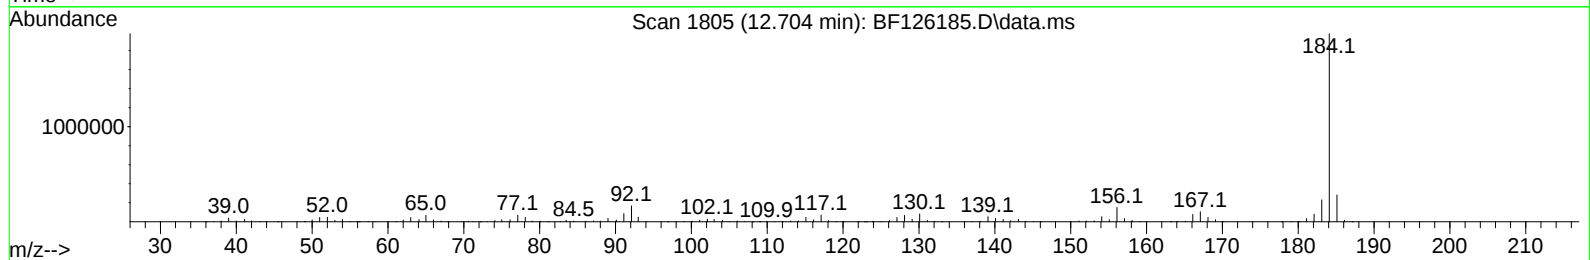


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF120321\  
Data File : BF126185.D  
Acq On : 3 Dec 2021 10:32  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 16:49:23 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF120321.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Dec 03 16:45:52 2021  
Response via : Initial Calibration

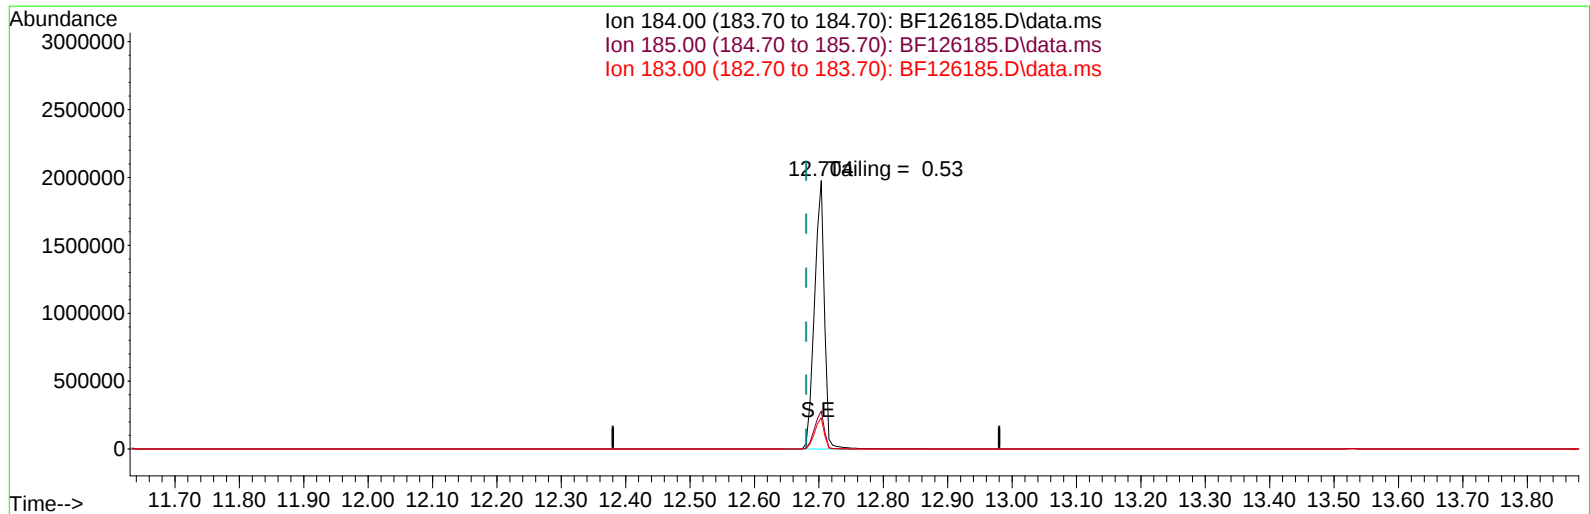

TIC: BF126185.D\data.ms

**(77) Benzidine**

12.704min (+ 0.023) 0.00 ng

response 2117624

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 14.20  |
| 183.00 | 10.10  | 11.64  |
| 0.00   | 0.00   | 0.00   |