
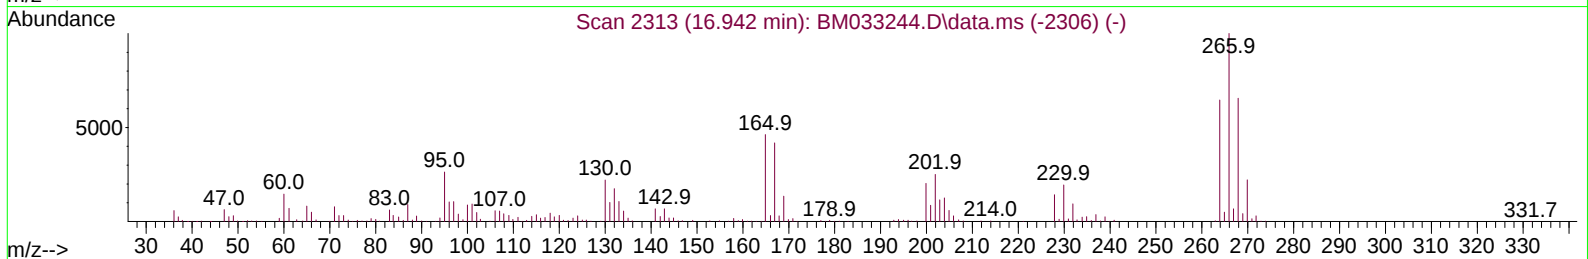
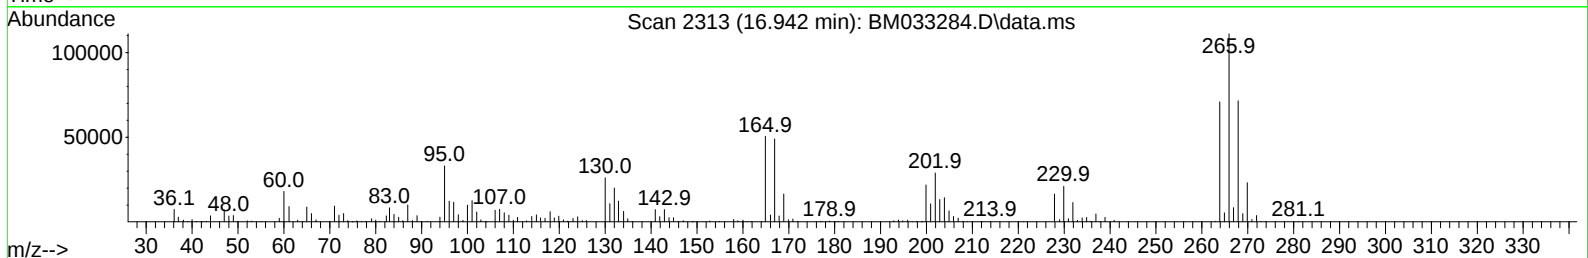


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120321\
 Data File : BM033284.D
 Acq On : 03 Dec 2021 13:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 14:36:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

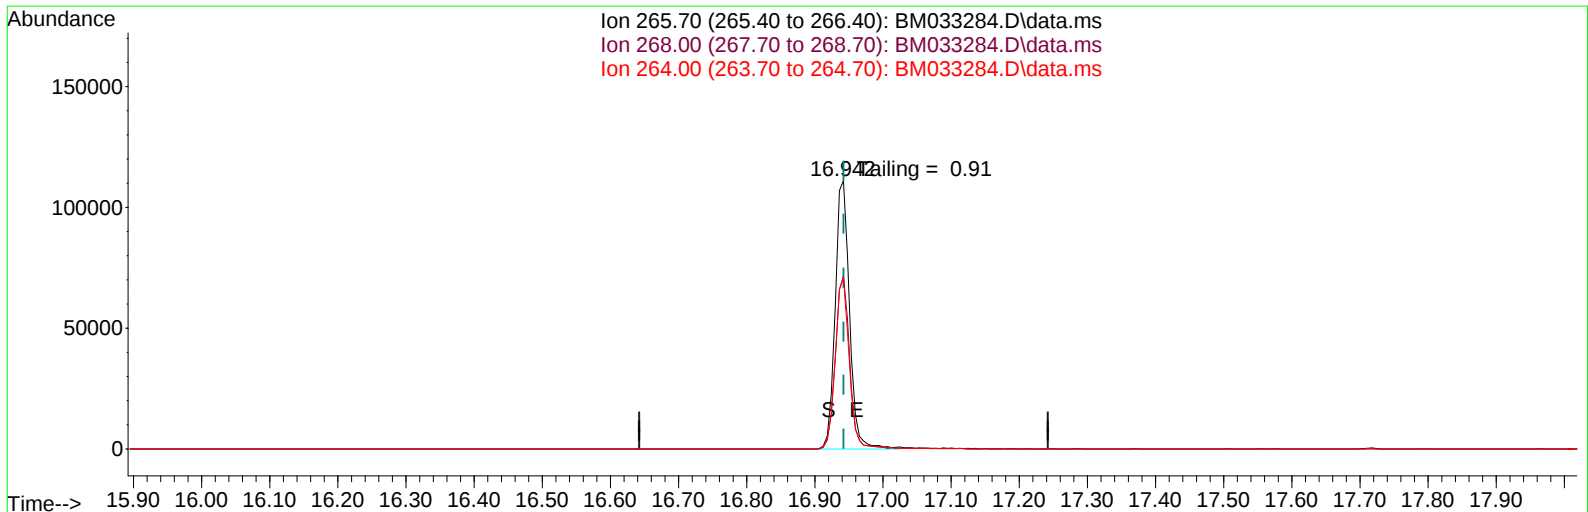

TIC: BM033284.D\data.ms

(70) Pentachlorophenol (C)




16.942min (-0.000) 0.00 ng

response 161812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.43
264.00	65.10	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120321\
 Data File : BM033284.D
 Acq On : 03 Dec 2021 13:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 03 14:36:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

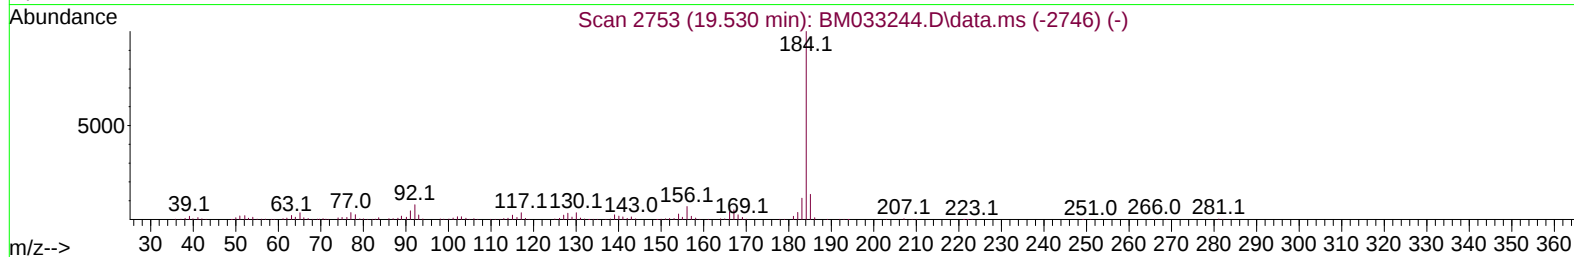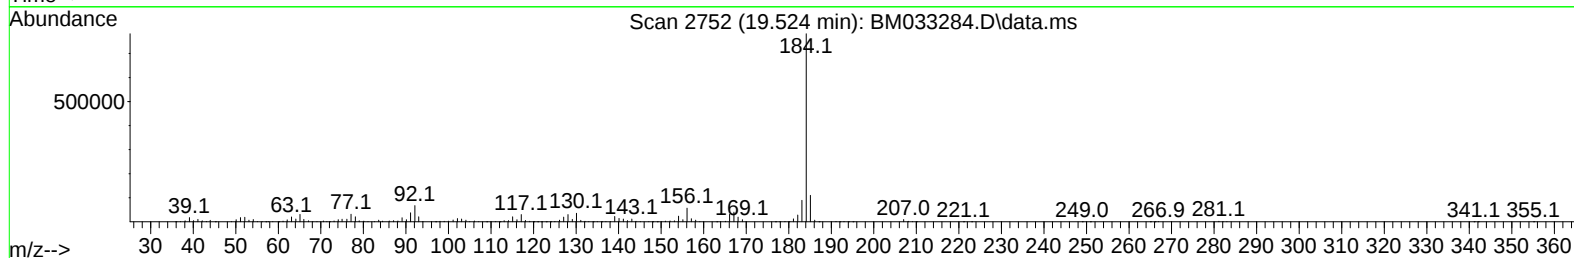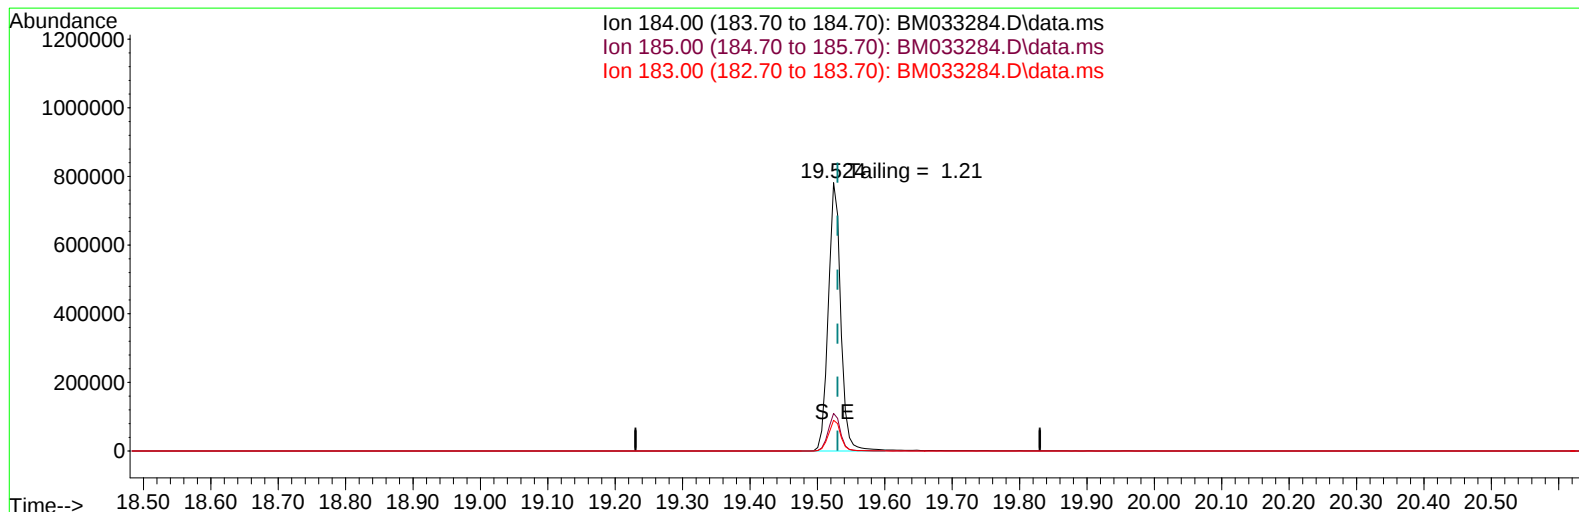

TIC: BM033284.D\data.ms

(77) Benzidine**19.524min (-0.006) 481841.66 ng****response 1007654**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.05
183.00	11.20	11.46
0.00	0.00	0.00