

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120321\
 Data File : BM033287.D
 Acq On : 03 Dec 2021 15:37
 Operator : CG/JU
 Sample : M4798-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-1-4.5

Quant Time: Dec 03 16:08:13 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	120753	20.000	ng	0.00
21) Naphthalene-d8	10.725	136	489112	20.000	ng	#-0.01
39) Acenaphthene-d10	14.554	164	311052	20.000	ng	0.00
64) Phenanthrene-d10	17.295	188	629249	20.000	ng	# 0.00
76) Chrysene-d12	21.447	240	618923	20.000	ng	# 0.00
86) Perylene-d12	23.783	264	646849	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.519	112	909522	124.383	ng	0.01
7) Phenol-d6	7.119	99	1206826	123.231	ng	0.02
23) Nitrobenzene-d5	9.089	82	862613	81.874	ng	-0.01
42) 2,4,6-Tribromophenol	16.042	330	358458	105.716	ng	0.00
45) 2-Fluorobiphenyl	13.177	172	1599794	72.534	ng	0.00
79) Terphenyl-d14	19.901	244	2378068	75.977	ng	0.00
Target Compounds						
						Qvalue
38) 1-Methylnaphthalene	12.601	142	209348	12.216	ng	100
52) Acenaphthene	14.618	154	74992	4.373	ng	95
55) Dibenzofuran	14.954	168	74412	2.609	ng	# 1
58) Fluorene	15.601	166	132226	5.922	ng	# 81
60) Diethylphthalate	15.360	149	66630	3.038	ng	# 66
71) Phenanthrene	17.336	178	207413	5.997	ng	# 81
75) Fluoranthene	19.342	202	99897	2.513	ng	83
78) Pyrene	19.701	202	172056	4.223	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120321\
Data File : BM033287.D
Acq On : 03 Dec 2021 15:37
Operator : CG/JU
Sample : M4798-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-1-4.5

Quant Time: Dec 03 16:08:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 24 15:16:33 2021
Response via : Initial Calibration




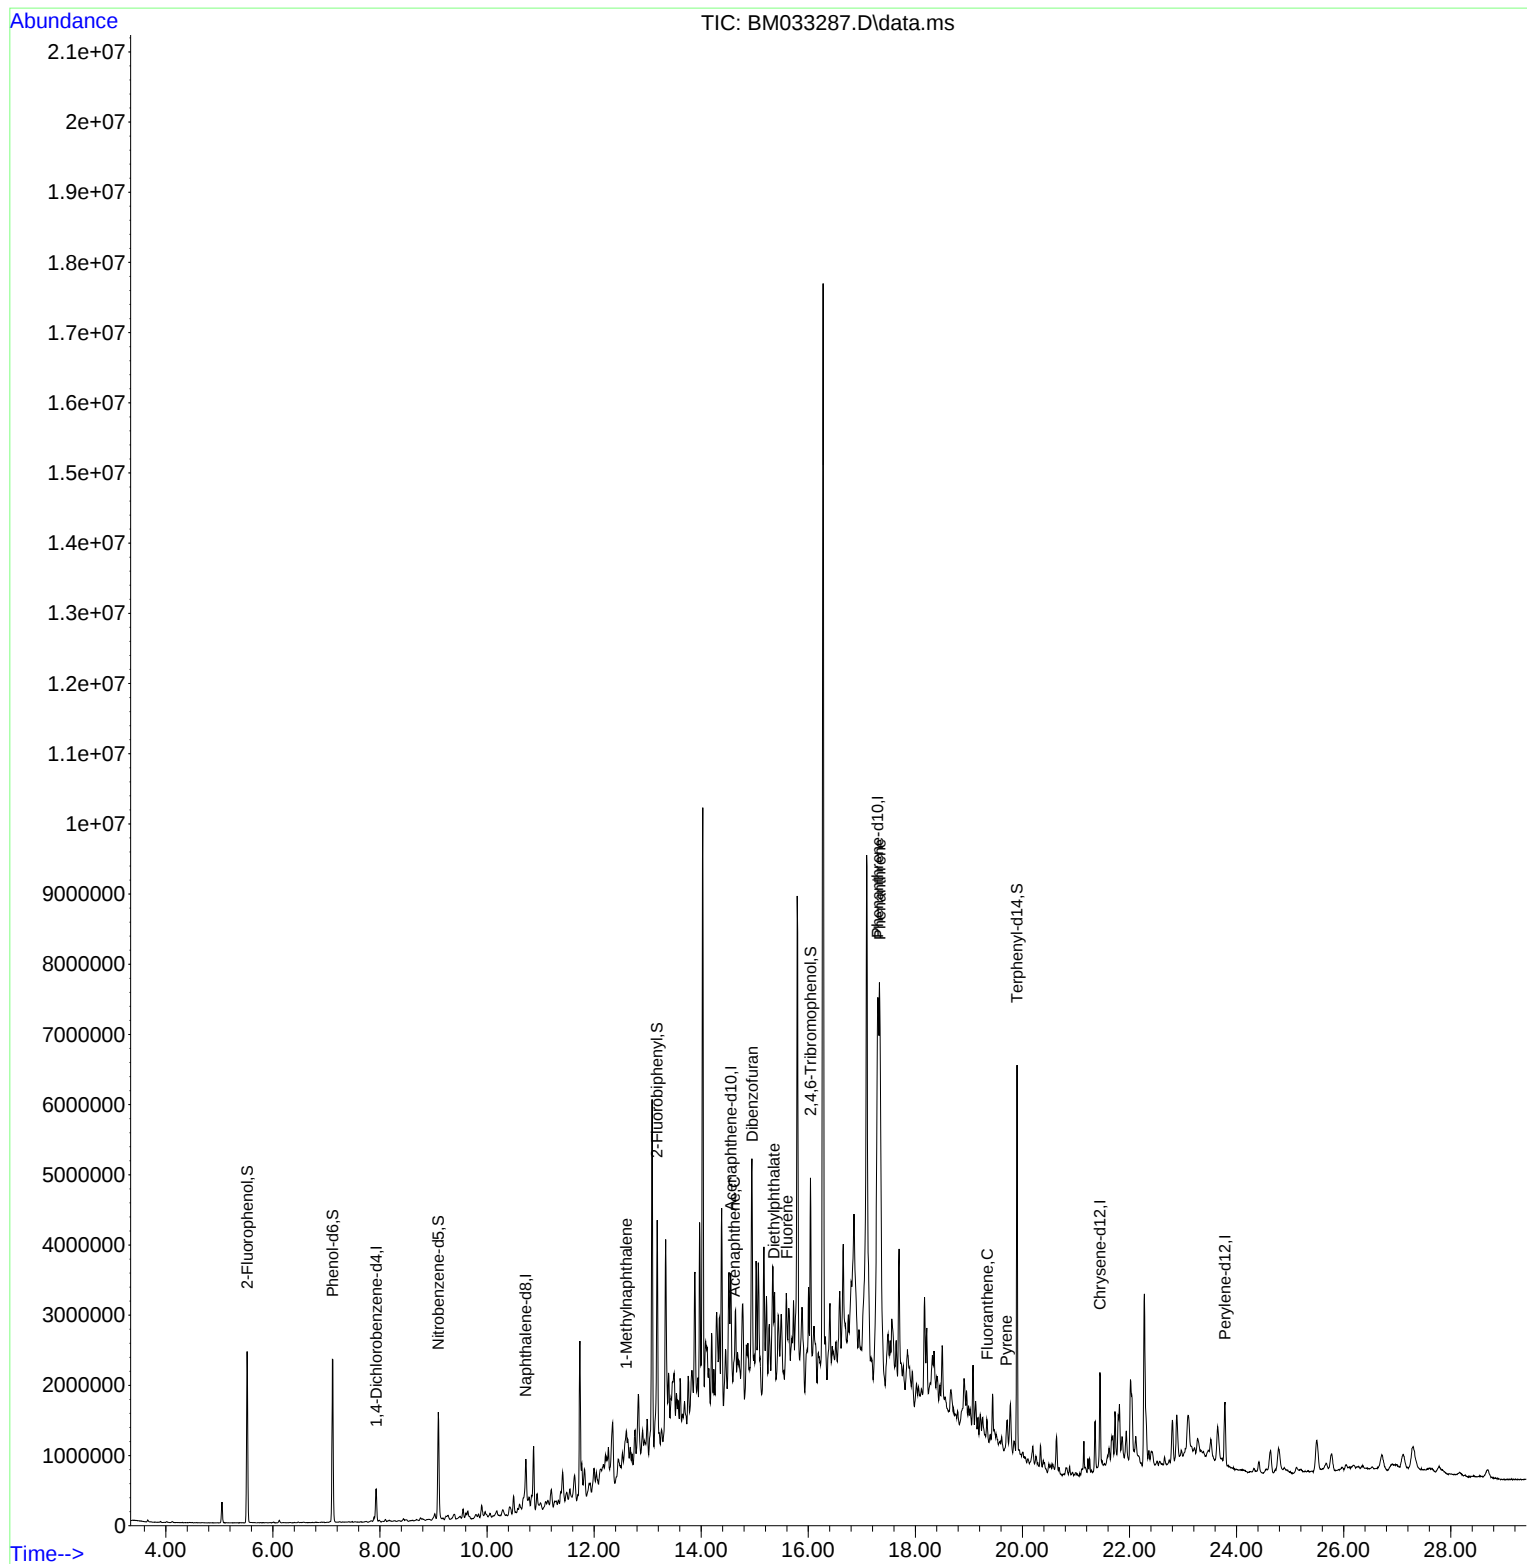




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.931 min Scan# 71
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion:152 Resp: 120753
Ion Ratio Lower Upper
152 100
150 157.3 122.4 183.6
115 63.3 53.8 80.8

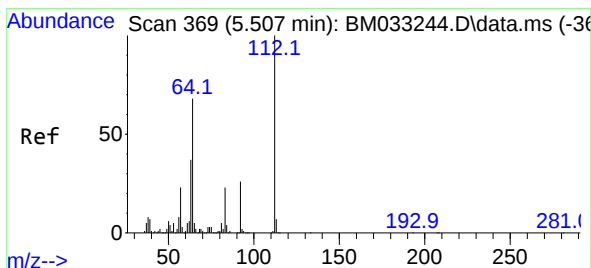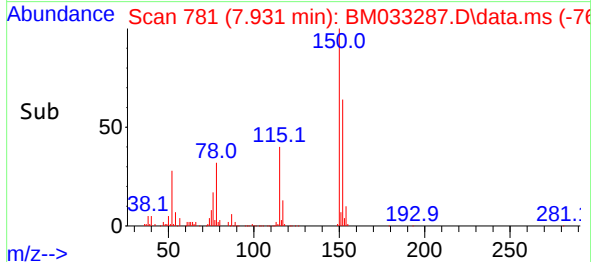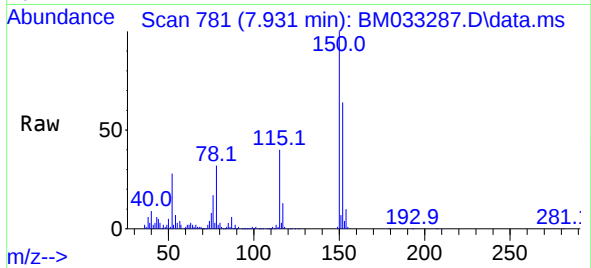

#5
2-Fluorophenol
Concen: 124.383 ng
RT: 5.519 min Scan# 371
Delta R.T. 0.012 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion:112 Resp: 909522
Ion Ratio Lower Upper
112 100
64 68.9 53.7 80.5
63 37.9 33.9 50.9


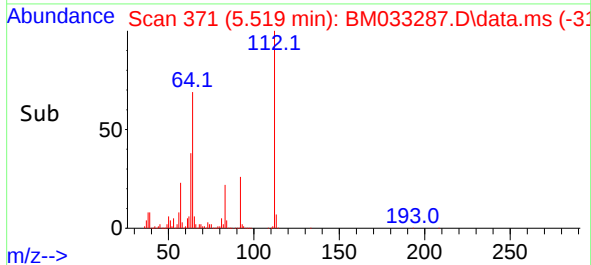

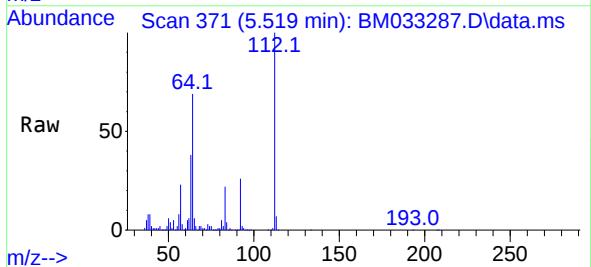




#7
Phenol-d6
Concen: 123.231 ng
RT: 7.119 min Scan# 64
Delta R.T. 0.023 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion: 99 Resp: 1206826
Ion Ratio Lower Upper
99 100
42 22.3 23.0 34.6#
71 38.3 37.8 56.8

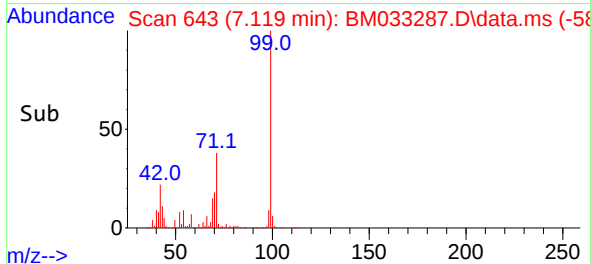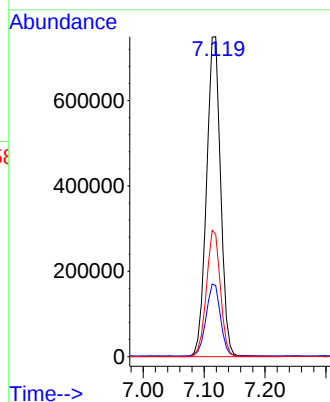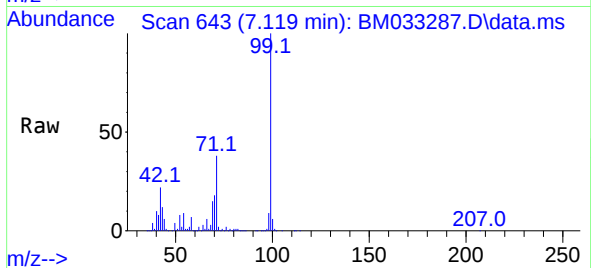

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.725 min Scan# 1256
Delta R.T. -0.012 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion:136 Resp: 489112
Ion Ratio Lower Upper
136 100
137 11.2 8.7 13.1
54 11.2 7.4 11.0#
68 8.8 3.8 5.8#


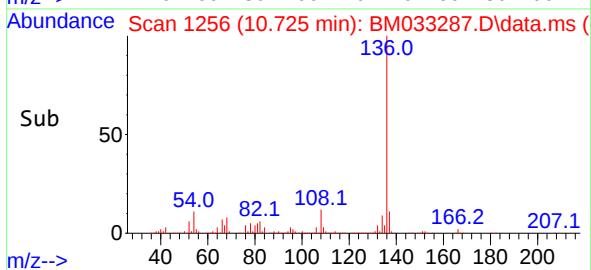

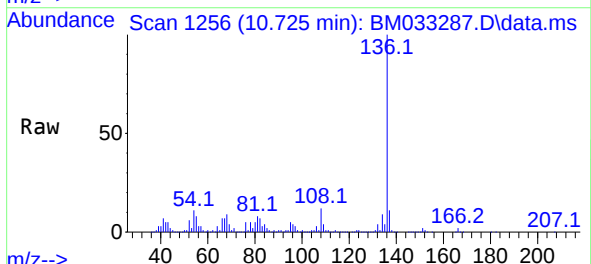




#23
Nitrobenzene-d5
Concen: 81.874 ng
RT: 9.089 min Scan# 91
Delta R.T. -0.012 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion: 82 Resp: 862613
Ion Ratio Lower Upper
82 100
128 36.9 29.0 43.6
54 55.2 45.8 68.8

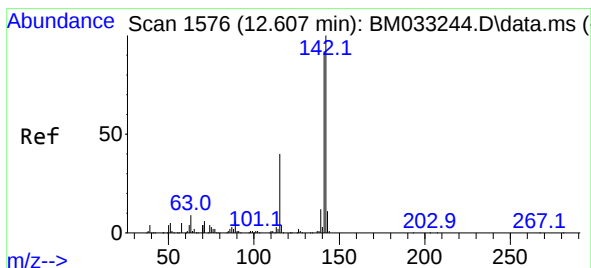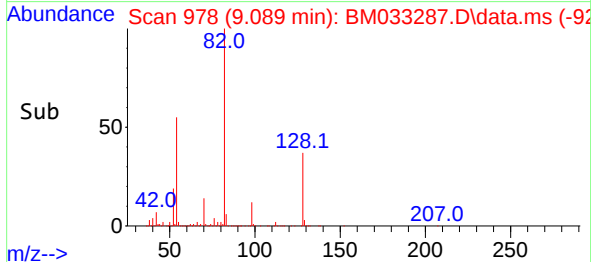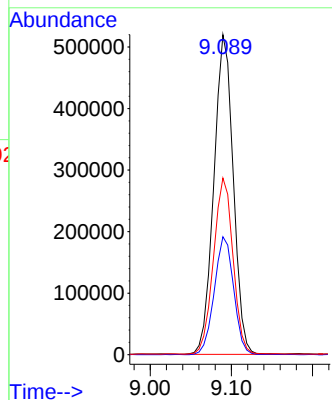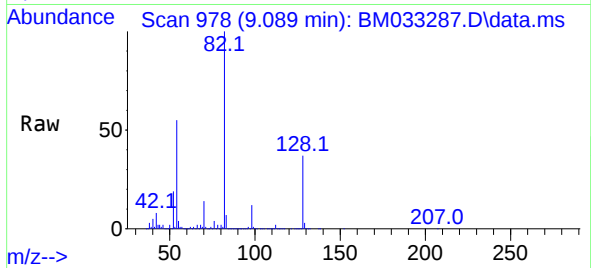

#38
1-Methylnaphthalene
Concen: 12.216 ng
RT: 12.601 min Scan# 1575
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion: 142 Resp: 209348
Ion Ratio Lower Upper
142 100
141 94.4 75.6 113.4
116 5.8 4.0 6.0


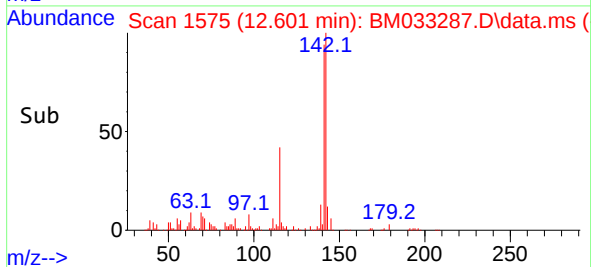
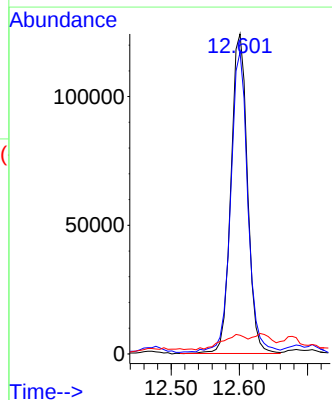
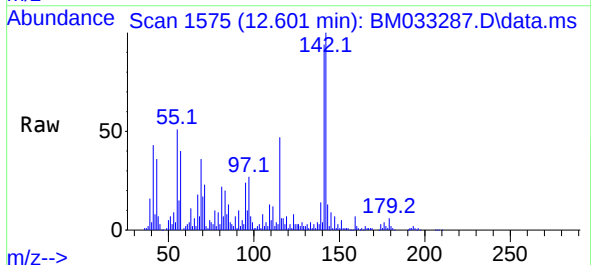




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.554 min Scan# 1908
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion:164 Resp: 311052
Ion Ratio Lower Upper
164 100
162 99.3 80.6 121.0
160 44.0 35.1 52.7

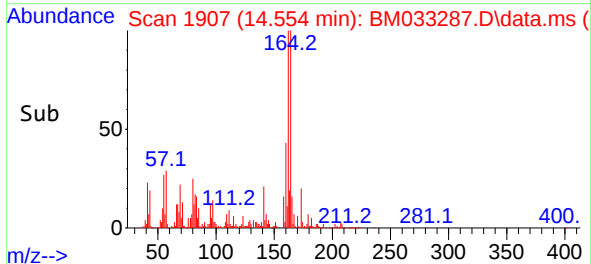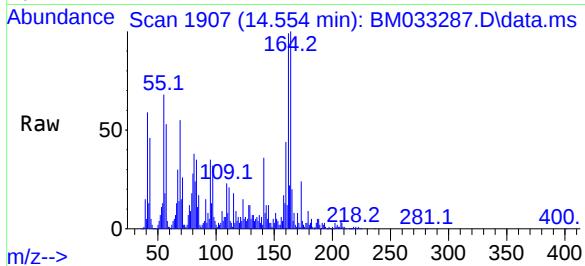

#42
2,4,6-Tribromophenol
Concen: 105.716 ng
RT: 16.042 min Scan# 2160
Delta R.T. -0.000 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion:330 Resp: 358458
Ion Ratio Lower Upper
330 100
332 97.7 75.7 113.5
141 49.6 50.7 76.1#


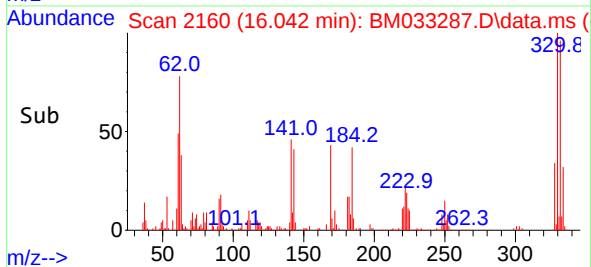

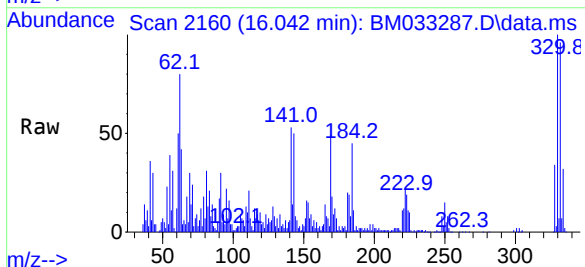




#45
2-Fluorobiphenyl
Concen: 72.534 ng
RT: 13.177 min Scan# 1
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion:172 Resp: 1599794
Ion Ratio Lower Upper
172 100
171 34.9 28.1 42.1
170 22.6 18.6 27.8

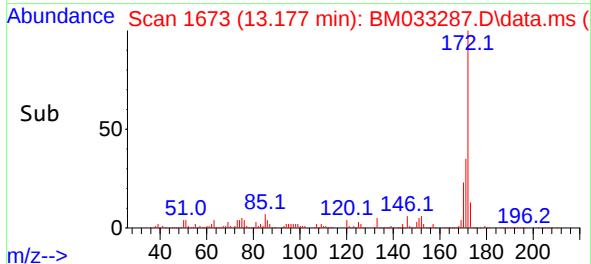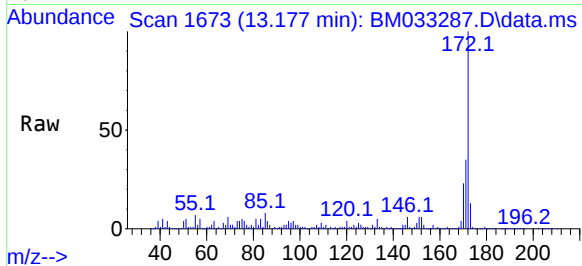

#52
Acenaphthene
Concen: 4.373 ng
RT: 14.618 min Scan# 1918
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion:154 Resp: 74992
Ion Ratio Lower Upper
154 100
153 117.5 92.4 138.6
152 62.9 43.7 65.5


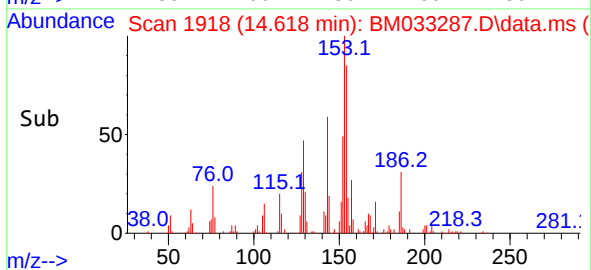

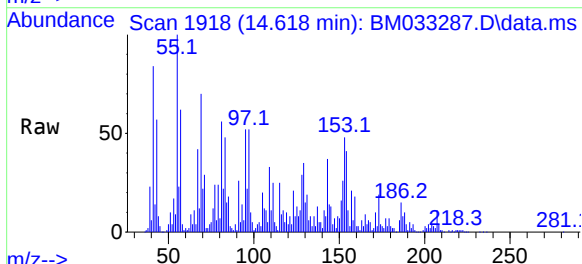




#55
Dibenzenofuran
Concen: 2.609 ng
RT: 14.954 min Scan# 1976
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion:168 Resp: 74412
Ion Ratio Lower Upper
168 100
139 90.5 35.0 52.4#
169 172.2 10.8 16.2#

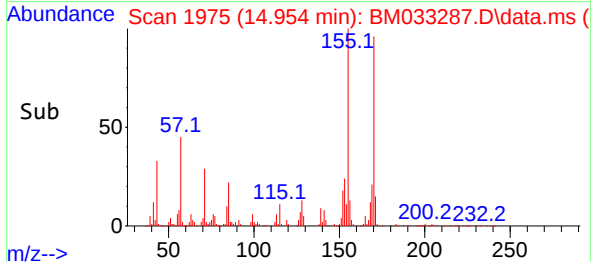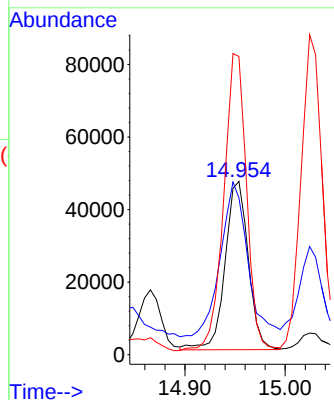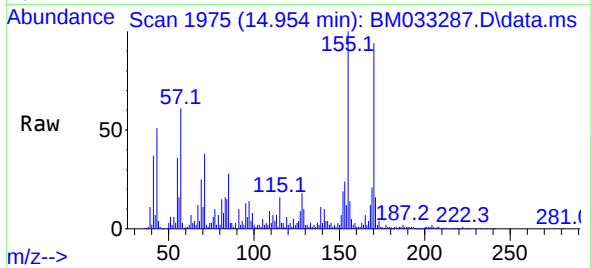

#58
Fluorene
Concen: 5.922 ng
RT: 15.601 min Scan# 2085
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion:166 Resp: 132226
Ion Ratio Lower Upper
166 100
165 115.3 79.3 118.9
167 29.3 10.6 16.0#


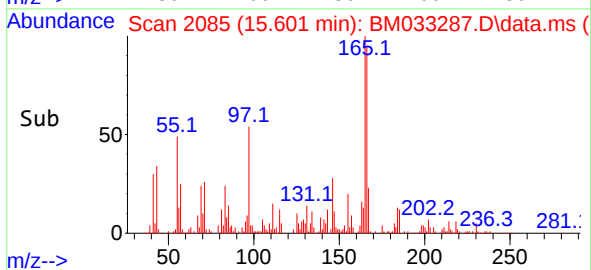
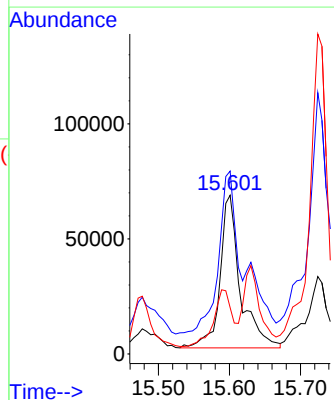
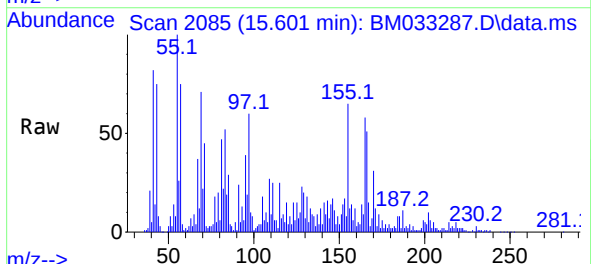




#60
Diethylphthalate
Concen: 3.038 ng
RT: 15.360 min Scan# 2044
Delta R.T. -0.018 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion:149 Resp: 66630
Ion Ratio Lower Upper
149 100
177 35.5 15.7 23.5#
150 24.7 9.6 14.4#

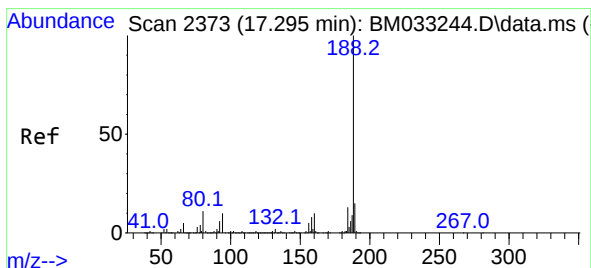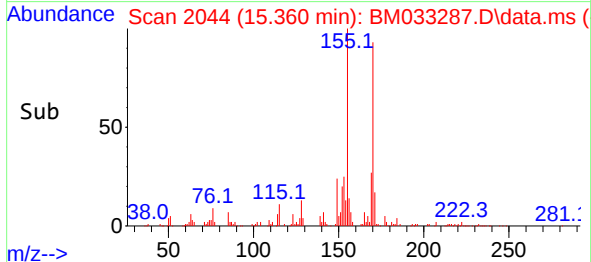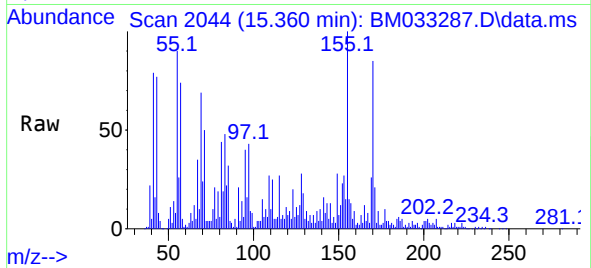

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.295 min Scan# 2373
Delta R.T. -0.000 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion:188 Resp: 629249
Ion Ratio Lower Upper
188 100
94 12.0 6.3 9.5#
80 13.5 7.3 10.9#


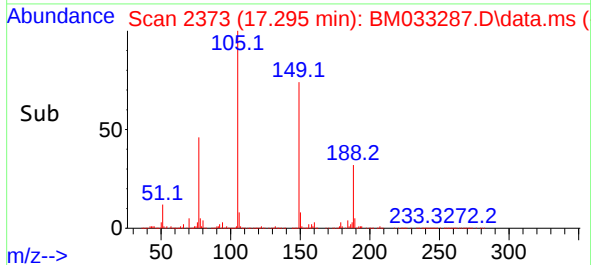

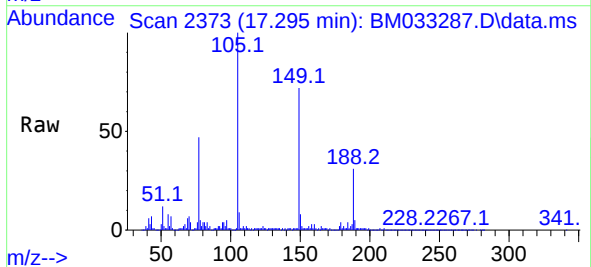




#71
Phenanthrene
Concen: 5.997 ng
RT: 17.336 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion:178 Resp: 207413
Ion Ratio Lower Upper
178 100
176 20.3 15.6 23.4
179 32.6 12.4 18.6#

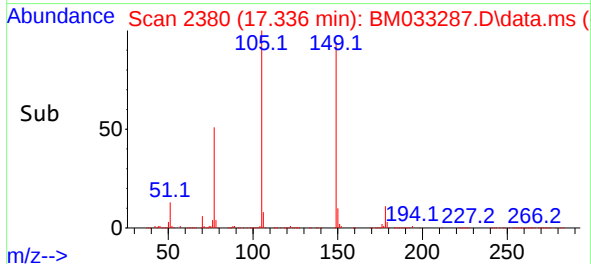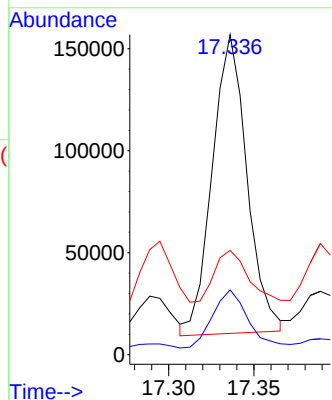

#75
Fluoranthene
Concen: 2.513 ng
RT: 19.342 min Scan# 2721
Delta R.T. -0.000 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion:202 Resp: 99897
Ion Ratio Lower Upper
202 100
101 15.8 0.0 29.9
203 24.3 0.0 36.8


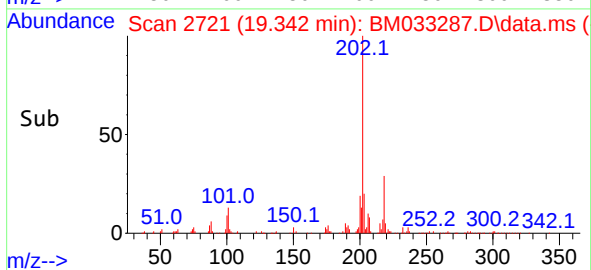
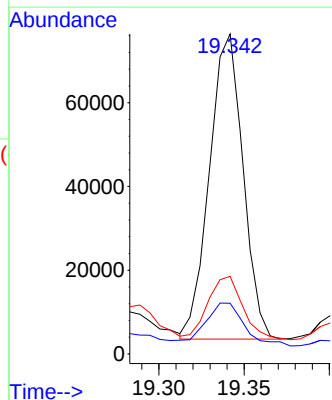
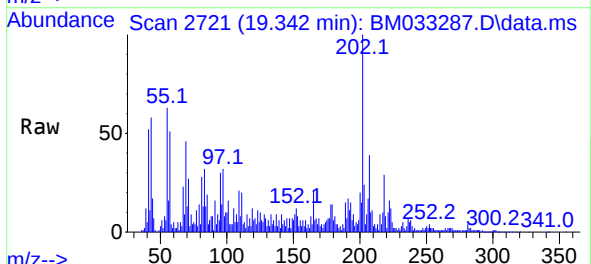


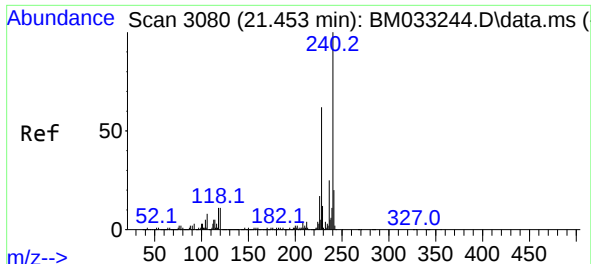

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.447 min Scan# 30
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37




Instrument :
BNA_M
ClientSampleId :
SB-1-4.5


Tgt Ion:240 Resp: 618923
Ion Ratio Lower Upper
240 100
120 12.0 7.8 11.6#
236 25.2 20.9 31.3

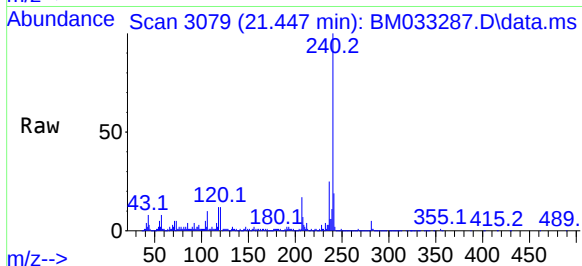

#78
Pyrene
Concen: 4.223 ng
RT: 19.701 min Scan# 2782
Delta R.T. -0.006 min
Lab File: BM033287.D
Acq: 03 Dec 2021 15:37

Tgt Ion:202 Resp: 172056
Ion Ratio Lower Upper
202 100
200 20.3 16.6 25.0
203 22.3 13.7 20.5#


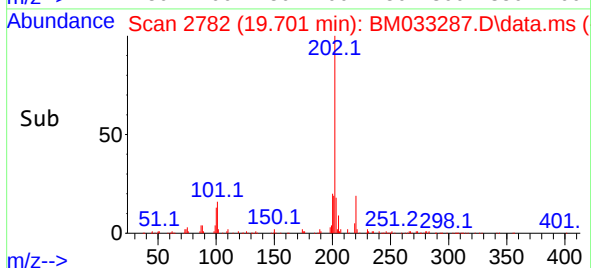
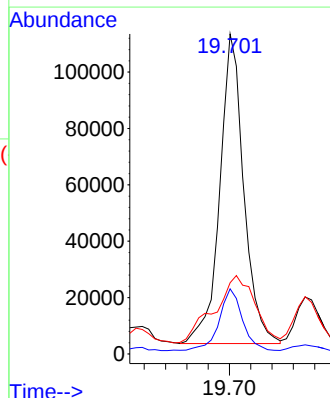
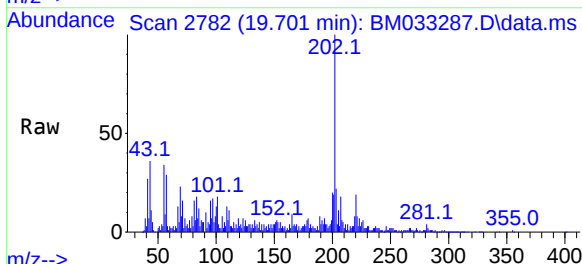




#79
 Terphenyl-d14
 Concen: 75.977 ng
 RT: 19.901 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BM033287.D
 Acq: 03 Dec 2021 15:37

Instrument :
 BNA_M
 ClientSampleId :
 SB-1-4.5

Tgt Ion:244 Resp: 2378068
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.5 9.7
 122 11.6 8.7 13.1

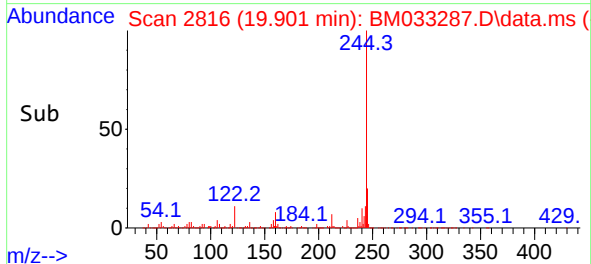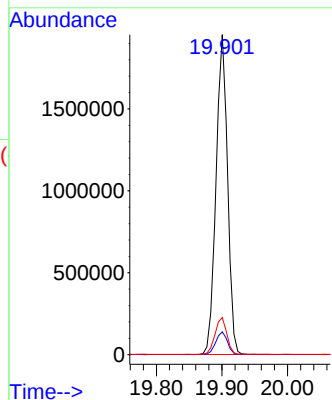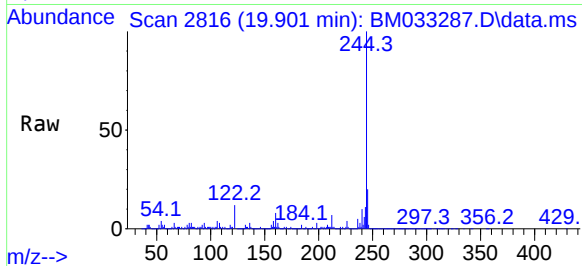

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.783 min Scan# 3476
 Delta R.T. -0.006 min
 Lab File: BM033287.D
 Acq: 03 Dec 2021 15:37

Tgt Ion:264 Resp: 646849
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.3 28.9
 265 22.1 18.3 27.5

