
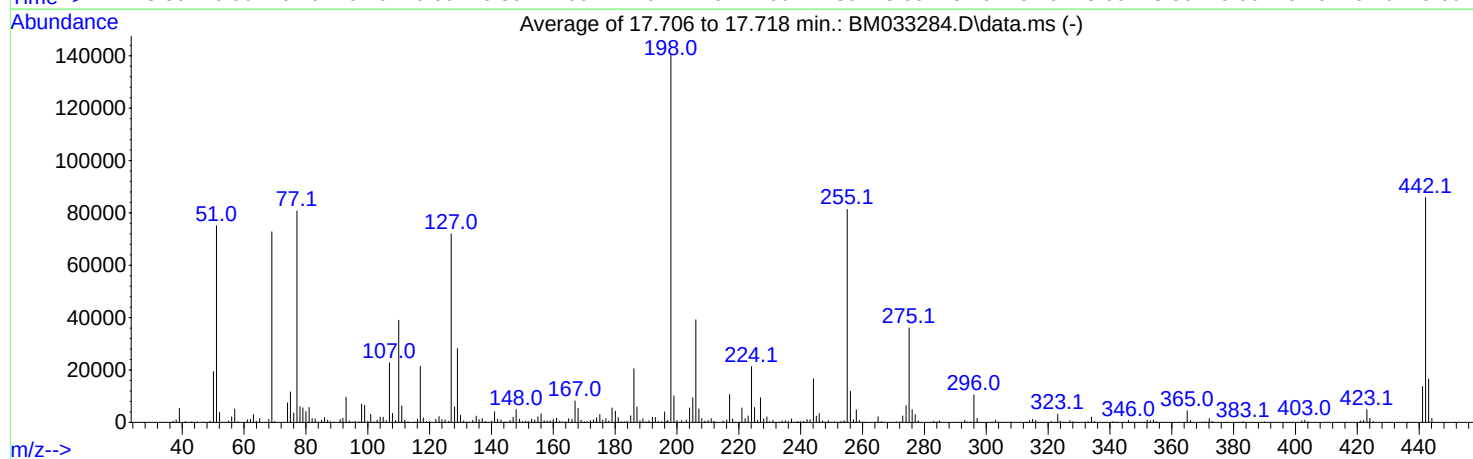


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120321\
 Data File : BM033284.D
 Acq On : 03 Dec 2021 13:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 06 13:01:33 2021

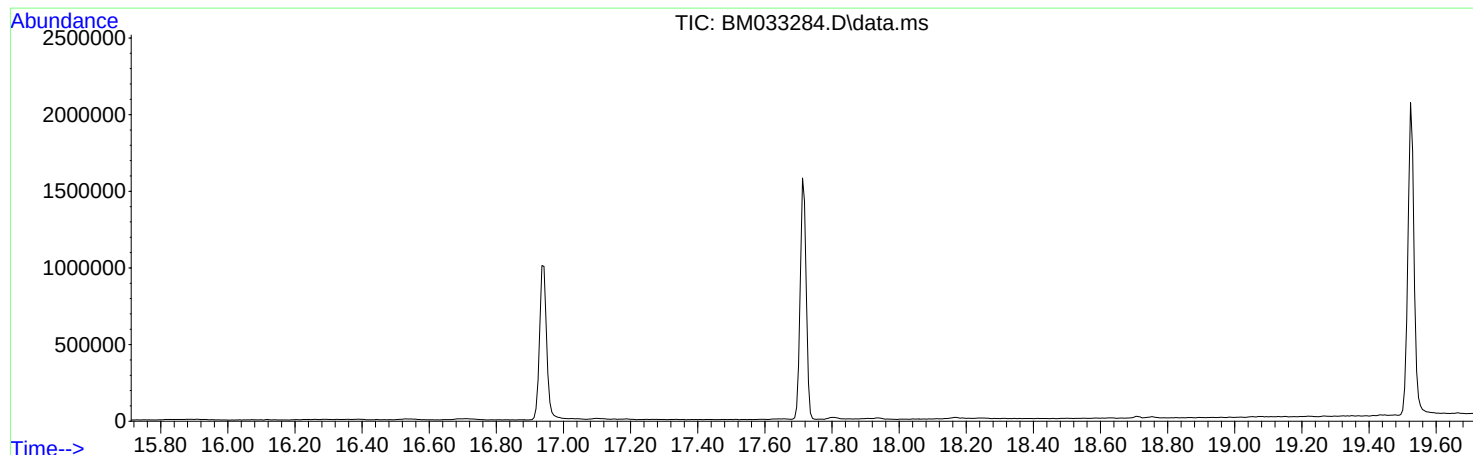




AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.4	75083	PASS
68	69	0.00	2	1.6	1142	PASS
69	198	0.00	100	51.8	72755	PASS
70	69	0.00	2	0.5	328	PASS
127	198	10	80	51.3	72008	PASS
197	198	0.00	2	0.5	734	PASS
198	198	100	100	100.0	140493	PASS
199	198	5	9	7.2	10176	PASS
275	198	10	60	25.7	36059	PASS
365	198	1	100	3.1	4419	PASS
441	198	0.01	100	9.7	13694	PASS
442	442	50	100	100.0	85915	PASS
443	442	15	24	19.3	16567	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120321\
 Data File : BM033284.D
 Acq On : 03 Dec 2021 13:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Dec 03 14:36:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

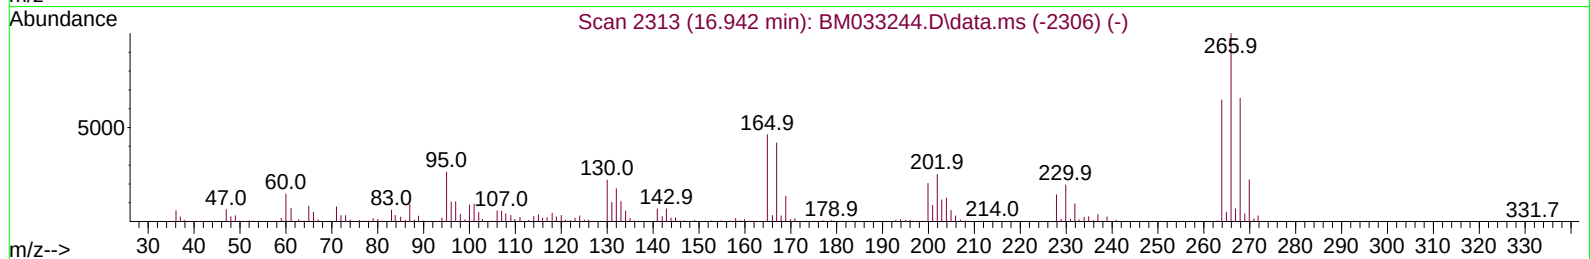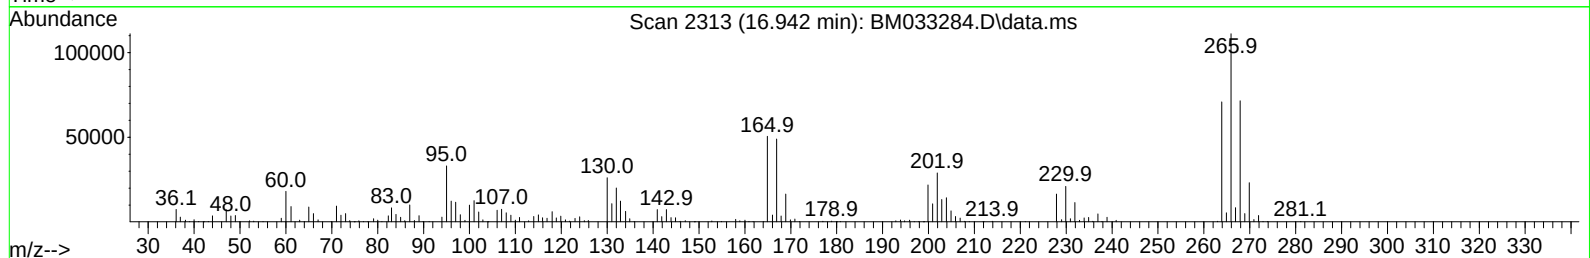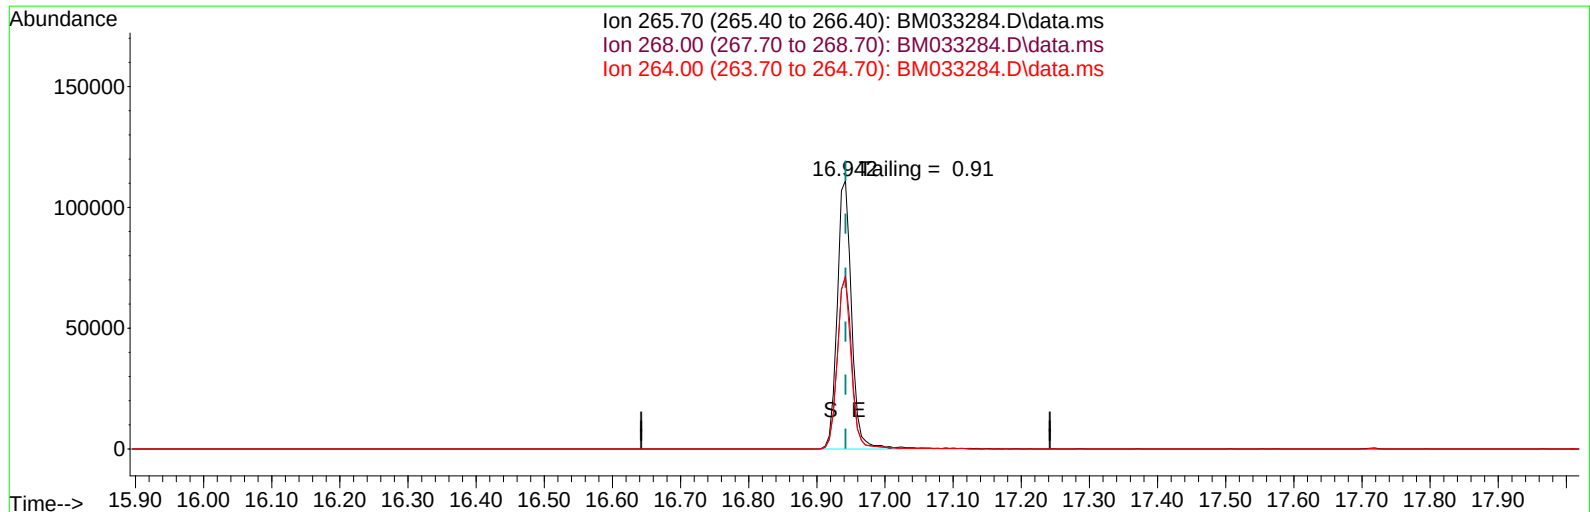

TIC: BM033284.D\data.ms

(70) Pentachlorophenol (C)

16.942min (-0.000) 0.00 ng




response 161812

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.43
264.00	65.10	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120321\
 Data File : BM033284.D
 Acq On : 03 Dec 2021 13:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Dec 03 14:36:10 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

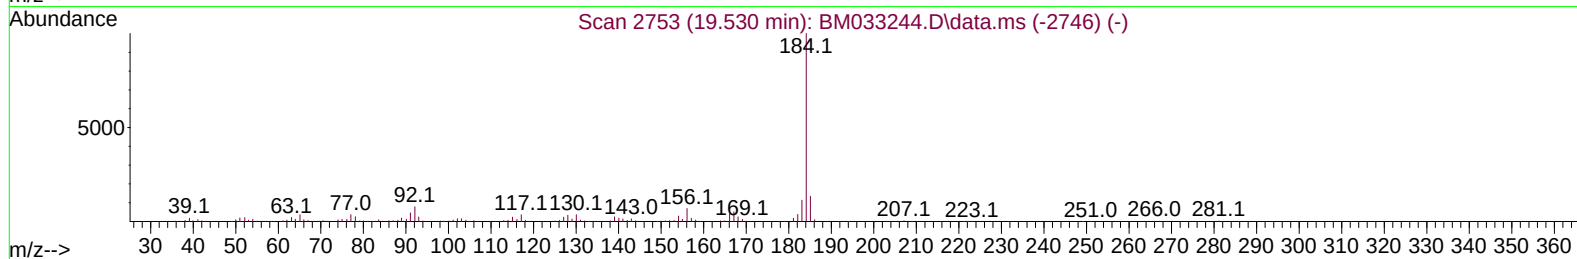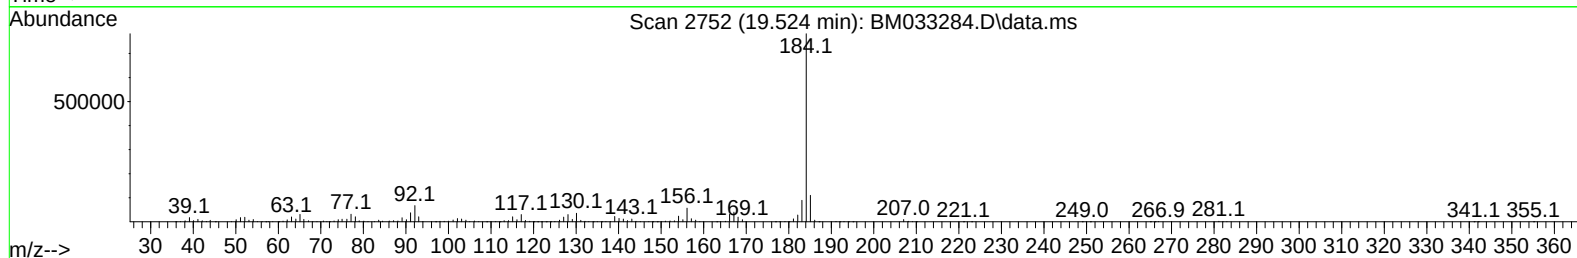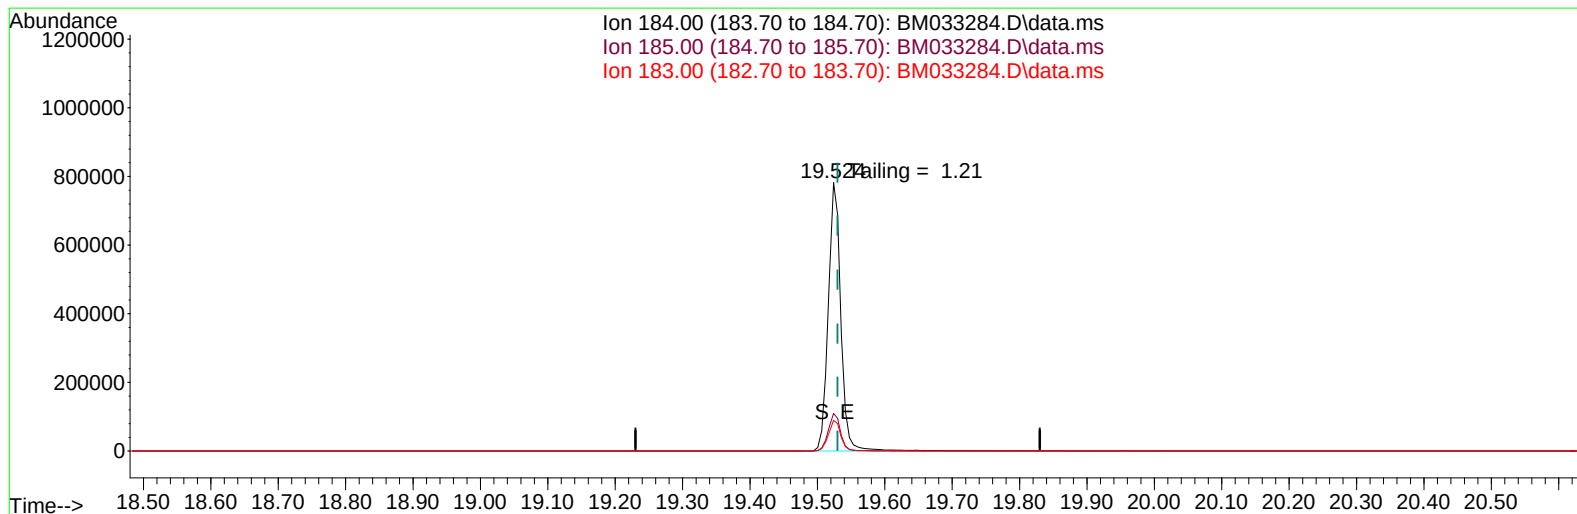

TIC: BM033284.D\data.ms

(77) Benzidine

19.524min (-0.006) 481841.66 ng

response 1007654

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	14.05
183.00	11.20	11.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/3/2021	BNA_M	<u>BM033284.D</u>
Compound Name	Response	Retention Time
DDT	487909	20.74
DDD	2828	20.31
DDE	244	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3072	490981	0.63

Instrument :
BNA_M
ClientSampleId :
DFTPP