
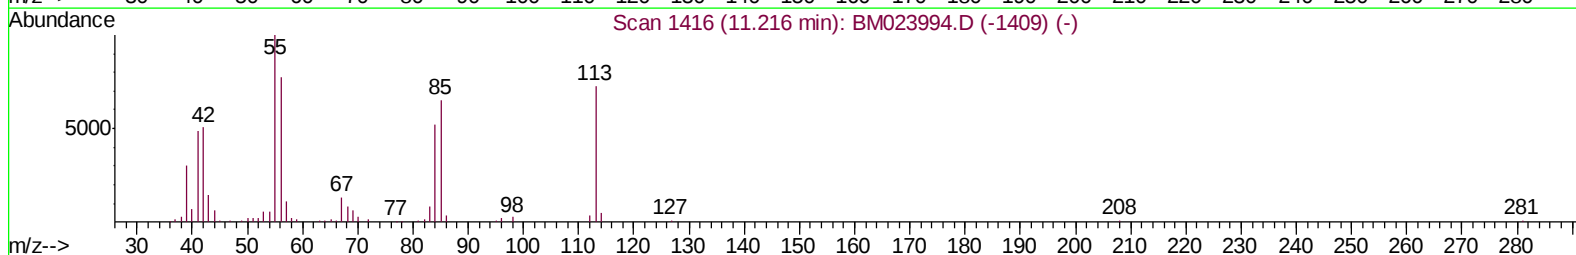
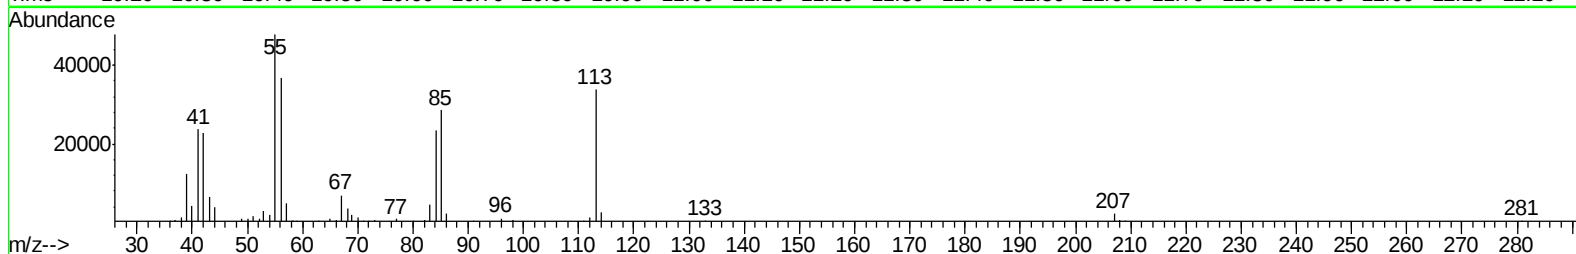


Data File : BM024009.D
Acq On : 04 Dec 2019 19:37
Operator : JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Dec 05 02:49:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 05 02:46:26 2019
Response via : Initial Calibration

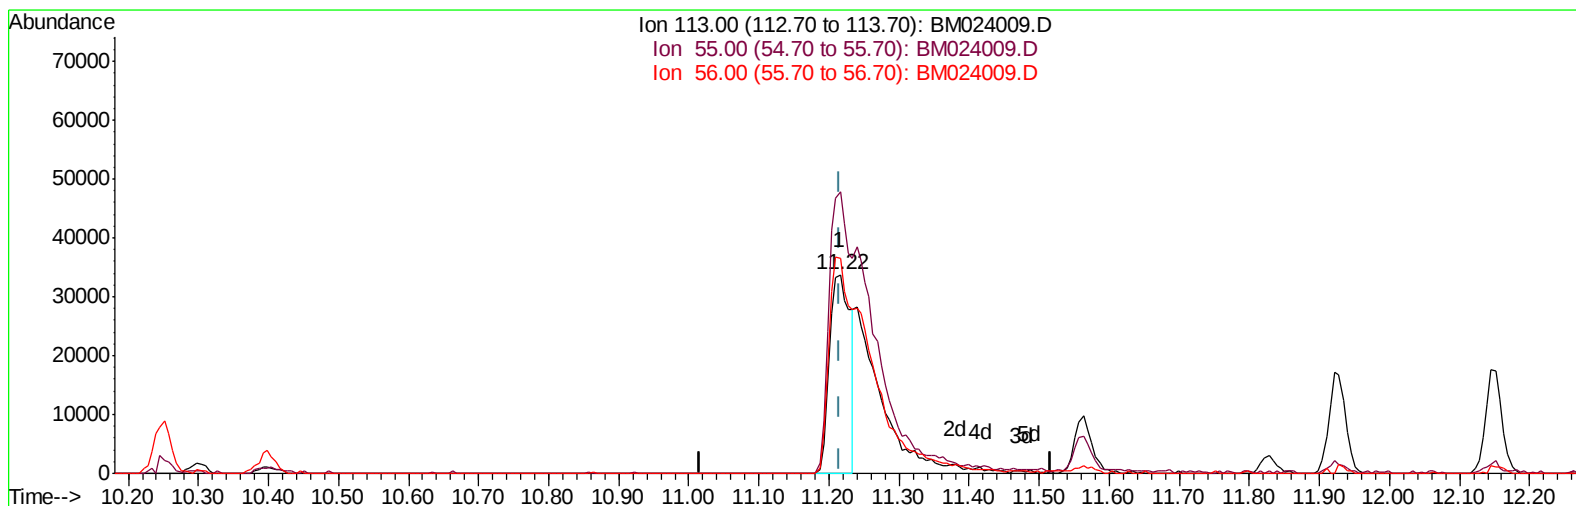

TIC: BM024009.D

(32) Caprolactam

11.216min (-0.000) 9.51ng/ul

response 70838

Ion	Exp%	Act%
113.00	100	100
55.00	137.60	141.61
56.00	106.90	108.43
0.00	0.00	0.00