
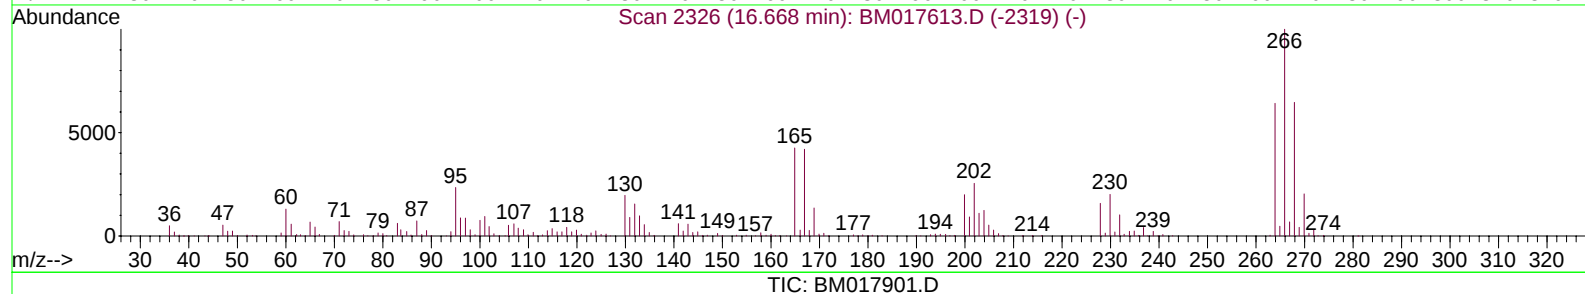
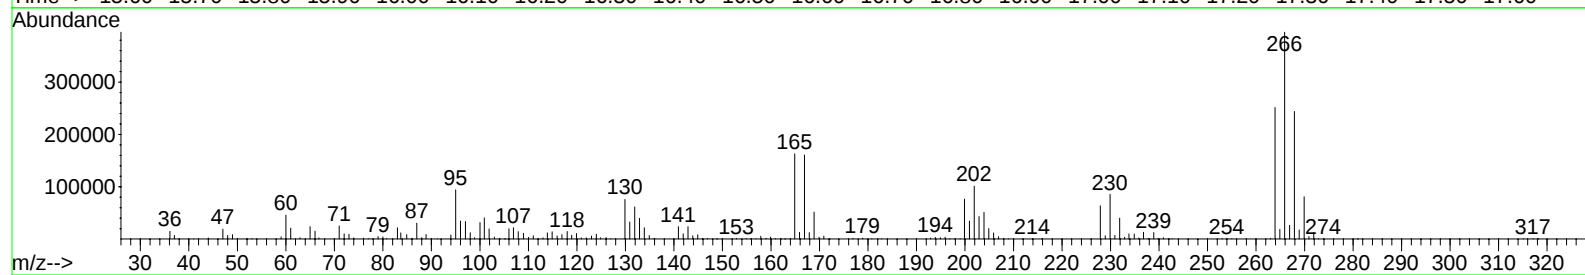


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM120518\
Data File : BM017901.D
Acq On : 04 Dec 2018 13:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 16:02:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

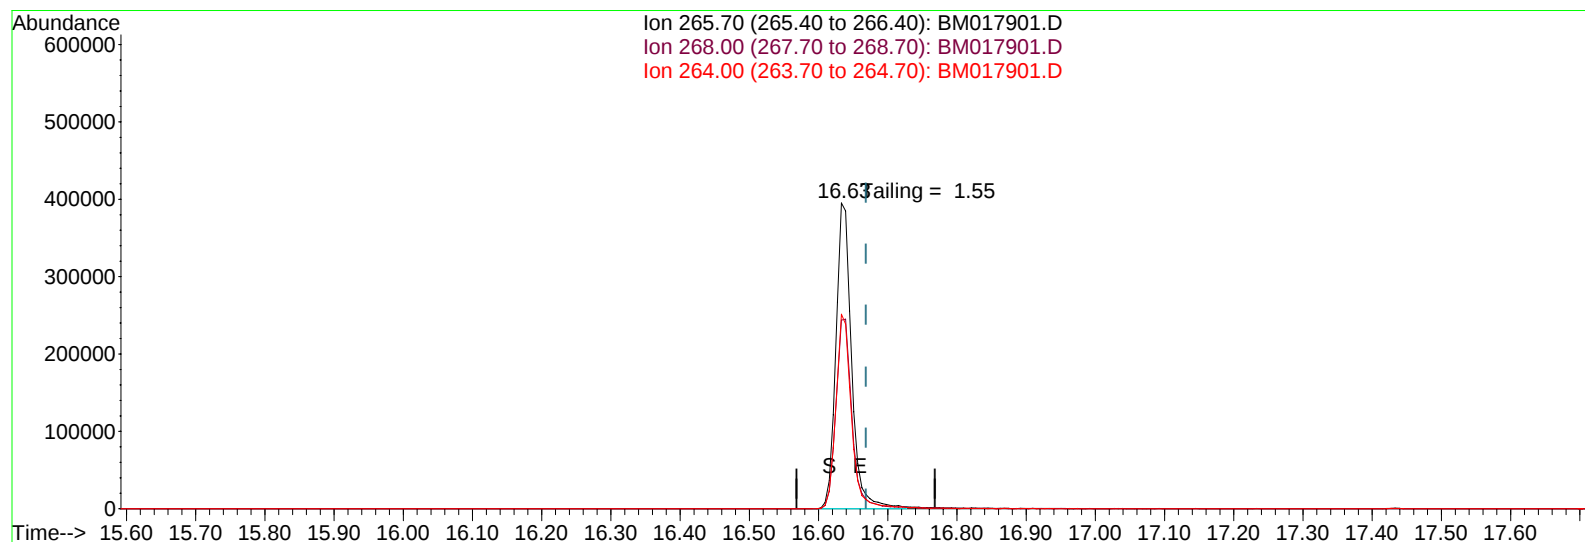

(70) Pentachlorophenol (C)




16.633min (-0.035) 101078.24ng

response 617550

Ion	Exp%	Act%
265.70	100	100
268.00	64.60	61.70
264.00	64.10	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM120518\
Data File : BM017901.D
Acq On : 04 Dec 2018 13:07
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 16:02:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 12 18:37:25 2018
Response via : Initial Calibration

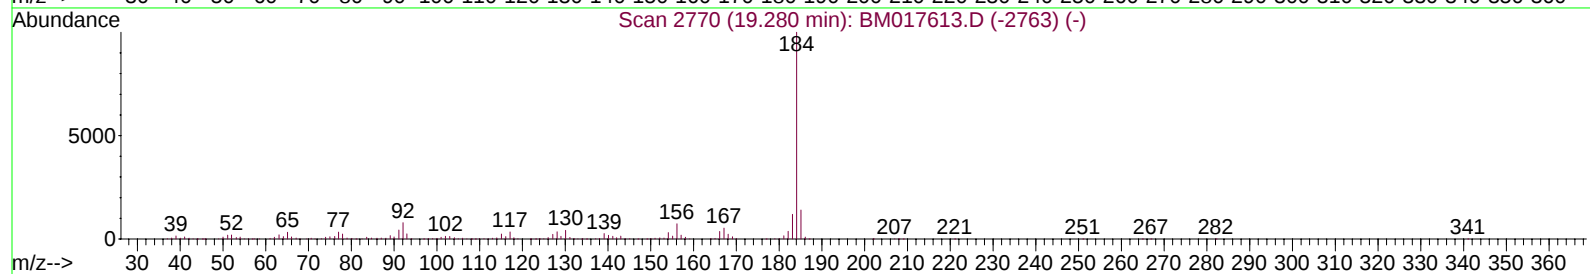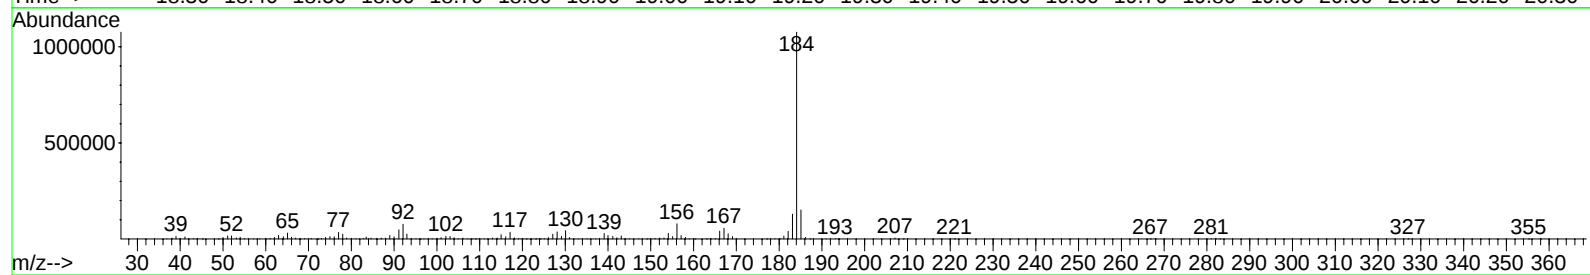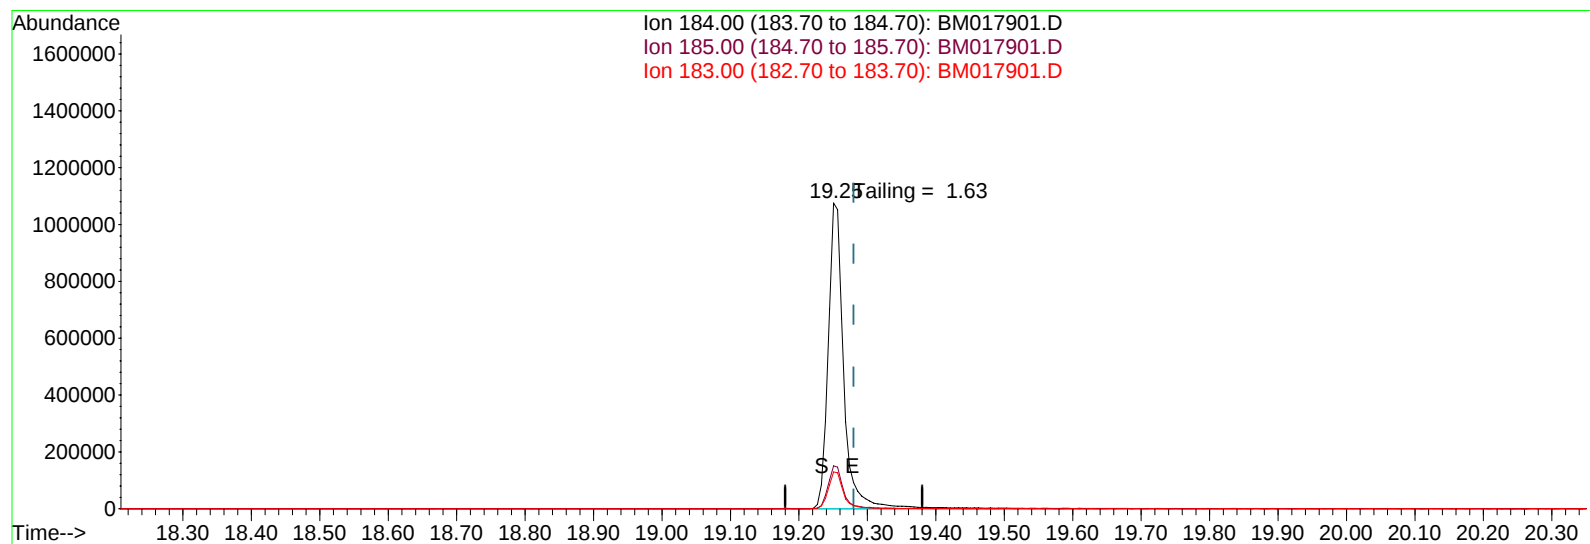

TIC: BM017901.D

(77) Benzidine

19.251min (-0.029) 17297.39ng

response 1667845

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.03
183.00	11.90	12.02
0.00	0.00	0.00