

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120518\
 Data File : BM017905.D
 Acq On : 04 Dec 2018 16:45
 Operator : JU/SJ
 Sample : J6074-05 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 003-WC-NY2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.451	76	79	86	rBV	23720	37739	1.52%	0.124%
2	4.769	298	303	310	rBV	50233	70675	2.85%	0.233%
3	5.210	371	378	392	rBV	1262827	1861227	74.95%	6.131%
4	6.769	636	643	658	rBV	1209738	2109166	84.94%	6.948%
5	7.116	696	702	714	rBV	1367671	2223379	89.54%	7.324%
6	7.581	771	781	788	rBV	1026286	1631374	65.70%	5.374%
7	7.892	827	834	843	rBV	1028842	1642927	66.16%	5.412%
8	8.733	970	977	993	rBV	669006	1239272	49.91%	4.082%
9	10.345	1242	1251	1267	rBV	1195181	2131749	85.85%	7.023%
10	12.839	1668	1675	1690	rBV	1502547	2429223	97.82%	8.002%
11	13.698	1814	1821	1829	rBV	129478	231129	9.31%	0.761%
12	14.227	1904	1911	1919	rBV2	1536985	2436575	98.12%	8.027%
13	14.292	1919	1922	1930	rVB2	18791	28819	1.16%	0.095%
14	15.727	2160	2166	2180	rBV	1027113	1630867	65.67%	5.372%
15	16.633	2317	2320	2326	rVB5	22819	29758	1.20%	0.098%
16	16.980	2373	2379	2385	rBV	1569656	2383578	95.99%	7.852%
17	17.892	2529	2534	2543	rBV3	87792	153459	6.18%	0.506%
18	18.821	2690	2692	2697	rBV6	21771	32670	1.32%	0.108%
19	19.050	2727	2731	2739	rBV	140313	218335	8.79%	0.719%
20	19.180	2750	2753	2760	rBV6	55055	113261	4.56%	0.373%
21	19.415	2789	2793	2797	rBV	119379	160796	6.48%	0.530%
22	19.627	2824	2829	2838	rBV	1681310	2126503	85.63%	7.005%
23	21.115	3078	3082	3086	rBV	494181	569279	22.92%	1.875%
24	21.191	3090	3095	3099	rVV	1806502	2380915	95.88%	7.843%
25	23.374	3460	3466	3474	rVB	1317005	2483251	100.00%	8.180%


Sum of corrected areas: 30355926

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120518\
Data File : BM017905.D
Acq On : 04 Dec 2018 16:45
Operator : JU/SJ
Sample : J6074-05 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
003-WC-NY2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

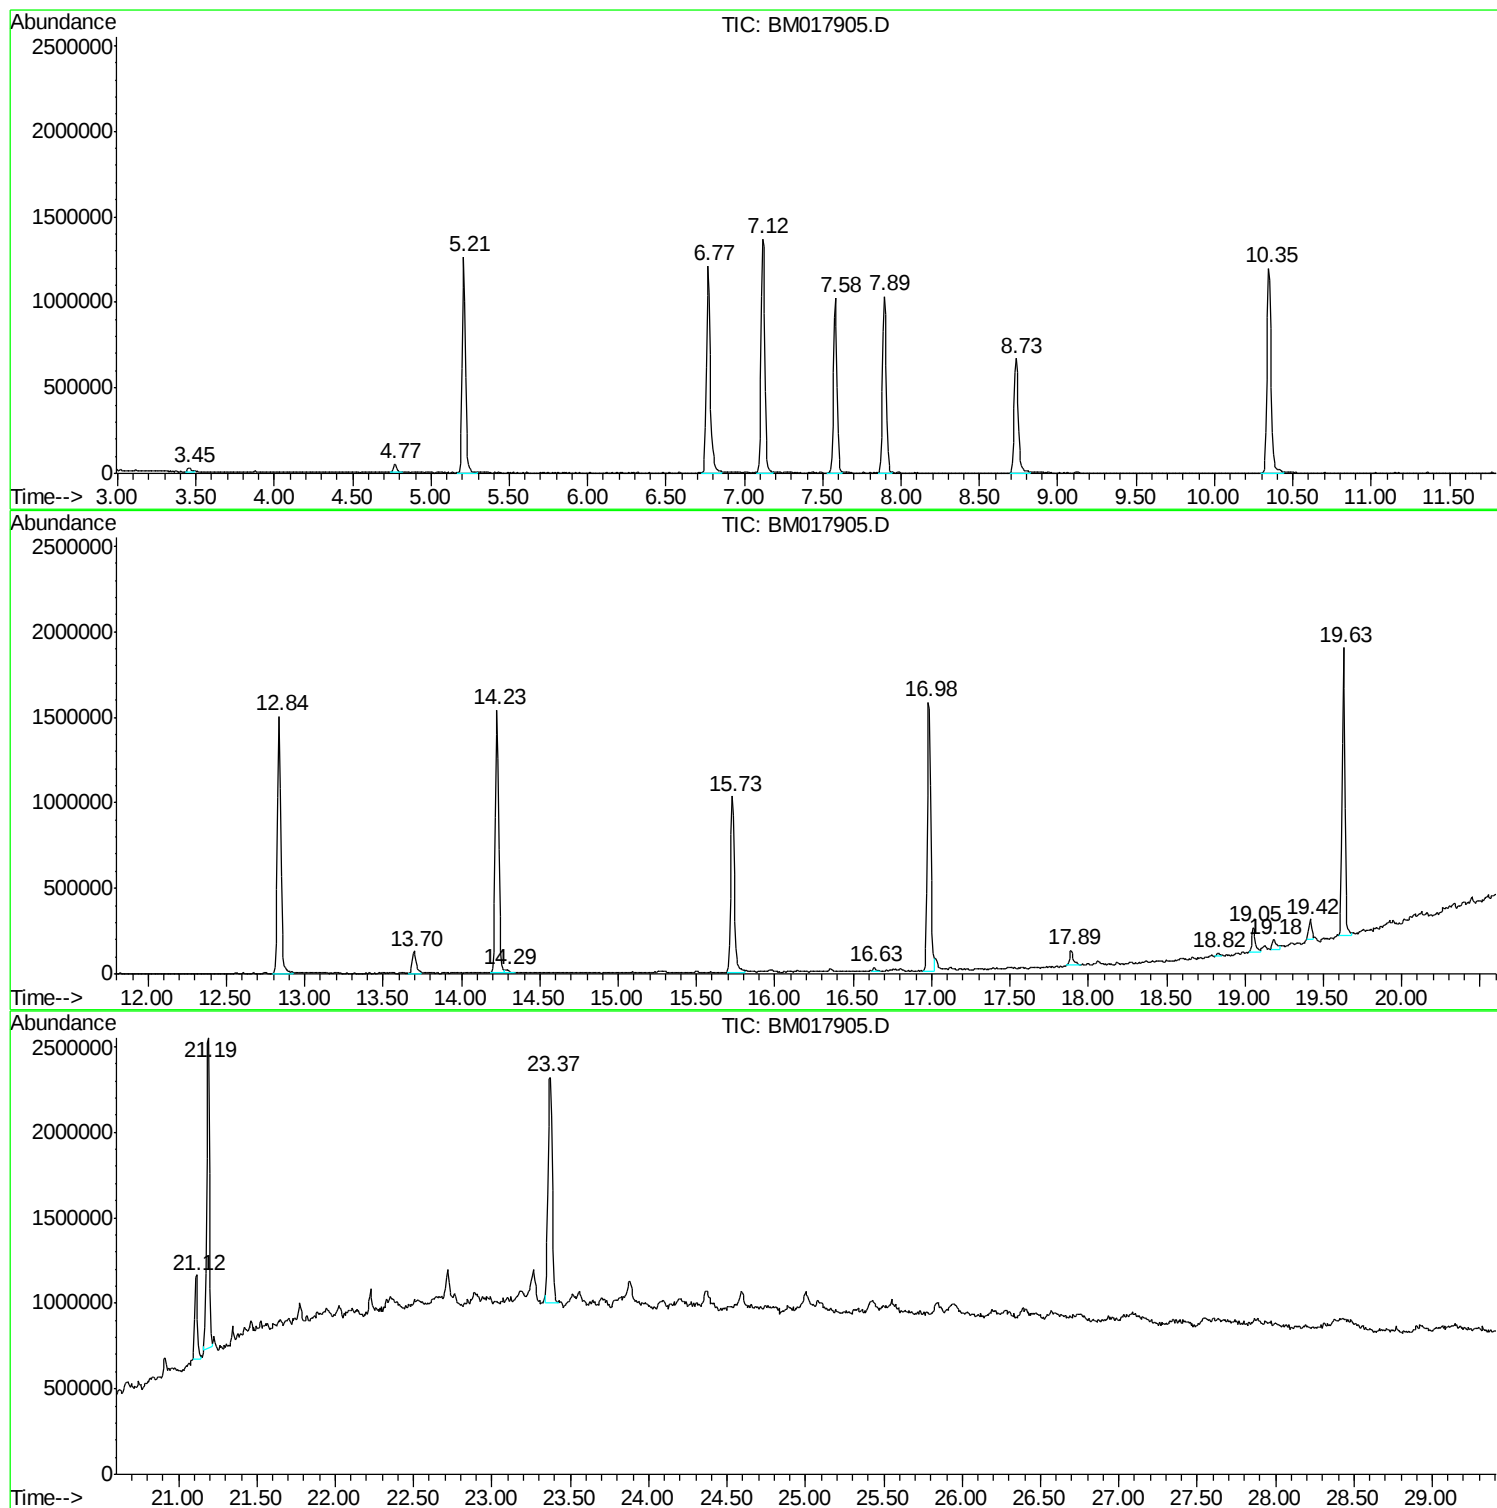

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120518\
Data File : BM017905.D
Acq On : 04 Dec 2018 16:45
Operator : JU/SJ
Sample : J6074-05 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
003-WC-NY2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.12 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.12	27.26 ng	2223380	1,4-Dichlorobenzene-d4	7.58

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Xenon	132	Xe	007440-63-3	9

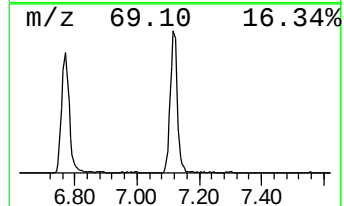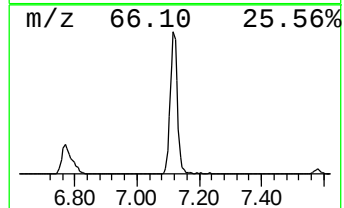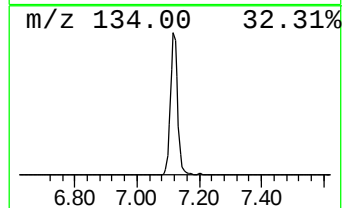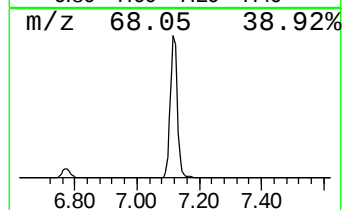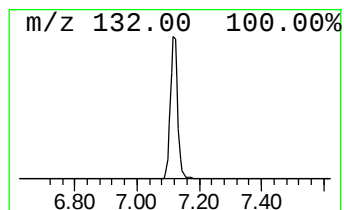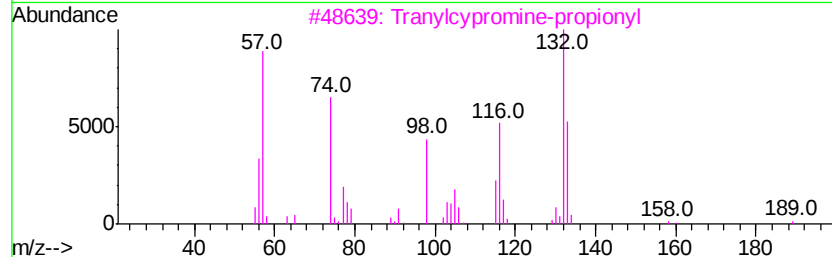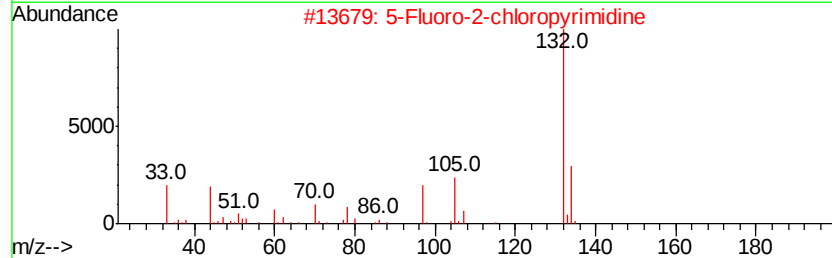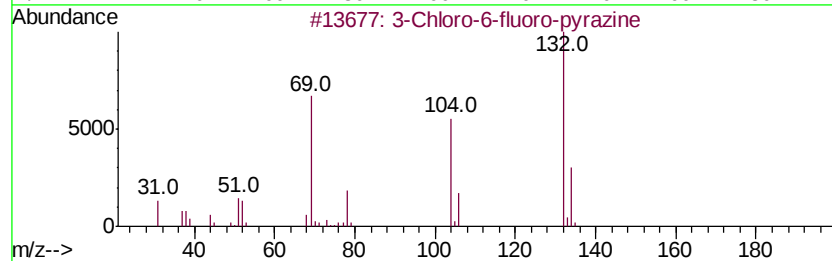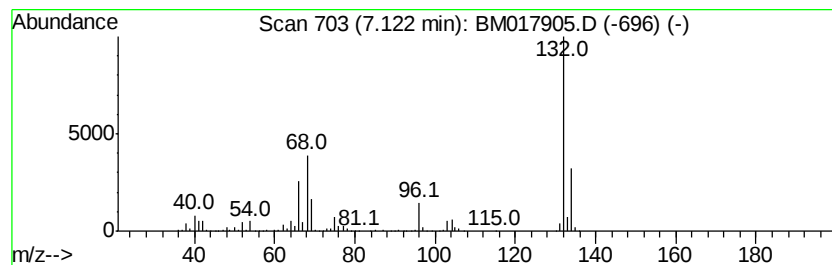

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120518\
Data File : BM017905.D
Acq On : 04 Dec 2018 16:45
Operator : JU/SJ
Sample : J6074-05 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
003-WC-NY2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.12	7.12	27.3	ng	2223380	1	7.58	1631370	20.0