


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120518\
 Data File : BM017901.D
 Acq On : 04 Dec 2018 13:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

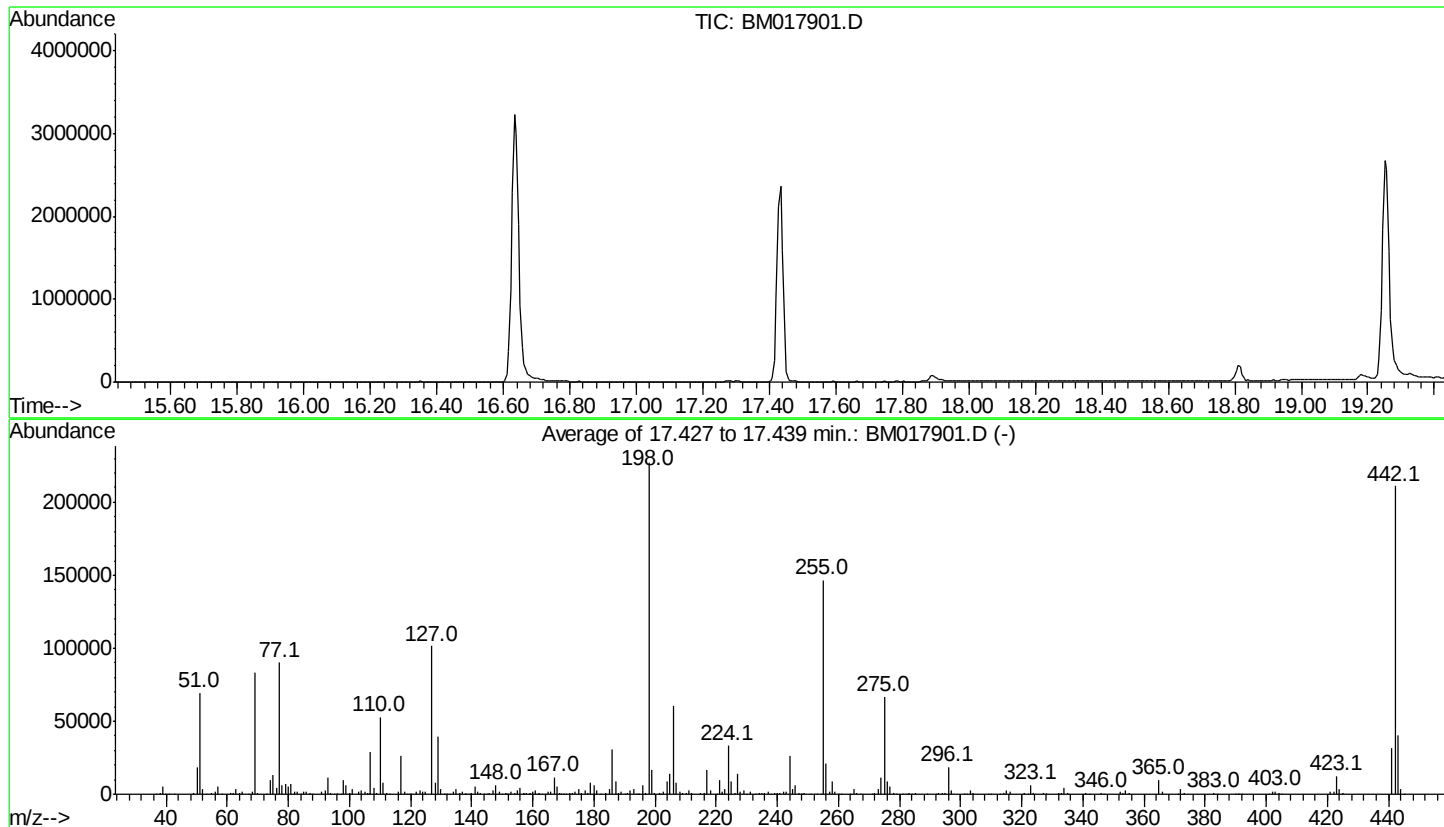

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	69600	PASS
68	69	0.00	2	1.8	1485	PASS
69	198	0.00	100	36.5	82917	PASS
70	69	0.00	2	0.7	543	PASS
127	198	10	80	44.6	101397	PASS
197	198	0.00	2	0.6	1268	PASS
198	198	100	100	100.0	227093	PASS
199	198	5	9	7.2	16316	PASS
275	198	10	60	29.5	66920	PASS
365	198	1	100	4.4	10083	PASS
441	198	0.01	100	13.8	31354	PASS
442	198	50	100	92.9	211072	PASS
443	442	15	24	19.2	40573	PASS