


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120518\
 Data File : BM017918.D
 Acq On : 05 Dec 2018 01:10
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

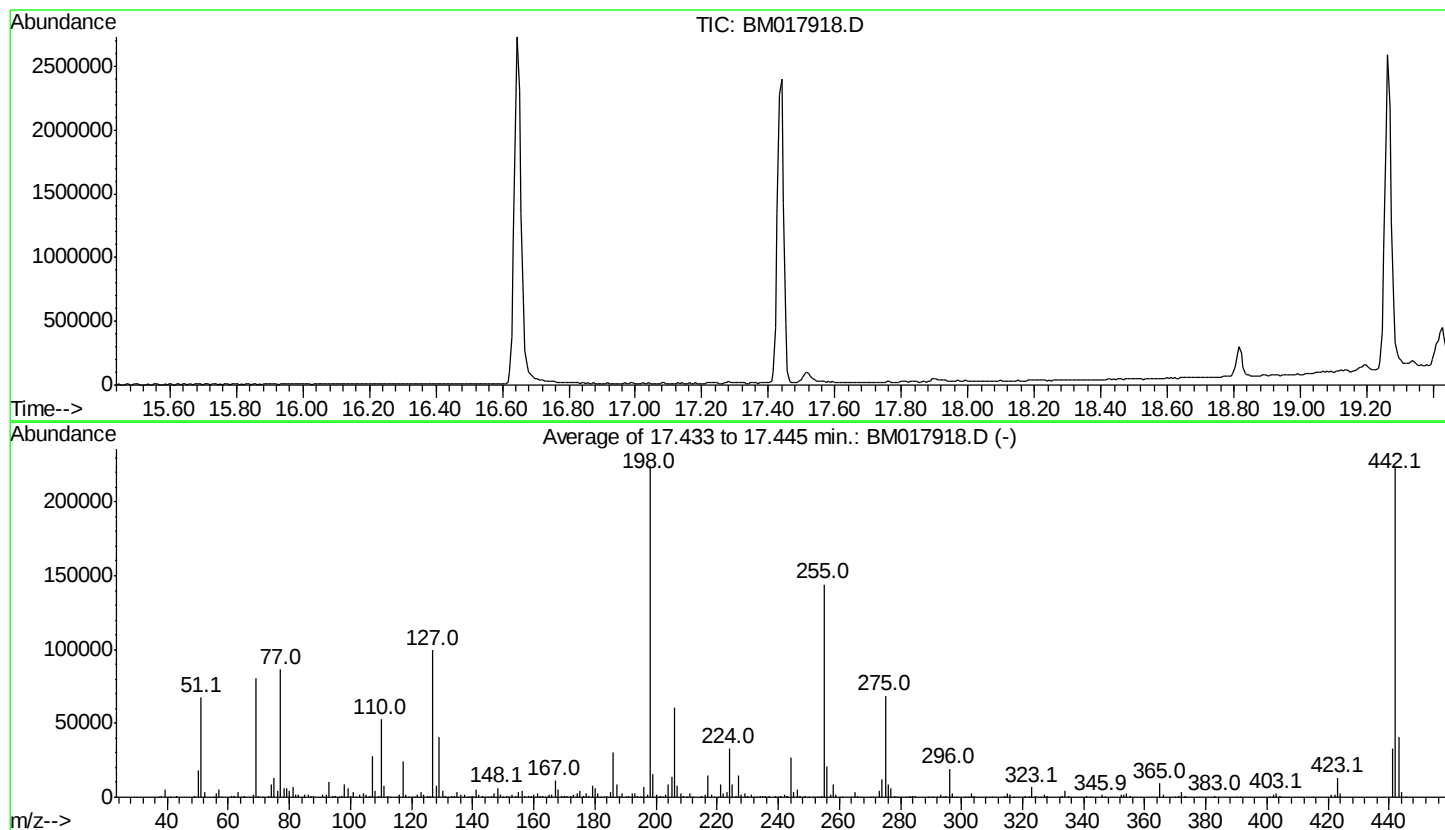

AutoFind: Scans 2456, 2457, 2458; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	67576	PASS
68	69	0.00	2	1.7	1352	PASS
69	198	0.00	100	35.7	80255	PASS
70	69	0.00	2	0.6	484	PASS
127	198	10	80	44.3	99360	PASS
197	198	0.00	2	0.8	1768	PASS
198	198	100	100	100.0	224533	PASS
199	198	5	9	6.8	15244	PASS
275	198	10	60	30.6	68626	PASS
365	198	1	100	4.2	9366	PASS
441	198	0.01	100	14.8	33224	PASS
442	198	50	100	99.9	224384	PASS
443	442	15	24	18.3	41056	PASS