

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120520\
 Data File : BM028044.D
 Acq On : 05 Dec 2020 10:52
 Operator : JU/CG
 Sample : PB133357BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK357

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120320.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	44	48	55	rBV	60204	79206	2.38%	0.195%
2	3.934	123	127	151	rBV	773508	1226912	36.84%	3.026%
3	4.293	183	188	195	rVB	8814	13818	0.41%	0.034%
4	5.381	368	373	377	rVB5	2874	6034	0.18%	0.015%
5	7.416	711	719	732	rBV	864769	1396784	41.94%	3.445%
6	7.598	742	750	759	rBV	666045	1067047	32.04%	2.632%
7	7.810	778	786	797	rVB	885901	1441333	43.27%	3.555%
8	8.287	860	867	877	rVB	640194	1015370	30.49%	2.505%
9	8.987	979	986	1001	rBV	1009354	1614625	48.48%	3.983%
10	9.463	1058	1067	1078	rBV	789923	1288581	38.69%	3.179%
11	10.192	1183	1191	1202	rBV	628228	998607	29.98%	2.463%
12	10.728	1273	1282	1293	rBV	955344	1609540	48.33%	3.970%
13	11.122	1341	1349	1357	rBV	825873	1370497	41.15%	3.381%
14	11.245	1363	1370	1379	rBV	970370	1629785	48.93%	4.020%
15	12.686	1610	1615	1620	rBV2	15742	24276	0.73%	0.060%
16	14.304	1883	1890	1896	rBV	1507105	2024466	60.78%	4.994%
17	14.357	1896	1899	1906	rVB7	4637	7757	0.23%	0.019%
18	14.610	1933	1942	1950	rBV	1734266	2553948	76.68%	6.300%
19	14.910	1986	1993	2001	rVB2	1101265	1636006	49.12%	4.036%
20	15.069	2013	2020	2033	rBV	692381	980505	29.44%	2.419%
21	15.304	2056	2060	2065	rVB5	4361	6749	0.20%	0.017%
22	15.686	2120	2125	2130	rVB5	2018	4880	0.15%	0.012%
23	15.886	2153	2159	2169	rBV	2045366	3006346	90.26%	7.416%
24	15.992	2171	2177	2185	rBV	594046	786199	23.60%	1.939%
25	16.127	2194	2200	2207	rVB	24785	34419	1.03%	0.085%
26	16.663	2284	2291	2296	rBV3	7908	11172	0.34%	0.028%
27	17.310	2395	2401	2404	rBV7	3567	5887	0.18%	0.015%
28	17.421	2416	2420	2425	rVB3	4638	7841	0.24%	0.019%
29	17.627	2447	2455	2465	rBV	1239044	1719958	51.64%	4.243%
30	17.727	2465	2472	2486	rVV	2095963	3058972	91.84%	7.546%
31	19.615	2790	2793	2796	rBV	18710	22635	0.68%	0.056%
32	19.868	2833	2836	2840	rVB	20838	23335	0.70%	0.058%
33	19.980	2849	2855	2862	rBV	2510260	3330647	100.00%	8.216%
34	21.733	3148	3153	3158	rBV	1377147	1723646	51.75%	4.252%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120520\
Data File : BM028044.D
Acq On : 05 Dec 2020 10:52
Operator : JU/CG
Sample : PB133357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK357

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120320.M
Title : SVOA CALIBRATION

35	23.986	3529	3536	3544	rVB	1623681	3126311	93.86%	7.712%
36	24.139	3556	3562	3576	rVB	855228	1685883	50.62%	4.159%


Sum of corrected areas: 40539977

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120520\
Data File : BM028044.D
Acq On : 05 Dec 2020 10:52
Operator : JU/CG
Sample : PB133357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK357

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120320.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

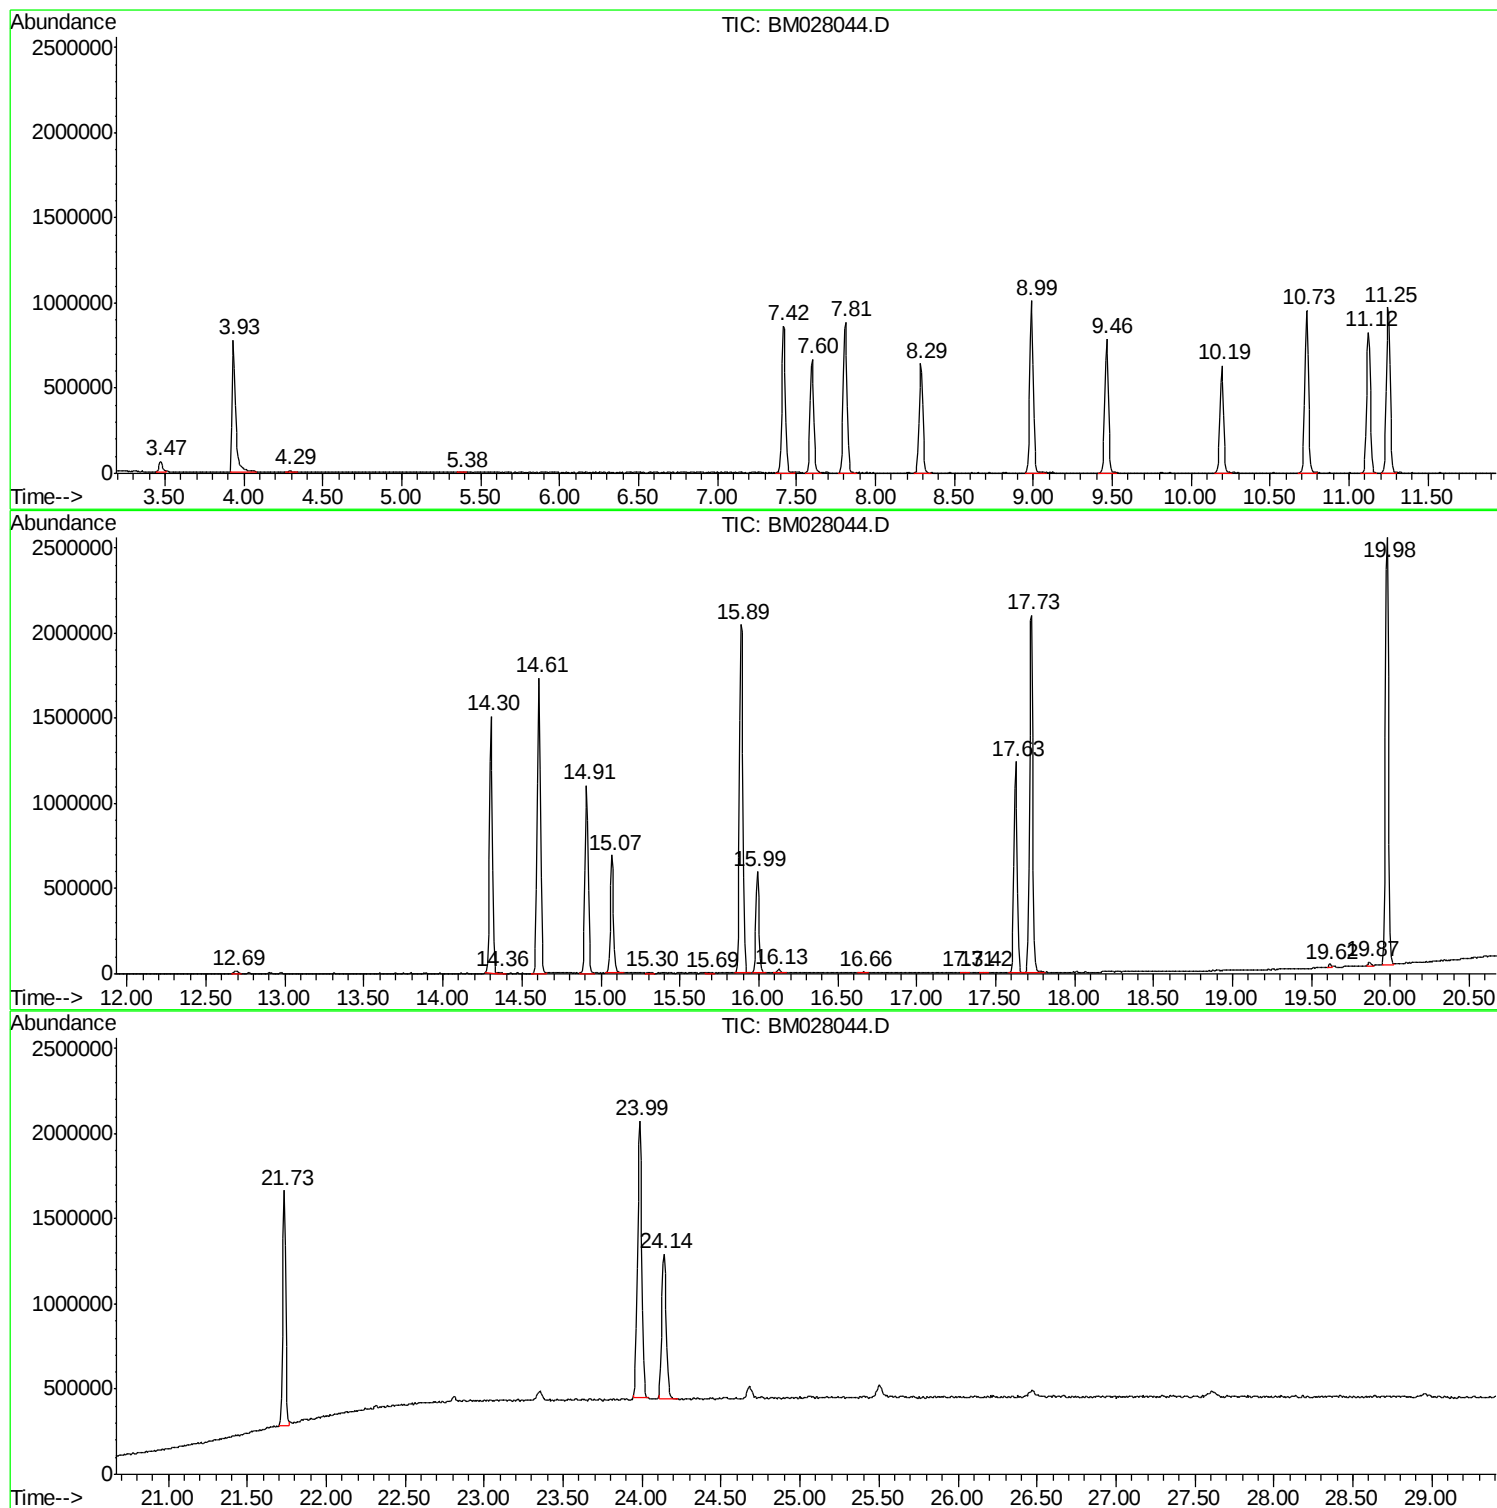

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120520\
Data File : BM028044.D
Acq On : 05 Dec 2020 10:52
Operator : JU/CG
Sample : PB133357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK357

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120320.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120520\
Data File : BM028044.D
Acq On : 05 Dec 2020 10:52
Operator : JU/CG
Sample : PB133357BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK357

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM120320.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc