


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM120618\
 Data File : BM017935.D
 Acq On : 05 Dec 2018 14:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

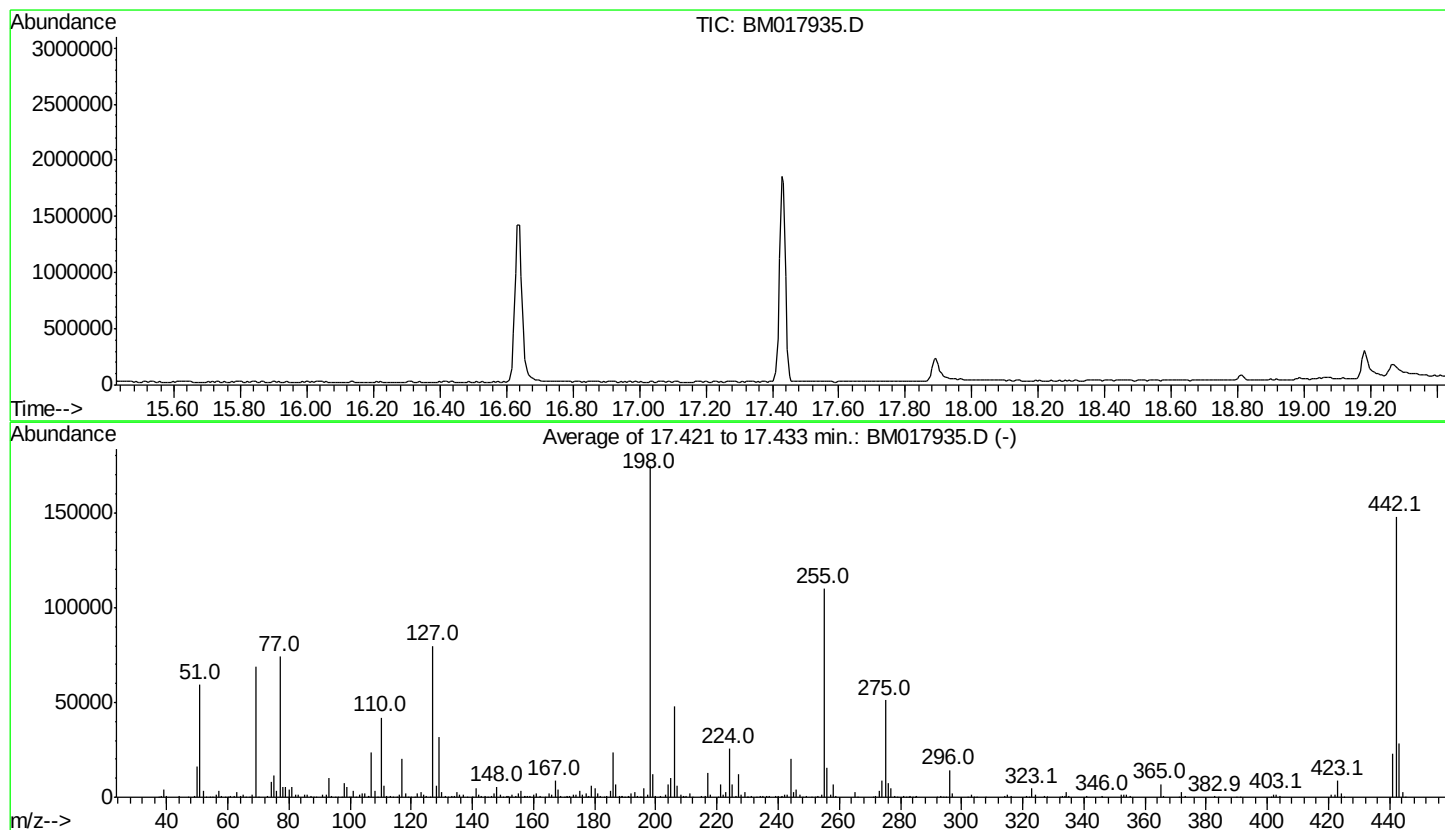

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	59271	PASS
68	69	0.00	2	2.0	1410	PASS
69	198	0.00	100	39.3	68785	PASS
70	69	0.00	2	0.4	266	PASS
127	198	10	80	45.6	79733	PASS
197	198	0.00	2	0.6	1069	PASS
198	198	100	100	100.0	174917	PASS
199	198	5	9	6.9	12048	PASS
275	198	10	60	29.3	51226	PASS
365	198	1	100	3.9	6850	PASS
441	198	0.01	100	13.0	22792	PASS
442	198	50	100	84.7	148082	PASS
443	442	15	24	19.2	28458	PASS