


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM120618\
 Data File : BM017953.D
 Acq On : 06 Dec 2018 02:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM111218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Nov 12 18:37:25 2018

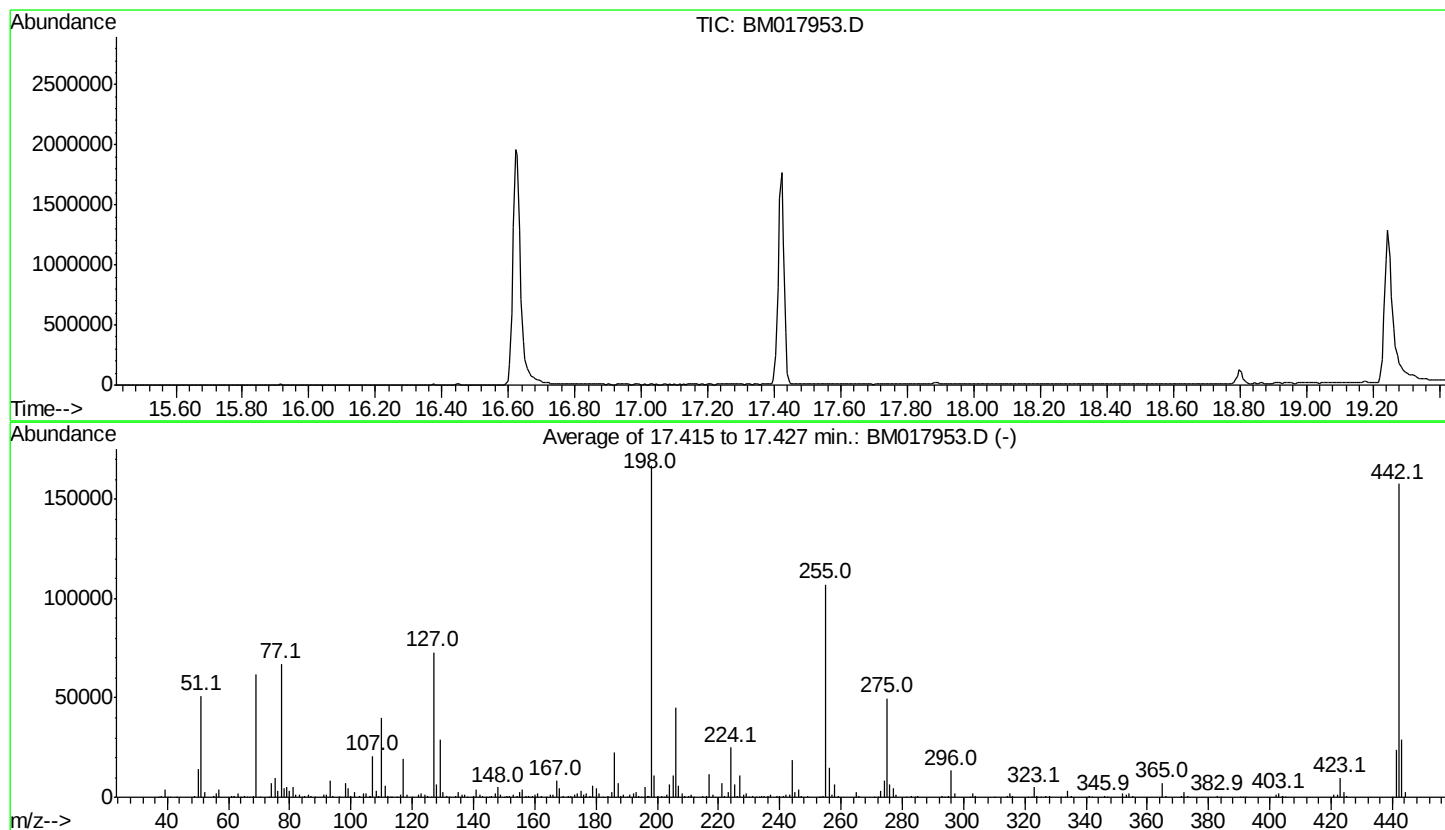

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	51133	PASS
68	69	0.00	2	0.8	468	PASS
69	198	0.00	100	37.2	62186	PASS
70	69	0.00	2	0.5	296	PASS
127	198	10	80	43.7	72976	PASS
197	198	0.00	2	0.3	456	PASS
198	198	100	100	100.0	167045	PASS
199	198	5	9	6.6	11059	PASS
275	198	10	60	29.8	49741	PASS
365	198	1	100	4.3	7202	PASS
441	198	0.01	100	14.2	23720	PASS
442	198	50	100	94.5	157930	PASS
443	442	15	24	18.4	29037	PASS