

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120619\
 Data File : BM024030.D
 Acq On : 06 Dec 2019 23:28
 Operator : JU
 Sample : K6007-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BM6

Quant Time: Dec 07 01:18:31 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 06 22:30:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	338346	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	1347974	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	790831	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1627203	20.00	ng/ul	0.00
78) Chrysene-d12	21.10	240	1602114	20.00	ng/ul	0.00
86) Perylene-d12	23.24	264	1953281	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.03	96	62362	8.20	ng/uL	0.00
5) Phenol-d5	6.67	99	1129874	38.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.83	67	711170	41.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.02	132	909685	39.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.19	113	857402	36.65	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	436364	41.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	488417	41.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	857987	38.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	1117884	45.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	2567608	41.78	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	3174679	44.08	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	379148	36.70	ng/ul	0.00
58) Fluorene-d10	15.14	176	2229856	43.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.28	200	347804	34.05	ng/ul	0.00
71) Anthracene-d10	16.99	188	3321987	42.75	ng/ul	0.00
79) Pyrene-d10	19.29	212	3551217	42.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.10	264	4456064	43.16	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.69	94	62768	2.058	ng/ul	94
45) Dimethylphthalate	13.60	163	1254028	20.848	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120619\
Data File : BM024030.D
Acq On : 06 Dec 2019 23:28
Operator : JU
Sample : K6007-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BM6

Quant Time: Dec 07 01:18:31 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM112719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 06 22:30:13 2019
Response via : Initial Calibration

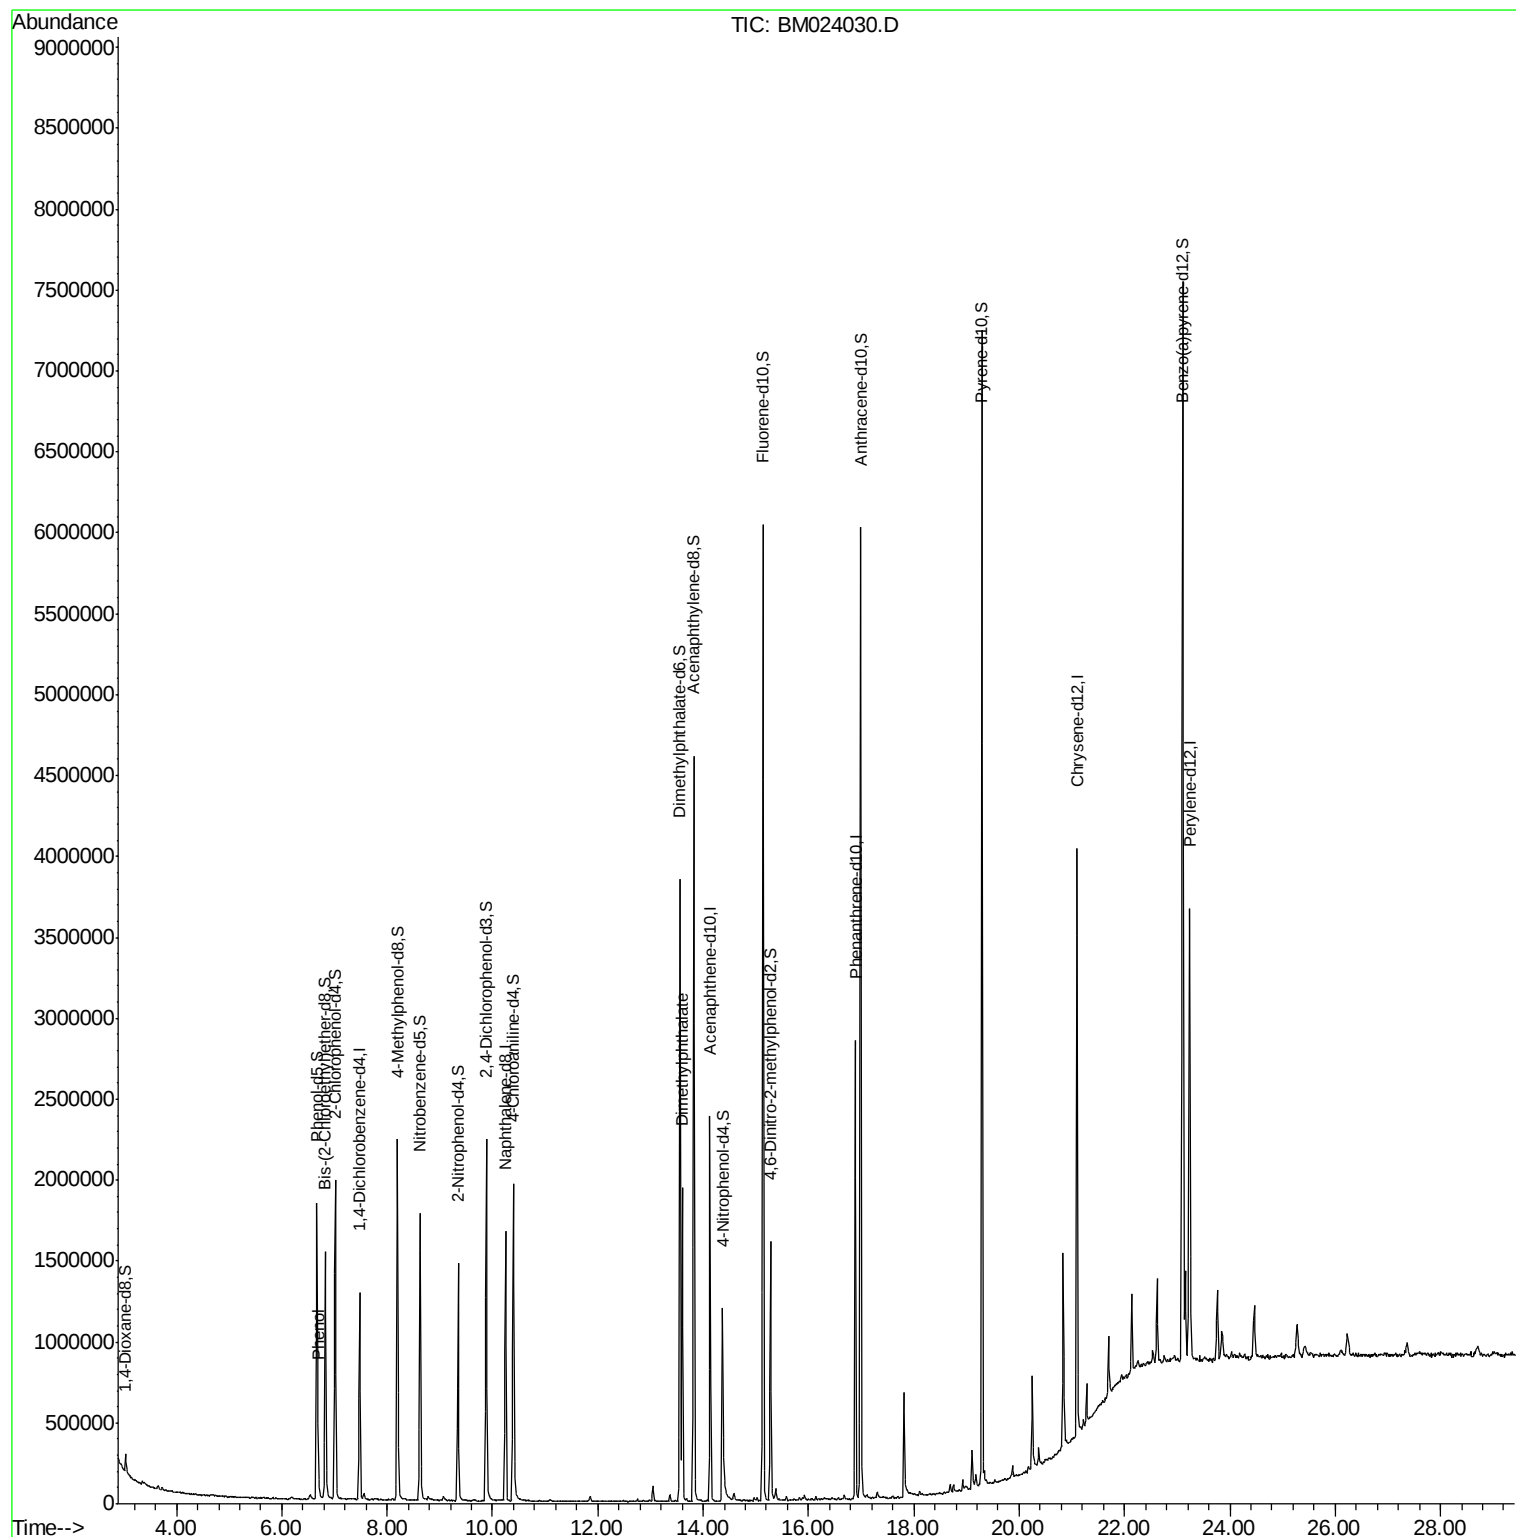

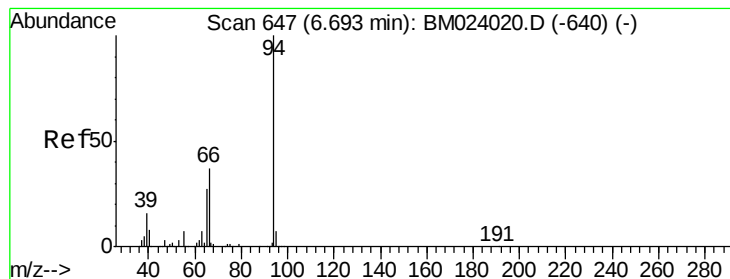





#6

Phenol

Concen: 2.058 ng/ul
 RT: 6.69 min Scan# 647
 Delta R.T. -0.01 min
 Lab File: BM024030.D
 Acq: 06 Dec 2019 23:28

Instrument :
 BNA_M
 ClientSampleId :
 C0BM6

Tot Ion: 94 Resp: 62768
 Ion Ratio Lower Upper
 94 100
 65 27.4 21.7 32.5
 66 42.3 28.8 43.2

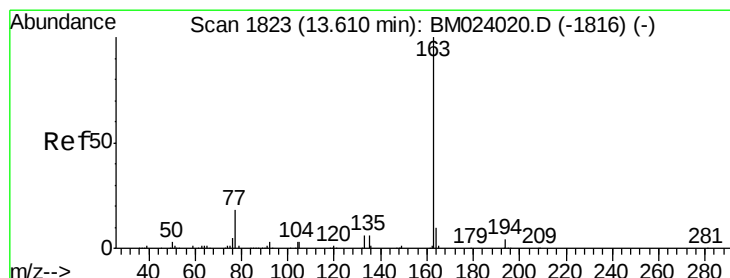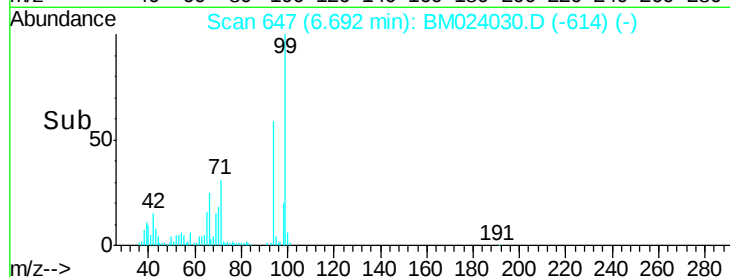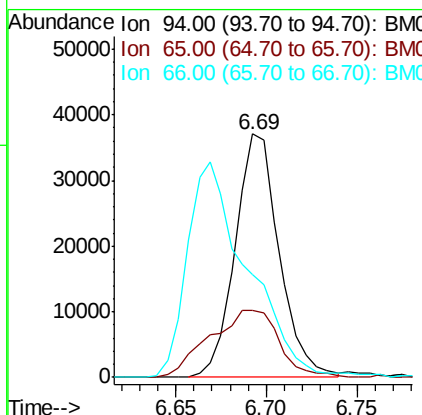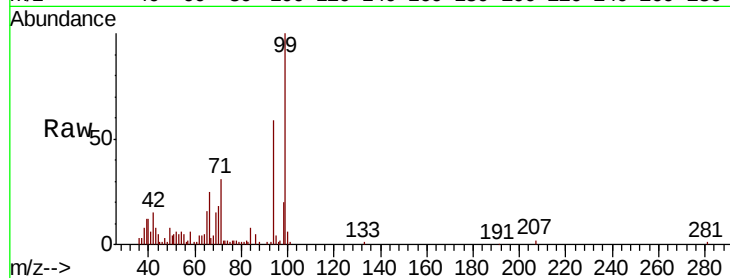

#45

Dimethylphthalate

Concen: 20.848 ng/ul
 RT: 13.60 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM024030.D
 Acq: 06 Dec 2019 23:28

Tgt Ion: 163 Resp: 1254028
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.3 4.9
 164 10.3 7.9 11.9

