
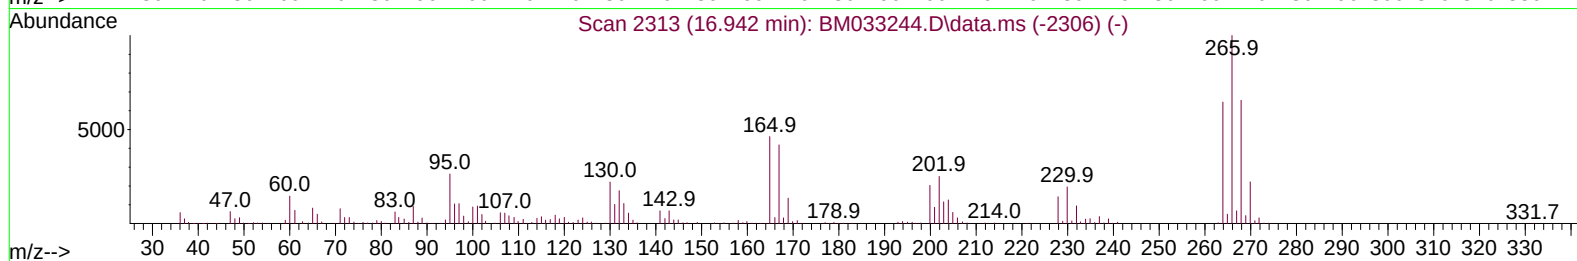
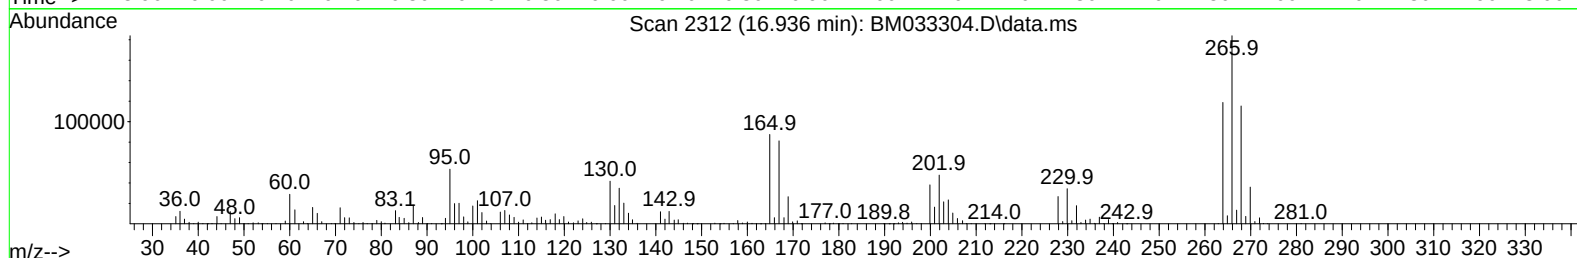


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120621\
Data File : BM033304.D
Acq On : 06 Dec 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 12:59:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 24 15:16:33 2021
Response via : Initial Calibration

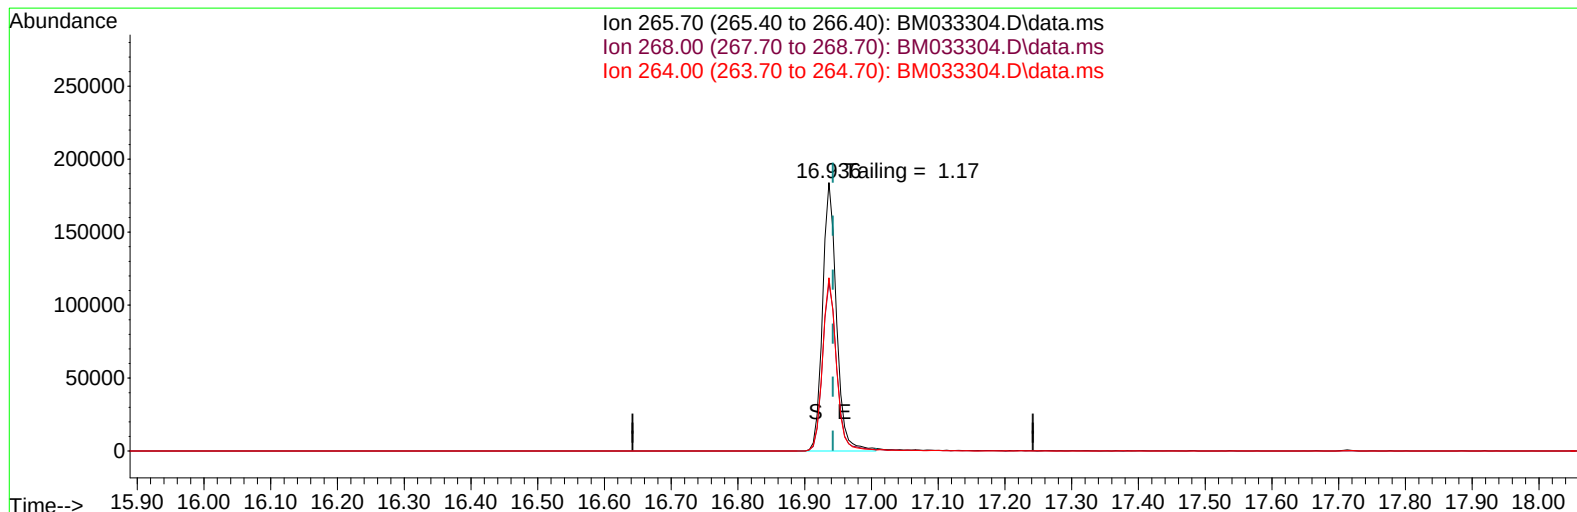

TIC: BM033304.D\data.ms

(70) Pentachlorophenol (C)




16.936min (-0.006) 195812.72 ng

response 268750

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.69
264.00	65.10	64.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120621\
 Data File : BM033304.D
 Acq On : 06 Dec 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 06 12:59:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

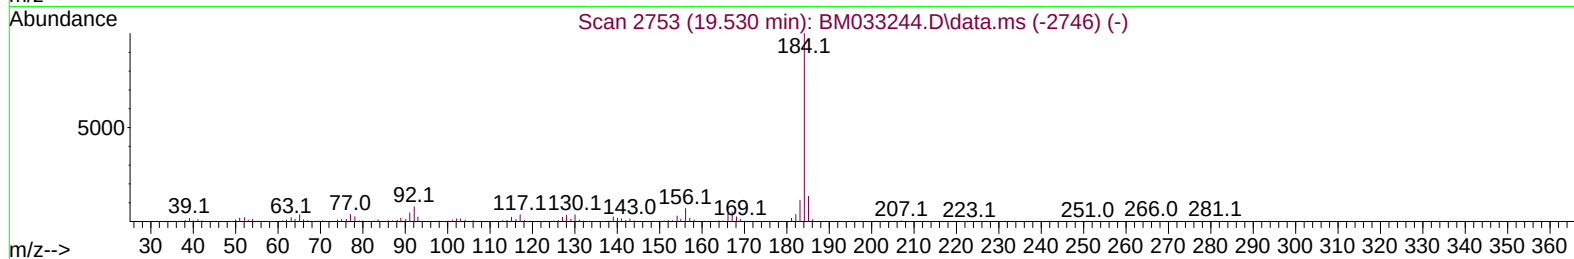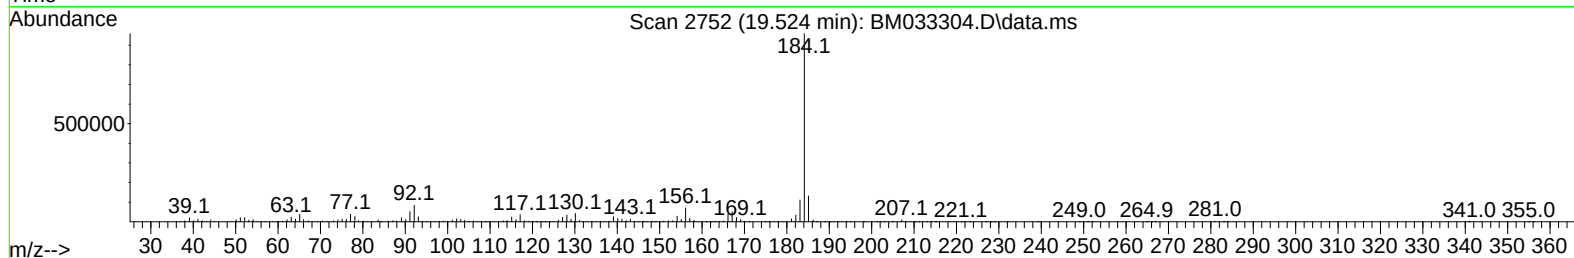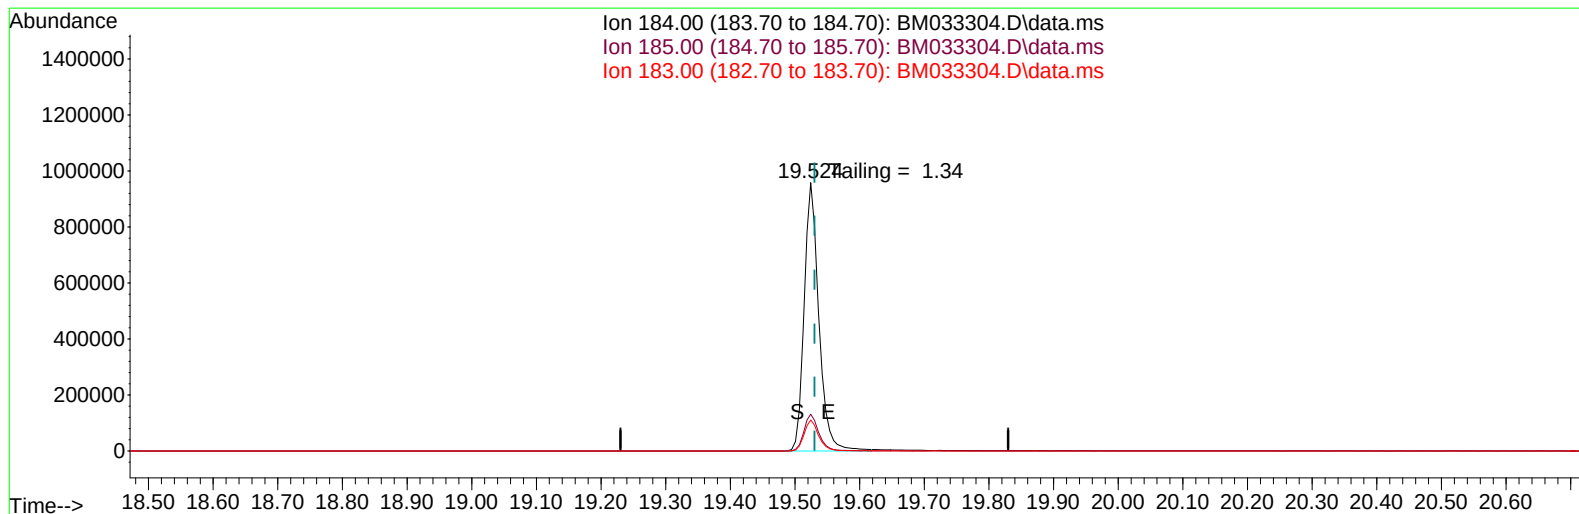

TIC: BM033304.D\data.ms

(77) Benzidine**19.524min (-0.006) 1260996.07 ng****response 1531199**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.72
183.00	11.20	11.57
0.00	0.00	0.00