


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120621\
 Data File : BM033304.D
 Acq On : 06 Dec 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 06 13:01:33 2021

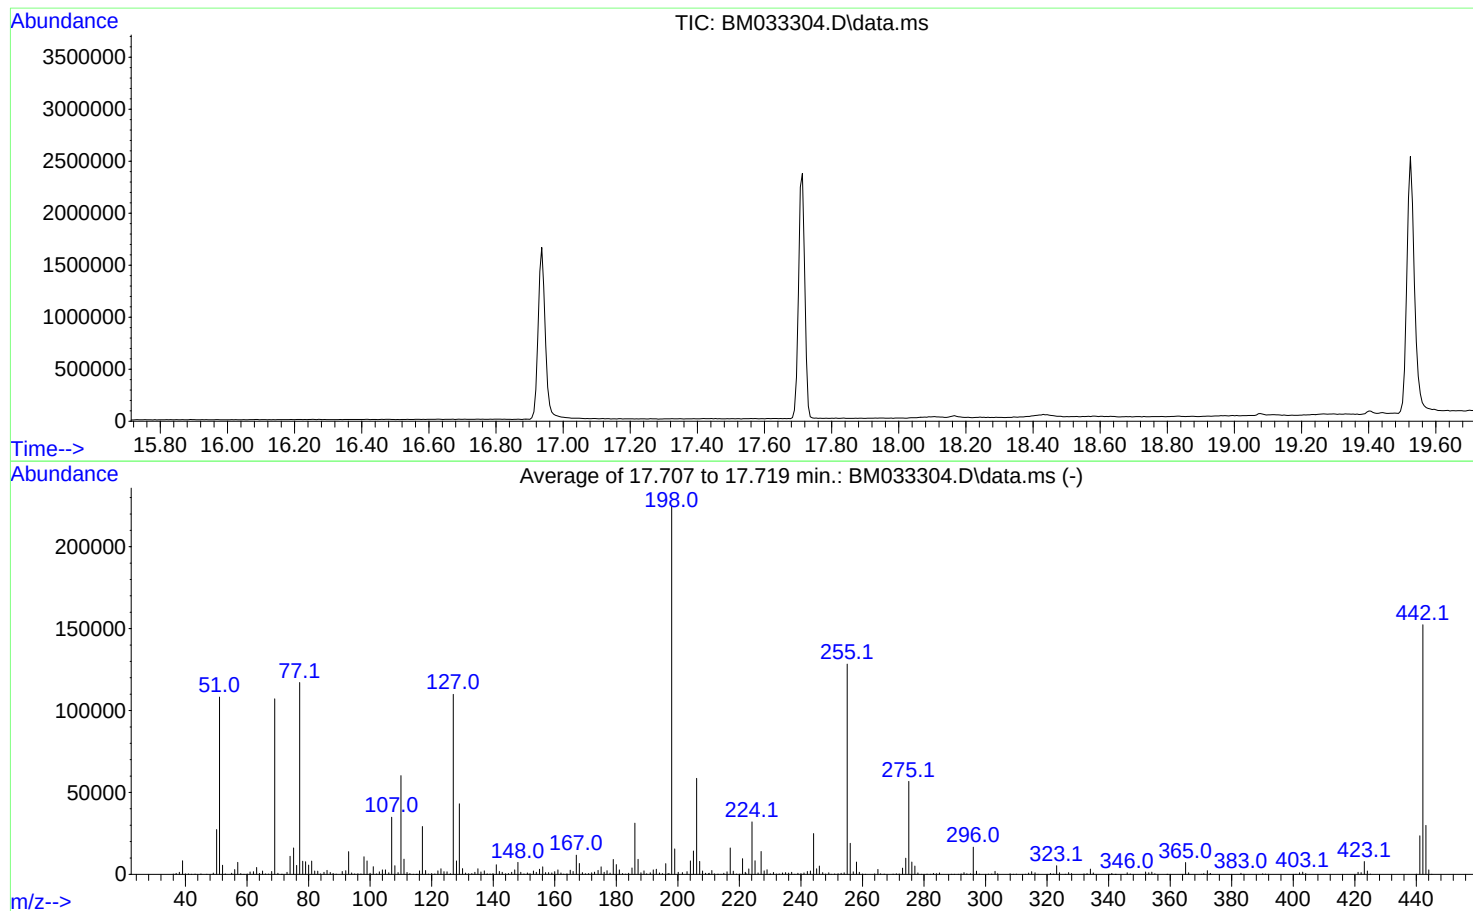




AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2436

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	108246	PASS
68	69	0.00	2	1.6	1753	PASS
69	198	0.00	100	47.7	107162	PASS
70	69	0.00	2	0.6	686	PASS
127	198	10	80	48.9	109901	PASS
197	198	0.00	2	0.3	612	PASS
198	198	100	100	100.0	224555	PASS
199	198	5	9	6.9	15521	PASS
275	198	10	60	25.3	56739	PASS
365	198	1	100	3.2	7256	PASS
441	198	0.01	100	10.5	23571	PASS
442	442	50	100	100.0	152331	PASS
443	442	15	24	19.6	29920	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120621\
Data File : BM033304.D
Acq On : 06 Dec 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 06 12:59:23 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 24 15:16:33 2021
Response via : Initial Calibration

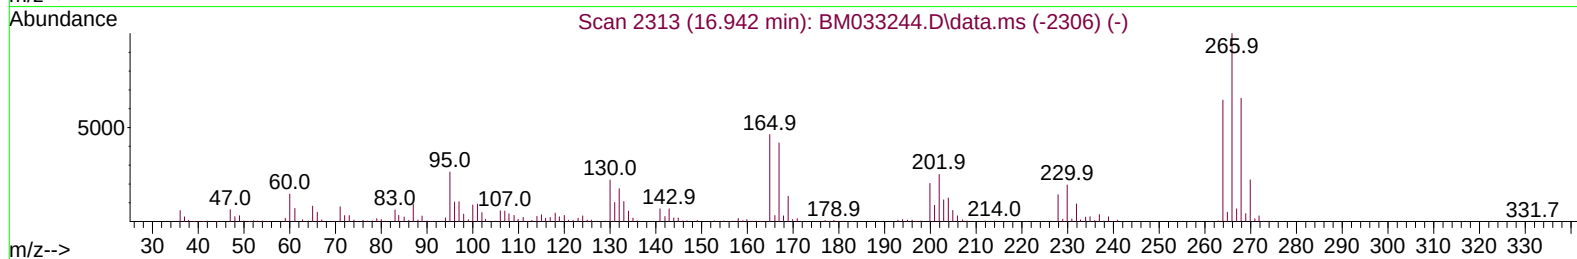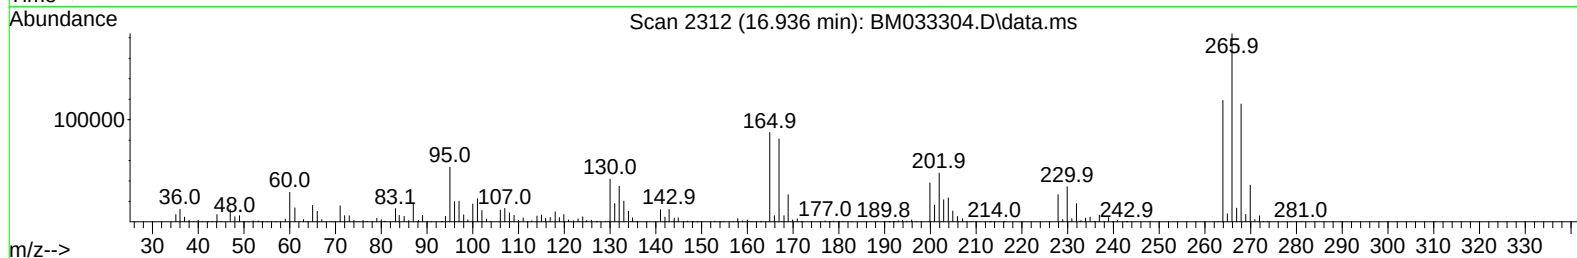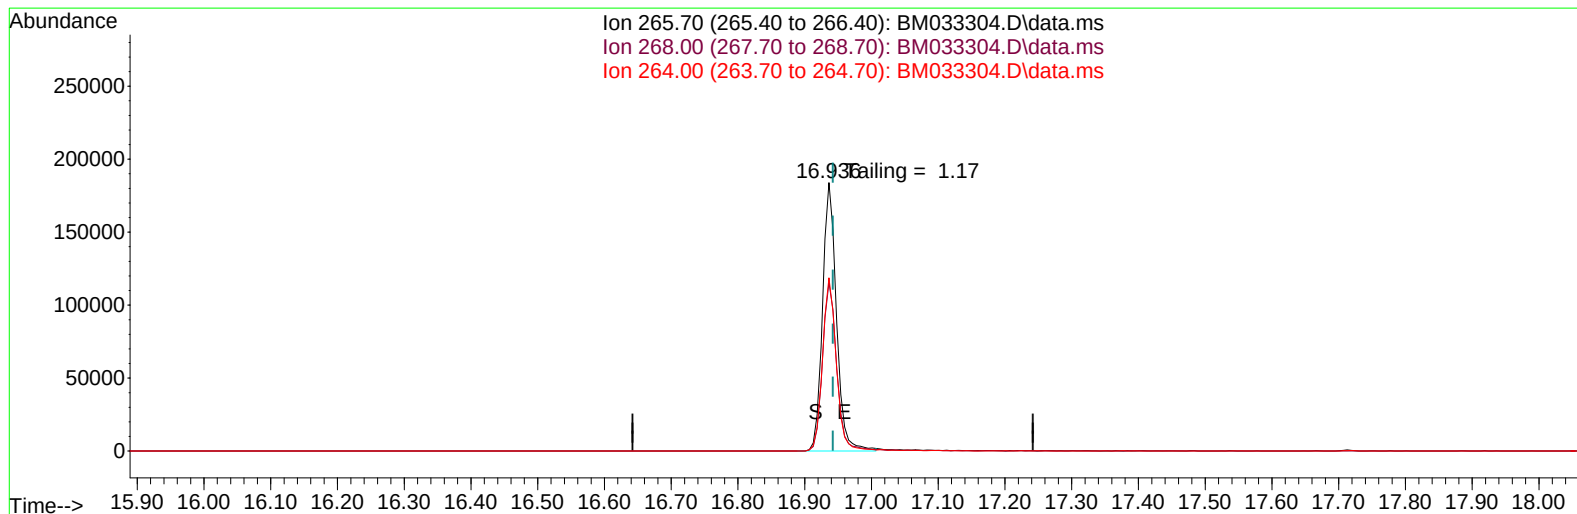

TIC: BM033304.D\data.ms

(70) Pentachlorophenol (C)

16.936min (-0.006) 195812.72 ng




response 268750

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.69
264.00	65.10	64.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120621\
 Data File : BM033304.D
 Acq On : 06 Dec 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Dec 06 12:59:23 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM112421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 24 15:16:33 2021
 Response via : Initial Calibration

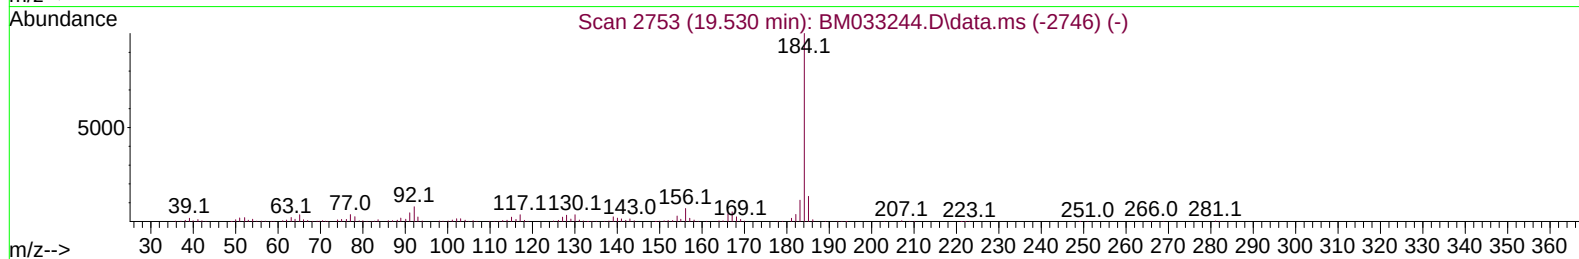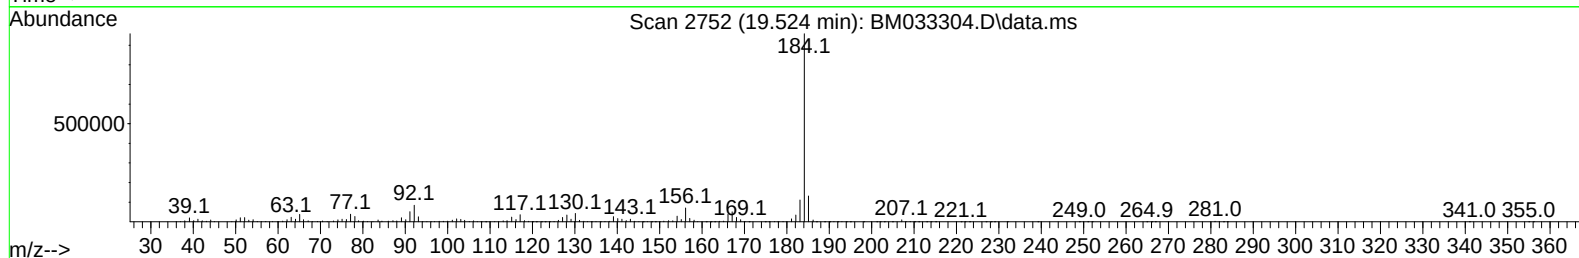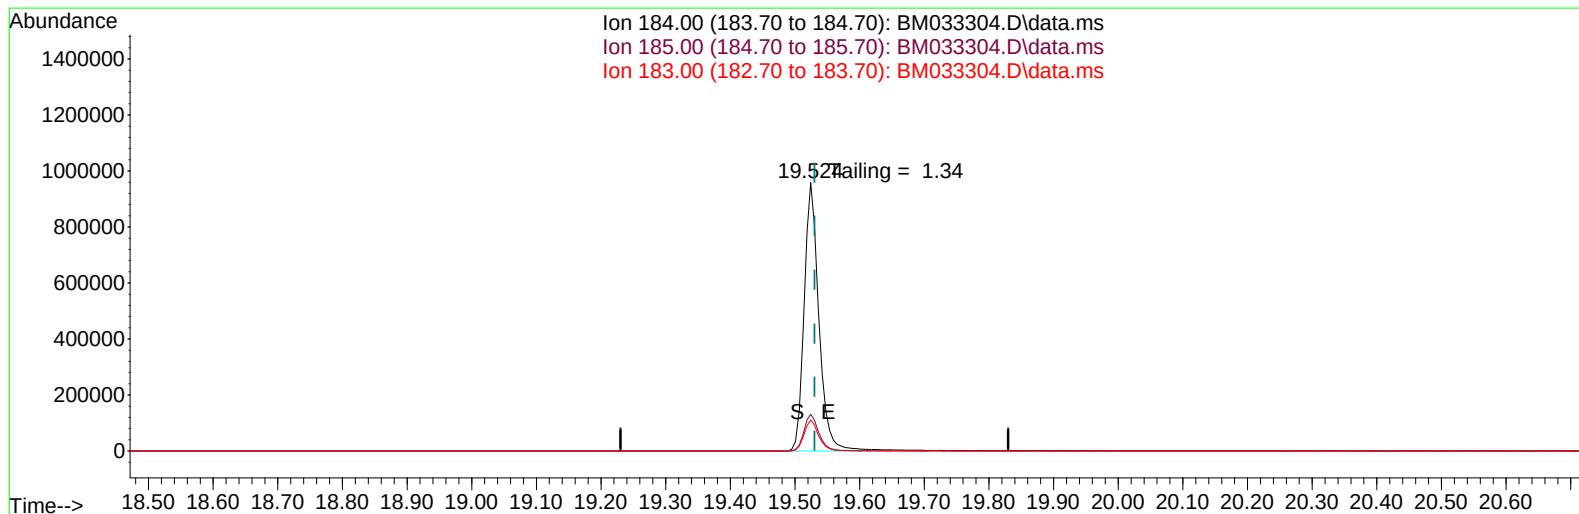

TIC: BM033304.D\data.ms

(77) Benzidine

19.524min (-0.006) 1260996.07 ng

response 1531199

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.30	13.72
183.00	11.20	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/6/2021	BNA_M	<u>BM033304.D</u>
Compound Name	Response	Retention Time
DDT	766322	20.74
DDD	12196	20.3
DDE	664	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12860	779182	1.65

Instrument :
BNA_M
ClientSampleId :
DFTPP