

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
 Data File : BM037852.D
 Acq On : 06 Dec 2022 12:30
 Operator : CG/JU
 Sample : PB149426BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK426

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037852.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	3	7	13	rVB	61694	86707	2.22%	0.174%
2	3.863	77	81	97	rBV	737774	1138040	29.10%	2.280%
3	4.199	134	138	142	rVB	19169	26153	0.67%	0.052%
4	5.040	279	281	283	rBV4	3663	4025	0.10%	0.008%
5	5.746	398	401	404	rBV5	5146	5569	0.14%	0.011%
6	6.693	561	562	567	rVB5	3568	4827	0.12%	0.010%
7	6.763	571	574	579	rVB6	2015	3998	0.10%	0.008%
8	7.063	621	625	627	rBV5	3153	4180	0.11%	0.008%
9	7.240	649	655	664	rBV	912265	1416041	36.21%	2.837%
10	7.410	678	684	696	rVV	751525	1136802	29.07%	2.278%
11	7.616	712	719	730	rVB	900519	1400912	35.82%	2.807%
12	7.951	771	776	779	rBV7	3003	4776	0.12%	0.010%
13	8.087	792	799	808	rBV	979153	1528126	39.07%	3.062%
14	8.193	815	817	820	rBV3	3029	3997	0.10%	0.008%
15	8.798	913	920	931	rBV	1100722	1707729	43.67%	3.422%
16	9.257	991	998	1006	rBV	826716	1352494	34.58%	2.710%
17	9.987	1114	1122	1134	rBV	674093	1088755	27.84%	2.182%
18	10.528	1205	1214	1230	rBV	1015414	1699826	43.46%	3.406%
19	10.910	1271	1279	1290	rVV	1325047	2185115	55.87%	4.378%
20	11.045	1295	1302	1316	rBV	993114	1695603	43.36%	3.398%
21	11.298	1342	1345	1349	rVB5	4179	5543	0.14%	0.011%
22	11.586	1390	1394	1397	rBV5	2995	4773	0.12%	0.010%
23	11.904	1444	1448	1451	rVB6	3017	4090	0.10%	0.008%
24	11.933	1451	1453	1457	rBV4	3405	4412	0.11%	0.009%
25	12.486	1543	1547	1552	rVB2	18768	29537	0.76%	0.059%
26	13.586	1731	1734	1735	rBV3	4175	5085	0.13%	0.010%
27	13.604	1735	1737	1741	rVB5	5541	6276	0.16%	0.013%
28	14.057	1810	1814	1818	rBV8	3550	5438	0.14%	0.011%
29	14.127	1819	1826	1841	rVV	1581368	2235472	57.16%	4.479%
30	14.416	1868	1875	1888	rBV	2009293	2946308	75.34%	5.904%
31	14.545	1892	1897	1905	rVV3	22187	63257	1.62%	0.127%
32	14.722	1919	1927	1938	rBV	1820532	2698191	68.99%	5.406%
33	14.910	1949	1959	1972	rBV	527665	946608	24.20%	1.897%
34	15.122	1991	1995	1998	rBV6	6008	8864	0.23%	0.018%
35	15.474	2052	2055	2062	rVB9	3637	7258	0.19%	0.015%
36	15.704	2084	2094	2107	rBV	2398357	3544434	90.63%	7.102%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
 Data File : BM037852.D
 Acq On : 06 Dec 2022 12:30
 Operator : CG/JU
 Sample : PB149426BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK426

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Title : SVOA CALIBRATION

37	15.821	2108	2114	2128	rVV	523026	833264	21.31%	1.670%
38	15.939	2132	2134	2140	rVV4	16094	26385	0.67%	0.053%
39	16.010	2144	2146	2150	rVB5	4001	4812	0.12%	0.010%
40	16.092	2157	2160	2162	rBV4	3207	3981	0.10%	0.008%
41	16.357	2199	2205	2207	rBV7	2827	4791	0.12%	0.010%
42	16.474	2222	2225	2227	rBV4	4007	4838	0.12%	0.010%
43	16.557	2236	2239	2241	rBV3	4113	4471	0.11%	0.009%
44	16.910	2296	2299	2303	rVB5	7203	9631	0.25%	0.019%
45	17.110	2329	2333	2335	rBV5	5227	6961	0.18%	0.014%
46	17.457	2386	2392	2403	rBV	2043713	2857908	73.08%	5.726%
47	17.557	2403	2409	2424	rVV	2609403	3620557	92.58%	7.255%
48	17.827	2453	2455	2458	rVB4	5932	4527	0.12%	0.009%
49	18.333	2537	2541	2550	rBV4	40426	81813	2.09%	0.164%
50	19.404	2721	2723	2729	rVB6	31052	36107	0.92%	0.072%
51	19.839	2791	2797	2805	rBV	2837844	3815262	97.56%	7.645%
52	20.809	2960	2962	2968	rVB	93031	100177	2.56%	0.201%
53	21.627	3096	3101	3110	rVB	2059144	2695711	68.93%	5.401%
54	23.950	3490	3496	3512	rVB2	1847009	3910832	100.00%	7.836%
55	24.115	3518	3524	3534	rVB2	1375772	2876105	73.54%	5.763%




Sum of corrected areas: 49907354

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
Data File : BM037852.D
Acq On : 06 Dec 2022 12:30
Operator : CG/JU
Sample : PB149426BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

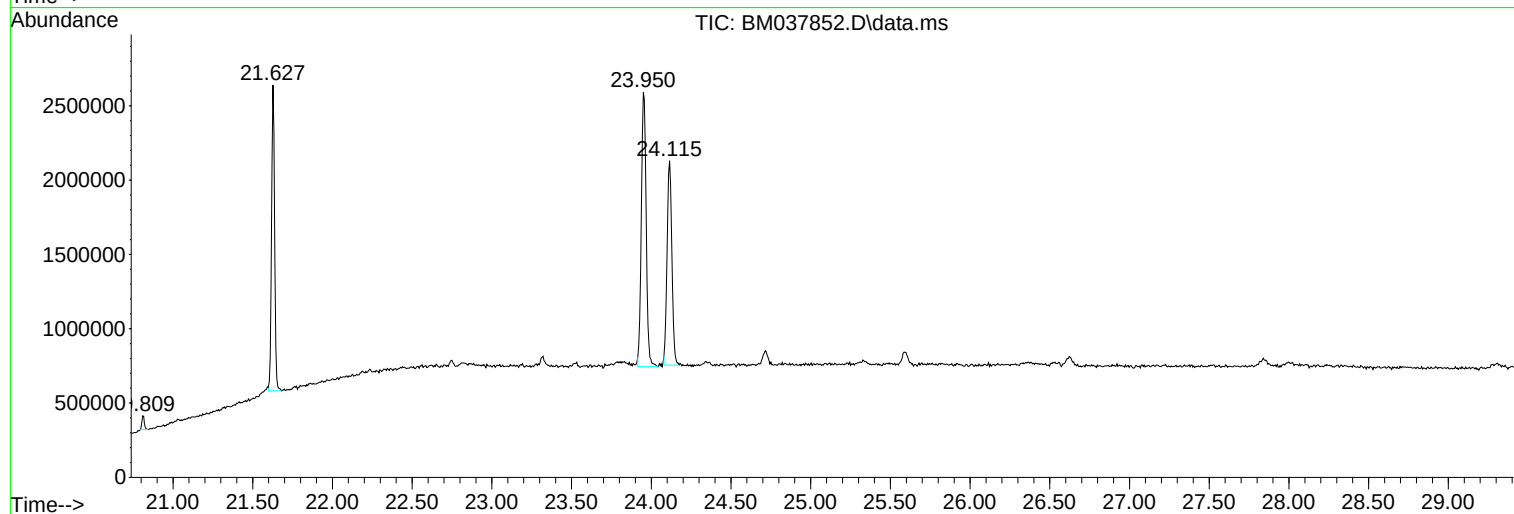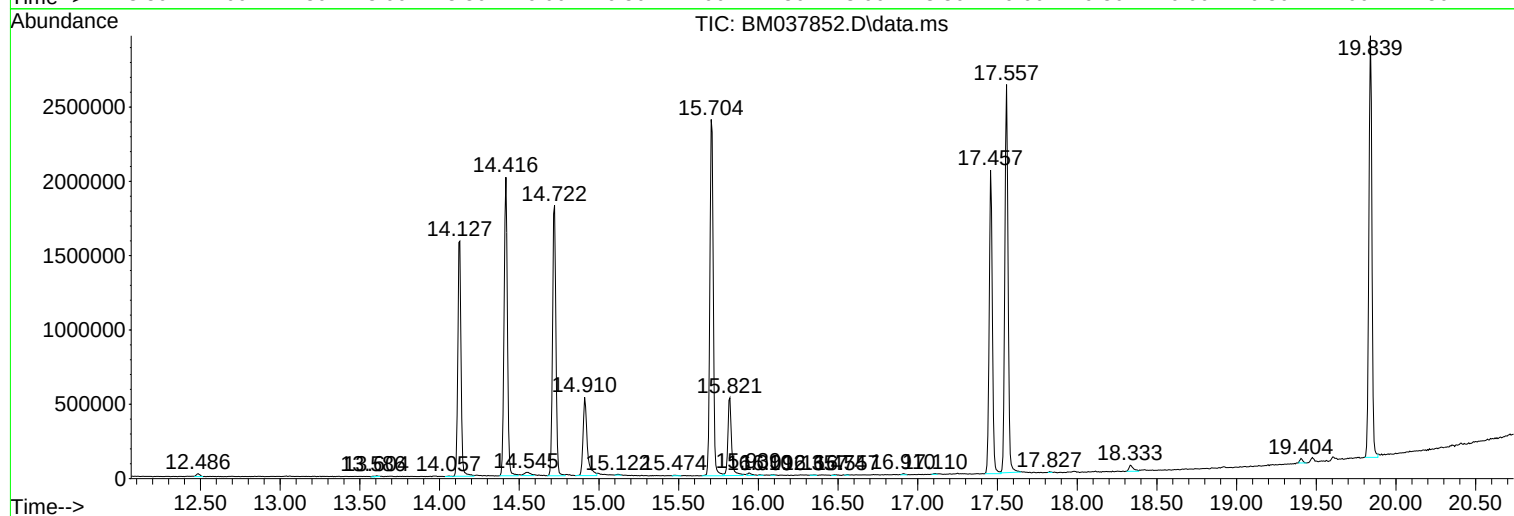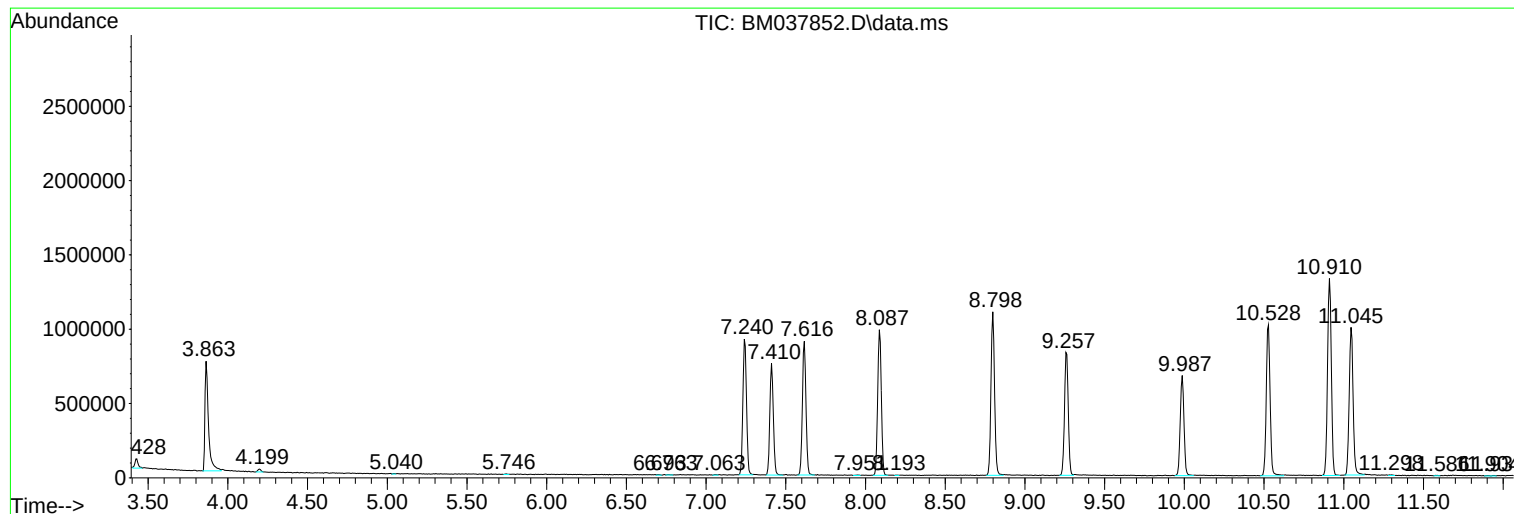

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
Data File : BM037852.D
Acq On : 06 Dec 2022 12:30
Operator : CG/JU
Sample : PB149426BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
Data File : BM037852.D
Acq On : 06 Dec 2022 12:30
Operator : CG/JU
Sample : PB149426BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK426

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc