

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
 Data File : BM037865.D
 Acq On : 06 Dec 2022 21:49
 Operator : CG/JU
 Sample : N5738-15MEDL 30X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBNJ4MEDL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.199	134	138	143	rVB2	13914	22129	0.13%	0.073%
2	7.246	651	656	665	rVB	20967	37092	0.21%	0.122%
3	7.410	679	684	688	rBV2	19421	31338	0.18%	0.103%
4	7.616	713	719	724	rBV2	22166	36681	0.21%	0.121%
5	8.087	792	799	806	rBV	761944	1213462	7.00%	4.003%
6	8.804	915	921	926	rBV3	21880	41151	0.24%	0.136%
7	9.263	993	999	1007	rVB2	21866	42346	0.24%	0.140%
8	9.987	1117	1122	1130	rVB4	14816	28950	0.17%	0.095%
9	10.528	1207	1214	1221	rBV3	20696	38585	0.22%	0.127%
10	10.910	1269	1279	1287	rBV	1061880	1737939	10.03%	5.733%
11	11.057	1299	1304	1309	rBV7	9161	18558	0.11%	0.061%
12	14.122	1818	1825	1834	rBV	41472	67173	0.39%	0.222%
13	14.416	1869	1875	1882	rBV	44682	70719	0.41%	0.233%
14	14.716	1918	1926	1945	rBV	1388325	2152565	12.42%	7.100%
15	15.339	2025	2032	2048	rBV	527993	847072	4.89%	2.794%
16	15.704	2090	2094	2102	rVB	64148	90714	0.52%	0.299%
17	17.110	2325	2333	2349	rBV	11235832	17331055	100.00%	57.168%
18	17.457	2386	2392	2404	rBV	1748503	2456269	14.17%	8.102%
19	17.557	2404	2409	2415	rVB	69043	105494	0.61%	0.348%
20	18.068	2491	2496	2500	rBV6	27462	36053	0.21%	0.119%
21	18.333	2538	2541	2545	rBV6	16427	24714	0.14%	0.082%
22	19.833	2793	2796	2802	rBV2	66840	88295	0.51%	0.291%
23	21.621	3096	3100	3110	rVB	1415787	1900928	10.97%	6.270%
24	24.109	3517	3523	3532	rVB2	913282	1896559	10.94%	6.256%


Sum of corrected areas: 30315841

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
Data File : BM037865.D
Acq On : 06 Dec 2022 21:49
Operator : CG/JU
Sample : N5738-15MEDL 30X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBNJ4MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

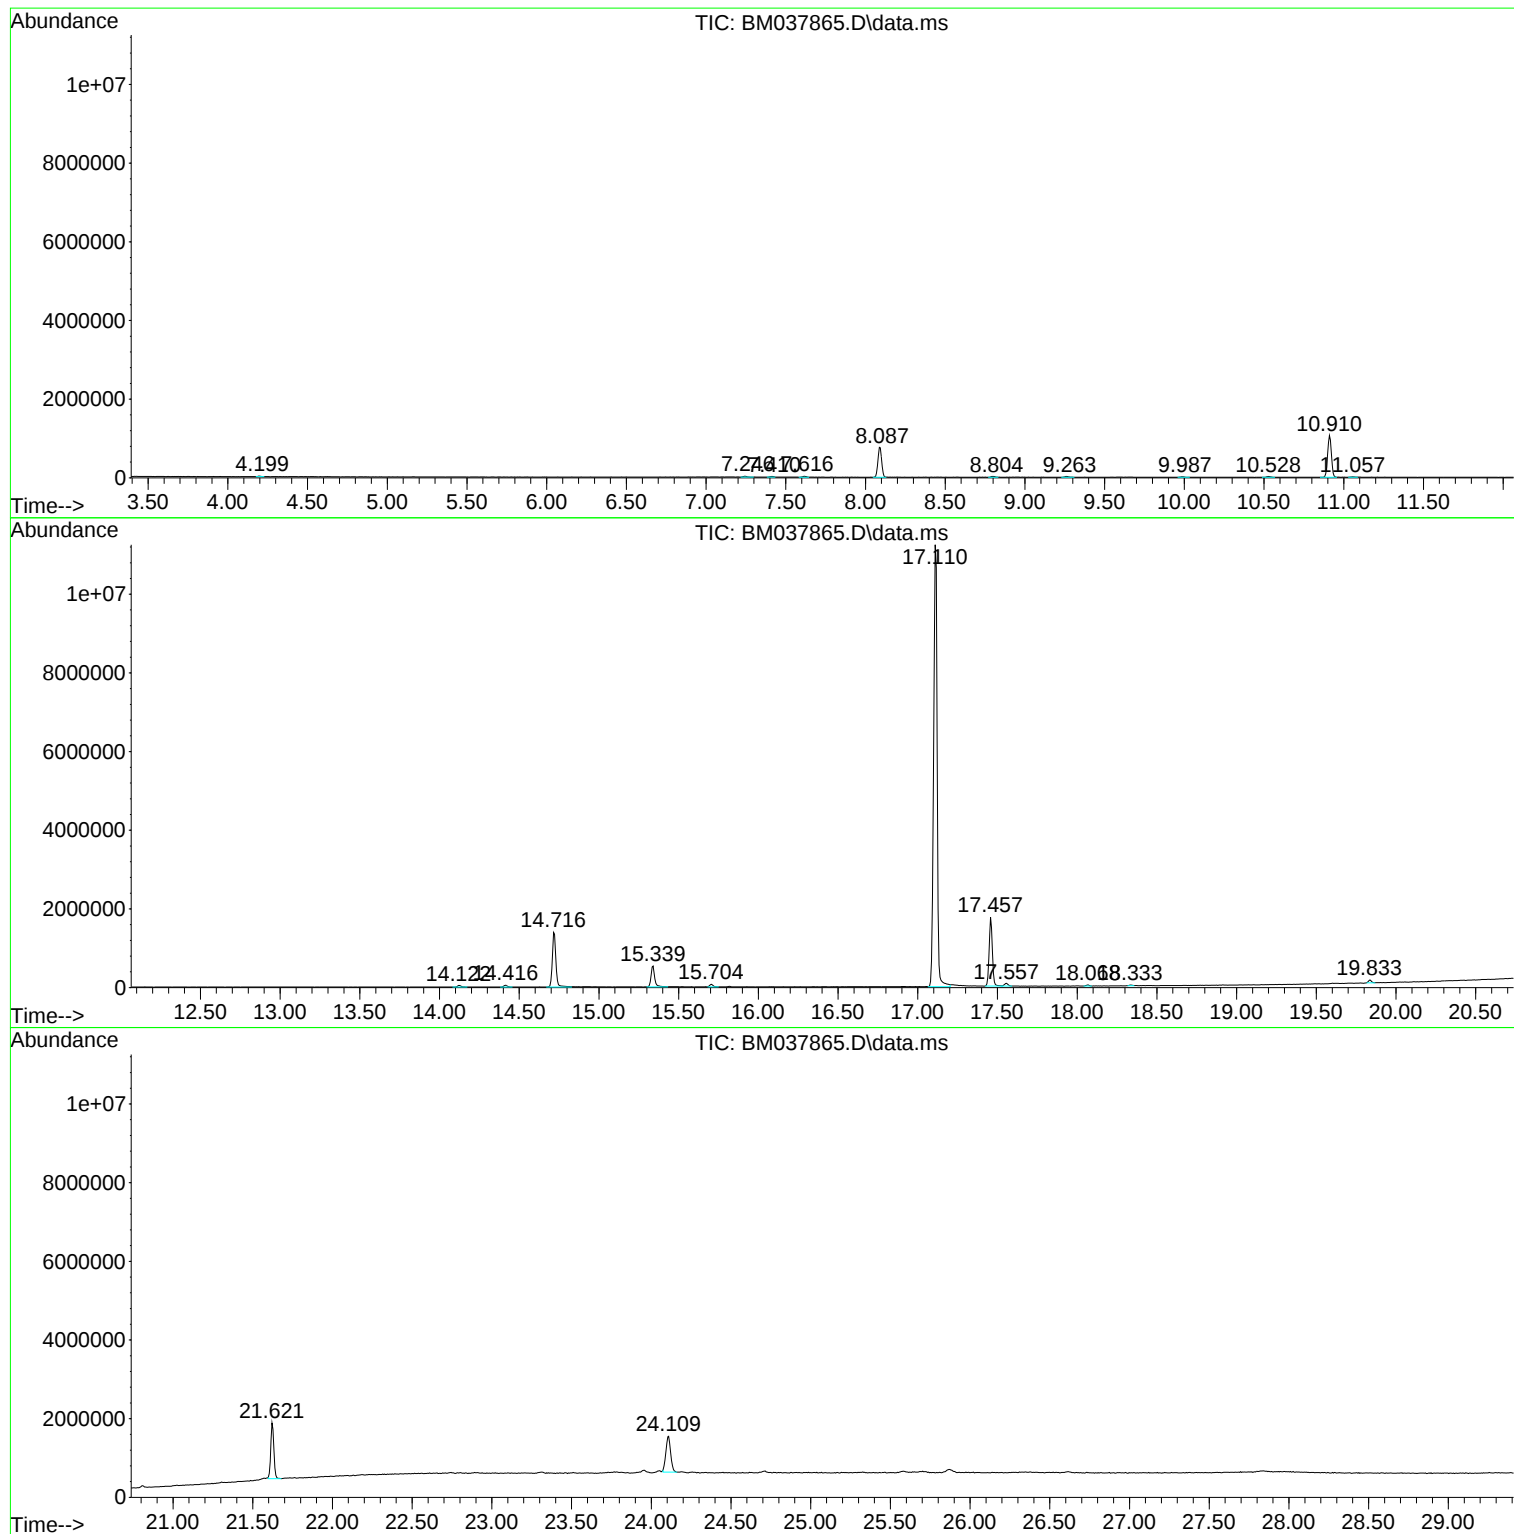

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
Data File : BM037865.D
Acq On : 06 Dec 2022 21:49
Operator : CG/JU
Sample : N5738-15MEDL 30X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBNJ4MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120622\
Data File : BM037865.D
Acq On : 06 Dec 2022 21:49
Operator : CG/JU
Sample : N5738-15MEDL 30X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBNJ4MEDL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120122.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
