

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017990.D
 Acq On : 07 Dec 2018 07:50
 Operator : JU/SJ
 Sample : J6170-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9M06

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:39:52 AM

Quant Time: Dec 07 12:19:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 07 08:24:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	143926	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	551494	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	276666	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	570762	20.00	ng/ul	0.00
77) Chrysene-d12	21.17	240	604209	20.00	ng/ul	0.00
85) Perylene-d12	23.35	264	640169	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	4269	1.36	ng/uL	0.00
5) Phenol-d5	6.75	99	64437	4.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	187964	23.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	227896	22.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	116386	10.84	ng/ul	0.00
19) Nitrobenzene-d5	8.71	128	122424	28.90	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	133346	27.47	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.96	165	210669	22.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	11435m	1.44	ng/ul	0.06
43) Dimethylphthalate-d6	13.63	166	678255	28.25	ng/ul	0.00
46) Acenaphthylene-d8	13.90	160	864635	29.76	ng/ul	0.00
51) 4-Nitrophenol-d4	14.55	143	9905m	2.27	ng/ul	0.11
57) Fluorene-d10	15.21	176	583615	28.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	76297	18.70	ng/ul	0.00
70) Anthracene-d10	17.06	188	852809	30.01	ng/ul	0.00
78) Pyrene-d10	19.37	212	947862	32.42	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.21	264	1091946	31.45	ng/ul	0.00

Target Compounds				Ovalue	
6) Phenol	6.78	94	16739	1.276	ng/ul 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM017990.D
Acq On : 07 Dec 2018 07:50
Operator : JU/SJ
Sample : J6170-03
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F9M06

Manual Integrations
APPROVED

Sohil
12/11/2018 8:39:52 AM

Quant Time: Dec 07 12:19:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 07 08:24:59 2018
Response via : Initial Calibration

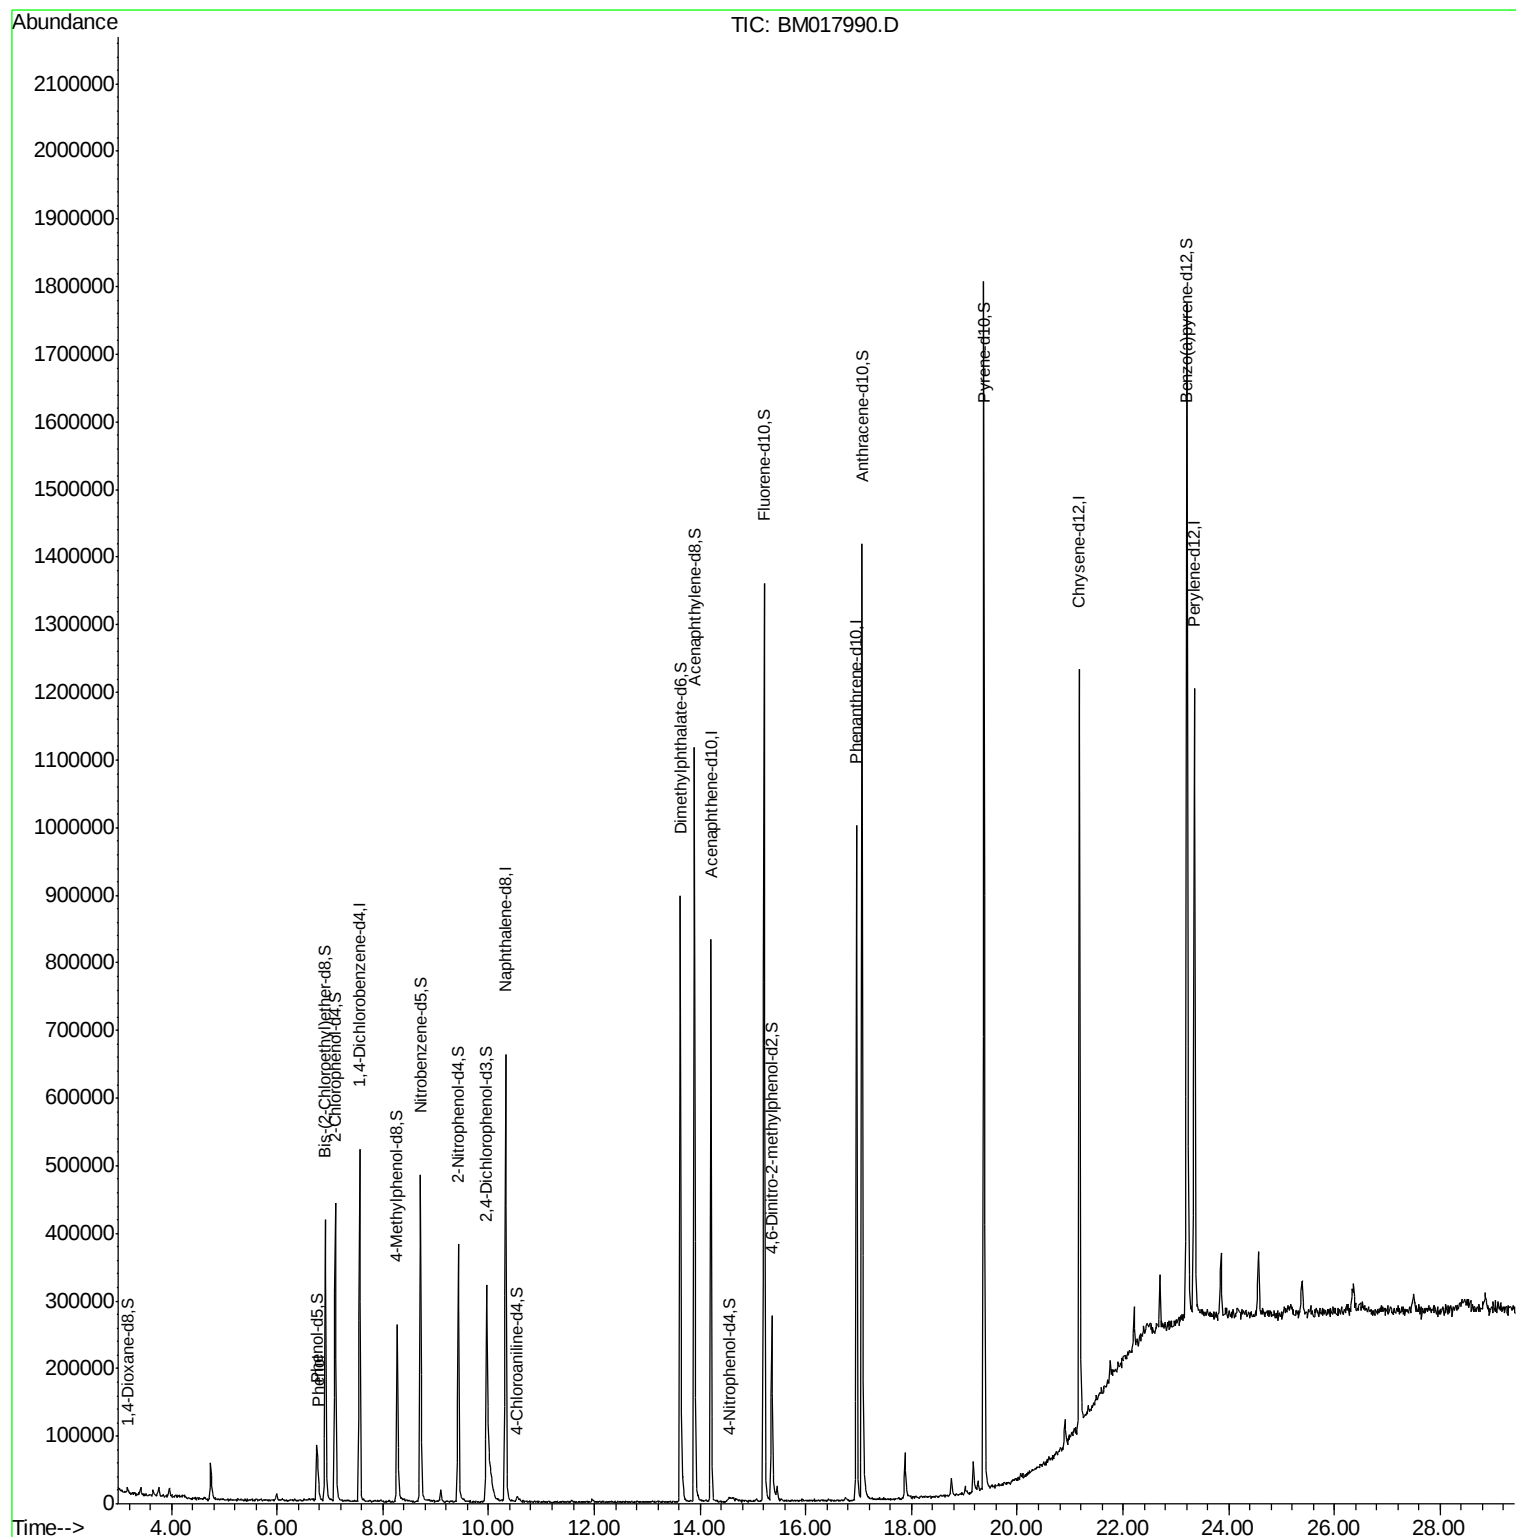

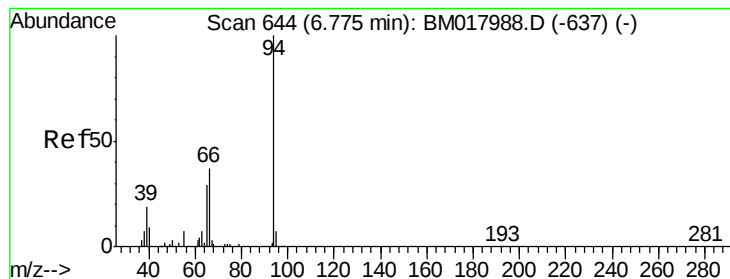

#6

Phenol

Concen: 1.276 ng/ul

RT: 6.78 min Scan# 645

Delta R.T. 0.01 min

Lab File: BM017990.D

Acq: 07 Dec 2018 07:50

Instrument :

BNA_M

ClientSampleId :

F9M06

Tot Ion: 94 Resp: 16739

Ion Ratio Lower Upper

94 100

65 26.2 24.7 37.1

66 51.4 34.6 51.8

Manual Integrations

APPROVED

Sohil

12/11/2018 8:39:52 AM

