

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017993.D
 Acq On : 07 Dec 2018 09:38
 Operator : JU/SJ
 Sample : J6170-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9M09

Manual Integrations
 APPROVED

Sohil
 12/11/2018 8:39:55 AM

Quant Time: Dec 07 12:51:21 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 07 08:24:59 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	143122	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	550757	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	287130	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	612210	20.00	ng/ul	0.00
77) Chrysene-d12	21.17	240	680428	20.00	ng/ul	0.00
85) Perylene-d12	23.35	264	735665	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	4241m	1.36	ng/uL	0.00
5) Phenol-d5	6.76	99	52314	4.00	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.91	67	133116	16.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	161179	15.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.27	113	90541	8.48	ng/ul	0.00
19) Nitrobenzene-d5	8.72	128	86447	20.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.43	143	93312	19.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.97	165	150271m	16.29	ng/ul	0.01
29) 4-Chloroaniline-d4	10.56	131	5903m	0.75	ng/ul	0.08
43) Dimethylphthalate-d6	13.63	166	528170	21.20	ng/ul	0.00
46) Acenaphthylene-d8	13.89	160	645230	21.40	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	10003m	2.21	ng/ul	0.09
57) Fluorene-d10	15.21	176	458375	21.31	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.36	200	63542	14.52	ng/ul	0.00
70) Anthracene-d10	17.06	188	684067	22.44	ng/ul	0.00
78) Pyrene-d10	19.37	212	774016	23.51	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.21	264	912857	22.88	ng/ul	0.00

Target Compounds					Ovalue	
6) Phenol	6.77	94	26839	2.057	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM017993.D
Acq On : 07 Dec 2018 09:38
Operator : JU/SJ
Sample : J6170-06
Misc :
ALS Vial : 32 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
F9M09

Quant Time: Dec 07 12:51:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 07 08:24:59 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/11/2018 8:39:55 AM

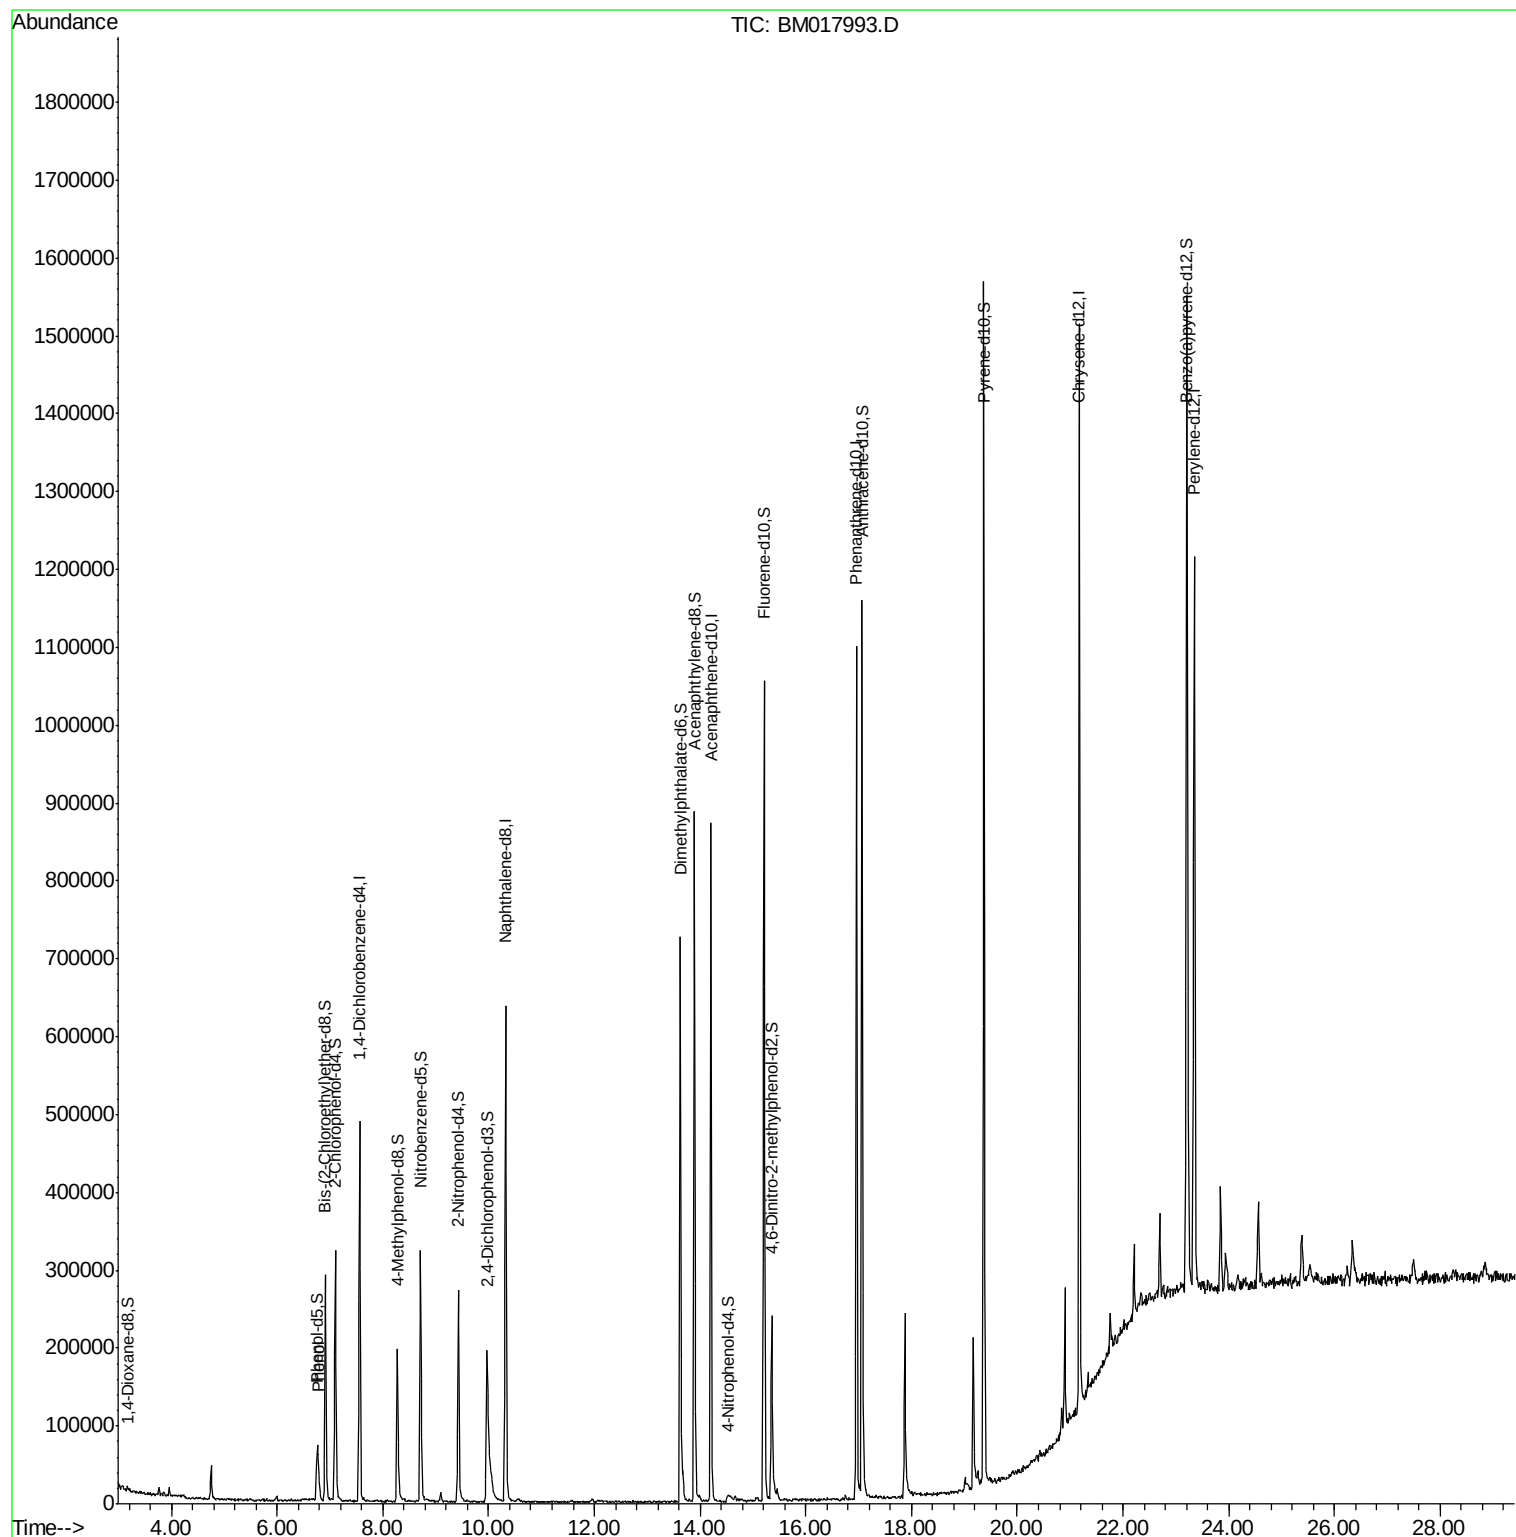

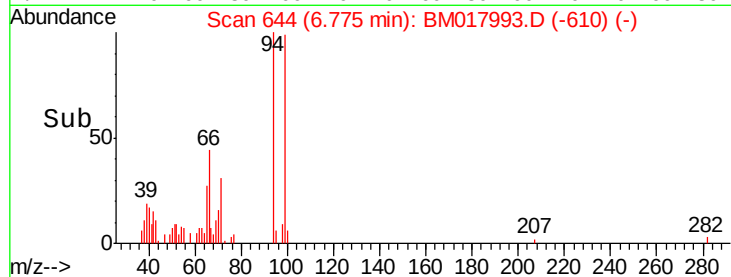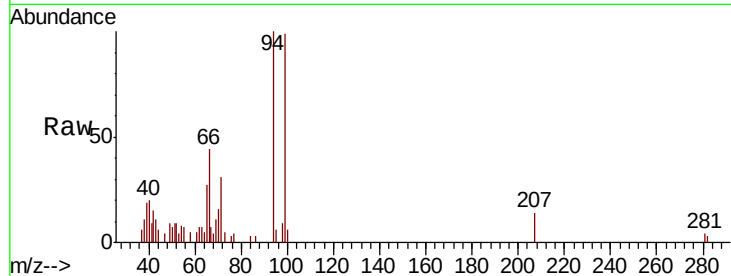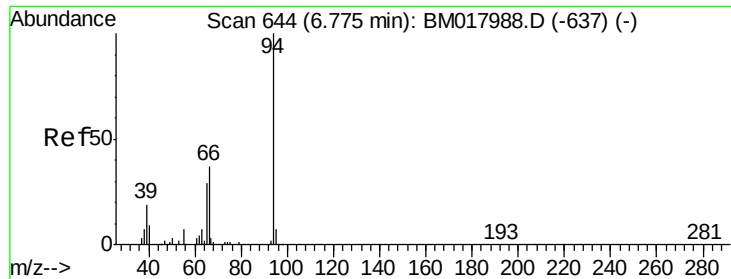

#6

Phenol

Concen: 2.057 ng/ul

RT: 6.77 min Scan# 644

Delta R.T. 0.00 min

Lab File: BM017993.D

Acq: 07 Dec 2018 09:38

Tot Ion:	94	Resp:	26839
Ion Ratio	Lower	Upper	
94	100		
65	27.3	24.7	37.1
66	43.8	34.6	51.8

Instrument :

BNA_M

ClientSampleId :

F9M09

Manual Integrations
APPROVED

Sohil
12/11/2018 8:39:55 AM

