

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017967.D
 Acq On : 06 Dec 2018 15:25
 Operator : JU/SJ
 Sample : J6096-26
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4174

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	34	rBV2	10615	11925	0.43%	0.047%
2	3.263	45	47	48	rVV2	3138	2799	0.10%	0.011%
3	3.299	51	53	57	rVB4	3578	4724	0.17%	0.019%
4	3.363	61	64	68	rBV5	4064	4428	0.16%	0.017%
5	3.463	79	81	84	rBV3	2947	2865	0.10%	0.011%
6	3.699	118	121	122	rBV3	3300	3017	0.11%	0.012%
7	3.763	127	132	137	rVB7	4956	11098	0.40%	0.044%
8	3.851	145	147	152	rBV2	7353	7962	0.29%	0.031%
9	4.128	190	194	196	rBV4	2949	4888	0.18%	0.019%
10	4.210	203	208	212	rVB5	6904	10336	0.37%	0.041%
11	4.287	217	221	222	rBV3	2587	3520	0.13%	0.014%
12	4.346	229	231	235	rBV2	3078	2846	0.10%	0.011%
13	4.775	299	304	309	rVB4	4463	8455	0.31%	0.033%
14	5.134	361	365	366	rBV2	1966	2918	0.11%	0.011%
15	5.593	437	443	447	rBV6	2321	4068	0.15%	0.016%
16	5.657	448	454	459	rBV3	14435	24918	0.90%	0.098%
17	6.575	605	610	613	rBV5	2082	3257	0.12%	0.013%
18	6.757	634	641	654	rVB2	100649	219948	7.94%	0.864%
19	6.910	662	667	679	rVV	381723	643484	23.22%	2.528%
20	7.098	692	699	713	rBV	449366	793607	28.63%	3.118%
21	7.210	717	718	723	rVV3	2348	2990	0.11%	0.012%
22	7.563	771	778	788	rBV	435025	733966	26.48%	2.884%
23	7.634	788	790	792	rBV3	3596	3281	0.12%	0.013%
24	7.722	802	805	809	rBV2	2026	3205	0.12%	0.013%
25	8.275	893	899	910	rBV	302071	558556	20.15%	2.195%
26	8.428	922	925	928	rBV4	1755	2872	0.10%	0.011%
27	8.586	948	952	957	rBV5	2231	4006	0.14%	0.016%
28	8.663	959	965	967	rBV5	4897	8213	0.30%	0.032%
29	8.716	967	974	984	rVV	455234	796343	28.73%	3.129%
30	8.910	1005	1007	1010	rVB4	2628	3043	0.11%	0.012%
31	9.104	1035	1040	1043	rBV4	2430	3239	0.12%	0.013%
32	9.186	1051	1054	1059	rVB4	1821	2858	0.10%	0.011%
33	9.428	1088	1095	1109	rBV	383224	679955	24.53%	2.672%
34	9.539	1113	1114	1118	rVB3	3553	2939	0.11%	0.012%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017967.D
 Acq On : 06 Dec 2018 15:25
 Operator : JU/SJ
 Sample : J6096-26
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4174

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

35	9.969	1179	1187	1215	rBV	334442	961302	34.68%	3.777%
36	10.328	1241	1248	1258	rBV	589761	978367	35.30%	3.844%
37	11.686	1473	1479	1486	rBV7	4968	12917	0.47%	0.051%
38	11.957	1519	1525	1532	rBV4	7020	14981	0.54%	0.059%
39	12.551	1619	1626	1631	rBV4	4741	8034	0.29%	0.032%
40	12.810	1665	1670	1674	rBV3	6358	9288	0.34%	0.036%
41	13.057	1706	1712	1716	rBV4	3320	5853	0.21%	0.023%
42	13.204	1730	1737	1738	rBV4	2853	4331	0.16%	0.017%
43	13.633	1802	1810	1827	rBV	814268	1290712	46.57%	5.071%
44	13.898	1848	1855	1866	rBV	1124490	1687755	60.89%	6.631%
45	13.968	1866	1867	1872	rVB2	5860	6039	0.22%	0.024%
46	14.210	1902	1908	1920	rBV2	748217	1167409	42.12%	4.587%
47	14.304	1920	1924	1925	rVV2	4253	4007	0.14%	0.016%
48	14.515	1952	1960	1962	rBV5	13427	32844	1.19%	0.129%
49	14.910	2024	2027	2032	rVB5	3959	6170	0.22%	0.024%
50	15.021	2042	2046	2049	rVV2	2342	3488	0.13%	0.014%
51	15.063	2049	2053	2058	rVB2	3872	6418	0.23%	0.025%
52	15.210	2071	2078	2095	rVV	1311449	2101357	75.82%	8.257%
53	15.357	2098	2103	2116	rVV	325233	548872	19.80%	2.157%
54	15.457	2116	2120	2125	rVB2	14387	28224	1.02%	0.111%
55	15.974	2204	2208	2211	rBV2	1824	2811	0.10%	0.011%
56	16.074	2220	2225	2228	rBV3	2250	3565	0.13%	0.014%
57	16.968	2371	2377	2387	rVV	901942	1268320	45.76%	4.983%
58	17.068	2387	2394	2409	rVV	1414693	2153589	77.70%	8.462%
59	17.162	2409	2410	2416	rVB3	5372	5273	0.19%	0.021%
60	17.345	2440	2441	2444	rBV3	3263	2833	0.10%	0.011%
61	17.645	2488	2492	2495	rBV2	45119	46803	1.69%	0.184%
62	17.892	2528	2534	2540	rBV7	14924	30768	1.11%	0.121%
63	17.962	2542	2546	2548	rVV3	3690	5077	0.18%	0.020%
64	17.992	2549	2551	2556	rVB5	3028	3656	0.13%	0.014%
65	18.127	2568	2574	2577	rVV4	3090	5141	0.19%	0.020%
66	18.298	2601	2603	2607	rBV3	2933	3362	0.12%	0.013%
67	18.421	2622	2624	2629	rBV5	2061	3510	0.13%	0.014%
68	18.668	2664	2666	2669	rBV3	2980	3033	0.11%	0.012%
69	18.927	2708	2710	2713	rBV3	2895	4010	0.14%	0.016%
70	19.015	2721	2725	2728	rBV2	12741	17059	0.62%	0.067%
71	19.174	2748	2752	2757	rBV5	15838	28626	1.03%	0.112%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM017967.D
Acq On : 06 Dec 2018 15:25
Operator : JU/SJ
Sample : J6096-26
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4174

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Title : SVOA CALIBRATION

72	19.256	2764	2766	2774	rBV3	10955	20452	0.74%	0.080%
73	19.374	2780	2786	2795	rBV	1779169	2474443	89.28%	9.722%
74	19.445	2795	2798	2804	rVB2	31569	51163	1.85%	0.201%
75	19.633	2827	2830	2835	rBV5	9742	15730	0.57%	0.062%
76	20.139	2914	2916	2919	rBV4	7167	7250	0.26%	0.028%
77	21.186	3089	3094	3102	rBV	1028461	1509843	54.47%	5.932%
78	23.227	3434	3441	3453	rVB	1375568	2771639	100.00%	10.890%
79	23.362	3458	3464	3474	rVB	793330	1557969	56.21%	6.121%


Sum of corrected areas: 25450822

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM017967.D
Acq On : 06 Dec 2018 15:25
Operator : JU/SJ
Sample : J6096-26
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4174

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

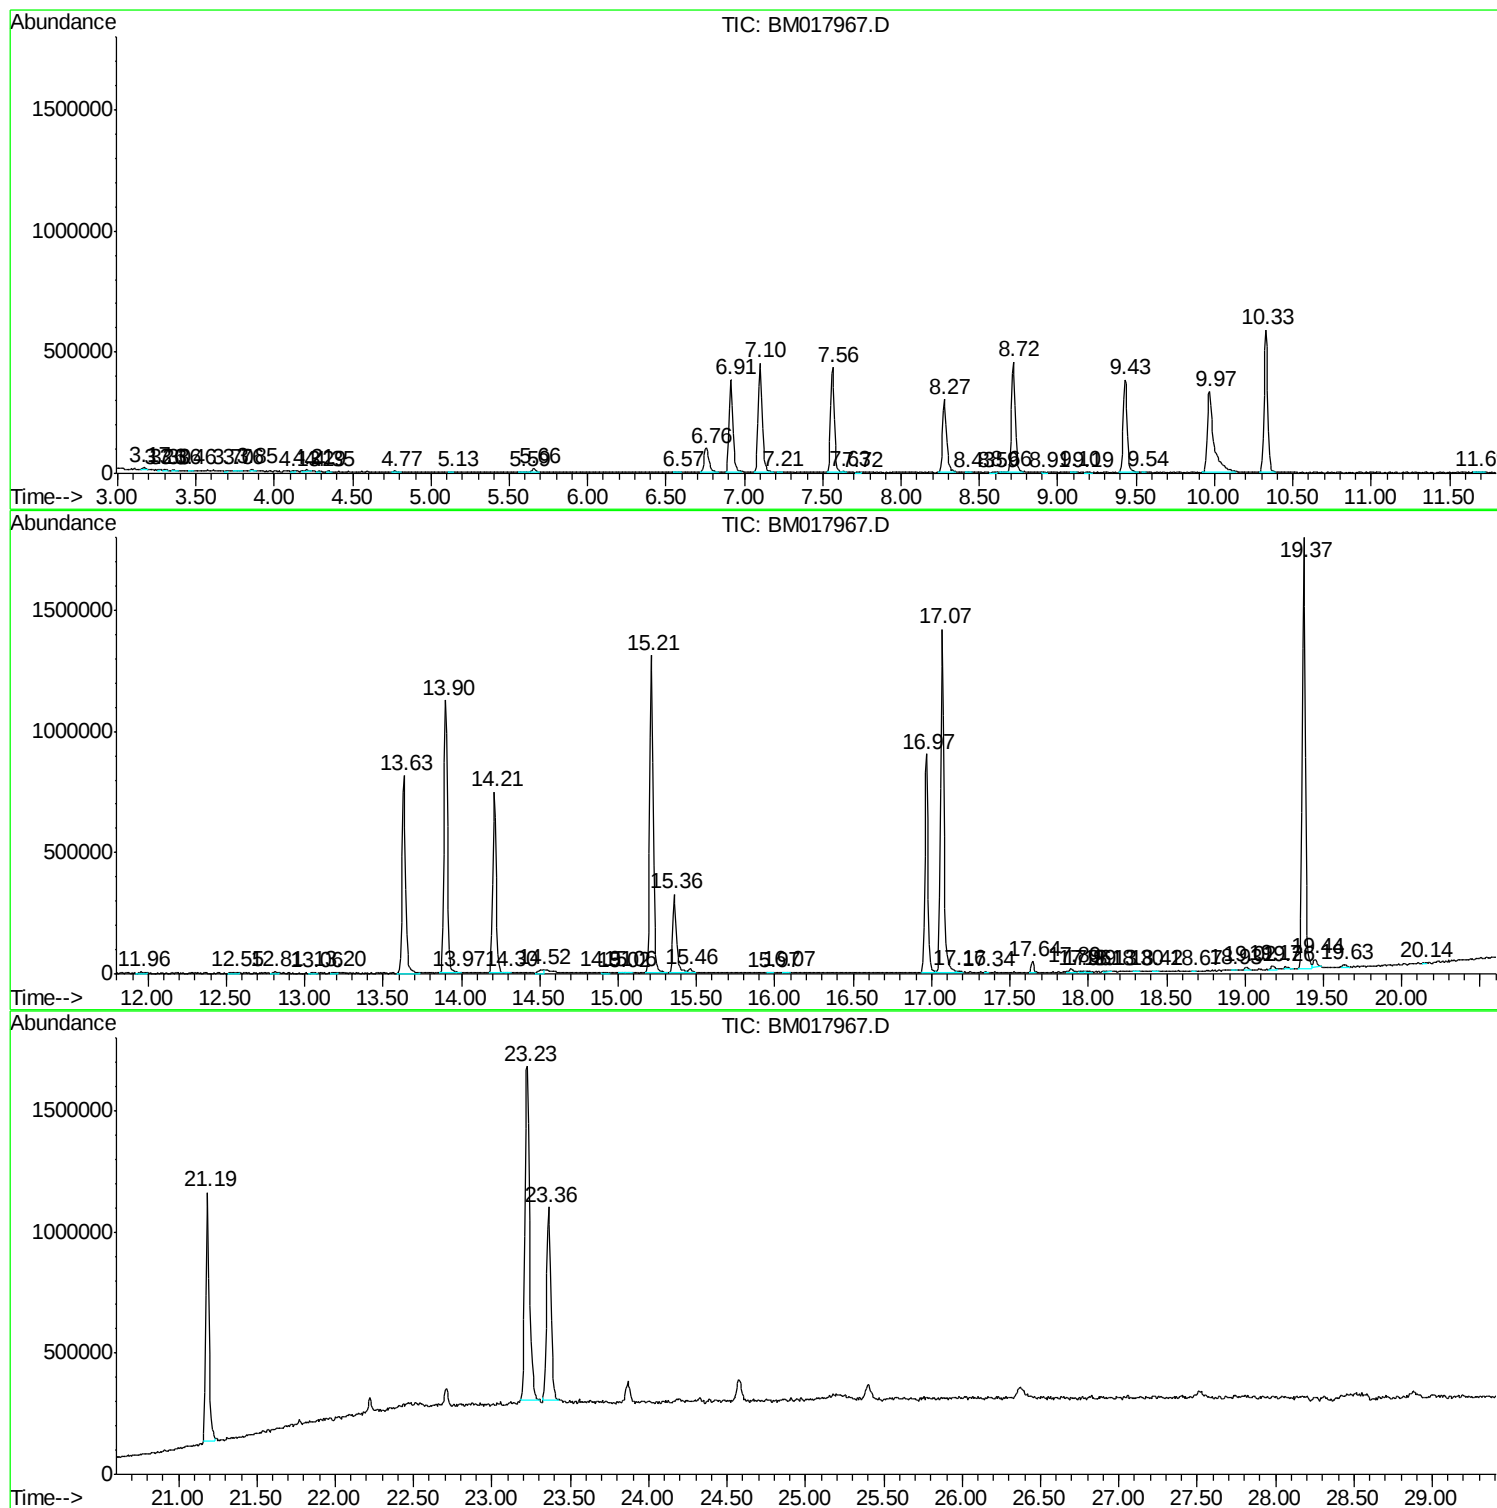

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM017967.D
Acq On : 06 Dec 2018 15:25
Operator : JU/SJ
Sample : J6096-26
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4174

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM017967.D
Acq On : 06 Dec 2018 15:25
Operator : JU/SJ
Sample : J6096-26
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4174

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc