

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017987.D
 Acq On : 07 Dec 2018 05:42
 Operator : JU/SJ
 Sample : PB115317BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK17

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.034	6	8	9	rVB2	4238	2963	0.10%	0.010%
2	3.046	9	10	17	rVB5	4848	9392	0.32%	0.032%
3	3.163	25	30	37	rBV	32539	53890	1.86%	0.184%
4	3.246	43	44	47	rBV3	3419	3292	0.11%	0.011%
5	3.269	47	48	52	rBV4	3591	4761	0.16%	0.016%
6	3.440	73	77	79	rBV4	2329	2922	0.10%	0.010%
7	4.328	226	228	231	rBV4	3117	3620	0.12%	0.012%
8	4.699	289	291	294	rVB3	2889	3349	0.12%	0.011%
9	5.010	341	344	346	rBV4	2835	3035	0.10%	0.010%
10	5.357	401	403	407	rBV3	2002	3543	0.12%	0.012%
11	5.410	410	412	415	rVB3	3166	3340	0.12%	0.011%
12	5.598	442	444	449	rVB2	2205	3085	0.11%	0.011%
13	6.145	533	537	540	rVB4	2432	3661	0.13%	0.013%
14	6.281	556	560	563	rVV4	2327	3764	0.13%	0.013%
15	6.657	622	624	628	rBV3	2348	3404	0.12%	0.012%
16	6.745	633	639	653	rBV	448473	831148	28.65%	2.843%
17	6.910	661	667	682	rVB	405086	650925	22.44%	2.227%
18	7.092	692	698	711	rBV	548043	936398	32.28%	3.203%
19	7.228	719	721	725	rVB4	2975	3599	0.12%	0.012%
20	7.557	771	777	790	rVB	518687	861910	29.71%	2.948%
21	8.269	891	898	920	rBV	539840	1017021	35.05%	3.479%
22	8.710	966	973	987	rBV	449199	807067	27.82%	2.761%
23	9.051	1027	1031	1033	rVB4	2402	3005	0.10%	0.010%
24	9.086	1033	1037	1040	rBV3	2489	3592	0.12%	0.012%
25	9.269	1066	1068	1072	rBV2	2890	3273	0.11%	0.011%
26	9.428	1088	1095	1109	rBV	378163	671738	23.15%	2.298%
27	9.528	1109	1112	1116	rVB3	3826	5294	0.18%	0.018%
28	9.957	1178	1185	1198	rBV	461064	925698	31.91%	3.167%
29	10.151	1216	1218	1221	rVB3	3763	3114	0.11%	0.011%
30	10.322	1240	1247	1260	rBV	664272	1128479	38.90%	3.860%
31	10.480	1267	1274	1298	rBV	331005	913552	31.49%	3.125%
32	11.122	1379	1383	1387	rBV3	2359	3674	0.13%	0.013%
33	11.969	1523	1527	1531	rVV4	6348	10492	0.36%	0.036%
34	13.627	1803	1809	1826	rBV	842464	1426396	49.16%	4.879%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017987.D
 Acq On : 07 Dec 2018 05:42
 Operator : JU/SJ
 Sample : PB115317BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK17

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

35	13.898	1847	1855	1870	rBV	1097160	1735538	59.82%	5.937%
36	14.204	1901	1907	1921	rVB2	833531	1310999	45.19%	4.485%
37	14.333	1927	1929	1936	rVB3	1851	2963	0.10%	0.010%
38	14.463	1944	1951	1967	rBV2	111390	395158	13.62%	1.352%
39	15.210	2071	2078	2093	rBV	1364786	2158769	74.41%	7.384%
40	15.351	2097	2102	2115	rVV	299467	541179	18.65%	1.851%
41	15.457	2116	2120	2129	rVV5	19979	38597	1.33%	0.132%
42	16.168	2237	2241	2243	rBV2	2838	3403	0.12%	0.012%
43	16.751	2338	2340	2344	rVB3	3862	5519	0.19%	0.019%
44	16.962	2370	2376	2387	rBV2	1011062	1424362	49.09%	4.872%
45	17.062	2387	2393	2413	rVB2	1421296	2243902	77.34%	7.676%
46	17.768	2509	2513	2515	rBV4	2753	3623	0.12%	0.012%
47	18.321	2603	2607	2611	rBV3	1915	3828	0.13%	0.013%
48	18.551	2644	2646	2647	rBV2	3603	3005	0.10%	0.010%
49	18.580	2649	2651	2654	rVV3	2935	3396	0.12%	0.012%
50	19.009	2720	2724	2727	rBV3	13199	17674	0.61%	0.060%
51	19.256	2763	2766	2772	rBV5	10959	15611	0.54%	0.053%
52	19.374	2779	2786	2799	rBV	1648261	2583319	89.04%	8.837%
53	21.180	3087	3093	3107	rBV	1086958	1789661	61.69%	6.122%
54	23.209	3432	3438	3454	rBV	1510745	2901261	100.00%	9.924%
55	23.350	3456	3462	3474	rVB2	879622	1737631	59.89%	5.944%


Sum of corrected areas: 29233794

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM017987.D
Acq On : 07 Dec 2018 05:42
Operator : JU/SJ
Sample : PB115317BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK17

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

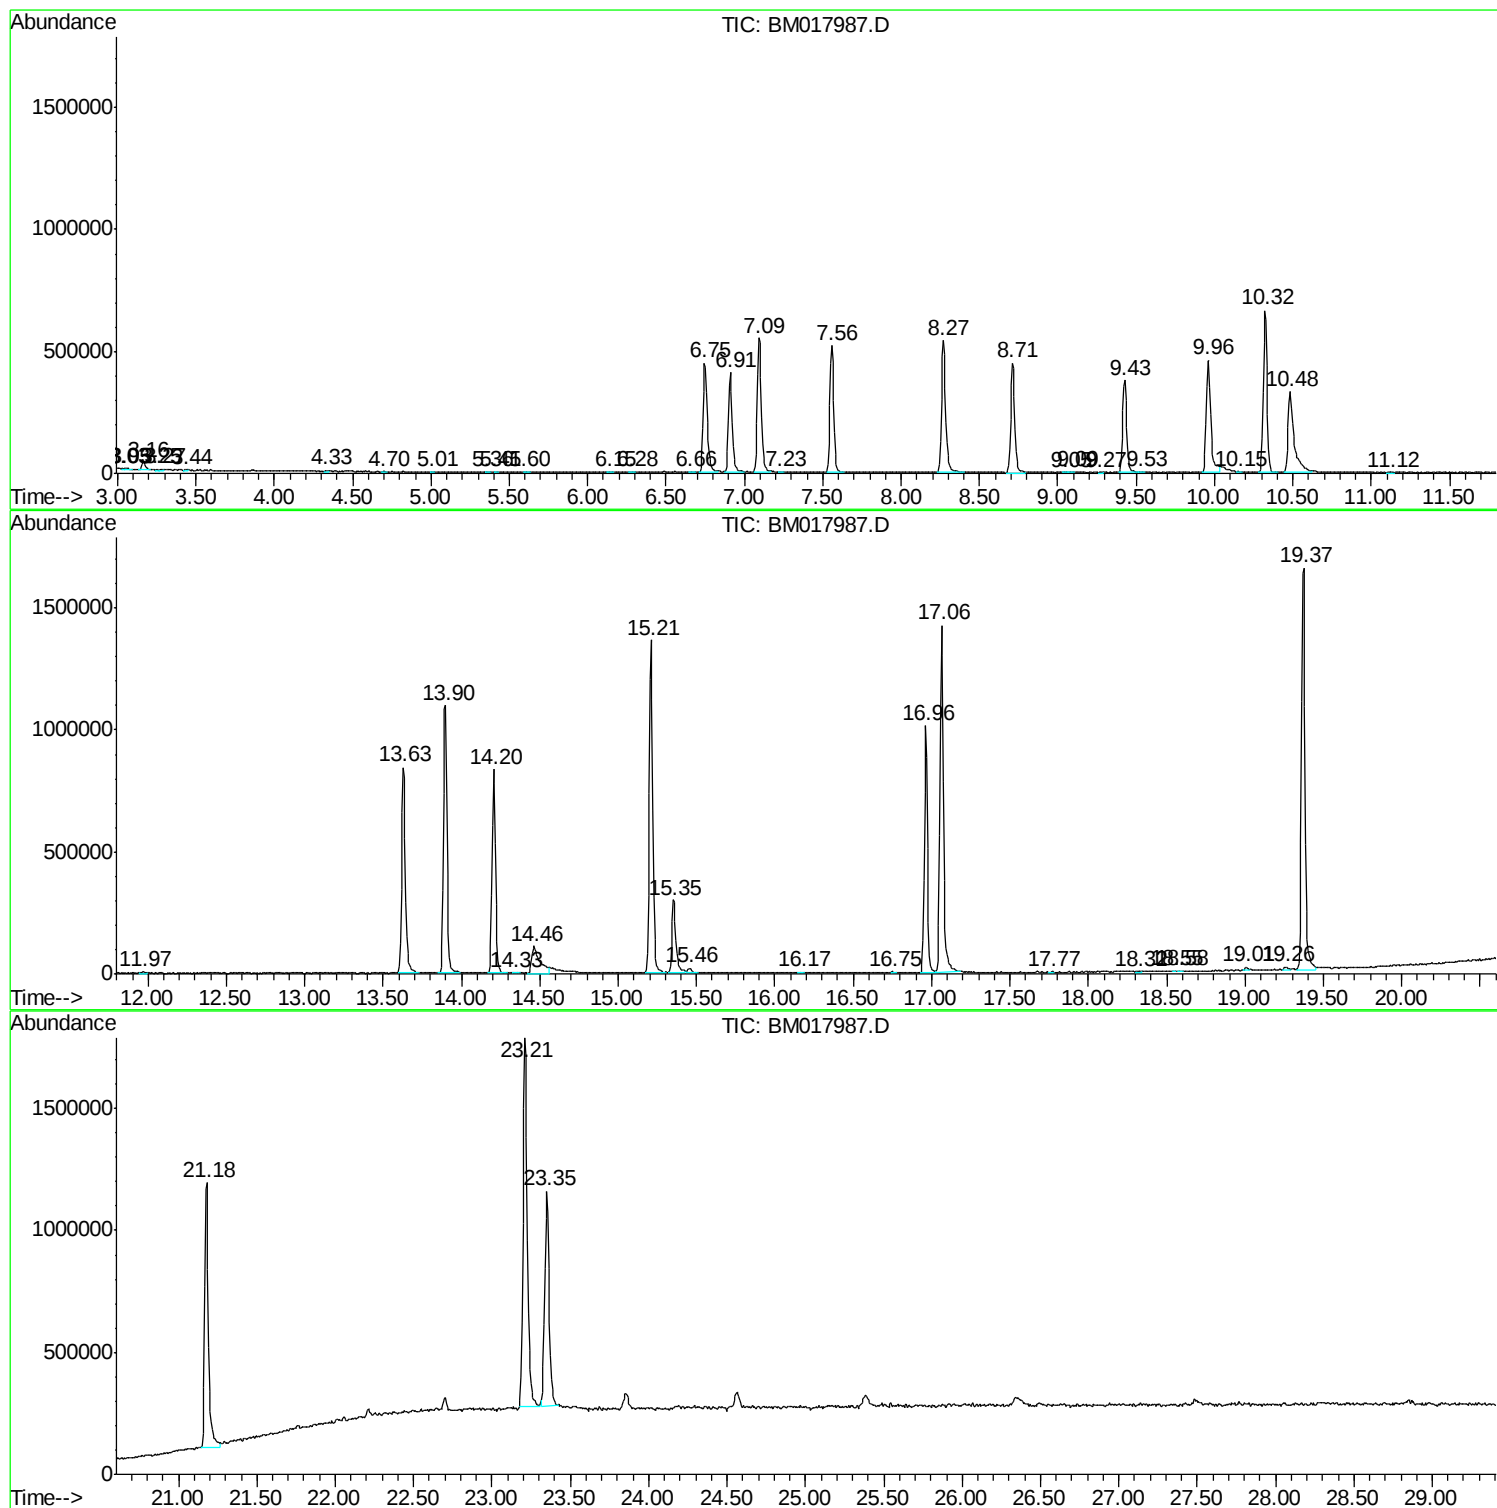

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM017987.D
Acq On : 07 Dec 2018 05:42
Operator : JU/SJ
Sample : PB115317BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK17

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM017987.D
Acq On : 07 Dec 2018 05:42
Operator : JU/SJ
Sample : PB115317BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK17

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc