

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017989.D
 Acq On : 07 Dec 2018 07:14
 Operator : JU/SJ
 Sample : PB115316BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK16

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.163	26	30	40	rVV	34937	55785	1.95%	0.192%
2	3.258	44	46	49	rVB3	2929	2927	0.10%	0.010%
3	3.757	129	131	134	rBV4	3745	4408	0.15%	0.015%
4	4.052	177	181	183	rBV5	4039	5016	0.18%	0.017%
5	4.199	204	206	208	rVB2	4413	3705	0.13%	0.013%
6	4.228	208	211	217	rBV6	4385	7420	0.26%	0.026%
7	4.528	259	262	265	rVV4	3322	4326	0.15%	0.015%
8	4.752	296	300	302	rVB4	2752	3979	0.14%	0.014%
9	4.963	333	336	338	rBV3	2701	3142	0.11%	0.011%
10	5.069	353	354	358	rBV3	2251	3236	0.11%	0.011%
11	5.134	363	365	369	rBV4	2448	3037	0.11%	0.010%
12	5.275	386	389	390	rBV3	2910	2911	0.10%	0.010%
13	5.652	449	453	456	rBV4	3266	5908	0.21%	0.020%
14	5.904	495	496	500	rBV2	2841	3034	0.11%	0.010%
15	5.957	502	505	509	rBV4	2978	5124	0.18%	0.018%
16	6.151	536	538	540	rBV2	2629	3166	0.11%	0.011%
17	6.751	634	640	651	rBV	437732	817062	28.55%	2.809%
18	6.910	660	667	683	rBV	413706	663300	23.18%	2.280%
19	7.098	692	699	713	rVV	555228	934059	32.64%	3.211%
20	7.328	734	738	740	rVB3	2911	3726	0.13%	0.013%
21	7.557	770	777	787	rBV	504160	854005	29.84%	2.936%
22	7.757	809	811	815	rBV2	2328	3488	0.12%	0.012%
23	7.998	848	852	856	rBV5	2125	4292	0.15%	0.015%
24	8.057	859	862	864	rBV3	2717	3163	0.11%	0.011%
25	8.269	892	898	914	rBV	540032	1025128	35.82%	3.524%
26	8.551	944	946	949	rVV3	2321	3119	0.11%	0.011%
27	8.592	949	953	955	rVV3	2202	3228	0.11%	0.011%
28	8.716	967	974	985	rBV	464303	820757	28.68%	2.822%
29	8.875	998	1001	1004	rBV3	2053	3241	0.11%	0.011%
30	9.428	1088	1095	1109	rBV	393605	686319	23.98%	2.359%
31	9.963	1178	1186	1199	rBV	482768	940760	32.87%	3.234%
32	10.328	1240	1248	1257	rVB	656349	1115983	39.00%	3.837%
33	10.486	1267	1275	1302	rBV	342659	928816	32.46%	3.193%
34	11.957	1520	1525	1526	rBV2	4152	4326	0.15%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017989.D
 Acq On : 07 Dec 2018 07:14
 Operator : JU/SJ
 Sample : PB115316BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK16

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

35	11.975	1526	1528	1532	rVB3	4949	6591	0.23%	0.023%
36	13.633	1803	1810	1828	rVV	824564	1417388	49.53%	4.873%
37	13.898	1848	1855	1869	rBV	1117788	1747300	61.06%	6.007%
38	14.210	1901	1908	1921	rBV2	813337	1293953	45.22%	4.448%
39	14.463	1943	1951	1970	rBV3	114720	421223	14.72%	1.448%
40	14.616	1976	1977	1984	rVB5	5899	9532	0.33%	0.033%
41	14.680	1987	1988	1992	rVB4	3323	3305	0.12%	0.011%
42	15.057	2048	2052	2056	rVB2	3164	3948	0.14%	0.014%
43	15.210	2071	2078	2091	rVV	1383623	2151706	75.19%	7.397%
44	15.357	2097	2103	2115	rBV	298826	533481	18.64%	1.834%
45	15.457	2117	2120	2128	rVB5	18476	26790	0.94%	0.092%
46	15.639	2147	2151	2156	rVB5	2316	4188	0.15%	0.014%
47	15.798	2173	2178	2181	rVB4	2195	3115	0.11%	0.011%
48	16.168	2238	2241	2244	rBV3	3218	3663	0.13%	0.013%
49	16.445	2284	2288	2290	rVB2	3453	5201	0.18%	0.018%
50	16.480	2293	2294	2298	rVV4	2397	2975	0.10%	0.010%
51	16.757	2337	2341	2343	rBV4	4361	6532	0.23%	0.022%
52	16.874	2360	2361	2365	rBV2	2582	3074	0.11%	0.011%
53	16.963	2370	2376	2387	rBV	1043270	1418604	49.57%	4.877%
54	17.063	2387	2393	2410	rVV	1407111	2206287	77.10%	7.585%
55	18.010	2552	2554	2556	rVB2	3721	2898	0.10%	0.010%
56	18.215	2586	2589	2590	rBV2	2661	2869	0.10%	0.010%
57	18.457	2624	2630	2635	rVB6	3248	5840	0.20%	0.020%
58	19.009	2720	2724	2729	rBV2	11059	15850	0.55%	0.054%
59	19.180	2750	2753	2754	rBV3	4354	4316	0.15%	0.015%
60	19.262	2763	2767	2772	rBV2	11723	16885	0.59%	0.058%
61	19.374	2780	2786	2798	rBV	1700014	2521846	88.13%	8.670%
62	20.321	2945	2947	2949	rBV3	6996	5092	0.18%	0.018%
63	21.180	3088	3093	3106	rBV	1087900	1708998	59.72%	5.875%
64	23.215	3433	3439	3453	rVB	1446171	2861667	100.00%	9.838%
65	23.356	3457	3463	3475	rVB	856007	1740539	60.82%	5.984%


Sum of corrected areas: 29087552

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM017989.D
Acq On : 07 Dec 2018 07:14
Operator : JU/SJ
Sample : PB115316BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

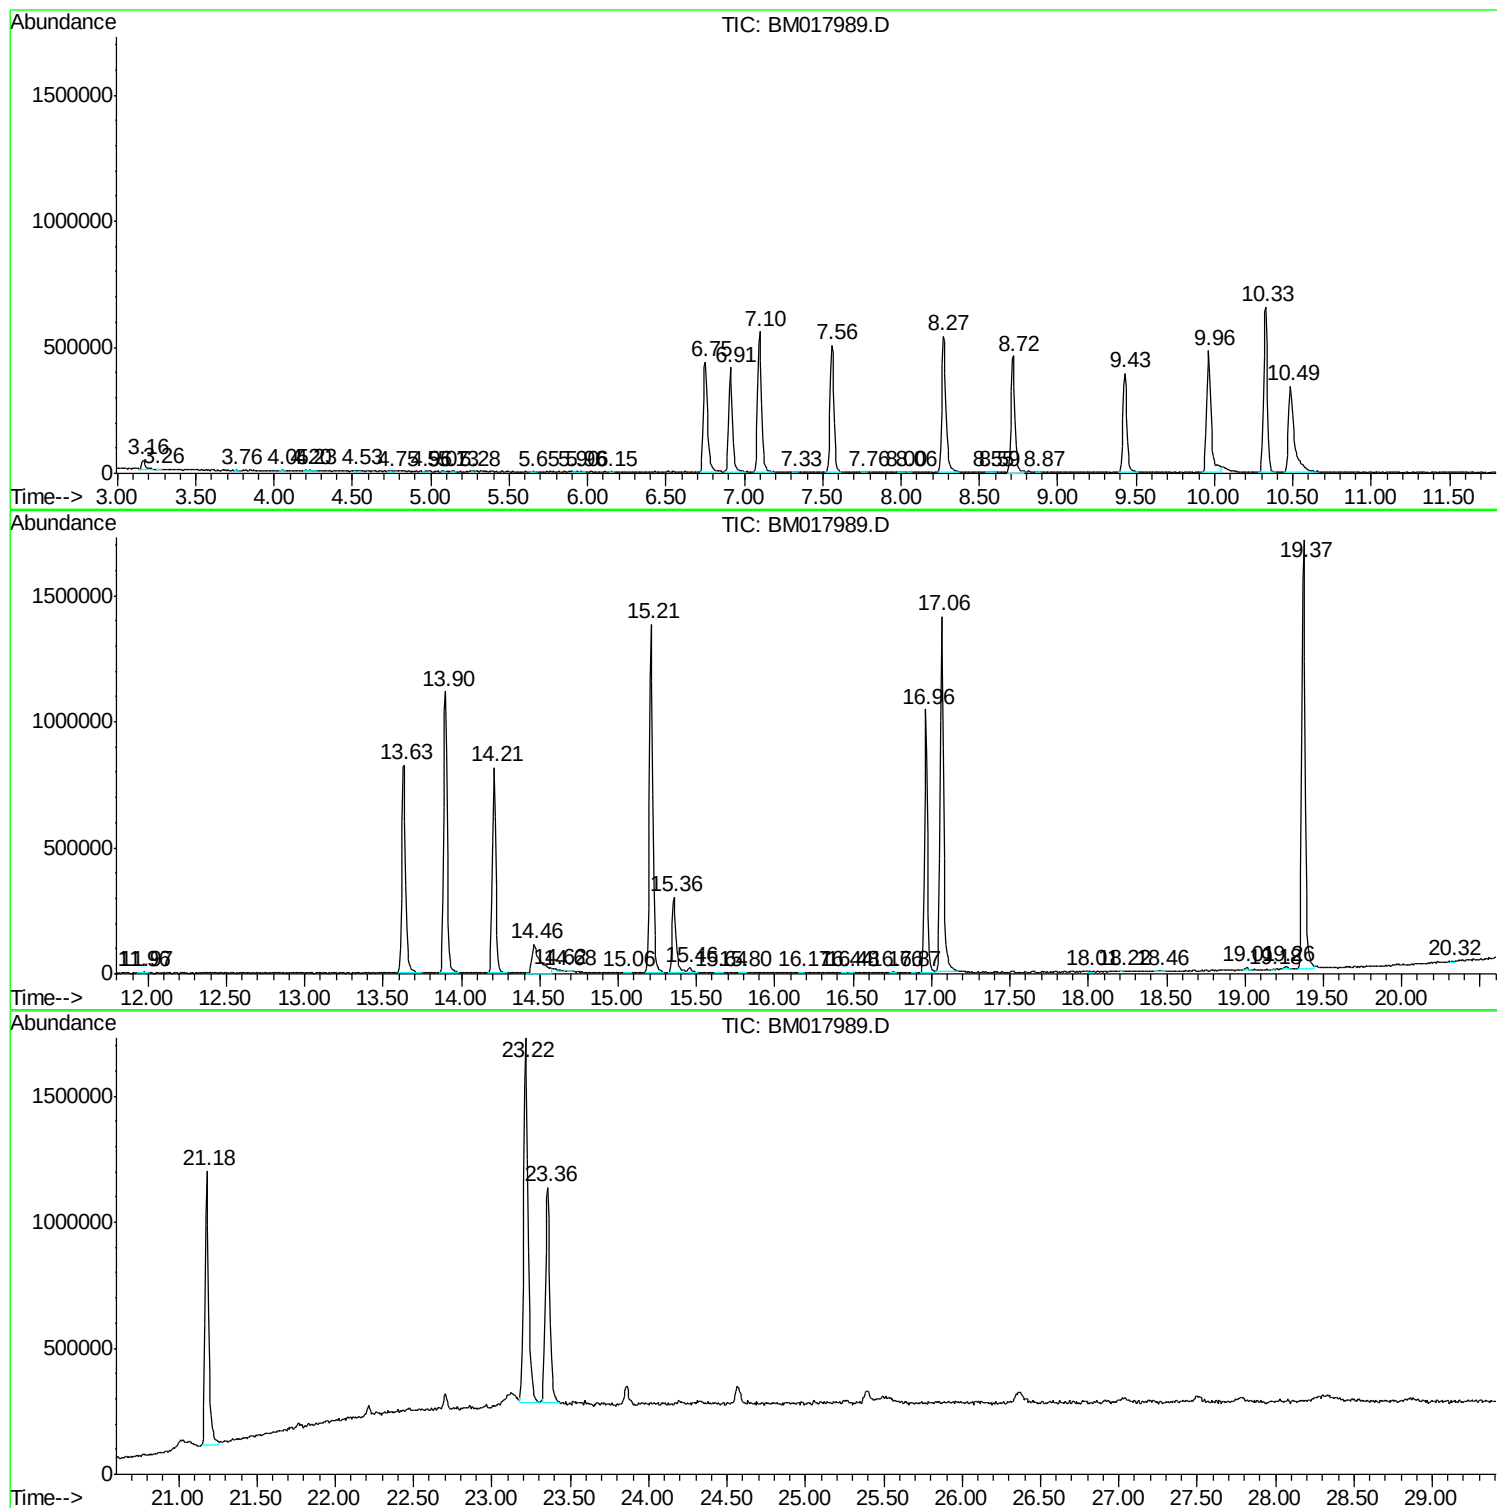

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM017989.D
Acq On : 07 Dec 2018 07:14
Operator : JU/SJ
Sample : PB115316BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM017989.D
Acq On : 07 Dec 2018 07:14
Operator : JU/SJ
Sample : PB115316BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc