

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM017995.D
 Acq On : 07 Dec 2018 10:50
 Operator : JU/SJ
 Sample : J6170-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9J06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	4	6	8	rVB3	5410	4157	0.13%	0.015%
2	3.122	20	23	25	rBV3	3678	4025	0.13%	0.014%
3	3.163	28	30	33	rVB3	8535	9117	0.29%	0.032%
4	3.681	115	118	119	rBV2	3299	3179	0.10%	0.011%
5	3.757	126	131	138	rBV	12717	26188	0.83%	0.092%
6	3.857	144	148	150	rBV3	3773	5023	0.16%	0.018%
7	3.952	162	164	170	rVV3	12193	19482	0.62%	0.069%
8	4.751	291	300	306	rBV2	39437	67975	2.15%	0.239%
9	5.551	433	436	440	rBV3	3410	4773	0.15%	0.017%
10	5.987	503	510	515	rBV2	10660	16694	0.53%	0.059%
11	6.751	633	640	656	rVB2	92315	232193	7.34%	0.818%
12	6.910	661	667	681	rBV	435414	698399	22.09%	2.460%
13	7.098	692	699	710	rBV	470381	836375	26.45%	2.947%
14	7.557	769	777	787	rBV	505650	852732	26.97%	3.004%
15	7.634	787	790	794	rVB3	4370	6307	0.20%	0.022%
16	8.269	892	898	911	rBV	284223	530685	16.78%	1.870%
17	8.639	955	961	962	rVB3	2353	3209	0.10%	0.011%
18	8.710	967	973	985	rBV	506017	882430	27.91%	3.109%
19	9.098	1035	1039	1044	rVB2	9060	11796	0.37%	0.042%
20	9.422	1087	1094	1106	rBV	406030	743474	23.52%	2.619%
21	9.963	1179	1186	1209	rBV	341544	988580	31.27%	3.483%
22	10.322	1240	1247	1259	rBV	657327	1110772	35.13%	3.913%
23	11.969	1521	1527	1534	rBV3	5484	11380	0.36%	0.040%
24	12.075	1540	1545	1546	rBV3	2762	4558	0.14%	0.016%
25	13.627	1802	1809	1829	rBV	986564	1543336	48.81%	5.437%
26	13.892	1848	1854	1869	rBV	1218161	1890925	59.81%	6.662%
27	14.204	1901	1907	1917	rBV2	820187	1314387	41.57%	4.631%
28	14.516	1955	1960	1961	rBV3	8116	10221	0.32%	0.036%
29	15.063	2050	2053	2055	rVB2	3124	3226	0.10%	0.011%
30	15.210	2071	2078	2091	rBV	1468199	2303753	72.86%	8.116%
31	15.351	2096	2102	2115	rVV	336373	623457	19.72%	2.196%
32	15.451	2115	2119	2126	rVV4	22057	42841	1.36%	0.151%
33	15.504	2126	2128	2132	rVV3	4694	4640	0.15%	0.016%
34	15.568	2137	2139	2143	rBV4	2496	3241	0.10%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM017995.D
Acq On : 07 Dec 2018 10:50
Operator : JU/SJ
Sample : J6170-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9J06

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Title : SVOA CALIBRATION

35	16.751	2335	2340	2344	rBV4	5247	7676	0.24%	0.027%
36	16.962	2369	2376	2386	rBV	994677	1451534	45.91%	5.114%
37	17.062	2387	2393	2412	rVB	1535936	2386118	75.47%	8.406%
38	17.209	2417	2418	2422	rVV2	3653	4167	0.13%	0.015%
39	17.874	2527	2531	2541	rBV5	24038	51625	1.63%	0.182%
40	18.580	2648	2651	2656	rBV6	2539	4302	0.14%	0.015%
41	18.809	2688	2690	2695	rBV4	2343	3487	0.11%	0.012%
42	18.927	2708	2710	2715	rVB4	2558	3505	0.11%	0.012%
43	19.003	2719	2723	2728	rBV2	13586	25093	0.79%	0.088%
44	19.104	2738	2740	2742	rBV2	4199	3246	0.10%	0.011%
45	19.133	2742	2745	2747	rBV3	3624	4789	0.15%	0.017%
46	19.168	2747	2751	2756	rBV7	16493	23981	0.76%	0.084%
47	19.256	2763	2766	2769	rBV2	10613	13773	0.44%	0.049%
48	19.368	2779	2785	2801	rBV	1976875	2767383	87.53%	9.750%
49	19.656	2832	2834	2836	rBV2	4678	3335	0.11%	0.012%
50	19.680	2836	2838	2842	rVB3	4606	5656	0.18%	0.020%
51	20.898	3042	3045	3051	rBV6	32237	50076	1.58%	0.176%
52	21.174	3087	3092	3106	rBV	1215433	1810391	57.26%	6.378%
53	23.209	3431	3438	3448	rBV	1665951	3161674	100.00%	11.139%
54	23.344	3455	3461	3471	rVB2	904040	1789420	56.60%	6.304%


Sum of corrected areas: 28384761

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM017995.D
Acq On : 07 Dec 2018 10:50
Operator : JU/SJ
Sample : J6170-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9J06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

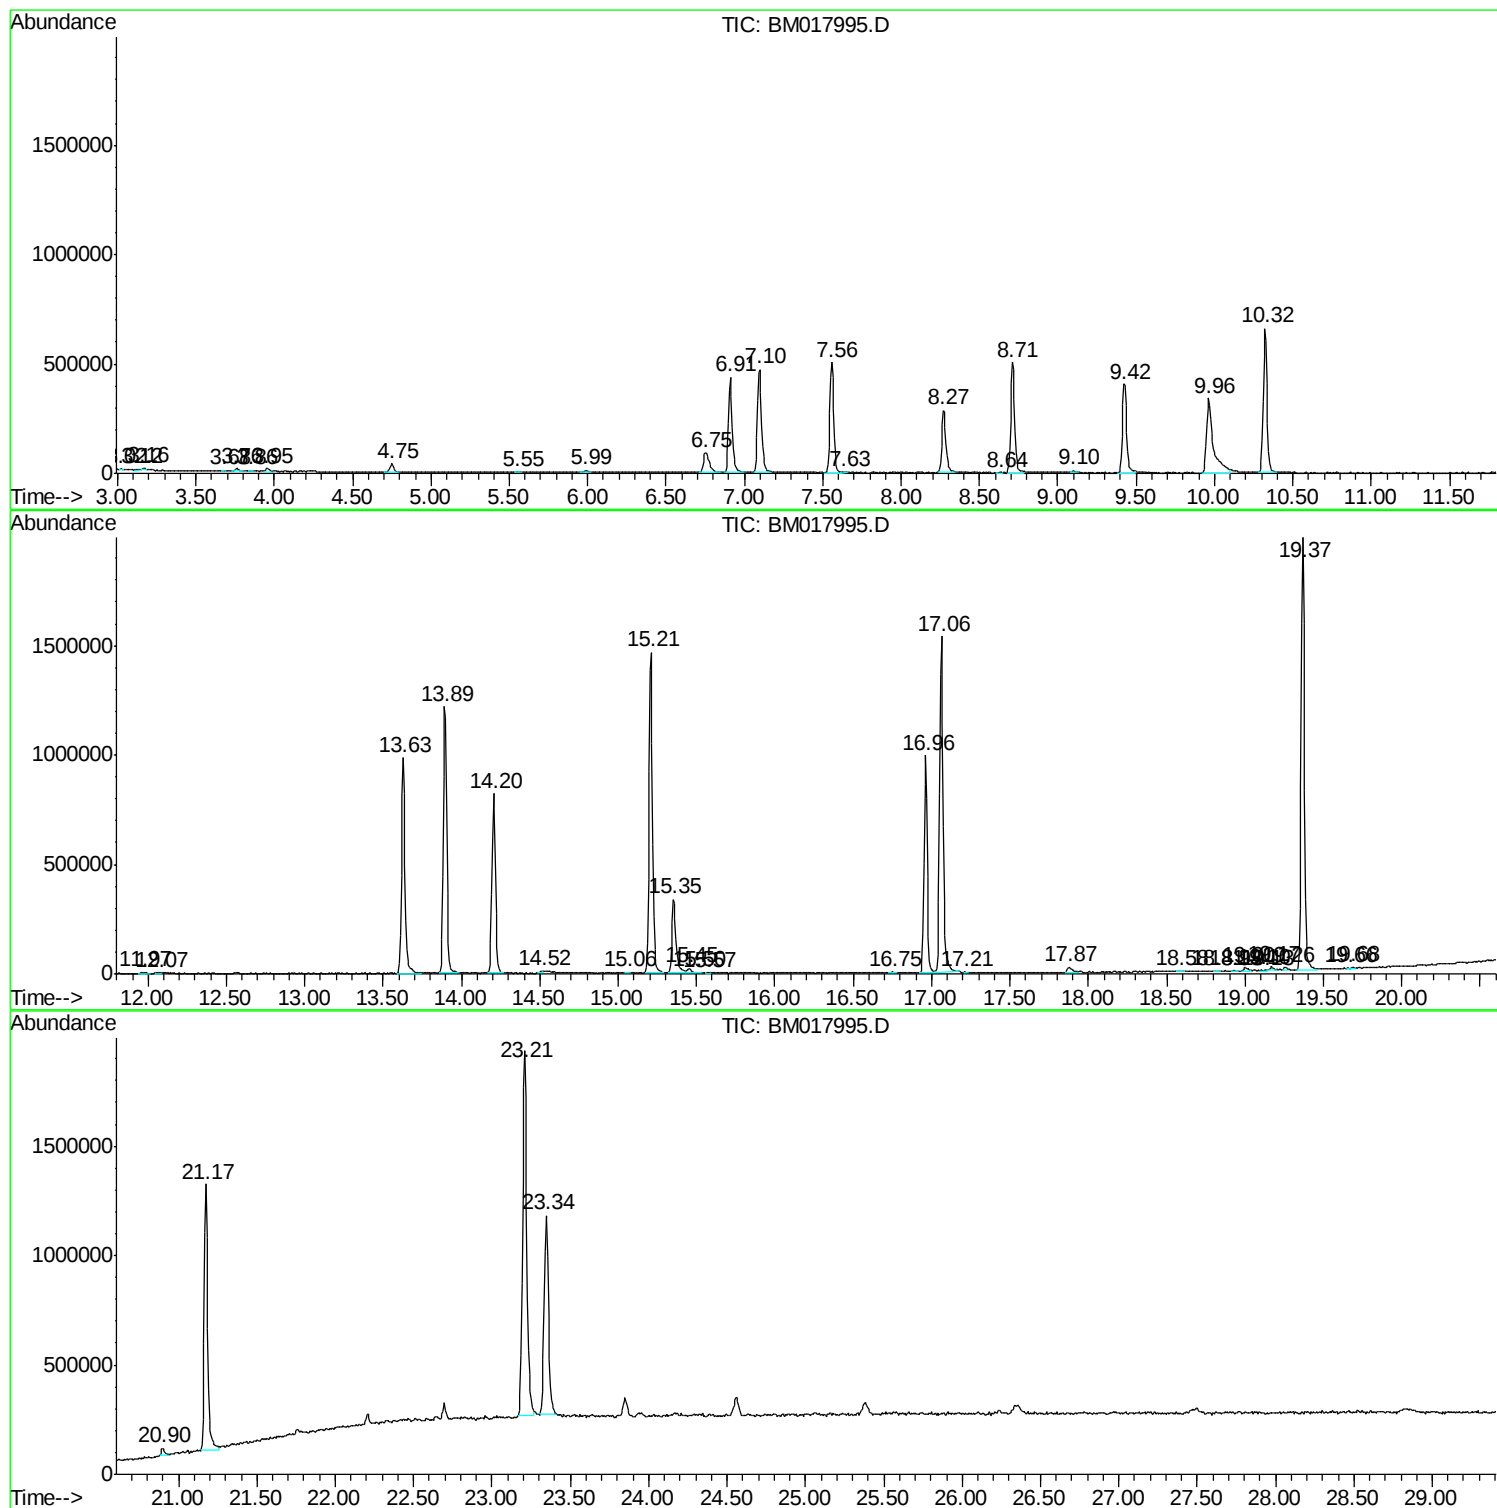

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM017995.D
Acq On : 07 Dec 2018 10:50
Operator : JU/SJ
Sample : J6170-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9J06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM017995.D
Acq On : 07 Dec 2018 10:50
Operator : JU/SJ
Sample : J6170-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9J06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc