

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM018009.D
 Acq On : 07 Dec 2018 20:49
 Operator : JU/SJ
 Sample : PB115265BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	6	9	12	rBV3	3114	3604	0.16%	0.016%
2	3.163	26	30	37	rVB	24568	36134	1.65%	0.158%
3	3.257	44	46	47	rBV2	2284	2218	0.10%	0.010%
4	3.381	65	67	70	rBV2	2774	3084	0.14%	0.013%
5	3.410	70	72	75	rVB3	2520	2437	0.11%	0.011%
6	3.599	103	104	107	rVB2	2942	2225	0.10%	0.010%
7	3.663	112	115	116	rVB3	4149	2975	0.14%	0.013%
8	3.704	119	122	125	rBV5	2366	3360	0.15%	0.015%
9	3.910	155	157	162	rBV2	1929	3080	0.14%	0.013%
10	4.104	189	190	192	rBV2	3018	2307	0.11%	0.010%
11	4.469	248	252	255	rVB3	2431	3618	0.16%	0.016%
12	5.316	394	396	401	rVB4	3540	3610	0.16%	0.016%
13	5.404	408	411	412	rBV	2453	2430	0.11%	0.011%
14	5.598	441	444	448	rBV3	2528	3285	0.15%	0.014%
15	5.787	473	476	478	rVV3	2428	2379	0.11%	0.010%
16	6.192	542	545	548	rBV5	2001	2298	0.10%	0.010%
17	6.310	560	565	566	rBV4	1910	2778	0.13%	0.012%
18	6.398	579	580	582	rBV	3591	2613	0.12%	0.011%
19	6.745	633	639	654	rBV	304101	589270	26.86%	2.571%
20	6.910	660	667	680	rBV	284158	473109	21.57%	2.065%
21	7.092	691	698	711	rBV	403014	705263	32.15%	3.078%
22	7.198	715	716	720	rVB3	2505	2385	0.11%	0.010%
23	7.445	756	758	761	rVB2	2129	2276	0.10%	0.010%
24	7.557	770	777	785	rBV	446764	751722	34.27%	3.280%
25	7.710	801	803	807	rVB3	2162	2443	0.11%	0.011%
26	7.816	818	821	823	rVB2	2569	2239	0.10%	0.010%
27	8.116	870	872	878	rBV3	1878	3406	0.16%	0.015%
28	8.269	891	898	912	rBV	389939	735465	33.53%	3.209%
29	8.363	912	914	917	rVV4	4938	5375	0.25%	0.023%
30	8.386	917	918	925	rVV5	3251	4286	0.20%	0.019%
31	8.710	966	973	991	rBV	329587	592921	27.03%	2.587%
32	9.045	1025	1030	1033	rVV4	2160	2948	0.13%	0.013%
33	9.086	1033	1037	1040	rVB3	2121	2731	0.12%	0.012%
34	9.316	1073	1076	1079	rVV2	1844	3180	0.14%	0.014%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
 Data File : BM018009.D
 Acq On : 07 Dec 2018 20:49
 Operator : JU/SJ
 Sample : PB115265BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Title : SVOA CALIBRATION

35	9.422	1088	1094	1109	rVV	267828	493458	22.49%	2.153%
36	9.522	1109	1111	1118	rVB3	2656	5149	0.23%	0.022%
37	9.869	1167	1170	1172	rVB2	2207	2444	0.11%	0.011%
38	9.963	1179	1186	1196	rBV	320490	647359	29.51%	2.825%
39	10.322	1240	1247	1256	rBV	594164	988417	45.06%	4.313%
40	10.480	1267	1274	1297	rBV	244859	706181	32.19%	3.082%
41	11.339	1414	1420	1422	rVV2	1546	2783	0.13%	0.012%
42	11.969	1525	1527	1531	rVB3	3352	4344	0.20%	0.019%
43	12.027	1534	1537	1540	rVB	1687	2268	0.10%	0.010%
44	12.186	1561	1564	1567	rVB3	2143	2415	0.11%	0.011%
45	12.474	1610	1613	1616	rBV2	2112	2436	0.11%	0.011%
46	13.627	1802	1809	1823	rBV	650753	1057738	48.22%	4.616%
47	13.892	1847	1854	1867	rBV	831113	1282182	58.45%	5.595%
48	14.204	1901	1907	1919	rVV2	761889	1187614	54.14%	5.183%
49	14.310	1923	1925	1929	rVV2	2568	2538	0.12%	0.011%
50	14.474	1946	1953	1962	rBV2	63082	202027	9.21%	0.882%
51	14.698	1990	1991	1995	rVB3	3115	2411	0.11%	0.011%
52	14.845	2013	2016	2018	rVB2	2243	2464	0.11%	0.011%
53	14.945	2030	2033	2037	rVB4	2957	4103	0.19%	0.018%
54	14.974	2037	2038	2042	rBV	2999	2845	0.13%	0.012%
55	15.062	2050	2053	2057	rBV4	1782	2381	0.11%	0.010%
56	15.210	2071	2078	2092	rBV	978646	1625575	74.10%	7.094%
57	15.351	2096	2102	2115	rVV	191280	348448	15.88%	1.521%
58	15.451	2115	2119	2126	rVB4	14358	22102	1.01%	0.096%
59	15.727	2161	2166	2168	rBV2	2109	3474	0.16%	0.015%
60	16.315	2262	2266	2269	rBV3	2299	2951	0.13%	0.013%
61	16.668	2323	2326	2329	rBV3	2306	3243	0.15%	0.014%
62	16.751	2335	2340	2345	rBV4	3638	4827	0.22%	0.021%
63	16.962	2369	2376	2387	rBV	902065	1299536	59.24%	5.671%
64	17.062	2387	2393	2413	rVB	1059561	1697570	77.38%	7.408%
65	17.239	2421	2423	2427	rBV4	1831	2592	0.12%	0.011%
66	17.956	2541	2545	2547	rBV2	1984	2235	0.10%	0.010%
67	18.015	2549	2555	2556	rBV4	3042	4680	0.21%	0.020%
68	18.039	2556	2559	2562	rBV4	2141	2846	0.13%	0.012%
69	18.321	2605	2607	2610	rBV4	2409	2772	0.13%	0.012%
70	18.950	2712	2714	2717	rBV4	2754	2609	0.12%	0.011%
71	19.003	2720	2723	2728	rVV2	6861	10818	0.49%	0.047%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM018009.D
Acq On : 07 Dec 2018 20:49
Operator : JU/SJ
Sample : PB115265BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Title : SVOA CALIBRATION

72	19.256	2762	2766	2770	rBV2	8669	10523	0.48%	0.046%
73	19.368	2779	2785	2802	rBV2	1182709	1963680	89.51%	8.569%
74	19.697	2839	2841	2843	rBV3	3667	3217	0.15%	0.014%
75	19.803	2857	2859	2861	rBV3	4603	4163	0.19%	0.018%
76	19.933	2879	2881	2883	rBV3	5165	5113	0.23%	0.022%
77	21.174	3087	3092	3106	rBV	951034	1564932	71.34%	6.829%
78	23.209	3432	3438	3450	rBV	1081986	2193765	100.00%	9.573%
79	23.350	3456	3462	3475	rVB2	811861	1566949	71.43%	6.838%


Sum of corrected areas: 22915631

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM120718\
Data File : BM018009.D
Acq On : 07 Dec 2018 20:49
Operator : JU/SJ
Sample : PB115265BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleID :
SBLK65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

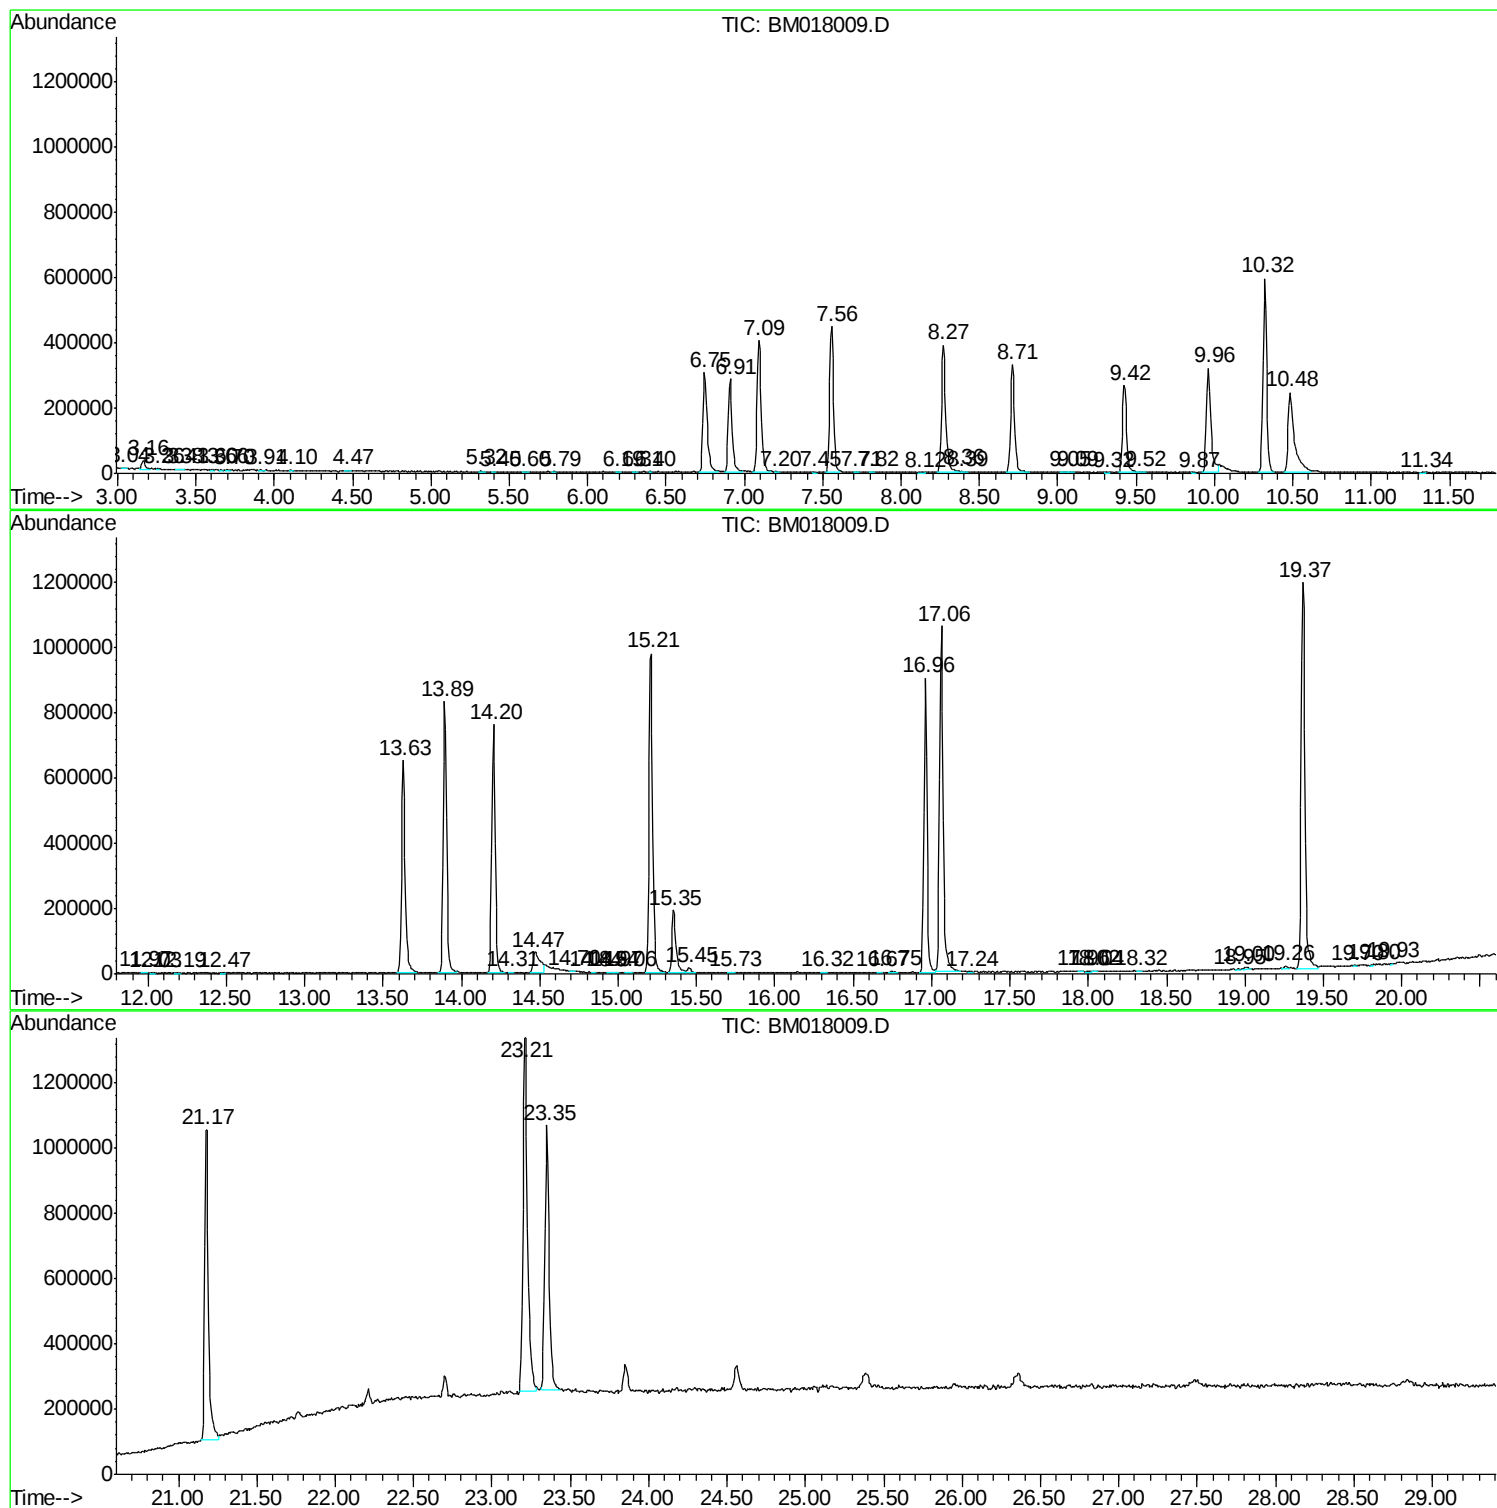

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM018009.D
Acq On : 07 Dec 2018 20:49
Operator : JU/SJ
Sample : PB115265BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM120718\
Data File : BM018009.D
Acq On : 07 Dec 2018 20:49
Operator : JU/SJ
Sample : PB115265BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK65

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc