

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120721\
Data File : BM033334.D
Acq On : 07 Dec 2021 22:03
Operator : CG/JU
Sample : PB141212BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141212BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120721.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.496	360	367	377	rBV	1647747	2436402	76.16%	13.167%
2	7.090	631	638	649	rBV	1593490	2540753	79.42%	13.731%
3	7.913	769	778	790	rVB	286899	455419	14.24%	2.461%
4	9.078	966	976	992	rBV	1002401	1680682	52.54%	9.083%
5	10.707	1246	1253	1267	rBV	321090	589240	18.42%	3.184%
6	13.160	1662	1670	1687	rBV	2121003	3199035	100.00%	17.289%
7	14.536	1898	1904	1915	rBV	435876	688533	21.52%	3.721%
8	16.024	2150	2157	2171	rBV	1367198	1940899	60.67%	10.489%
9	17.277	2364	2370	2381	rBV	453069	683090	21.35%	3.692%
10	19.889	2808	2814	2822	rBV	2554934	3148532	98.42%	17.016%
11	21.442	3073	3078	3083	rBV	405108	564836	17.66%	3.053%
12	23.765	3467	3473	3483	rVB2	289768	576296	18.01%	3.114%




Sum of corrected areas: 18503717

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120721\
Data File : BM033334.D
Acq On : 07 Dec 2021 22:03
Operator : CG/JU
Sample : PB141212BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141212BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

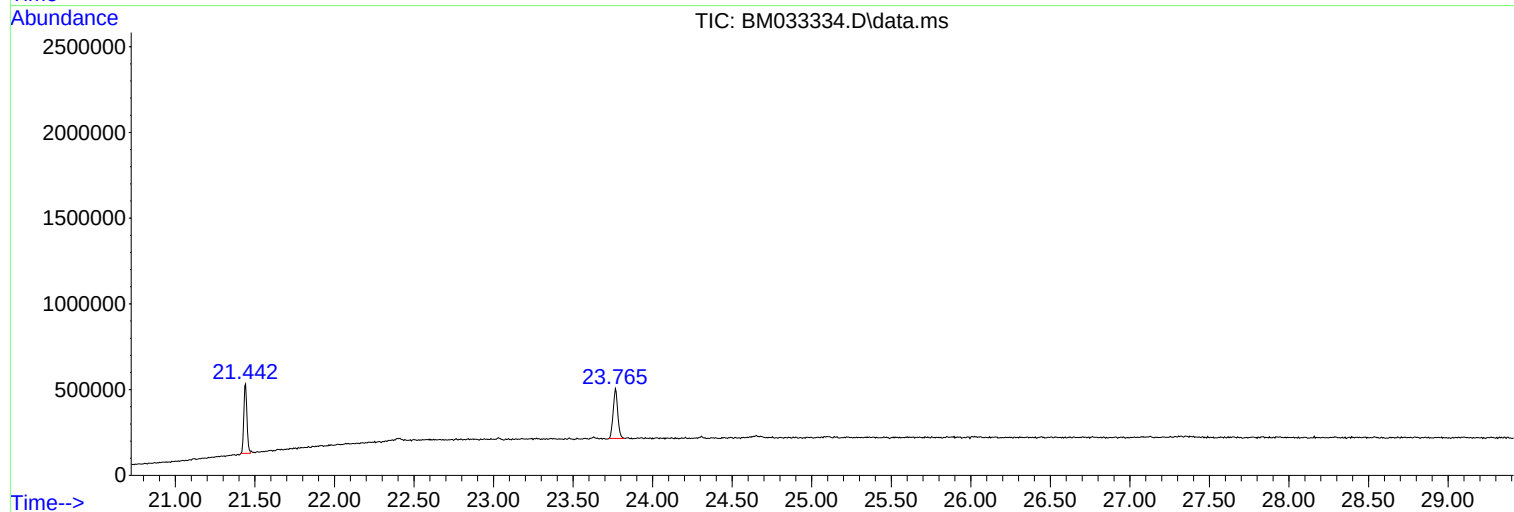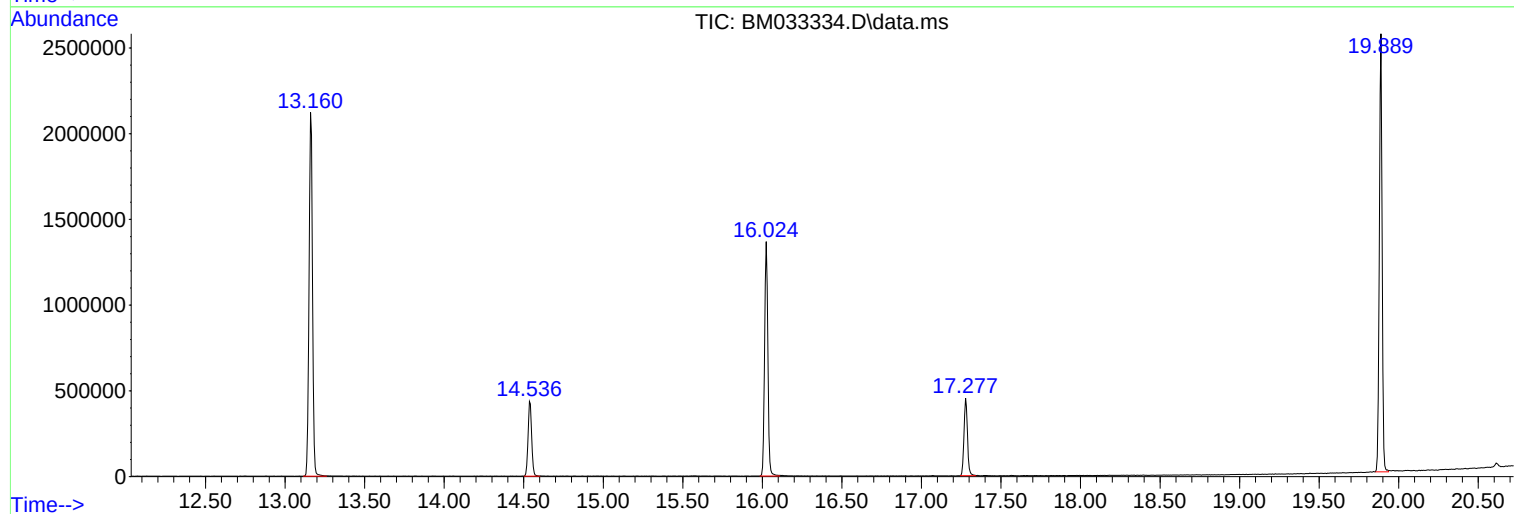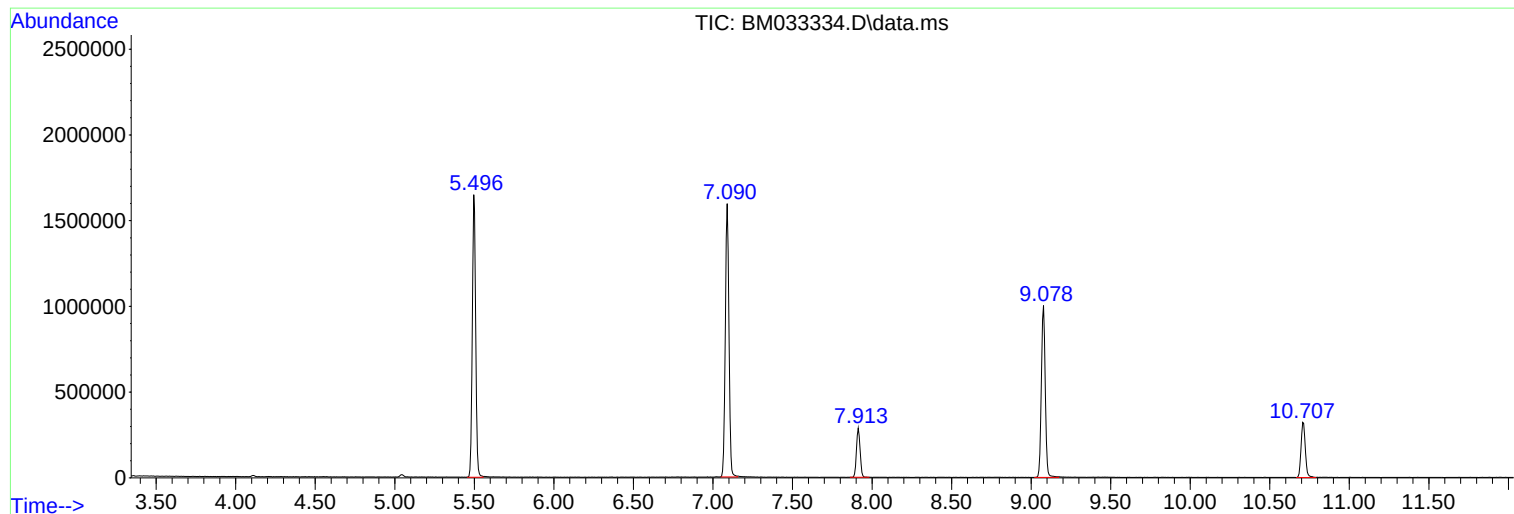

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120721\
Data File : BM033334.D
Acq On : 07 Dec 2021 22:03
Operator : CG/JU
Sample : PB141212BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141212BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120721\
Data File : BM033334.D
Acq On : 07 Dec 2021 22:03
Operator : CG/JU
Sample : PB141212BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141212BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------