


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120721\
 Data File : BM033324.D
 Acq On : 07 Dec 2021 15:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 08 02:33:11 2021

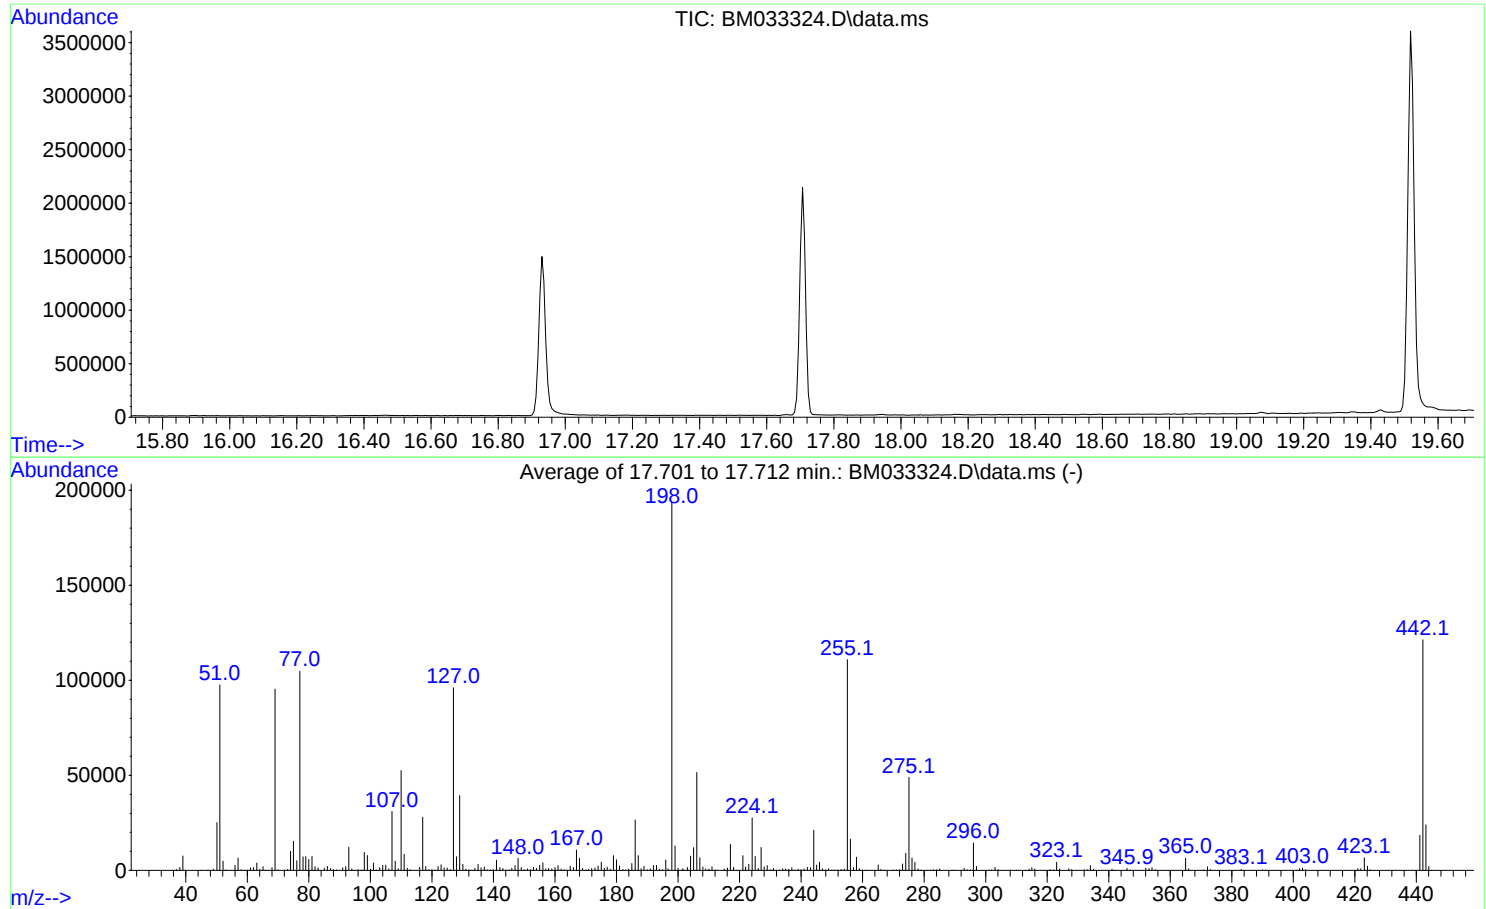

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.4	97598	PASS
68	69	0.00	2	1.5	1430	PASS
69	198	0.00	100	49.3	95356	PASS
70	69	0.00	2	0.2	236	PASS
127	198	10	80	49.7	96083	PASS
197	198	0.00	2	0.4	829	PASS
198	198	100	100	100.0	193515	PASS
199	198	5	9	6.6	12849	PASS
275	198	10	60	25.3	48867	PASS
365	198	1	100	3.3	6374	PASS
441	198	0.01	100	9.5	18401	PASS
442	442	50	100	100.0	121309	PASS
443	442	15	24	19.7	23926	PASS