

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120723\
 Data File : BM043184.D
 Acq On : 07 Dec 2023 16:53
 Operator : MA/JU
 Sample : SST02071
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SST020036

Quant Time: Dec 08 00:03:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 08 00:03:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	460759	20.000	ng/u1	0.00
20) Naphthalene-d8	10.816	136	2053038	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.633	164	1393405	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.374	188	3043198	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	2890826	20.000	ng/u1	0.00
88) Perylene-d12	23.938	264	2924631	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.404	96	84924	7.234	ng/uL	0.00
4) Pyridine-d5	3.816	84	639115	18.657	ng/u1	0.00
7) Phenol-d5	7.169	99	827560	18.574	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.351	67	534768	19.010	ng/u1	0.00
11) 2-Chlorophenol-d4	7.539	132	632205	18.129	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	665907	18.737	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	330885	18.909	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	314973	18.666	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.433	165	706654	18.789	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	1054576	19.468	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	2308382	18.899	ng/u1	0.00
49) Acenaphthylene-d8	14.333	160	2699697	19.104	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	407138	19.073	ng/u1	0.00
60) Fluorene-d10	15.621	176	2022892	18.999	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	260783	17.318	ng/u1	0.00
73) Anthracene-d10	17.474	188	3132779	19.028	ng/u1	0.00
81) Pyrene-d10	19.750	212	3536199	19.118	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.785	264	3206986	18.792	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.440	88	94938	7.362	ng/uL	100
5) Pyridine	3.840	79	666584	18.885	ng/u1	100
6) Benzaldehyde	7.157	77	526769	20.793	ng/u1	100
8) Phenol	7.192	94	821068	18.557	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.445	93	682991	18.911	ng/u1	100
12) 2-Chlorophenol	7.569	128	649210	18.351	ng/u1	100
13) 2-Methylphenol	8.451	108	634762	18.547	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.545	45	1170109	19.234	ng/u1	100
16) Acetophenone	8.845	105	1111781	19.081	ng/u1	100
17) N-Nitroso-di-n-propyla...	8.828	70	600362	18.831	ng/u1	100
18) 4-Methylphenol	8.786	108	701604	18.746	ng/u1	100
19) Hexachloroethane	9.086	117	274006	18.272	ng/u1	100
22) Nitrobenzene	9.228	77	794485	18.883	ng/u1	100
23) Isophorone	9.745	82	1724848	19.240	ng/u1	100
25) 2-Nitrophenol	9.933	139	350723	18.964	ng/u1	100
26) 2,4-Dimethylphenol	9.992	107	685372	18.902	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.239	93	994726	18.872	ng/u1	100
29) 2,4-Dichlorophenol	10.463	162	685302	18.773	ng/u1	100
30) Naphthalene	10.869	128	2354504	18.684	ng/u1	100
32) 4-Chloroaniline	10.986	127	998167	19.528	ng/u1	100
33) Hexachlorobutadiene	11.145	225	426001	18.729	ng/u1	100
34) Caprolactam	11.751	113	119078	10.843	ng/u1	100
35) 4-Chloro-3-methylphenol	12.098	107	731882	19.094	ng/u1	100
36) 2-Methylnaphthalene	12.474	142	1707717	18.836	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120723\
 Data File : BM043184.D
 Acq On : 07 Dec 2023 16:53
 Operator : MA/JU
 Sample : SST02071
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_M
 ClientSampleId :
 SST020036


Quant Time: Dec 08 00:03:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 08 00:03:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.686	142	1726257	18.759	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.833	216	877437	18.612	ng/ul	100
40) Hexachlorocyclopentadiene	12.804	237	488438	19.146	ng/ul	100
41) 2,4,6-Trichlorophenol	13.074	196	555761	18.945	ng/ul	100
42) 2,4,5-Trichlorophenol	13.139	196	613522	19.216	ng/ul	100
43) 1,1'-Biphenyl	13.480	154	2326334	18.873	ng/ul	100
44) 2-Chloronaphthalene	13.516	162	1784122	18.672	ng/ul	100
45) 2-Nitroaniline	13.727	65	484968	19.207	ng/ul	100
47) Dimethylphthalate	14.104	163	2278266	19.017	ng/ul	100
48) 2,6-Dinitrotoluene	14.221	165	424613	19.237	ng/ul	100
50) Acenaphthylene	14.363	152	3051527	19.106	ng/ul	100
51) 3-Nitroaniline	14.545	138	470801	19.373	ng/ul	100
52) Acenaphthene	14.698	153	1980729	18.801	ng/ul	100
53) 2,4-Dinitrophenol	14.751	184	147211	16.509	ng/ul	100
55) 4-Nitrophenol	14.845	109	301414	19.247	ng/ul	100
56) Dibenzofuran	15.033	168	2715686	18.871	ng/ul	100
57) 2,4-Dinitrotoluene	15.004	165	608012	19.293	ng/ul	100
58) 2,3,4,6-Tetrachlorophenol	15.251	232	507344	19.117	ng/ul	100
59) Diethylphthalate	15.463	149	2293687	19.034	ng/ul	100
61) Fluorene	15.680	166	2390978	19.194	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.680	204	1154160	18.753	ng/ul	100
63) 4-Nitroaniline	15.704	138	502962	20.282	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.757	198	299991	17.851	ng/ul	100
67) N-Nitrosodiphenylamine	15.892	169	1928168	18.894	ng/ul	100
68) 4-Bromophenyl-phenylether	16.568	248	685888	18.638	ng/ul	100
69) Hexachlorobenzene	16.668	284	814073	18.644	ng/ul	100
70) Atrazine	16.845	200	595540	19.792	ng/ul	100
71) Pentachlorophenol	17.015	266	447717	18.328	ng/ul	100
72) Phenanthrene	17.415	178	3641224	19.188	ng/ul	100
74) Anthracene	17.509	178	3698908	19.350	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.433	216	884325	18.368	ng/ul	100
76) Pentachlorobenzene	14.945	250	906775	18.533	ng/ul	100
77) Carbazole	17.780	167	3306368	19.672	ng/ul	100
78) Di-n-butylphthalate	18.351	149	4069723	19.926	ng/ul	100
80) Fluoranthene	19.421	202	4197028	19.780	ng/ul	100
82) Pyrene	19.780	202	4379632	19.843	ng/ul	100
83) Butylbenzylphthalate	20.686	149	1676244	19.092	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.456	252	1365440	19.335	ng/ul	100
85) Benzo(a)anthracene	21.521	228	4351856	19.634	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.468	149	2749784	19.841	ng/ul	100
87) Chrysene	21.574	228	3865271	19.525	ng/ul	100
89) Di-n-octyl phthalate	22.403	149	4135717	19.524	ng/ul	100
90) Benzo(b)fluoranthene	23.209	252	3914666	18.760	ng/ul	100
91) Benzo(k)fluoranthene	23.256	252	3923635	18.879	ng/ul	100
93) Benzo(a)pyrene	23.833	252	3617674	18.756	ng/ul	100
94) Indeno(1,2,3-cd)pyrene	26.438	276	4195595	19.096	ng/ul	100
95) Dibenzo(a,h)anthracene	26.468	278	3491586	19.007	ng/ul	100
96) Benzo(g,h,i)perylene	27.203	276	3159786	19.090	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Dec 08 00:03:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 08 00:03:45 2023
Response via : Initial Calibration




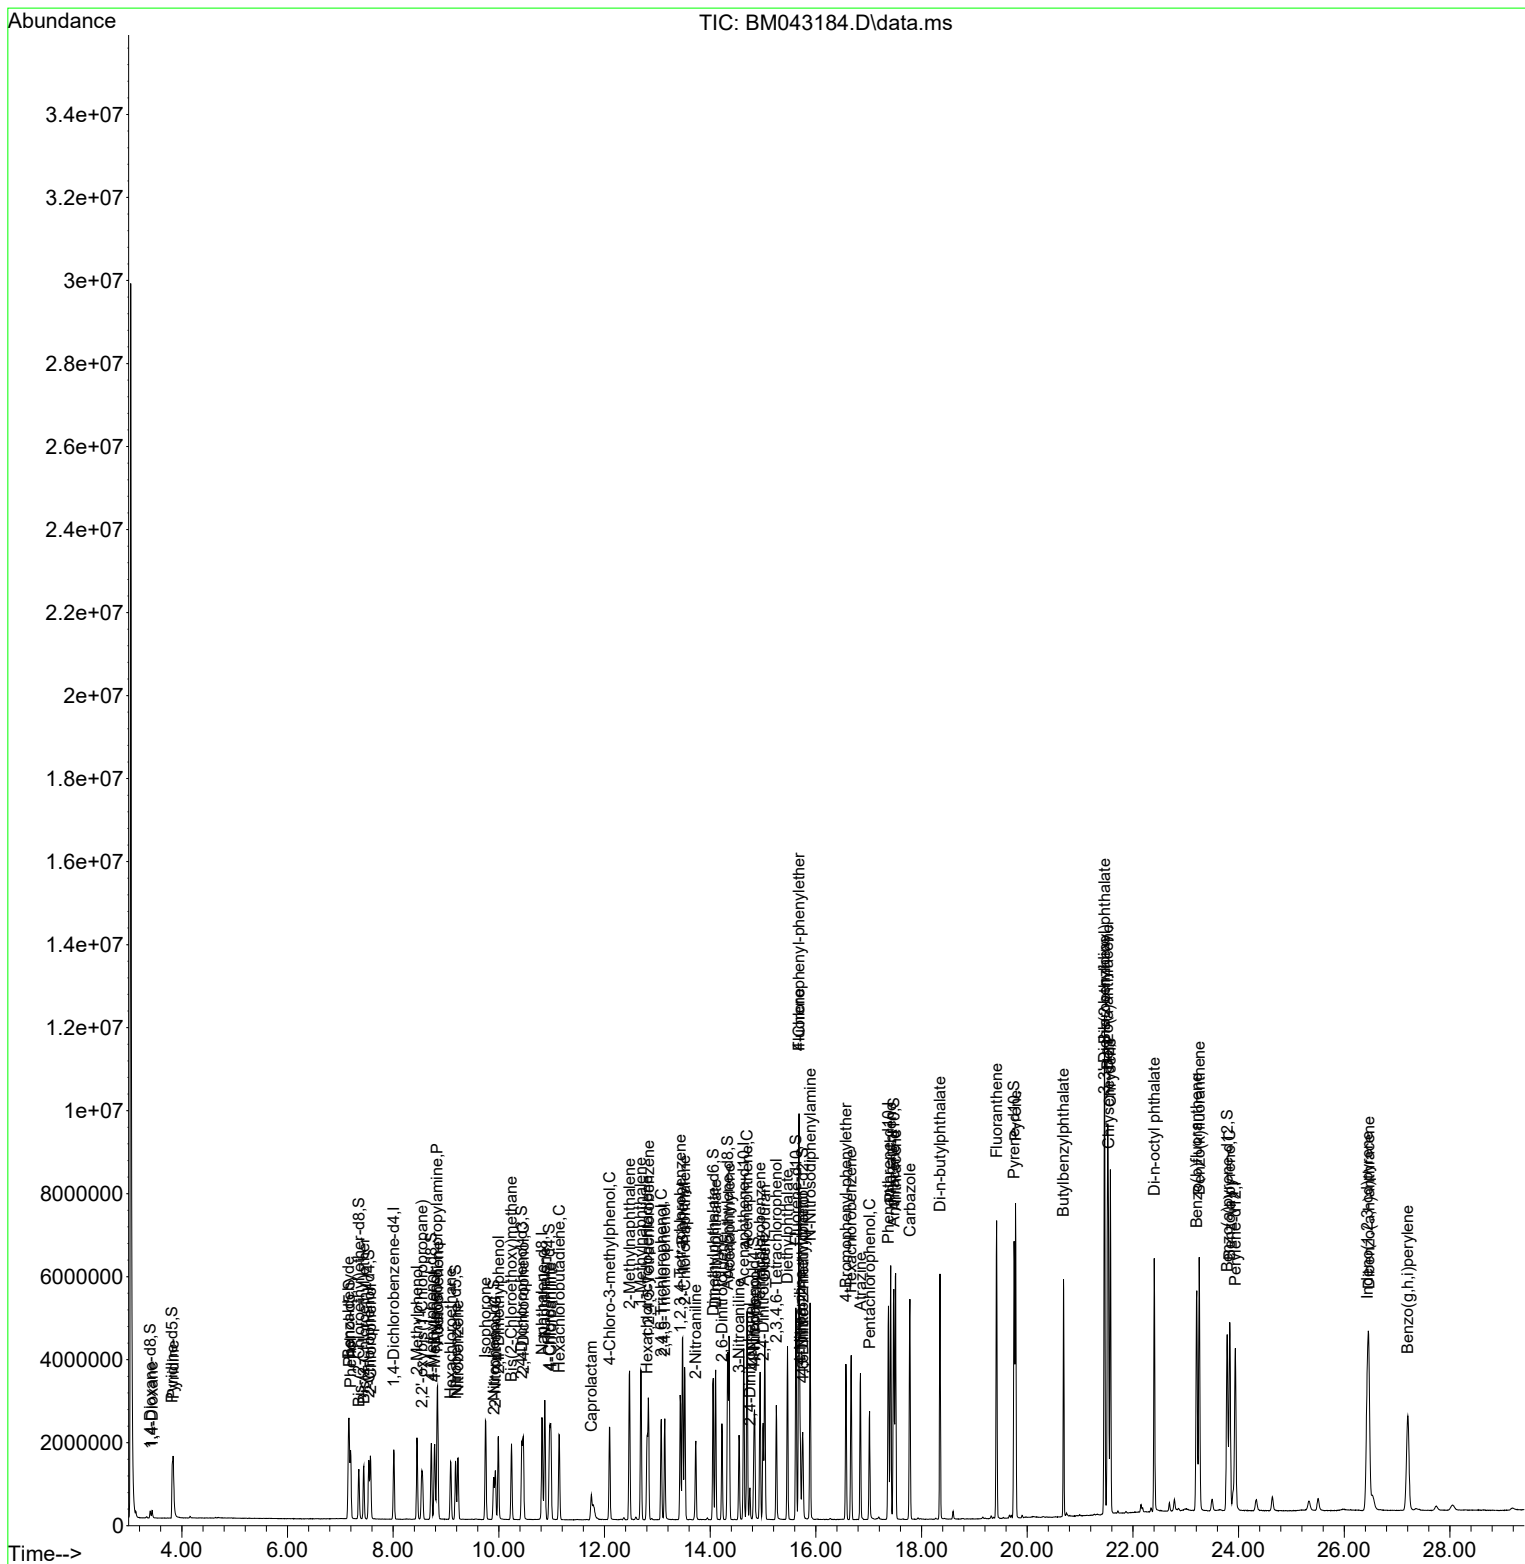




#2
1,4-Dioxane
Concen: 7.362 ng/uL
RT: 3.440 min Scan# 71
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion: 88 Resp: 94938
Ion Ratio Lower Upper
88 100
43 31.2 25.0 37.4
58 75.7 60.6 90.8



#5
Pyridine
Concen: 18.885 ng/uL
RT: 3.840 min Scan# 145
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion: 79 Resp: 666584
Ion Ratio Lower Upper
79 100
52 81.1 64.9 97.3
51 38.7 31.0 46.4









#6
Benzaldehyde
Concen: 20.793 ng/ul
RT: 7.157 min Scan# 709
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion: 77 Resp: 526769
Ion Ratio Lower Upper
77 100
105 95.4 76.3 114.5
106 93.3 74.6 112.0



#8
Phenol
Concen: 18.557 ng/ul
RT: 7.192 min Scan# 715
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion: 94 Resp: 821068
Ion Ratio Lower Upper
94 100
65 29.4 23.5 35.3
66 37.4 29.9 44.9









#10
Bis(2-Chloroethyl)ether
Concen: 18.911 ng/ul
RT: 7.445 min Scan# 758
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion: 93 Resp: 682991
Ion Ratio Lower Upper
93 100
63 78.7 63.0 94.4
95 32.5 26.0 39.0



#12
2-Chlorophenol
Concen: 18.351 ng/ul
RT: 7.569 min Scan# 779
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:128 Resp: 649210
Ion Ratio Lower Upper
128 100
64 47.9 38.3 57.5
130 33.3 26.6 40.0





#13

2-Methylphenol

Concen: 18.547 ng/ul

RT: 8.451 min Scan# 929

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Instrument :

BNA_M

ClientSampleId :





SSTD020036

Tgt Ion:108 Resp: 634762

Ion Ratio Lower Upper

108 100

107 89.7 71.8 107.6

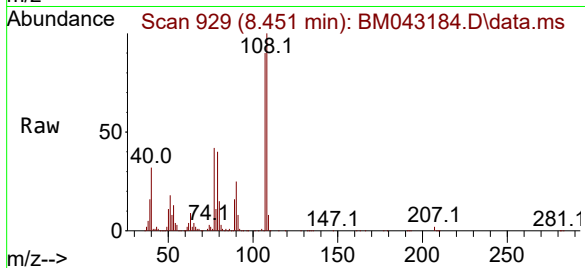

#14

2,2'-oxybis(1-Chloropropane)

Concen: 19.234 ng/ul

RT: 8.545 min Scan# 945

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53




Tgt Ion: 45 Resp: 1170109


Ion Ratio Lower Upper

45 100

77 12.7 10.2 15.2

79 9.0 7.2 10.8




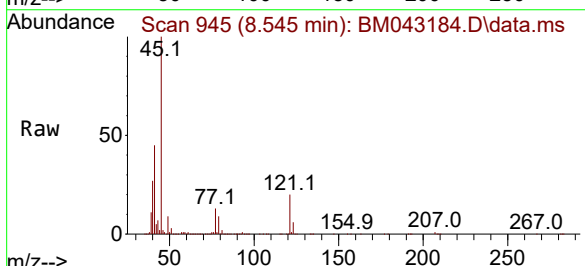




#16
Acetophenone
Concen: 19.081 ng/ul
RT: 8.845 min Scan# 996
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:105 Resp: 1111781
Ion Ratio Lower Upper
105 100
77 78.4 62.7 94.1
51 29.8 23.8 35.8

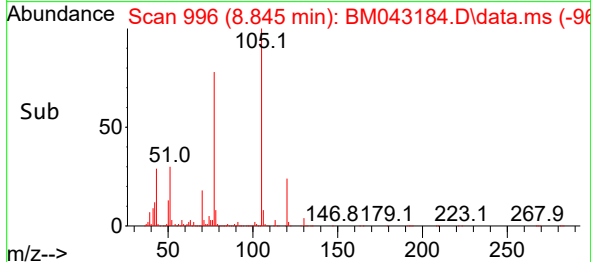

#17
N-Nitroso-di-n-propylamine
Concen: 18.831 ng/ul
RT: 8.828 min Scan# 993
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion: 70 Resp: 600362
Ion Ratio Lower Upper
70 100
42 65.4 52.3 78.5
101 8.8 7.0 10.6
130 20.2 16.2 24.2




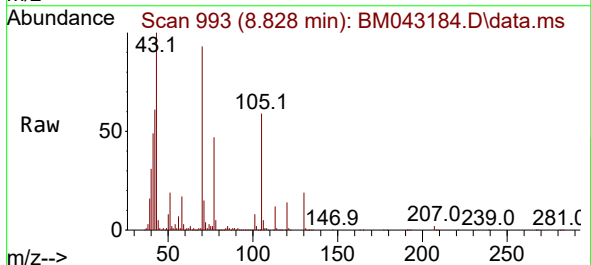




#18
4-Methylphenol
Concen: 18.746 ng/ul
RT: 8.786 min Scan# 986
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:108 Resp: 701604
Ion Ratio Lower Upper
108 100
107 108.0 86.4 129.6

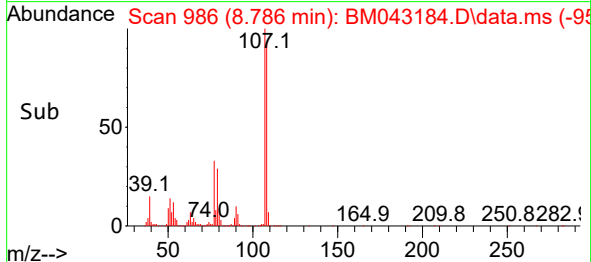

#19
Hexachloroethane
Concen: 18.272 ng/ul
RT: 9.086 min Scan# 1037
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:117 Resp: 274006
Ion Ratio Lower Upper
117 100
201 99.0 79.2 118.8
199 62.3 49.8 74.8




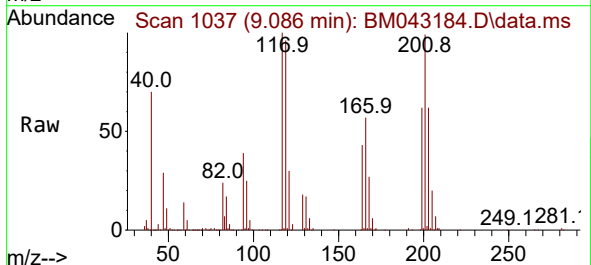


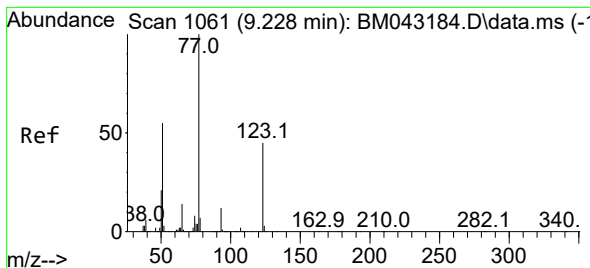

#22
Nitrobenzene
Concen: 18.883 ng/ul
RT: 9.228 min Scan# 1061
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion: 77 Resp: 794485
Ion Ratio Lower Upper
77 100
123 44.5 35.6 53.4
65 13.7 11.0 16.4

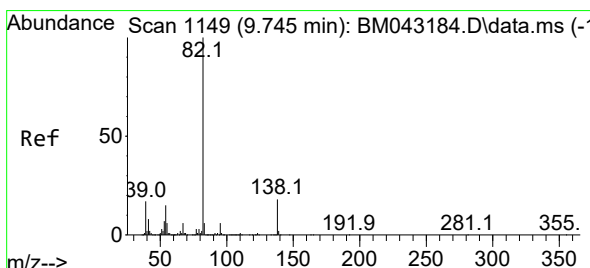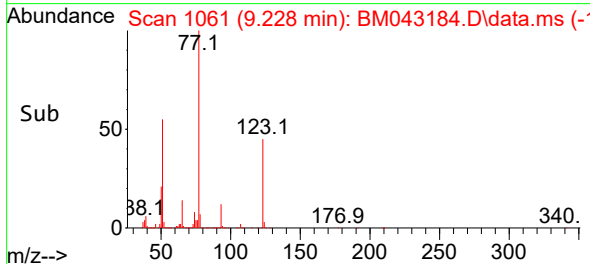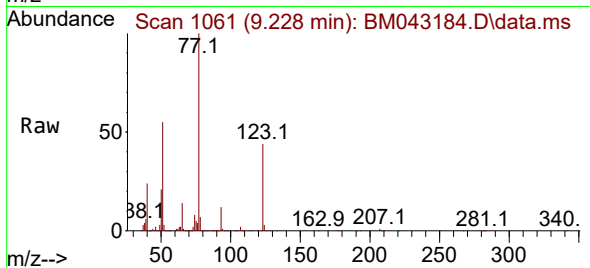

#23
Isophorone
Concen: 19.240 ng/ul
RT: 9.745 min Scan# 1149
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion: 82 Resp: 1724848
Ion Ratio Lower Upper
82 100
95 6.5 5.2 7.8
138 17.5 14.0 21.0


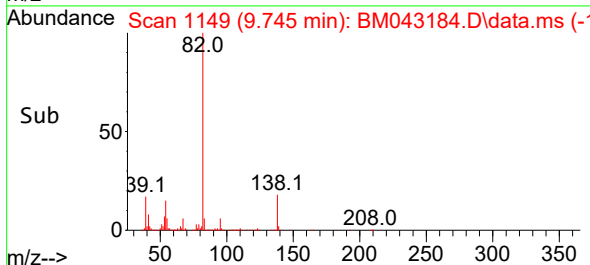

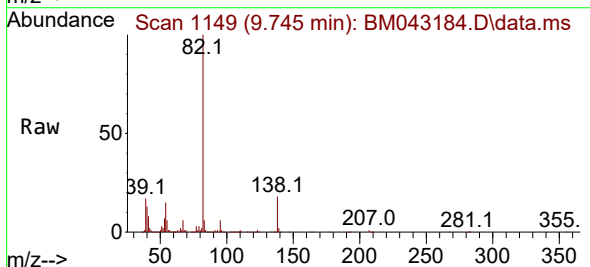


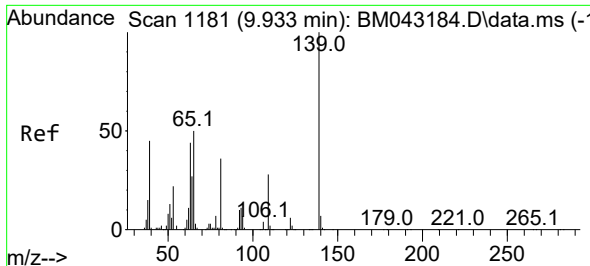

#25
2-Nitrophenol
Concen: 18.964 ng/ul
RT: 9.933 min Scan# 1181
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:139 Resp: 350723
Ion Ratio Lower Upper
139 100
65 50.7 40.6 60.8
109 28.2 22.6 33.8

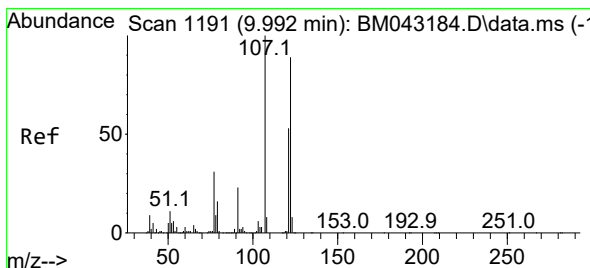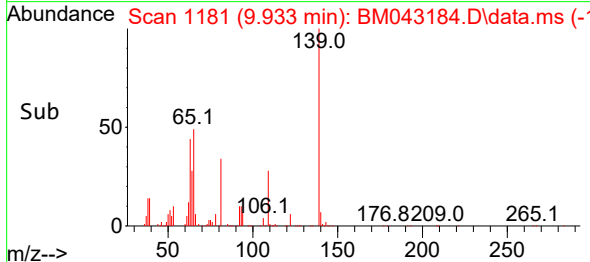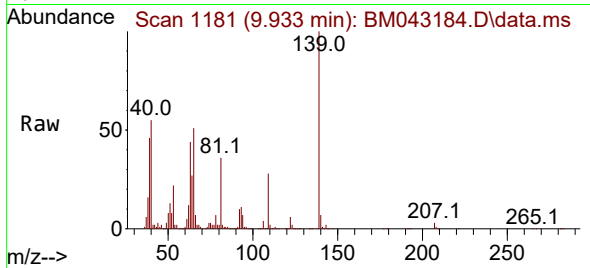

#26
2,4-Dimethylphenol
Concen: 18.902 ng/ul
RT: 9.992 min Scan# 1191
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:107 Resp: 685372
Ion Ratio Lower Upper
107 100
121 52.7 42.2 63.2
122 90.0 72.0 108.0


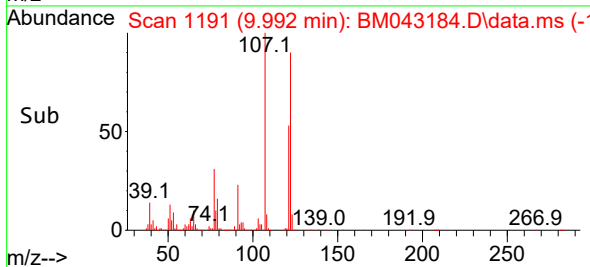

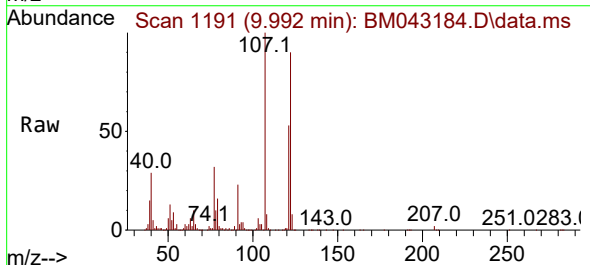




#27
 Bis(2-Chloroethoxy)methane
 Concen: 18.872 ng/ul
 RT: 10.239 min Scan# 1233
 Delta R.T. 0.000 min
 Lab File: BM043184.D
 Acq: 07 Dec 2023 16:53




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020036


Tgt Ion: 93 Resp: 994726
 Ion Ratio Lower Upper
 93 100
 95 32.7 26.2 39.2
 123 11.5 9.2 13.8

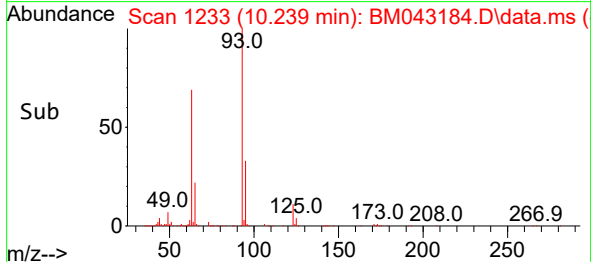

#29
 2,4-Dichlorophenol
 Concen: 18.773 ng/ul
 RT: 10.463 min Scan# 1271
 Delta R.T. 0.000 min
 Lab File: BM043184.D
 Acq: 07 Dec 2023 16:53

Tgt Ion: 162 Resp: 685302
 Ion Ratio Lower Upper
 162 100
 164 64.2 51.4 77.0
 98 33.6 26.9 40.3


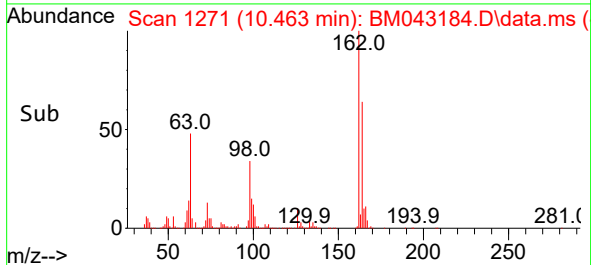






#30
Naphthalene
Concen: 18.684 ng/ul
RT: 10.869 min Scan# 1340
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:128 Resp: 2354504
Ion Ratio Lower Upper
128 100
129 11.2 9.0 13.4
127 13.0 10.4 15.6

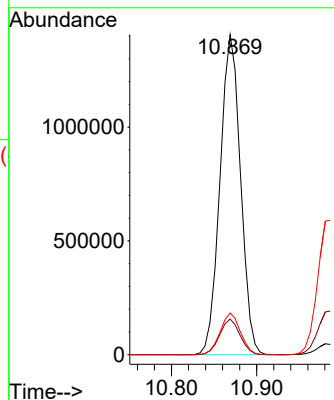

#32
4-Chloroaniline
Concen: 19.528 ng/ul
RT: 10.986 min Scan# 1360
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:127 Resp: 998167
Ion Ratio Lower Upper
127 100
129 32.5 26.0 39.0



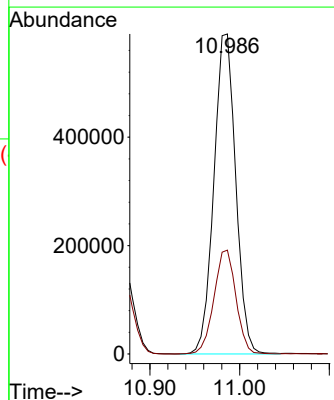





#33
Hexachlorobutadiene
Concen: 18.729 ng/ul
RT: 11.145 min Scan# 1387
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:225 Resp: 426001
Ion Ratio Lower Upper
225 100
223 62.8 50.2 75.4
227 65.0 52.0 78.0

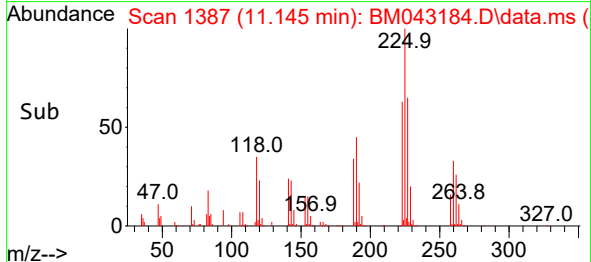

#34
Caprolactam
Concen: 10.843 ng/ul
RT: 11.751 min Scan# 1490
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:113 Resp: 119078
Ion Ratio Lower Upper
113 100
55 174.4 139.5 209.3
56 129.4 103.5 155.3




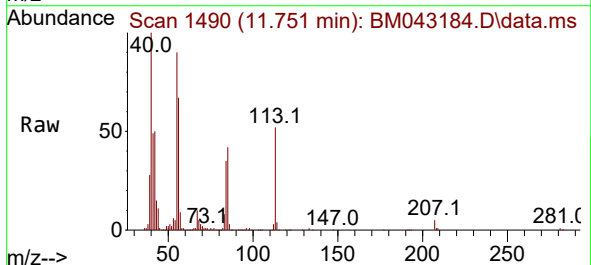




#35
4-Chloro-3-methylphenol
Concen: 19.094 ng/ul
RT: 12.098 min Scan# 1549
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:107 Resp: 731882
Ion Ratio Lower Upper
107 100
144 27.5 22.0 33.0
142 84.1 67.3 100.9

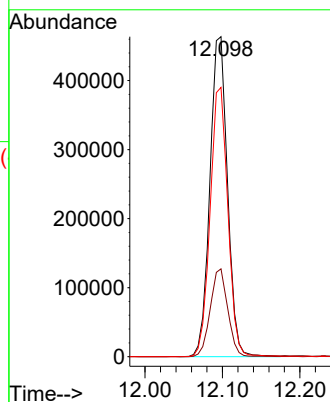

#36
2-Methylnaphthalene
Concen: 18.836 ng/ul
RT: 12.474 min Scan# 1613
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:142 Resp: 1707717
Ion Ratio Lower Upper
142 100
141 87.5 70.0 105.0

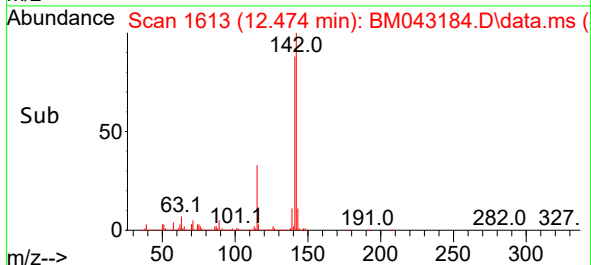



#37

1-Methylnaphthalene

Concen: 18.759 ng/ul

RT: 12.686 min Scan# 1

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Instrument :

BNA_M

ClientSampleId :

SSTD020036





Tgt Ion:142 Resp: 1726257

Ion Ratio Lower Upper

142 100

141 89.9 71.9 107.9

116 3.5 2.8 4.2



#39

1,2,4,5-Tetrachlorobenzene

Concen: 18.612 ng/ul

RT: 12.833 min Scan# 1674

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Tgt Ion:216 Resp: 877437




Ion Ratio Lower Upper


216 100

214 78.9 63.1 94.7

179 20.5 16.4 24.6

108 17.0 13.6 20.4









#40
Hexachlorocyclopentadiene
Concen: 19.146 ng/ul
RT: 12.804 min Scan# 1669
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:237 Resp: 488438
Ion Ratio Lower Upper
237 100
235 63.1 50.5 75.7
272 13.3 10.6 16.0

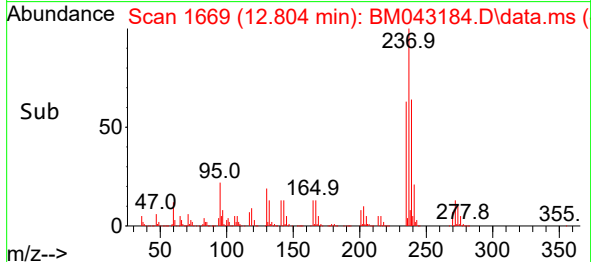

#41
2,4,6-Trichlorophenol
Concen: 18.945 ng/ul
RT: 13.074 min Scan# 1715
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:196 Resp: 555761
Ion Ratio Lower Upper
196 100
198 96.2 77.0 115.4
200 31.2 25.0 37.4




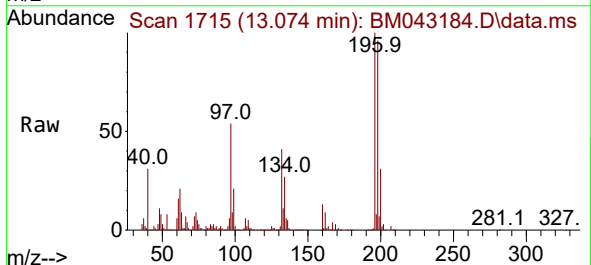




#42
2,4,5-Trichlorophenol
Concen: 19.216 ng/ul
RT: 13.139 min Scan# 1726
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:196 Resp: 613522
Ion Ratio Lower Upper
196 100
198 95.1 76.1 114.1
200 30.7 24.6 36.8



#43
1,1'-Biphenyl
Concen: 18.873 ng/ul
RT: 13.480 min Scan# 1784
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:154 Resp: 2326334
Ion Ratio Lower Upper
154 100
153 39.7 31.8 47.6
76 11.6 9.3 13.9







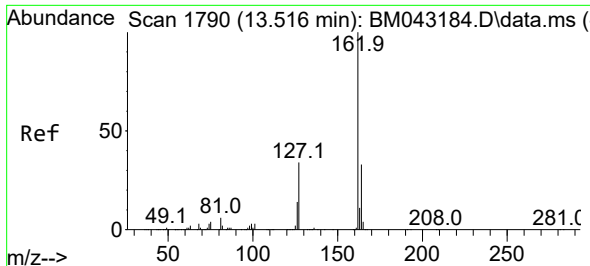

#44
2-Chloronaphthalene
Concen: 18.672 ng/ul
RT: 13.516 min Scan# 1790
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:162 Resp: 1784122
Ion Ratio Lower Upper
162 100
164 33.0 26.4 39.6
127 37.5 30.0 45.0

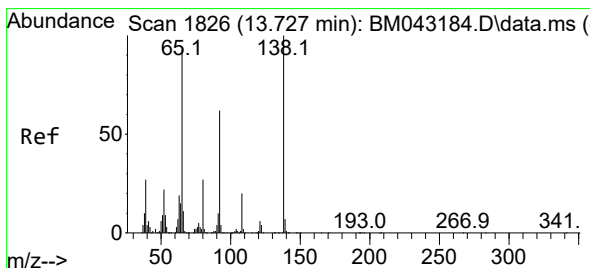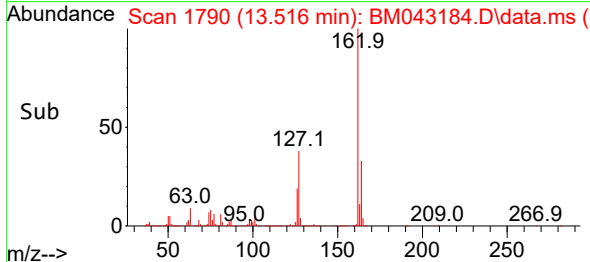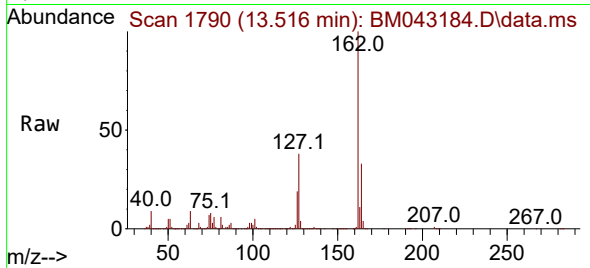

#45
2-Nitroaniline
Concen: 19.207 ng/ul
RT: 13.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion: 65 Resp: 484968
Ion Ratio Lower Upper
65 100
92 66.7 53.4 80.0
138 107.7 86.2 129.2


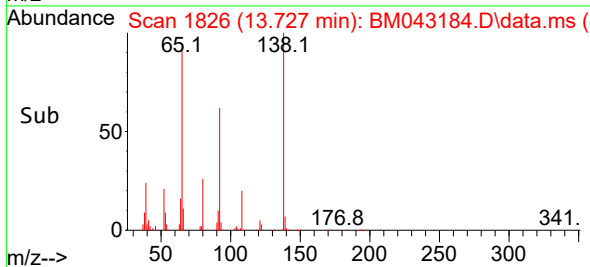

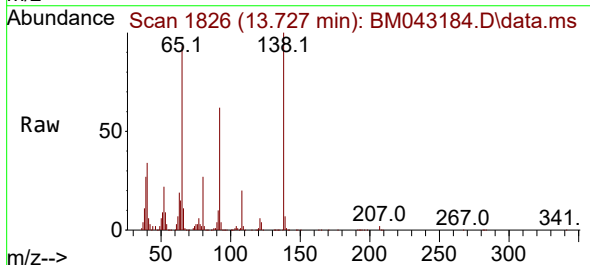




#47
Dimethylphthalate
Concen: 19.017 ng/ul
RT: 14.104 min Scan# 1890
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:163 Resp: 2278266
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 9.9 7.9 11.9

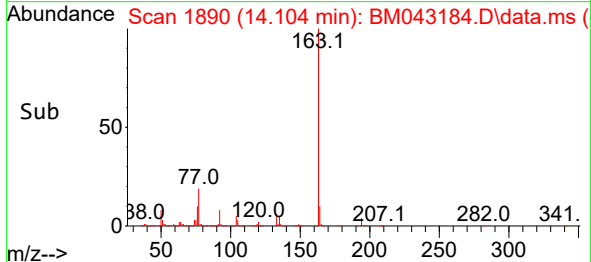

#48
2,6-Dinitrotoluene
Concen: 19.237 ng/ul
RT: 14.221 min Scan# 1910
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:165 Resp: 424613
Ion Ratio Lower Upper
165 100
89 59.4 47.5 71.3
121 21.4 17.1 25.7









#50
Acenaphthylene
Concen: 19.106 ng/ul
RT: 14.363 min Scan# 1934
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:152 Resp: 3051527
Ion Ratio Lower Upper
152 100
151 20.0 16.0 24.0
153 12.9 10.3 15.5

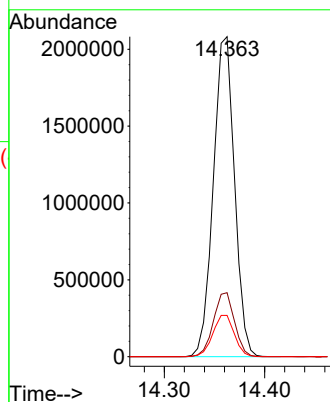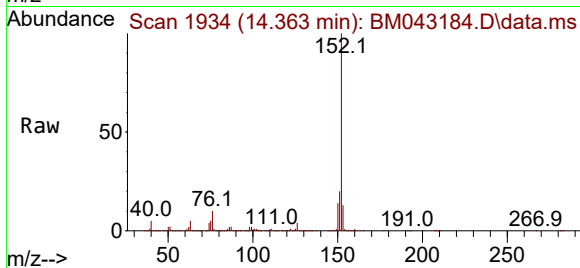

#51
3-Nitroaniline
Concen: 19.373 ng/ul
RT: 14.545 min Scan# 1965
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:138 Resp: 470801
Ion Ratio Lower Upper
138 100
108 11.7 9.4 14.0
92 109.9 87.9 131.9



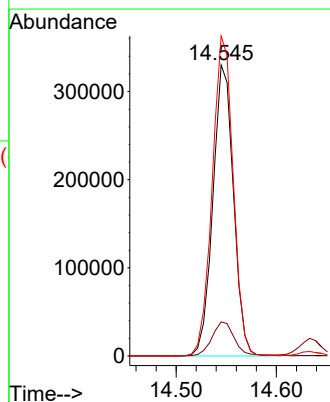





#52
Acenaphthene
Concen: 18.801 ng/ul
RT: 14.698 min Scan# 1991
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:153 Resp: 1980729
Ion Ratio Lower Upper
153 100
152 48.3 38.6 58.0
154 89.5 71.6 107.4



#53
2,4-Dinitrophenol
Concen: 16.509 ng/ul
RT: 14.751 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:184 Resp: 147211
Ion Ratio Lower Upper
184 100
63 65.3 52.2 78.4
154 59.8 47.8 71.8









#55
4-Nitrophenol
Concen: 19.247 ng/ul
RT: 14.845 min Scan# 2016
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:109 Resp: 301414
Ion Ratio Lower Upper
109 100
139 143.4 114.7 172.1
65 136.9 109.5 164.3

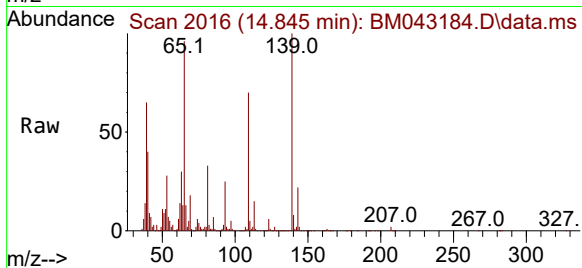

#56
Dibenzofuran
Concen: 18.871 ng/ul
RT: 15.033 min Scan# 2048
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:168 Resp: 2715686
Ion Ratio Lower Upper
168 100
139 35.8 28.6 43.0




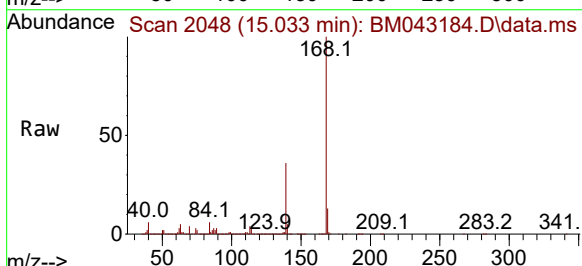




#57
2,4-Dinitrotoluene
Concen: 19.293 ng/ul
RT: 15.004 min Scan# 2043
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:165 Resp: 608012
Ion Ratio Lower Upper
165 100
63 43.3 34.6 52.0
182 2.6 2.1 3.1



#58
2,3,4,6-Tetrachlorophenol
Concen: 19.117 ng/ul
RT: 15.251 min Scan# 2085
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:232 Resp: 507344
Ion Ratio Lower Upper
232 100
131 46.2 37.0 55.4
130 2.4 1.9 2.9
166 32.6 26.1 39.1



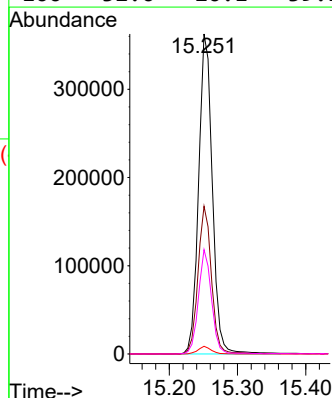





#59
Diethylphthalate
Concen: 19.034 ng/ul
RT: 15.463 min Scan# 2121
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:149 Resp: 2293687
Ion Ratio Lower Upper
149 100
177 22.7 18.2 27.2
150 12.5 10.0 15.0



#61
Fluorene
Concen: 19.194 ng/ul
RT: 15.680 min Scan# 2158
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:166 Resp: 2390978
Ion Ratio Lower Upper
166 100
165 96.9 77.5 116.3
167 13.4 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 18.753 ng/ul
RT: 15.680 min Scan# 2158
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:204 Resp: 1154160
Ion Ratio Lower Upper
204 100
206 32.7 26.2 39.2
141 55.3 44.2 66.4



#63
4-Nitroaniline
Concen: 20.282 ng/ul
RT: 15.704 min Scan# 2162
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:138 Resp: 502962
Ion Ratio Lower Upper
138 100
92 50.1 40.1 60.1
108 78.8 63.0 94.6


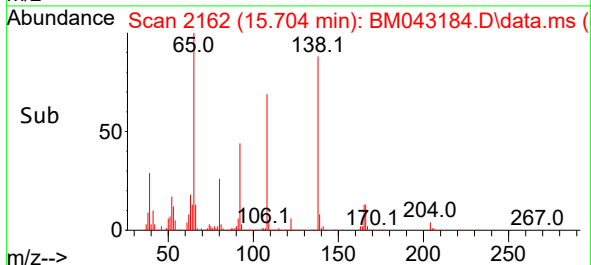






#66
4,6-Dinitro-2-methylphenol
Concen: 17.851 ng/ul
RT: 15.757 min Scan# 2171
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:198 Resp: 299991
Ion Ratio Lower Upper
198 100
182 4.0 3.2 4.8
77 25.1 20.1 30.1



#67
N-Nitrosodiphenylamine
Concen: 18.894 ng/ul
RT: 15.892 min Scan# 2194
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:169 Resp: 1928168
Ion Ratio Lower Upper
169 100
168 66.8 53.4 80.2
167 36.7 29.4 44.0









#68
4-Bromophenyl-phenylether
Concen: 18.638 ng/ul
RT: 16.568 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:248 Resp: 685888
Ion Ratio Lower Upper
248 100
250 98.6 78.9 118.3
141 75.2 60.2 90.2



#69
Hexachlorobenzene
Concen: 18.644 ng/ul
RT: 16.668 min Scan# 2326
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:284 Resp: 814073
Ion Ratio Lower Upper
284 100
142 33.4 26.7 40.1
249 30.0 24.0 36.0

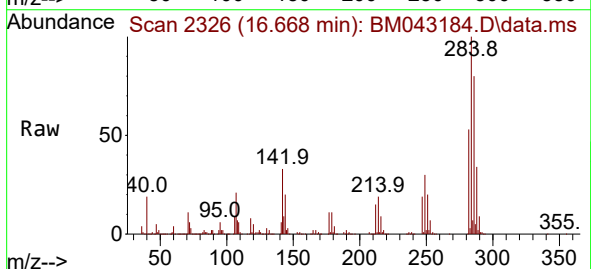



#70

Atrazine

Concen: 19.792 ng/ul

RT: 16.845 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Instrument :

BNA_M

ClientSampleId :

SSTD020036





Tgt Ion:200 Resp: 595540

Ion Ratio Lower Upper

200 100

173 25.7 20.6 30.8

215 49.3 39.4 59.2



#71

Pentachlorophenol

Concen: 18.328 ng/ul

RT: 17.015 min Scan# 2385

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53




Tgt Ion:266 Resp: 447717


Ion Ratio Lower Upper

266 100

264 63.1 50.5 75.7

268 63.0 50.4 75.6

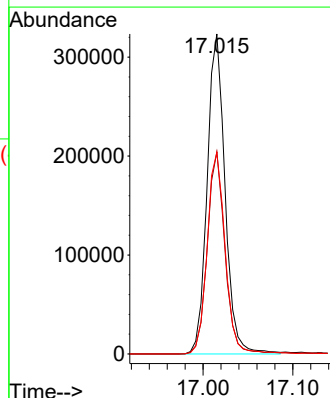



#72

Phenanthrene

Concen: 19.188 ng/ul

RT: 17.415 min Scan# 2453

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Instrument :

BNA_M

ClientSampleId :

SSTD020036





Tgt Ion:178 Resp: 3641224

Ion Ratio Lower Upper

178 100

179 15.2 12.2 18.2

176 19.6 15.7 23.5



#74

Anthracene

Concen: 19.350 ng/ul

RT: 17.509 min Scan# 2469

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53




Tgt Ion:178 Resp: 3698908


Ion Ratio Lower Upper

178 100

179 15.1 12.1 18.1

176 18.9 15.1 22.7









#75
1,2,3,4-Tetrachlorobenzene
Concen: 18.368 ng/uL
RT: 13.433 min Scan# 1776
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:216 Resp: 884325
Ion Ratio Lower Upper
216 100
214 77.7 62.2 93.2
218 47.0 37.6 56.4



#76
Pentachlorobenzene
Concen: 18.533 ng/uL
RT: 14.945 min Scan# 2033
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:250 Resp: 906775
Ion Ratio Lower Upper
250 100
248 64.8 51.8 77.8
252 64.9 51.9 77.9









#77
 Carbazole
 Concen: 19.672 ng/ul
 RT: 17.780 min Scan# 2515
 Delta R.T. 0.000 min
 Lab File: BM043184.D
 Acq: 07 Dec 2023 16:53




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020036


Tgt Ion:167 Resp: 3306368
 Ion Ratio Lower Upper
 167 100
 166 21.4 17.1 25.7
 139 12.4 9.9 14.9



#78
 Di-n-butylphthalate
 Concen: 19.926 ng/ul
 RT: 18.351 min Scan# 2612
 Delta R.T. 0.000 min
 Lab File: BM043184.D
 Acq: 07 Dec 2023 16:53

Tgt Ion:149 Resp: 4069723
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.2 10.8
 104 4.7 3.8 5.6









#80
Fluoranthene
Concen: 19.780 ng/ul
RT: 19.421 min Scan# 21
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:202 Resp: 4197028
Ion Ratio Lower Upper
202 100
101 10.2 8.2 12.2
100 7.6 6.1 9.1

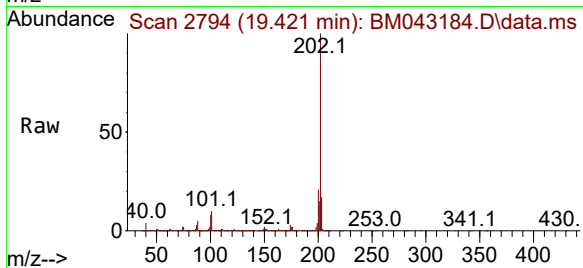

#82
Pyrene
Concen: 19.843 ng/ul
RT: 19.780 min Scan# 2855
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:202 Resp: 4379632
Ion Ratio Lower Upper
202 100
101 12.7 10.2 15.2
100 10.2 8.2 12.2

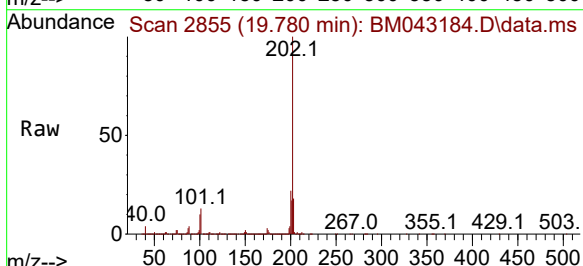



#83

Butylbenzylphthalate

Concen: 19.092 ng/ul

RT: 20.686 min Scan# 3009

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Instrument :

BNA_M

ClientSampleId :

SSTD020036





Tgt Ion:149 Resp: 1676244

Ion Ratio Lower Upper

149 100

91 71.1 56.9 85.3

206 20.1 16.1 24.1

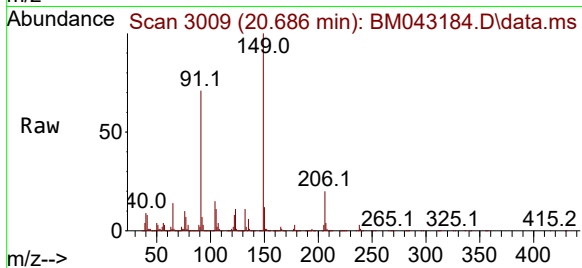

#84

3,3'-Dichlorobenzidine

Concen: 19.335 ng/ul

RT: 21.456 min Scan# 3140

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53




Tgt Ion:252 Resp: 1365440


Ion Ratio Lower Upper

252 100

254 64.1 51.3 76.9

126 11.0 8.8 13.2




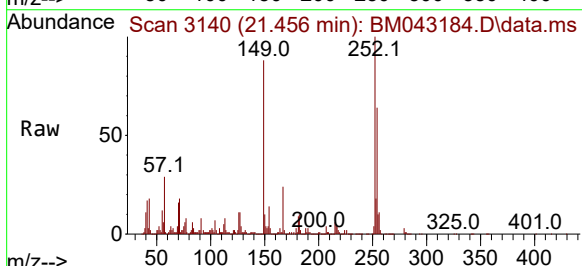




#85
Benzo(a)anthracene
Concen: 19.634 ng/ul
RT: 21.521 min Scan# 3151
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:228 Resp: 4351856
Ion Ratio Lower Upper
228 100
229 19.8 15.8 23.8
226 27.8 22.2 33.4

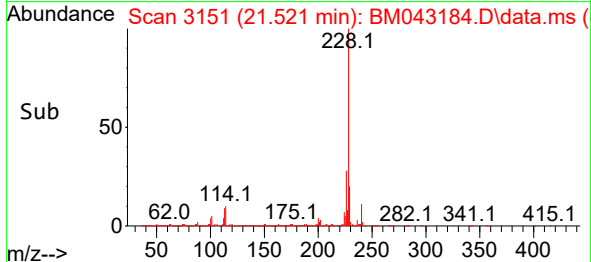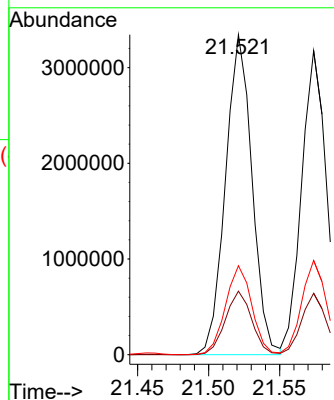

#86
Bis(2-ethylhexyl)phthalate
Concen: 19.841 ng/ul
RT: 21.468 min Scan# 3142
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:149 Resp: 2749784
Ion Ratio Lower Upper
149 100
167 28.3 22.6 34.0
279 4.6 3.7 5.5



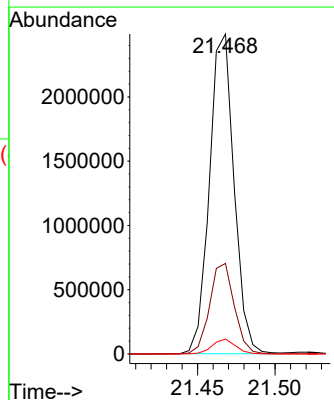





#87
Chrysene
Concen: 19.525 ng/ul
RT: 21.574 min Scan# 3160
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:228 Resp: 3865271
Ion Ratio Lower Upper
228 100
226 31.0 24.8 37.2
229 20.2 16.2 24.2



#89
Di-n-octyl phthalate
Concen: 19.524 ng/ul
RT: 22.403 min Scan# 3301
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:149 Resp: 4135717









#90
Benzo(b)fluoranthene
Concen: 18.760 ng/ul
RT: 23.209 min Scan# 3438
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53




Instrument :
BNA_M
ClientSampleId :
SSTD020036


Tgt Ion:252 Resp: 3914666
Ion Ratio Lower Upper
252 100
253 21.8 17.4 26.2
125 9.0 7.2 10.8



#91
Benzo(k)fluoranthene
Concen: 18.879 ng/ul
RT: 23.256 min Scan# 3446
Delta R.T. 0.000 min
Lab File: BM043184.D
Acq: 07 Dec 2023 16:53

Tgt Ion:252 Resp: 3923635
Ion Ratio Lower Upper
252 100
253 22.4 17.9 26.9
125 9.6 7.7 11.5





#93

Benzo(a)pyrene

Concen: 18.756 ng/ul

RT: 23.833 min Scan# 3

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Instrument :

BNA_M

ClientSampleId :

SSTD020036





Tgt Ion:252 Resp: 3617674

Ion Ratio Lower Upper

252 100

253 22.2 17.8 26.6

125 10.5 8.4 12.6



#94

Indeno(1,2,3-cd)pyrene

Concen: 19.096 ng/ul

RT: 26.438 min Scan# 3987

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53




Tgt Ion:276 Resp: 4195595


Ion Ratio Lower Upper

276 100

138 21.1 16.9 25.3

277 24.4 19.5 29.3





#95

Dibenzo(a,h)anthracene

Concen: 19.007 ng/ul

RT: 26.468 min Scan# 3992

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Instrument :

BNA_M

ClientSampleId :

SSTD020036





Tgt Ion:278 Resp: 3491586

Ion Ratio Lower Upper

278 100

139 14.9 11.9 17.9

279 24.3 19.4 29.2



#96

Benzo(g,h,i)perylene

Concen: 19.090 ng/ul

RT: 27.203 min Scan# 4117

Delta R.T. 0.000 min

Lab File: BM043184.D

Acq: 07 Dec 2023 16:53

Tgt Ion:276 Resp: 3159786

Ion Ratio Lower Upper

276 100

138 20.2 16.2 24.2

277 23.4 18.7 28.1

