
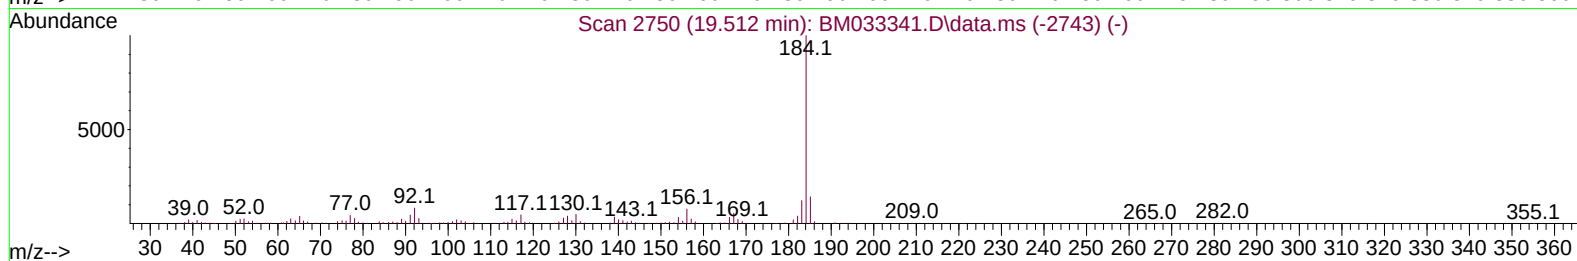
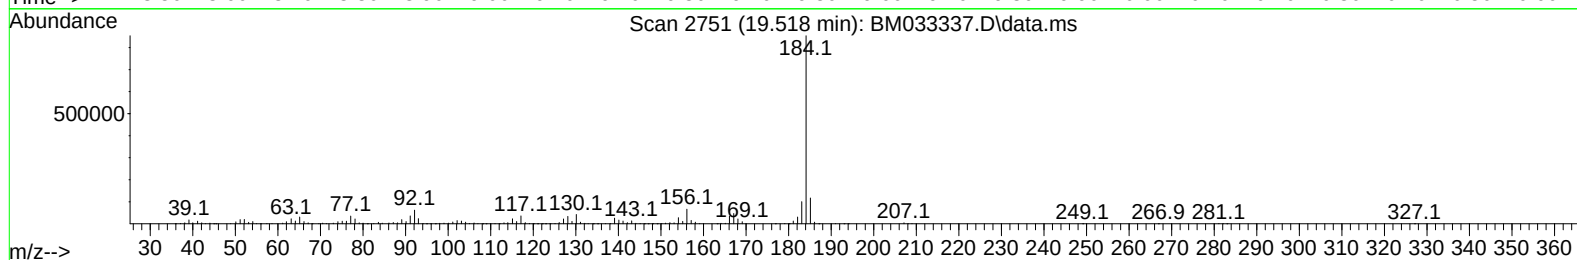


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
 Data File : BM033337.D
 Acq On : 08 Dec 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 12:26:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 07:11:07 2021
 Response via : Initial Calibration

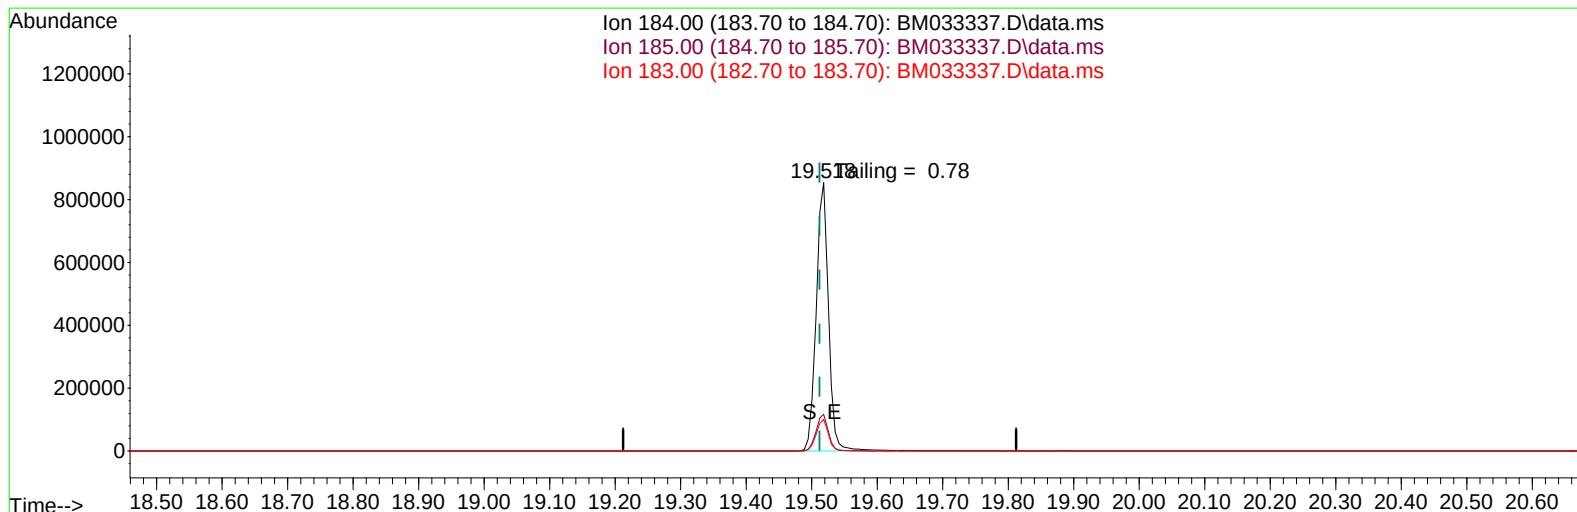

TIC: BM033337.D\data.ms

(77) Benzidine




19.518min (+ 0.006) 23323.84 ng

response 1116783

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.75
183.00	12.10	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
Data File : BM033337.D
Acq On : 08 Dec 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 12:26:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 07:11:07 2021
Response via : Initial Calibration

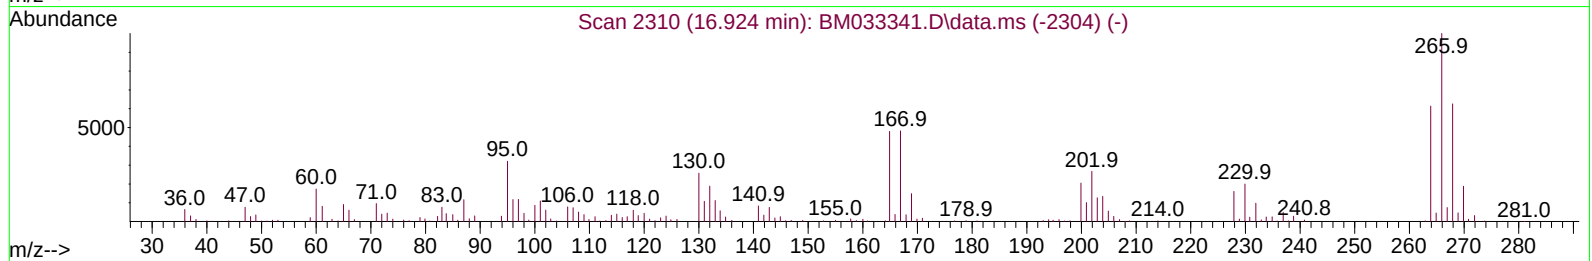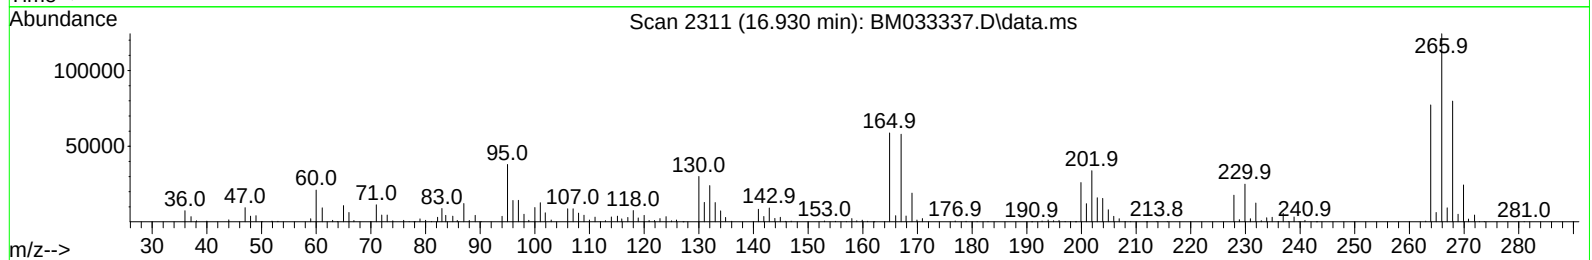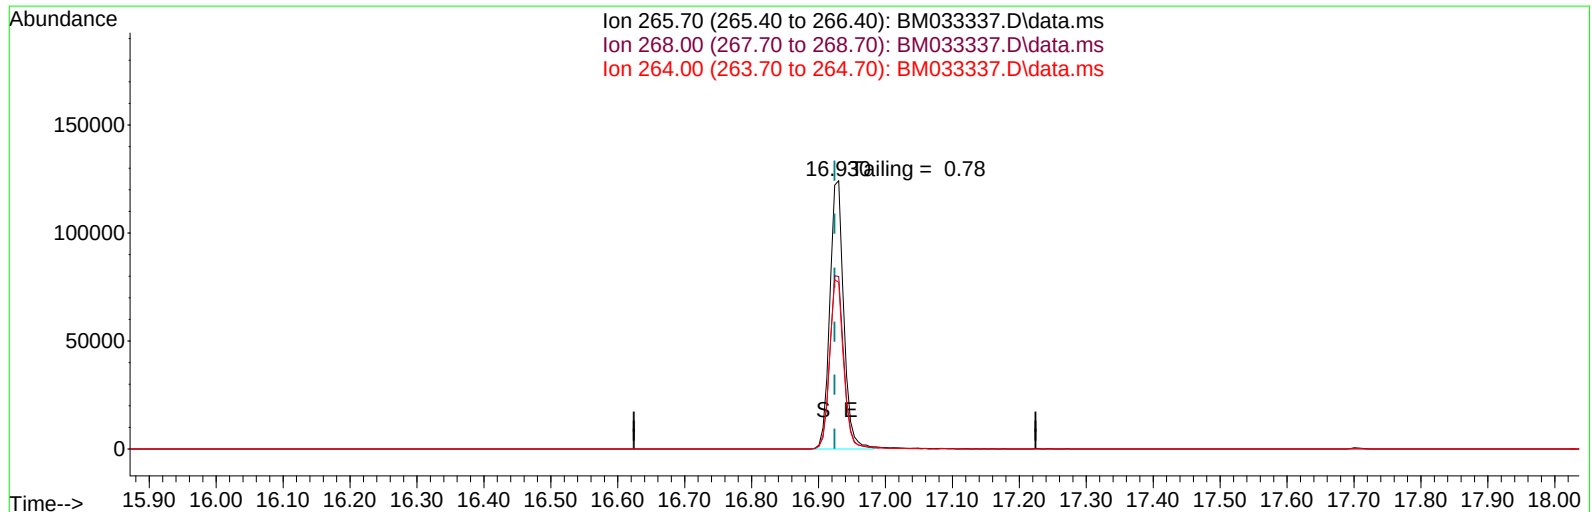

TIC: BM033337.D\data.ms

(70) Pentachlorophenol (C)

16.930min (+ 0.006) 454337.41 ng

response 181926

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.26
264.00	61.40	62.15
0.00	0.00	0.00