

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
 Data File : BM033347.D
 Acq On : 08 Dec 2021 17:24
 Operator : CG/JU
 Sample : PB141259BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB141259BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.496	360	367	379	rBV	1323987	1930336	73.76%	13.400%
2	7.084	630	637	652	rBV	1220902	1981280	75.71%	13.754%
3	7.913	772	778	787	rVB	209162	347813	13.29%	2.414%
4	9.072	968	975	990	rBV	752628	1313705	50.20%	9.119%
5	10.707	1246	1253	1267	rVB	236649	429365	16.41%	2.981%
6	13.160	1663	1670	1682	rBV	1583696	2393596	91.46%	16.616%
7	14.536	1896	1904	1912	rBV	321904	496012	18.95%	3.443%
8	16.024	2151	2157	2171	rBV	1011317	1479375	56.53%	10.269%
9	17.277	2364	2370	2384	rBV	330944	504134	19.26%	3.500%
10	19.883	2808	2813	2824	rBV	2063857	2617045	100.00%	18.167%
11	21.436	3073	3077	3085	rBV	346142	466401	17.82%	3.238%
12	23.765	3467	3473	3480	rVB	216786	446485	17.06%	3.099%




Sum of corrected areas: 14405547

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
Data File : BM033347.D
Acq On : 08 Dec 2021 17:24
Operator : CG/JU
Sample : PB141259BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141259BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

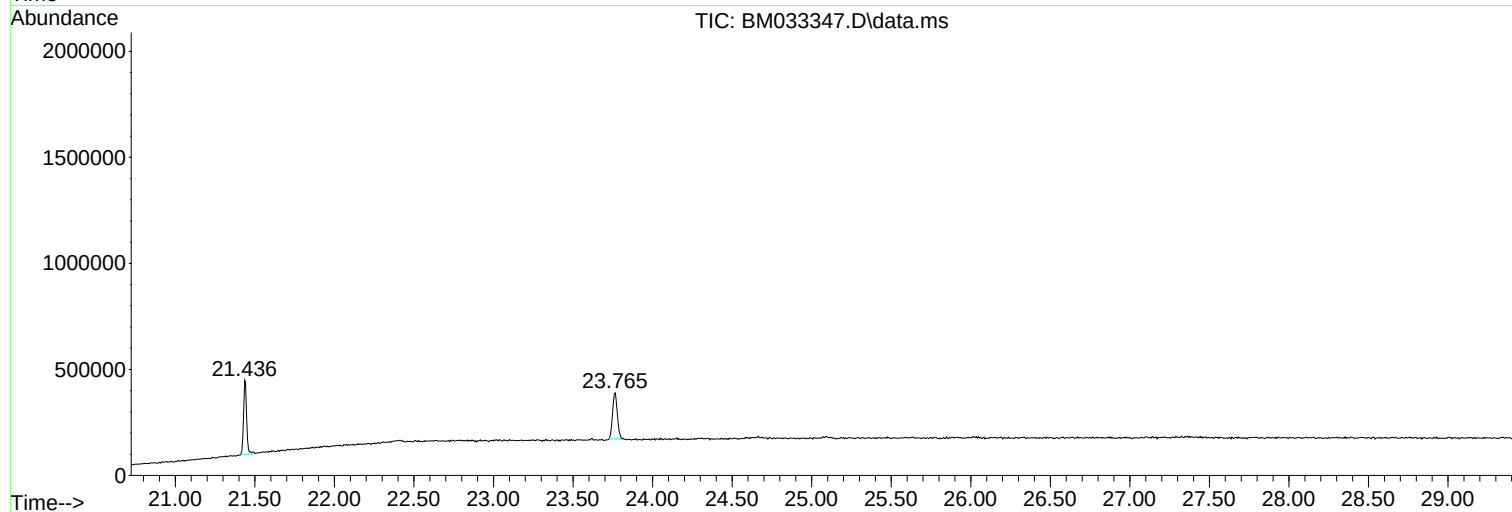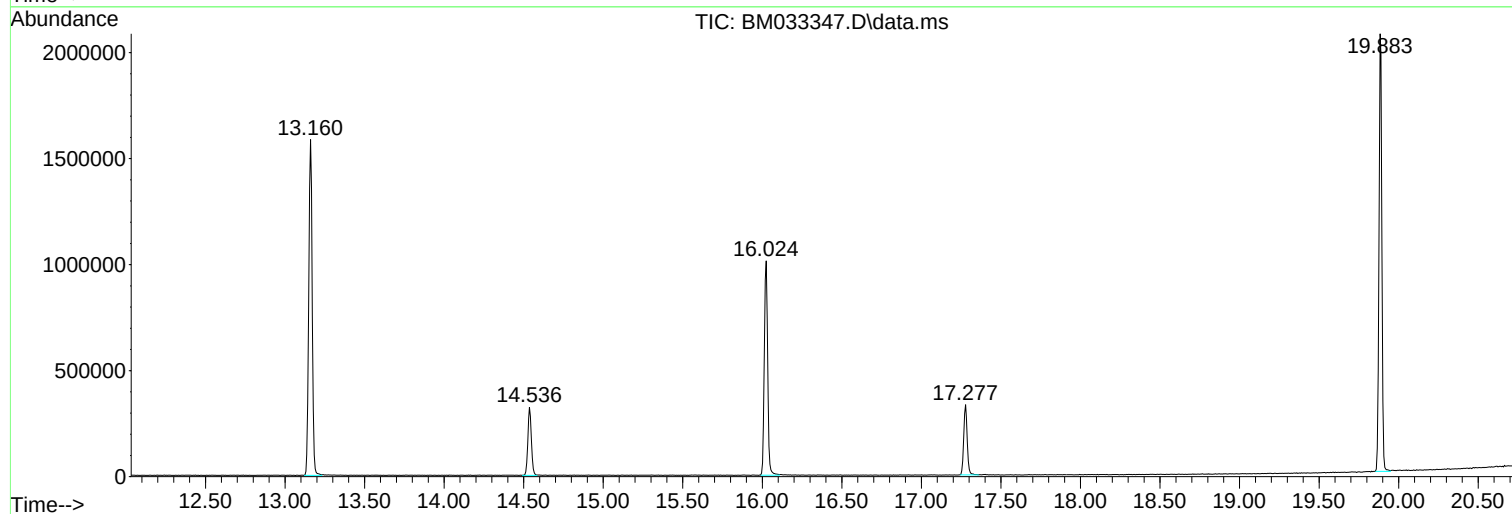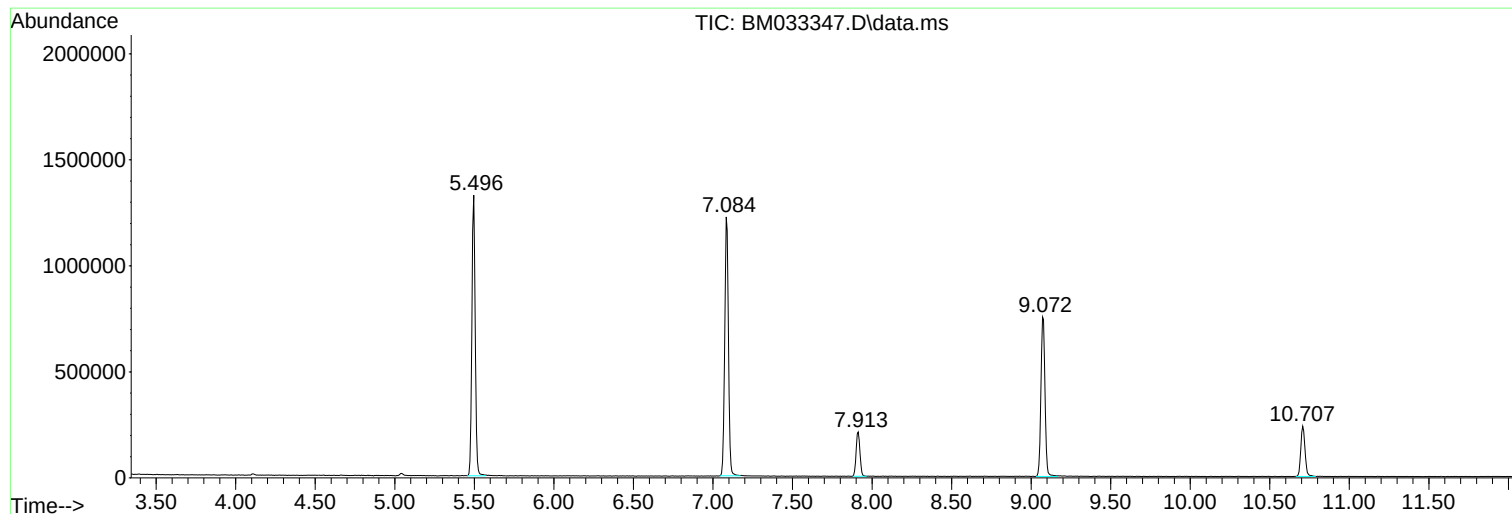

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
Data File : BM033347.D
Acq On : 08 Dec 2021 17:24
Operator : CG/JU
Sample : PB141259BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141259BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
Data File : BM033347.D
Acq On : 08 Dec 2021 17:24
Operator : CG/JU
Sample : PB141259BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB141259BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------