
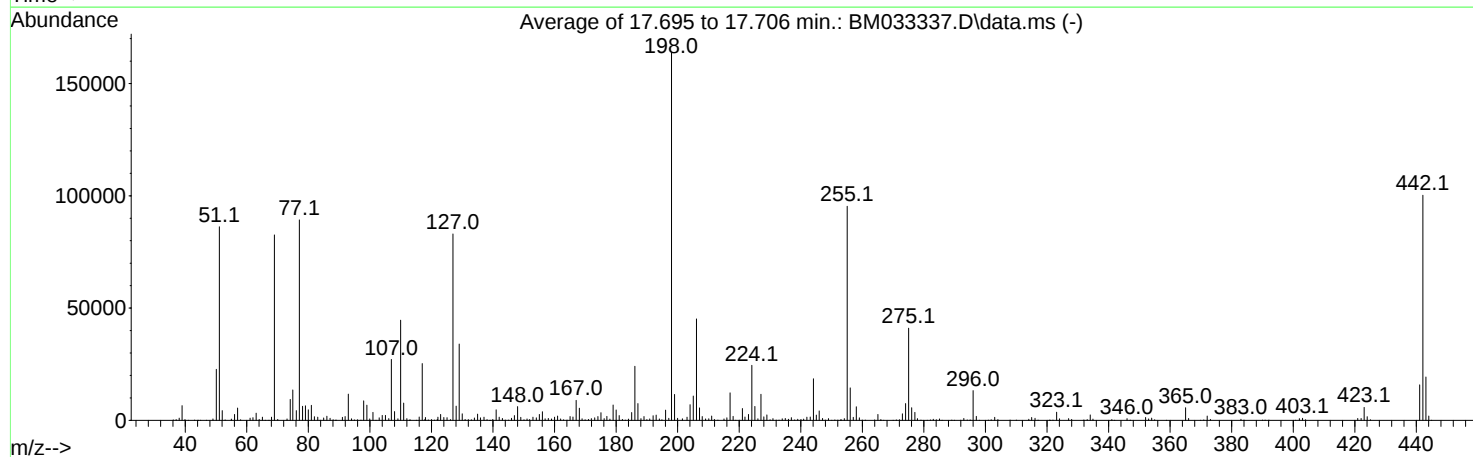


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
 Data File : BM033337.D
 Acq On : 08 Dec 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Dec 12 00:15:00 2021

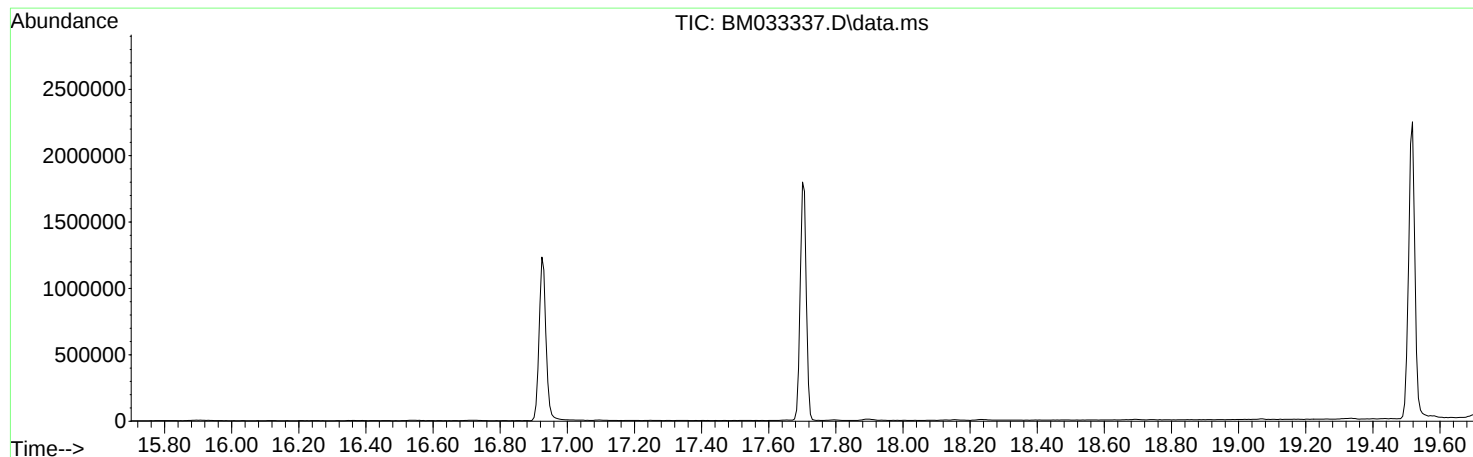

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.6	86251	PASS
68	69	0.00	2	1.7	1400	PASS
69	198	0.00	100	50.4	82611	PASS
70	69	0.00	2	0.5	441	PASS
127	198	10	80	50.7	82987	PASS
197	198	0.00	2	0.6	966	PASS
198	198	100	100	100.0	163829	PASS
199	198	5	9	7.0	11518	PASS
275	198	10	60	25.1	41085	PASS
365	198	1	100	3.4	5602	PASS
441	198	0.01	100	9.7	15819	PASS
442	442	50	100	100.0	100245	PASS
443	442	15	24	19.2	19295	PASS

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/8/2021	BNA_M	<u>BM033337.D</u>
Compound Name	Response	Retention Time
DDT	573439	20.736
DDD	4971	20.3
DDE	429	19.8
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5400	578839	0.93

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
 Data File : BM033337.D
 Acq On : 08 Dec 2021 09:47
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Dec 09 12:26:11 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 09 07:11:07 2021
 Response via : Initial Calibration

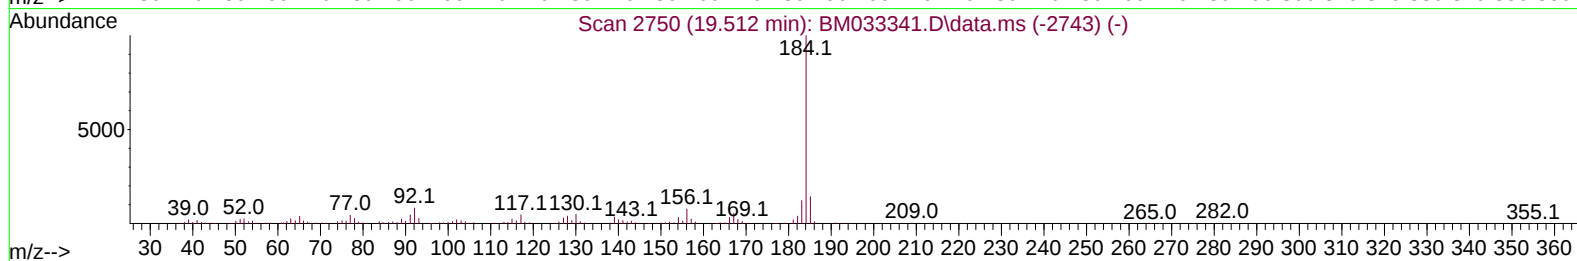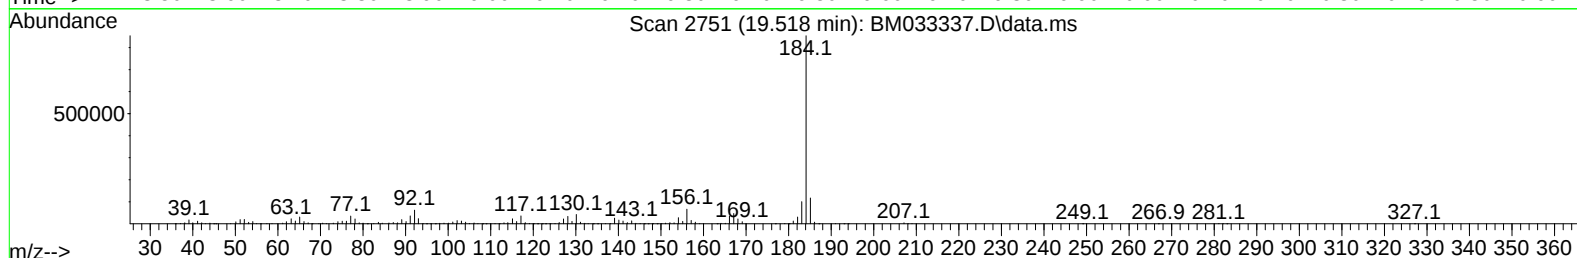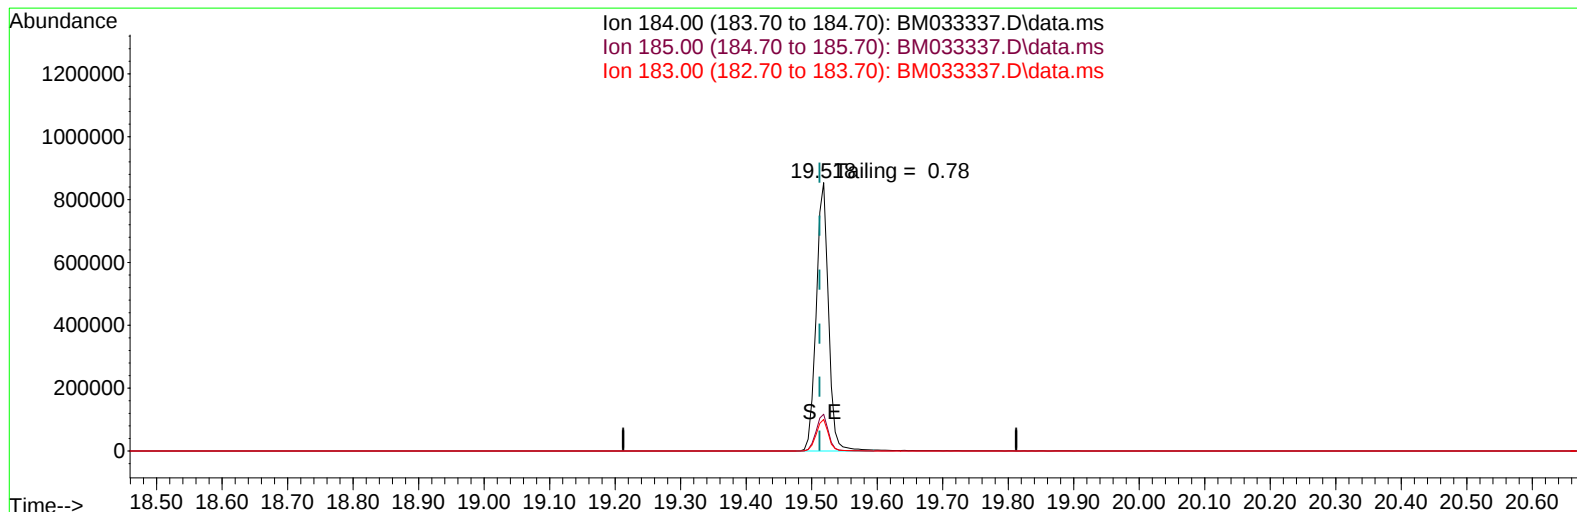

TIC: BM033337.D\data.ms

(77) Benzidine

19.518min (+ 0.006) 23323.84 ng




response 1116783

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.75
183.00	12.10	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120821\
Data File : BM033337.D
Acq On : 08 Dec 2021 09:47
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Dec 09 12:26:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 07:11:07 2021
Response via : Initial Calibration

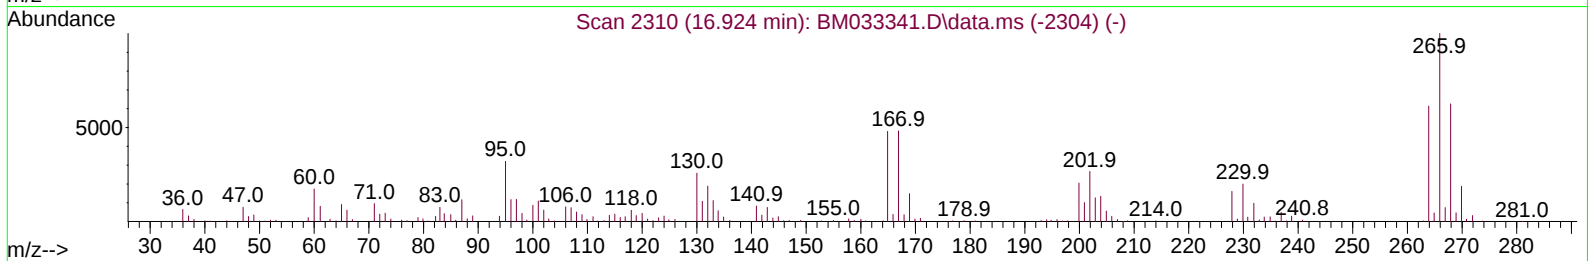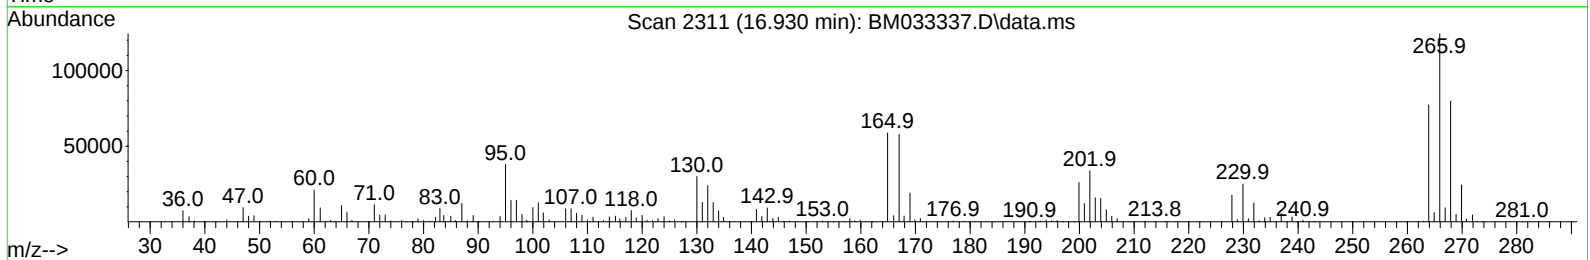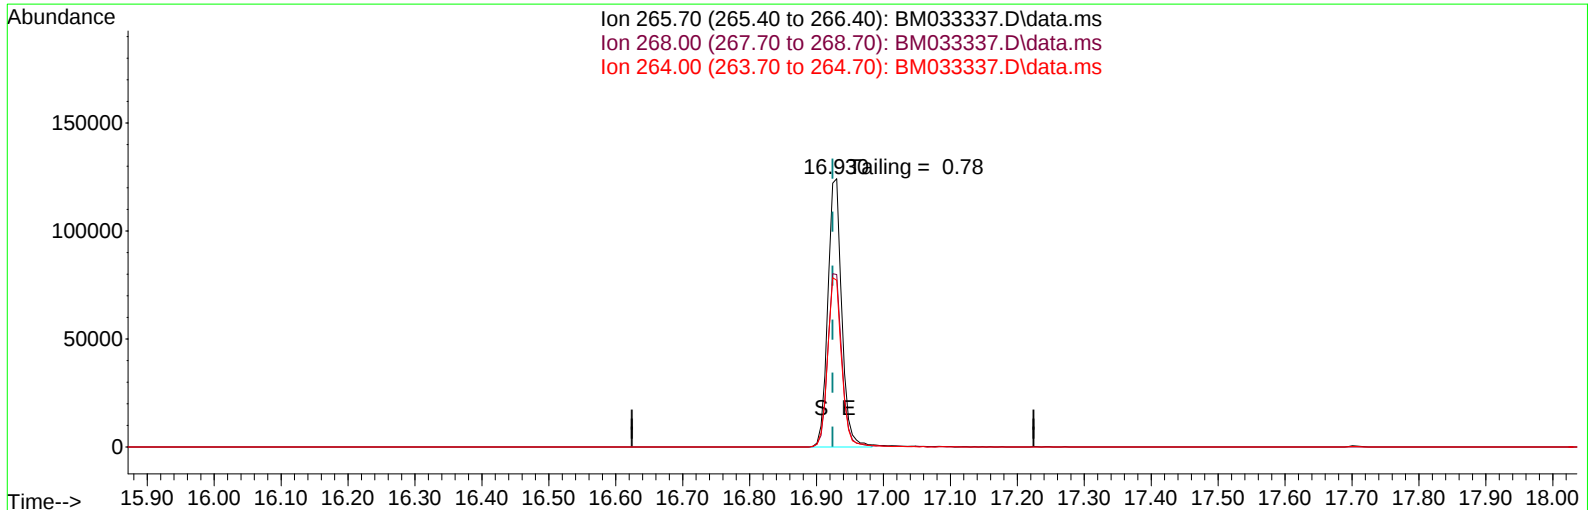

TIC: BM033337.D\data.ms

(70) Pentachlorophenol (C)

16.930min (+ 0.006) 454337.41 ng

response 181926

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	64.26
264.00	61.40	62.15
0.00	0.00	0.00