

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037881.D
 Acq On : 08 Dec 2022 11:36
 Operator : CG/JU
 Sample : N5832-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXK3

Quant Time: Dec 08 22:37:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 08 01:49:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	281029	20.000	ng/ul	0.00
20) Naphthalene-d8	10.910	136	1078588	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.715	164	569478	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.456	188	1084679	20.000	ng/ul	0.00
79) Chrysene-d12	21.633	240	904999	20.000	ng/ul	0.00
88) Perylene-d12	24.121	264	1140708	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	23090	3.731	ng/uL	0.00
4) Pyridine-d5	3.863	84	194363	10.586	ng/ul	0.00
7) Phenol-d5	7.239	99	513195	22.472	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	296460	21.319	ng/ul	0.00
11) 2-Chlorophenol-d4	7.610	132	422644	22.561	ng/ul	0.00
15) 4-Methylphenol-d8	8.792	113	394556	22.134	ng/ul	0.00
21) Nitrobenzene-d5	9.257	128	204920	23.996	ng/ul	0.00
24) 2-Nitrophenol-d4	9.980	143	212135	23.704	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	382320	22.491	ng/ul	0.00
31) 4-Chloroaniline-d4	11.045	131	310441	13.230	ng/ul	0.00
46) Dimethylphthalate-d6	14.121	166	1007631	24.819	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	1209860	24.382	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	146914	21.233	ng/ul	0.00
60) Fluorene-d10	15.704	176	901444	24.921	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.815	200	115768	19.963	ng/ul	0.00
73) Anthracene-d10	17.556	188	1323680	26.148	ng/ul	0.00
81) Pyrene-d10	19.839	212	1404724	25.840	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.962	264	1466214	25.734	ng/ul	0.02
Target Compounds						
					Qvalue	
8) Phenol	7.269	94	24776	1.082	ng/ul	99
16) Acetophenone	8.916	105	94206	3.360	ng/ul	97
30) Naphthalene	10.957	128	509322	8.750	ng/ul	99
36) 2-Methylnaphthalene	12.557	142	149306	3.955	ng/ul	95
37) 1-Methylnaphthalene	12.774	142	56913	1.474	ng/ul	97
43) 1,1'-Biphenyl	13.551	154	56408	1.232	ng/ul	99
50) Acenaphthylene	14.439	152	714335	13.092	ng/ul	99
52) Acenaphthene	14.780	153	196825	5.215	ng/ul	96
56) Dibenzofuran	15.110	168	402145	7.805	ng/ul	99
61) Fluorene	15.757	166	290892	6.923	ng/ul	98
71) Pentachlorophenol	17.104	266	69935	8.863	ng/ul	97
72) Phenanthrene	17.498	178	2311751	39.027	ng/ul	100
74) Anthracene	17.604	178	13743256	228.305	ng/ul	97
77) Carbazole	17.862	167	2329436	44.665	ng/ul	100
80) Fluoranthene	19.509	202	5105518	79.576	ng/ul	100
82) Pyrene	19.874	202	6096803	91.306	ng/ul	99
85) Benzo(a)anthracene	21.615	228	3606492	59.193	ng/ul	96
87) Chrysene	21.674	228	5676617	99.302	ng/ul	98
90) Benzo(b)fluoranthene	23.374	252	9718411	137.422	ng/ul	97
91) Benzo(k)fluoranthene	23.374	252	9718411	141.796	ng/ul	97
93) Benzo(a)pyrene	24.021	252	4341692	69.815	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	26.726	276	3557335	44.415	ng/ul	98
95) Dibenzo(a,h)anthracene	26.732	278	935798	13.860	ng/ul#	86
96) Benzo(g,h,i)perylene	27.538	276	2798697	43.766	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037881.D
Acq On : 08 Dec 2022 11:36
Operator : CG/JU
Sample : N5832-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXK3

Quant Time: Dec 08 22:37:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 08 01:49:06 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037881.D
Acq On : 08 Dec 2022 11:36
Operator : CG/JU
Sample : N5832-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXK3

Quant Time: Dec 08 22:37:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 08 01:49:06 2022
Response via : Initial Calibration




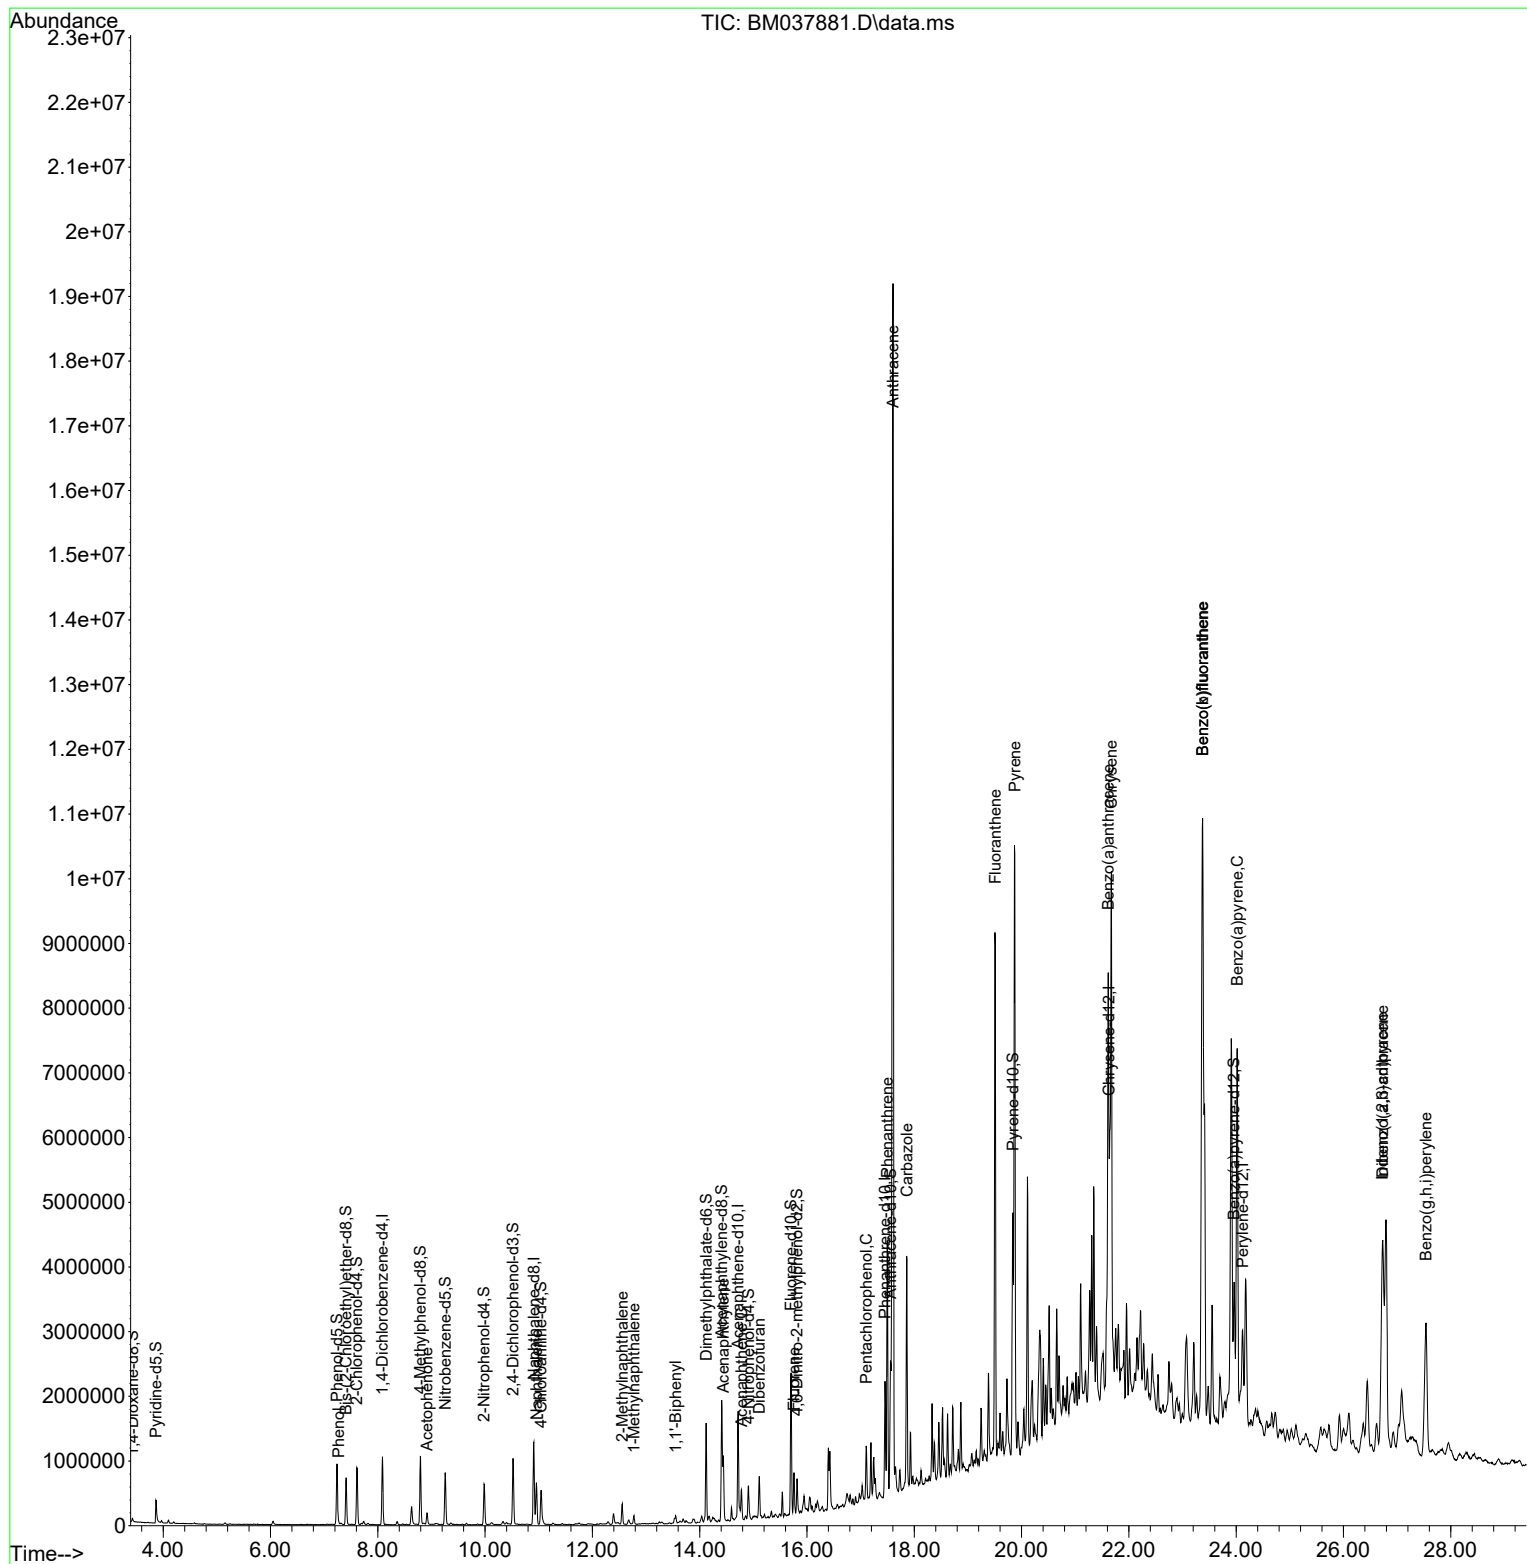




#8
Phenol
Concen: 1.082 ng/ul
RT: 7.269 min Scan# 659
Delta R.T. -0.000 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36




Instrument :
BNA_M
ClientSampleId :
DBXK3


Tgt Ion: 94 Resp: 24776
Ion Ratio Lower Upper
94 100
65 28.2 22.2 33.4
66 34.4 27.3 40.9

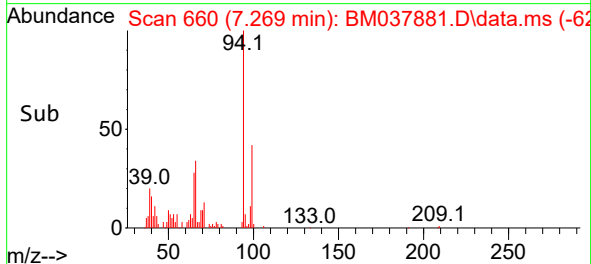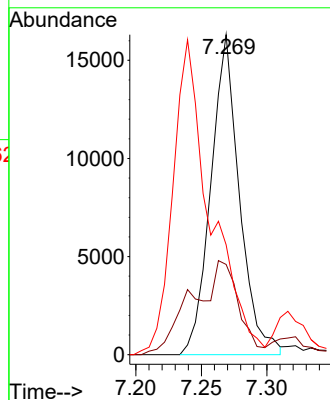

#16
Acetophenone
Concen: 3.360 ng/ul
RT: 8.916 min Scan# 940
Delta R.T. -0.006 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36

Tgt Ion: 105 Resp: 94206
Ion Ratio Lower Upper
105 100
77 72.3 59.7 89.5
51 31.9 27.2 40.8


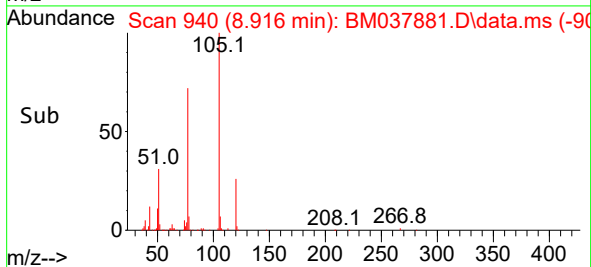
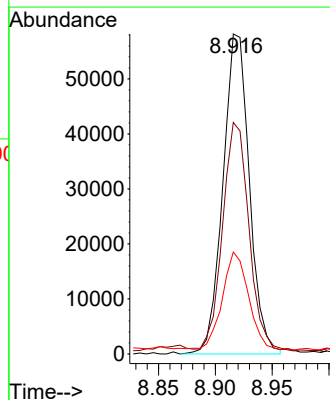
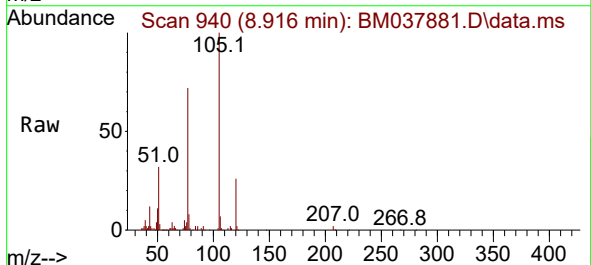




#30
Naphthalene
Concen: 8.750 ng/ul
RT: 10.957 min Scan# 1287
Delta R.T. -0.006 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36




Instrument :
BNA_M
ClientSampleId :
DBXK3


Tgt Ion:128 Resp: 509322
Ion Ratio Lower Upper
128 100
129 10.5 9.0 13.4
127 12.7 10.4 15.6

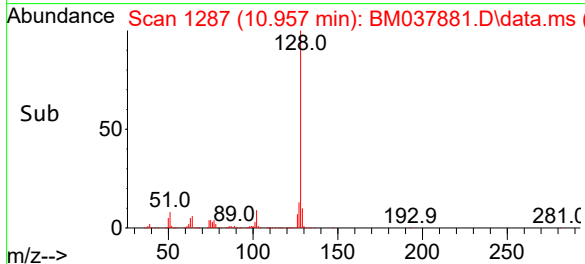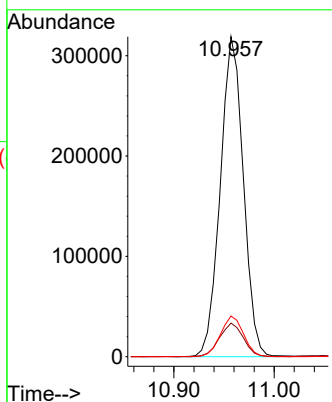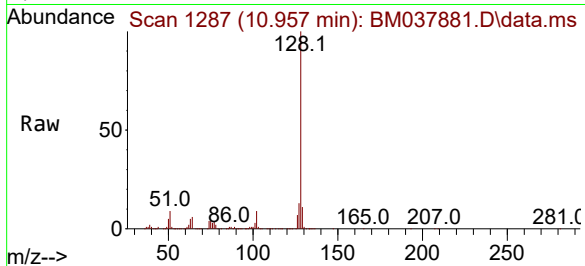

#36
2-Methylnaphthalene
Concen: 3.955 ng/ul
RT: 12.557 min Scan# 1559
Delta R.T. -0.000 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36

Tgt Ion:142 Resp: 149306
Ion Ratio Lower Upper
142 100
141 91.3 69.4 104.0


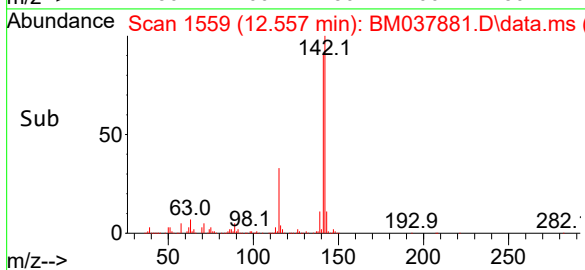
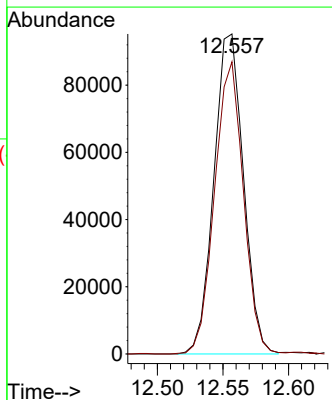
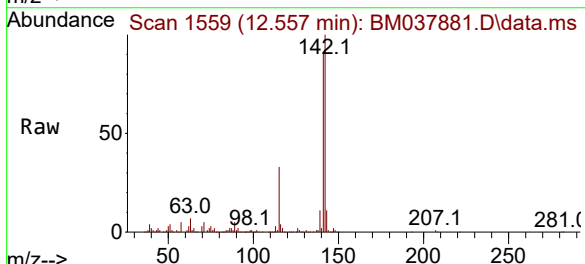




#37
1-Methylnaphthalene
Concen: 1.474 ng/ul
RT: 12.774 min Scan# 1596
Delta R.T. -0.000 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36




Instrument :
BNA_M
ClientSampleId :
DBXK3


Tgt Ion:142 Resp: 56913
Ion Ratio Lower Upper
142 100
141 87.6 72.4 108.6
116 4.3 2.9 4.3

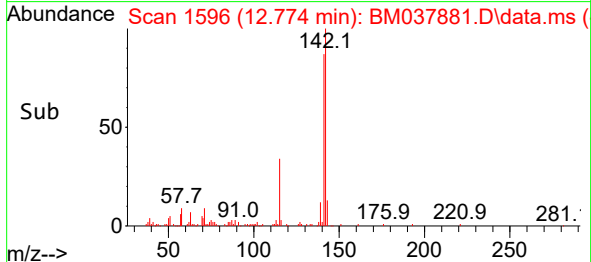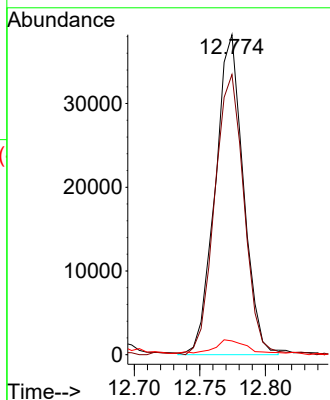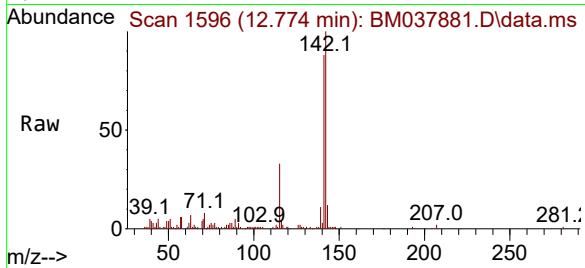

#43
1,1'-Biphenyl
Concen: 1.232 ng/ul
RT: 13.551 min Scan# 1728
Delta R.T. -0.006 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36

Tgt Ion:154 Resp: 56408
Ion Ratio Lower Upper
154 100
153 39.3 31.2 46.8
76 13.2 9.3 13.9


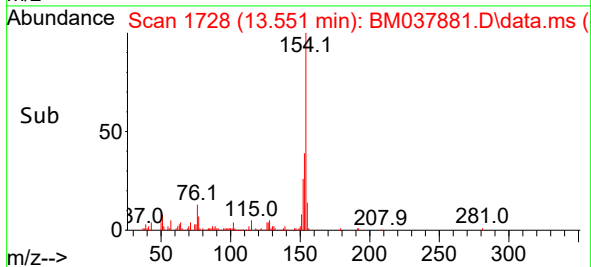
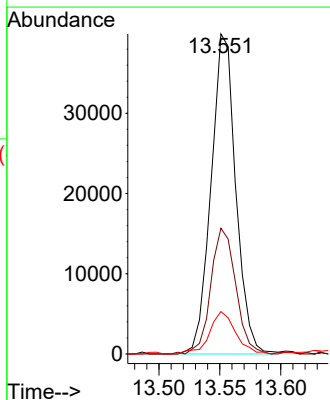
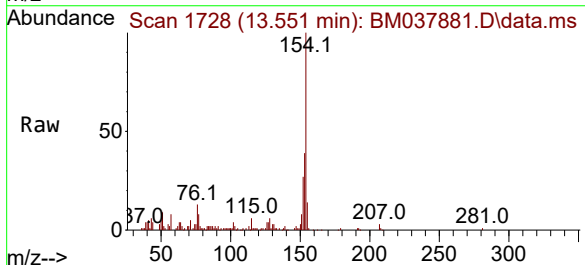




#50
Acenaphthylene
Concen: 13.092 ng/ul
RT: 14.439 min Scan# 1879
Delta R.T. -0.006 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36




Instrument :
BNA_M
ClientSampleId :
DBXK3


Tgt Ion:152 Resp: 714335
Ion Ratio Lower Upper
152 100
151 19.4 15.3 22.9
153 13.0 10.2 15.4

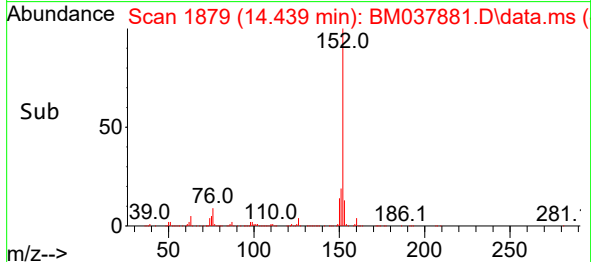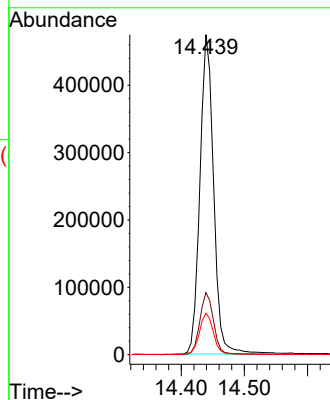

#52
Acenaphthene
Concen: 5.215 ng/ul
RT: 14.780 min Scan# 1937
Delta R.T. -0.000 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36

Tgt Ion:153 Resp: 196825
Ion Ratio Lower Upper
153 100
152 46.5 38.2 57.4
154 84.7 71.4 107.0


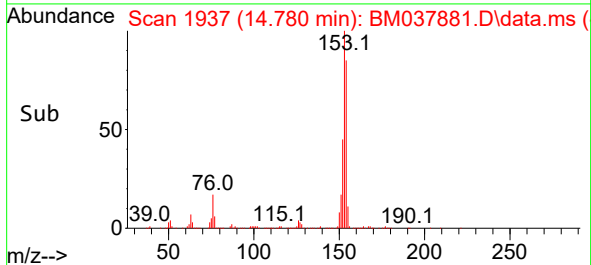
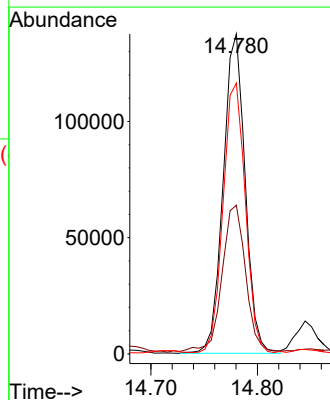
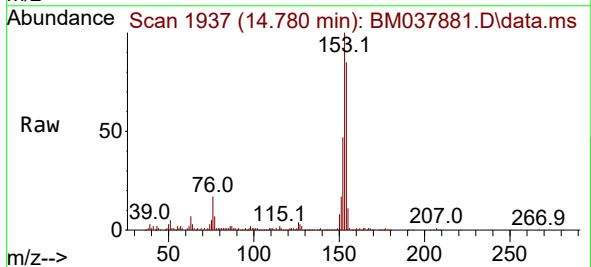




#56
Dibenzenofuran
Concen: 7.805 ng/ul
RT: 15.110 min Scan# 1993
Delta R.T. -0.006 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36




Instrument :
BNA_M
ClientSampleId :
DBXK3


Tgt Ion:168 Resp: 402145
Ion Ratio Lower Upper
168 100
139 35.5 28.1 42.1

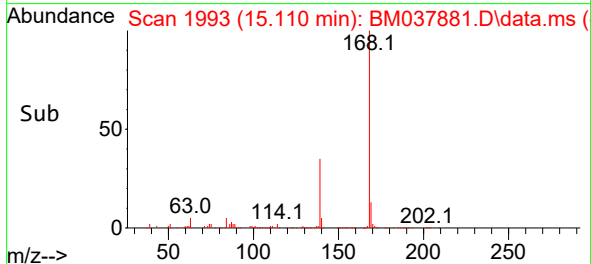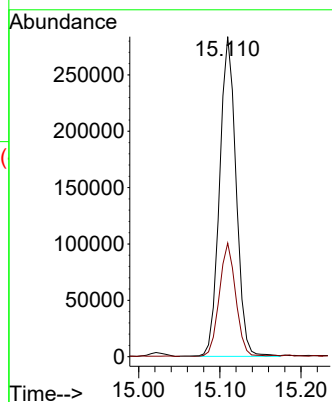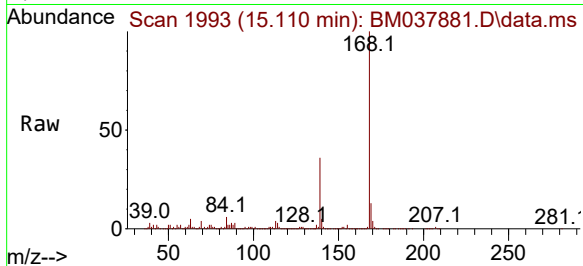

#61
Fluorene
Concen: 6.923 ng/ul
RT: 15.757 min Scan# 2103
Delta R.T. -0.006 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36

Tgt Ion:166 Resp: 290892
Ion Ratio Lower Upper
166 100
165 98.3 77.2 115.8
167 13.7 10.4 15.6

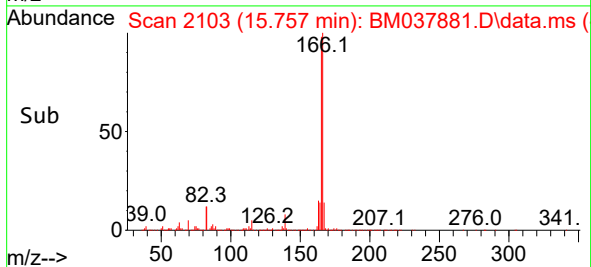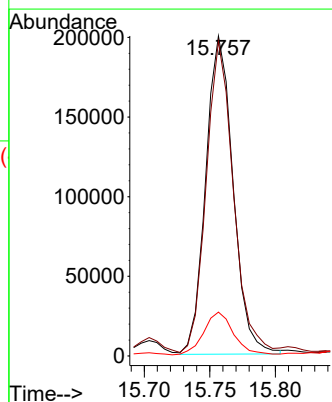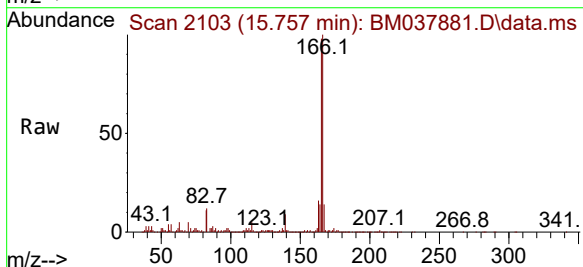



#71

Pentachlorophenol

Concen: 8.863 ng/ul

RT: 17.104 min Scan# 21

Delta R.T. -0.000 min

Lab File: BM037881.D

Acq: 08 Dec 2022 11:36

Instrument :

BNA_M

ClientSampleId :

DBXK3





Tgt Ion:266 Resp: 69935

Ion Ratio Lower Upper

266 100

264 58.5 50.1 75.1

268 64.3 50.6 75.8

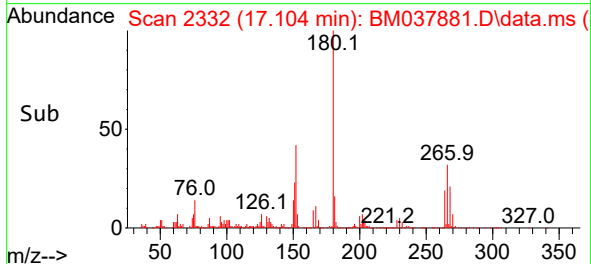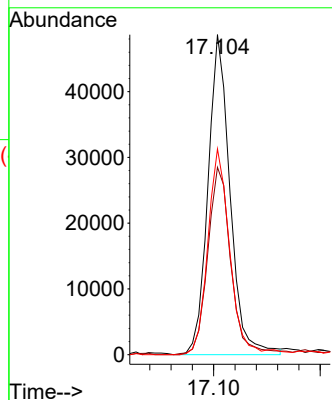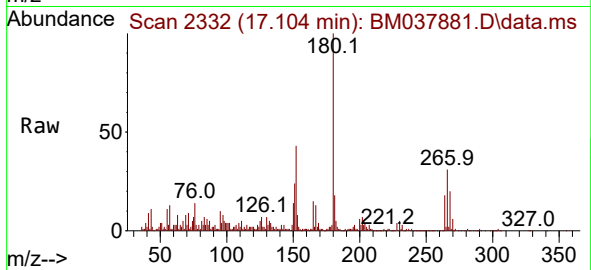

#72

Phenanthrene

Concen: 39.027 ng/ul

RT: 17.498 min Scan# 2399

Delta R.T. -0.000 min

Lab File: BM037881.D

Acq: 08 Dec 2022 11:36




Tgt Ion:178 Resp: 2311751


Ion Ratio Lower Upper

178 100

179 15.4 12.2 18.2

176 19.2 15.4 23.0


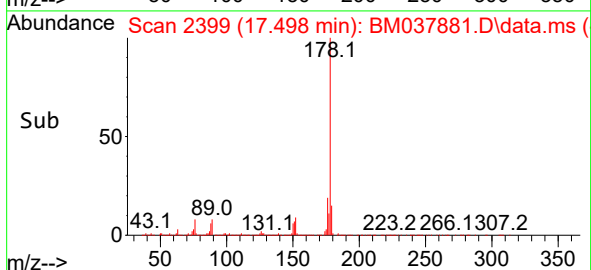
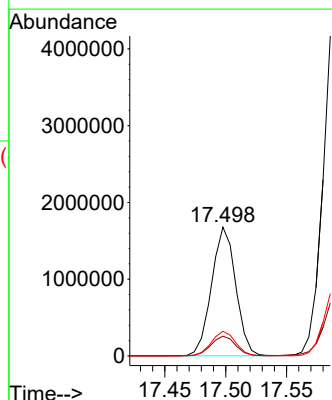





#74
 Anthracene
 Concen: 228.305 ng/ul
 RT: 17.604 min Scan# 2414
 Delta R.T. 0.012 min
 Lab File: BM037881.D
 Acq: 08 Dec 2022 11:36




Instrument :
 BNA_M
 ClientSampleId :
 DBXK3


Tgt Ion:178 Resp:13743256
 Ion Ratio Lower Upper
 178 100
 179 16.4 11.8 17.8
 176 20.1 15.0 22.6

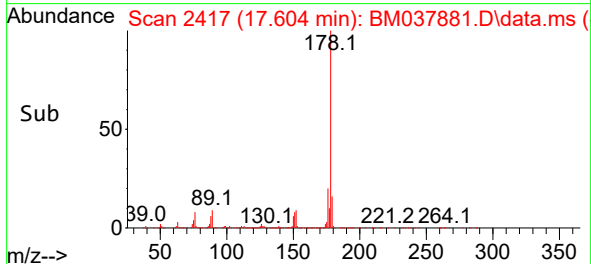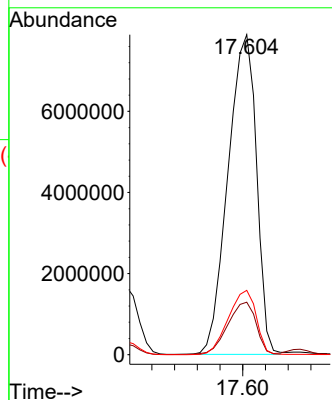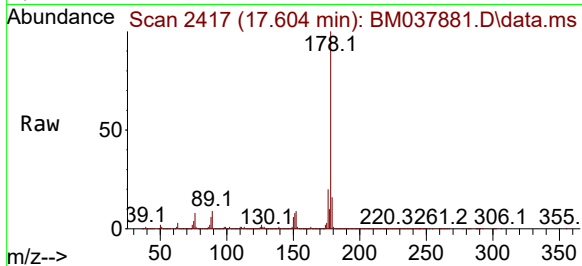

#77
 Carbazole
 Concen: 44.665 ng/ul
 RT: 17.862 min Scan# 2461
 Delta R.T. 0.006 min
 Lab File: BM037881.D
 Acq: 08 Dec 2022 11:36

Tgt Ion:167 Resp: 2329436
 Ion Ratio Lower Upper
 167 100
 166 20.9 16.7 25.1
 139 12.5 9.8 14.6


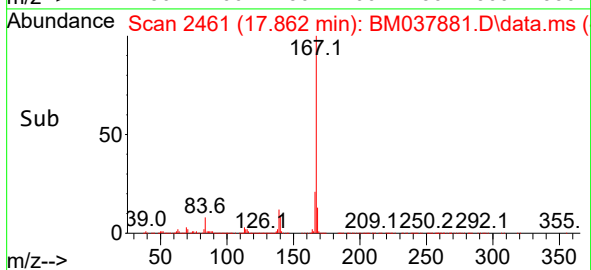
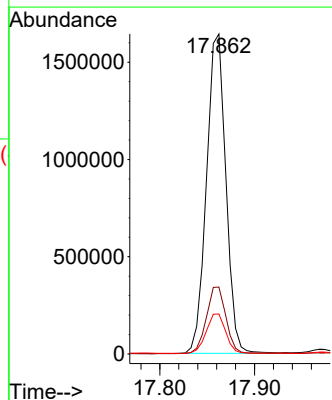
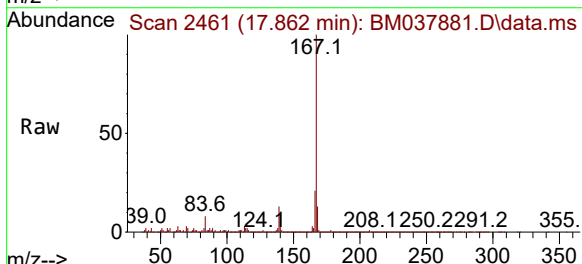




#80
 Fluoranthene
 Concen: 79.576 ng/ul
 RT: 19.509 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BM037881.D
 Acq: 08 Dec 2022 11:36




Instrument :
 BNA_M
 ClientSampleId :
 DBXK3


Tgt Ion:202 Resp: 5105518
 Ion Ratio Lower Upper
 202 100
 101 10.7 8.6 13.0
 100 8.2 6.6 10.0

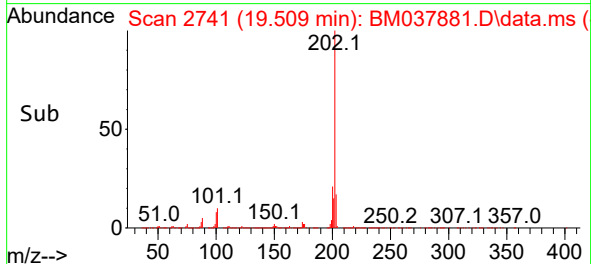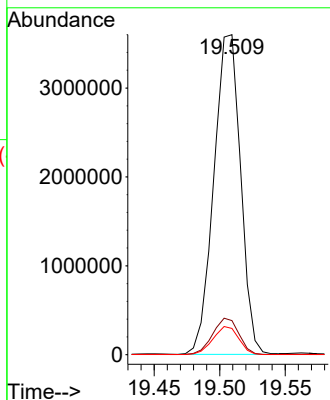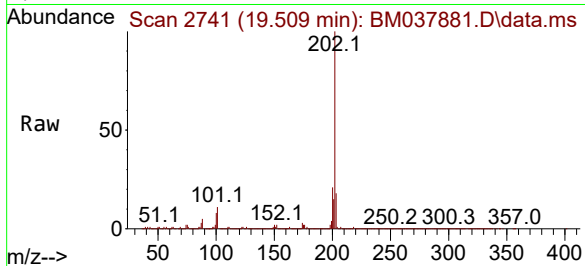

#82
 Pyrene
 Concen: 91.306 ng/ul
 RT: 19.874 min Scan# 2803
 Delta R.T. 0.006 min
 Lab File: BM037881.D
 Acq: 08 Dec 2022 11:36

Tgt Ion:202 Resp: 6096803
 Ion Ratio Lower Upper
 202 100
 101 12.8 10.0 15.0
 100 10.3 7.9 11.9

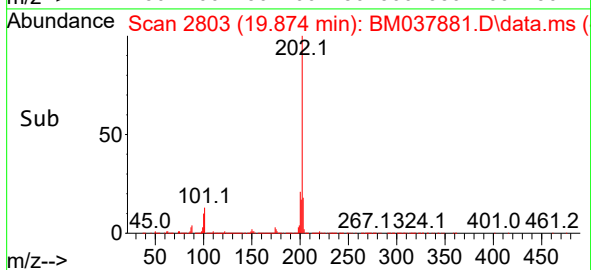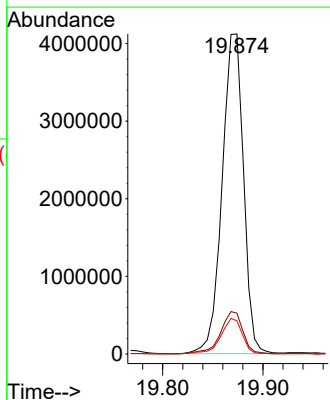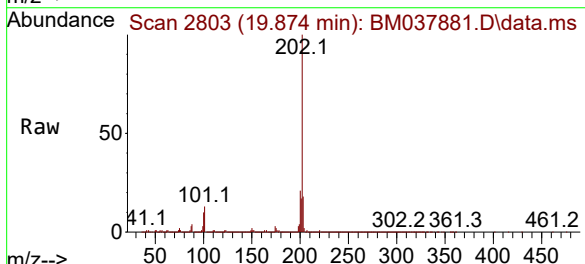



#85

Benzo(a)anthracene

Concen: 59.193 ng/ul

RT: 21.615 min Scan# 3099

Delta R.T. 0.006 min

Lab File: BM037881.D

Acq: 08 Dec 2022 11:36

Instrument :

BNA_M

ClientSampleId :

DBXK3





Tgt Ion:228 Resp: 3606492

Ion Ratio Lower Upper

228 100

229 21.0 15.5 23.3

226 29.2 21.8 32.8

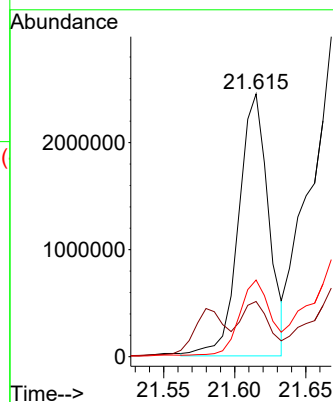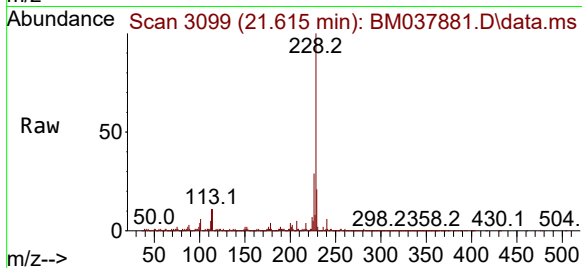

#87

Chrysene

Concen: 99.302 ng/ul

RT: 21.674 min Scan# 3109

Delta R.T. 0.012 min

Lab File: BM037881.D

Acq: 08 Dec 2022 11:36




Tgt Ion:228 Resp: 5676617


Ion Ratio Lower Upper

228 100

226 30.3 24.3 36.5

229 21.5 15.6 23.4


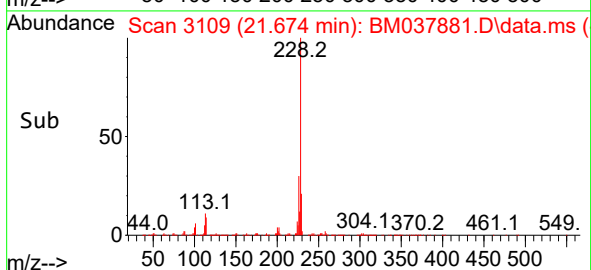
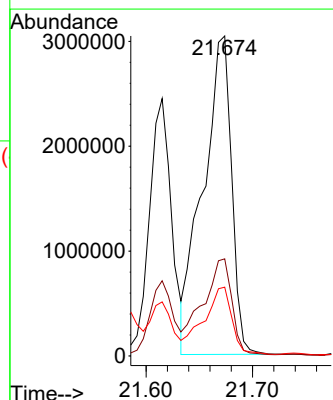
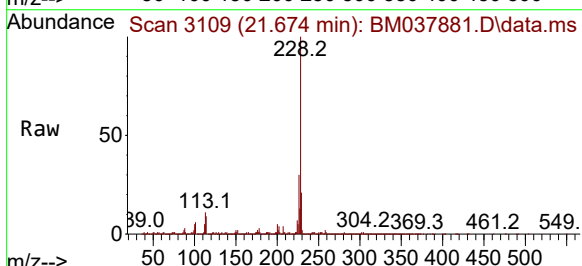




#90
Benzo(b)fluoranthene
Concen: 137.422 ng/ul
RT: 23.374 min Scan# 3398
Delta R.T. 0.029 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36




Instrument :
BNA_M
ClientSampleId :
DBXK3


Tgt Ion:252 Resp: 9718411
Ion Ratio Lower Upper
252 100
253 23.4 17.6 26.4
125 10.9 8.0 12.0

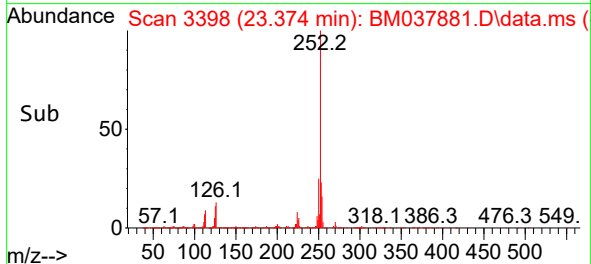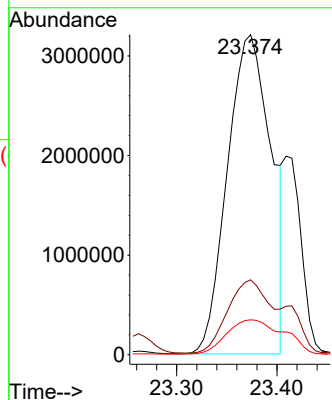

#91
Benzo(k)fluoranthene
Concen: 141.796 ng/ul
RT: 23.374 min Scan# 3398
Delta R.T. -0.024 min
Lab File: BM037881.D
Acq: 08 Dec 2022 11:36

Tgt Ion:252 Resp: 9718411
Ion Ratio Lower Upper
252 100
253 23.4 17.4 26.2
125 10.9 8.1 12.1

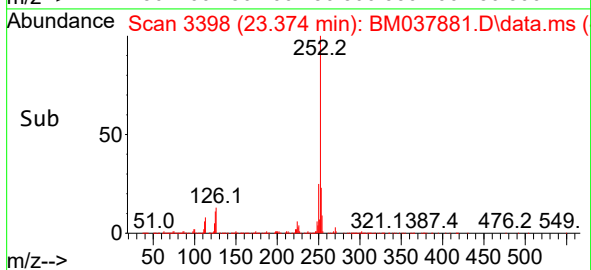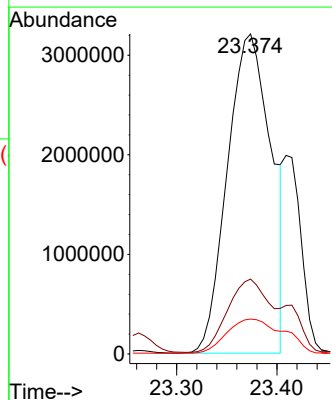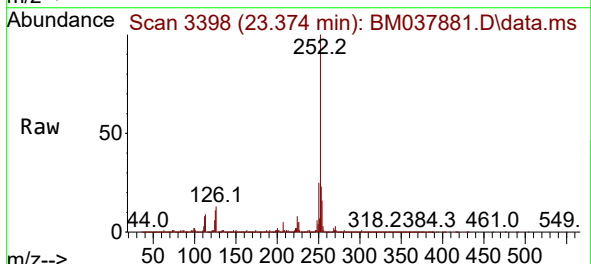



#93

Benzo(a)pyrene

Concen: 69.815 ng/ul

RT: 24.021 min Scan# 3

Delta R.T. 0.023 min

Lab File: BM037881.D

Acq: 08 Dec 2022 11:36

Instrument :

BNA_M

ClientSampleId :

DBXK3





Tgt Ion:252 Resp: 4341692

Ion Ratio Lower Upper

252 100

253 23.6 17.4 26.0

125 11.2 9.4 14.0

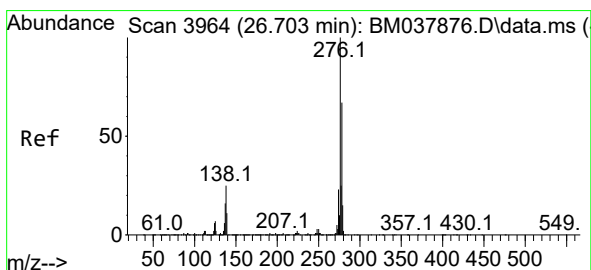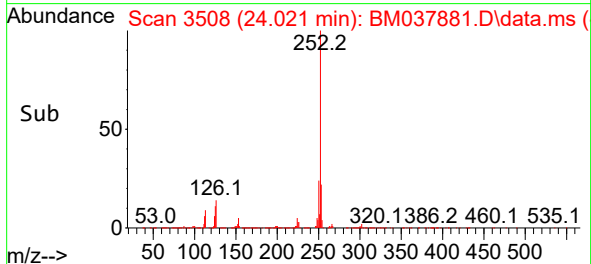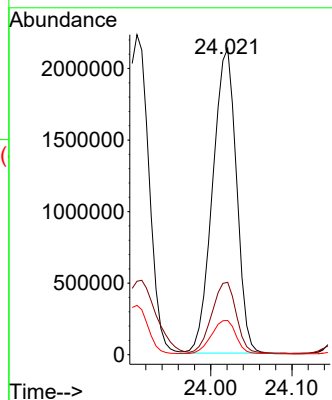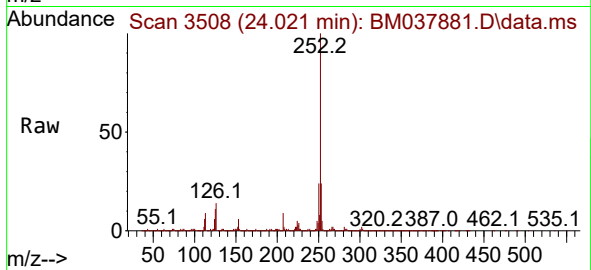

#94

Indeno(1,2,3-cd)pyrene

Concen: 44.415 ng/ul

RT: 26.726 min Scan# 3968

Delta R.T. 0.018 min

Lab File: BM037881.D

Acq: 08 Dec 2022 11:36




Tgt Ion:276 Resp: 3557335


Ion Ratio Lower Upper

276 100

138 22.3 19.3 28.9

277 24.6 19.8 29.8

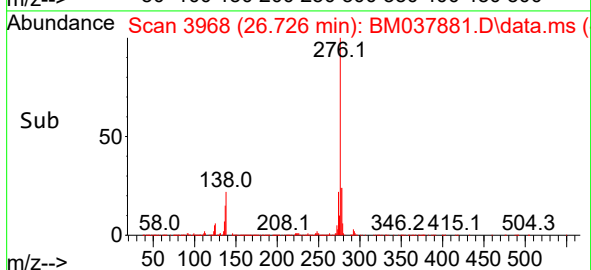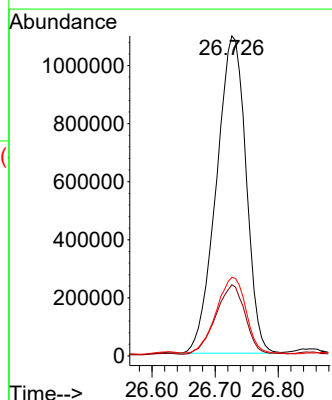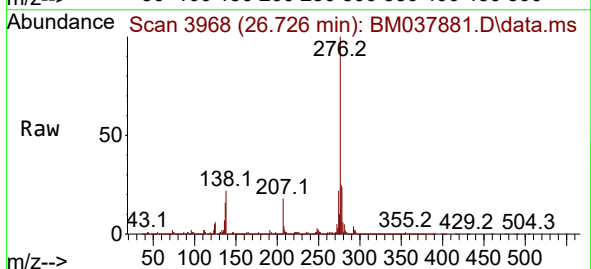



#95

Dibenzo(a,h)anthracene

Concen: 13.860 ng/ul

RT: 26.732 min Scan# 3969

Delta R.T. 0.006 min

Lab File: BM037881.D

Acq: 08 Dec 2022 11:36

Instrument :

BNA_M

ClientSampleId :

DBXK3





Tgt Ion:278 Resp: 935798

Ion Ratio Lower Upper

278 100

139 0.0 12.4 18.6#

279 24.6 19.8 29.6

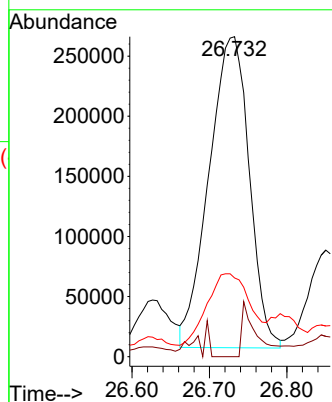

#96

Benzo(g,h,i)perylene

Concen: 43.766 ng/ul

RT: 27.538 min Scan# 4106

Delta R.T. 0.023 min

Lab File: BM037881.D

Acq: 08 Dec 2022 11:36

Tgt Ion:276 Resp: 2798697

Ion Ratio Lower Upper

276 100

138 21.8 17.1 25.7

277 24.4 18.2 27.4

