

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037890.D
 Acq On : 08 Dec 2022 17:13
 Operator : CG/JU
 Sample : PB149468BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK468

Quant Time: Dec 08 22:40:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 08 01:49:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.087	152	286774	20.000	ng/ul	0.00
20) Naphthalene-d8	10.910	136	1120385	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.716	164	577592	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.457	188	1062456	20.000	ng/ul	0.00
79) Chrysene-d12	21.621	240	890034	20.000	ng/ul	0.00
88) Perylene-d12	24.109	264	985273	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	26300	4.164	ng/uL	0.00
4) Pyridine-d5	3.863	84	379056	20.231	ng/ul	0.00
7) Phenol-d5	7.240	99	526796	22.606	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	323278	22.782	ng/ul	0.00
11) 2-Chlorophenol-d4	7.616	132	456226	23.865	ng/ul	0.00
15) 4-Methylphenol-d8	8.798	113	405308	22.281	ng/ul	0.00
21) Nitrobenzene-d5	9.263	128	220888	24.901	ng/ul	0.00
24) 2-Nitrophenol-d4	9.986	143	236613	25.453	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	383236	21.704	ng/ul	0.00
31) 4-Chloroaniline-d4	11.045	131	555077	22.774	ng/ul	0.00
46) Dimethylphthalate-d6	14.121	166	977623	23.741	ng/ul	0.00
49) Acenaphthylene-d8	14.410	160	1196061	23.765	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	138053	19.672	ng/ul	0.00
60) Fluorene-d10	15.704	176	839367	22.879	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.821	200	97184	17.109	ng/ul	0.00
73) Anthracene-d10	17.551	188	1234361	24.893	ng/ul	0.00
81) Pyrene-d10	19.839	212	1307974	24.464	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.944	264	1266092	25.727	ng/ul	0.00


Target Compounds					Qvalue
86) Bis(2-ethylhexyl)phtha...	21.515	149	40625	1.144 ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037890.D
Acq On : 08 Dec 2022 17:13
Operator : CG/JU
Sample : PB149468BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK468

Quant Time: Dec 08 22:40:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 08 01:49:06 2022
Response via : Initial Calibration

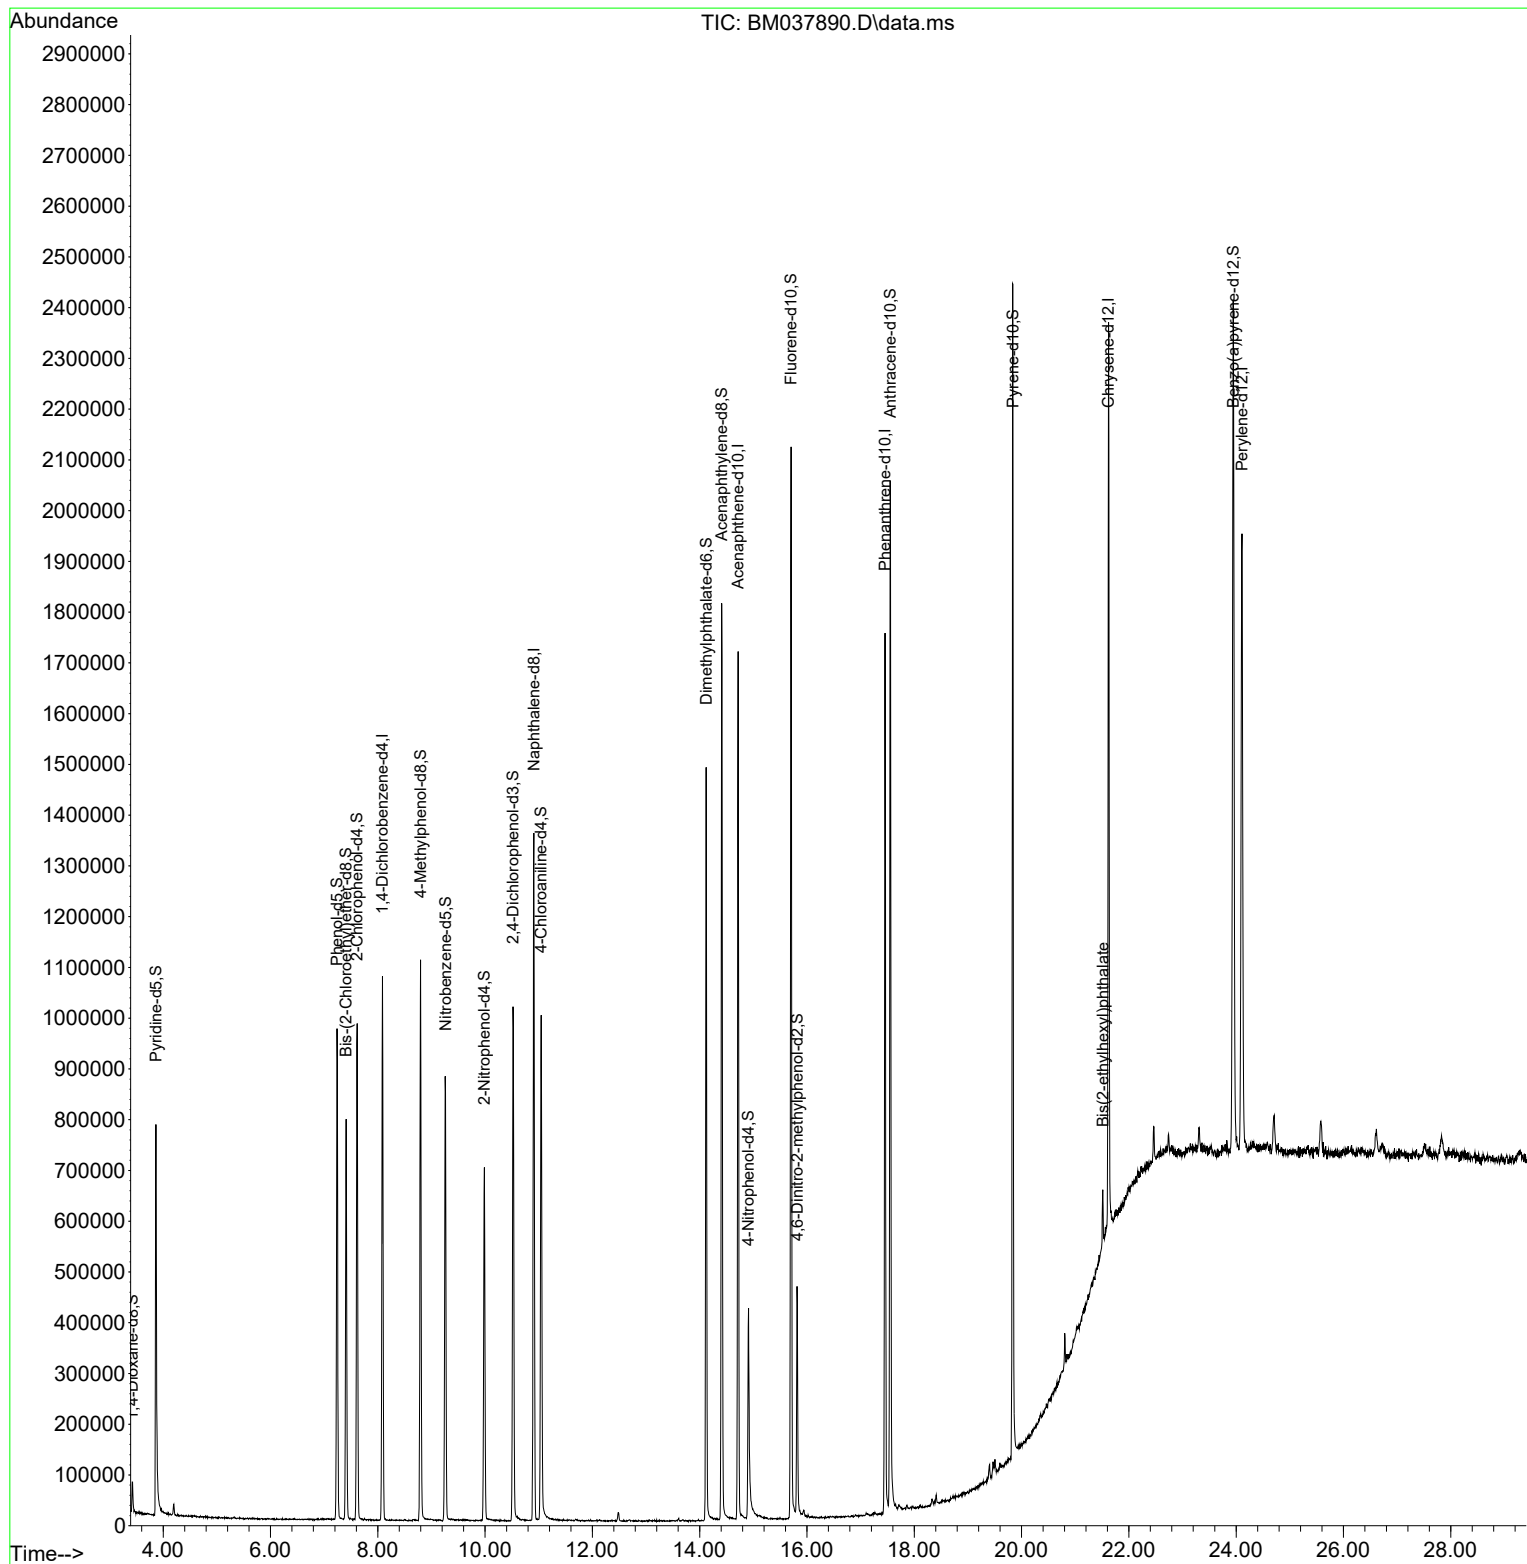

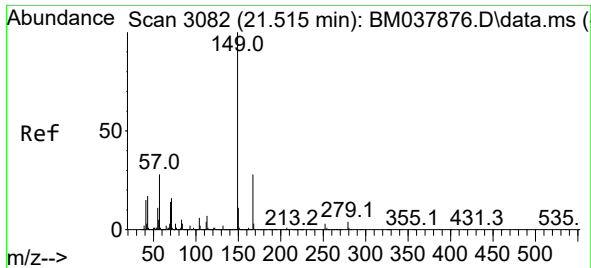

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.144 ng/ul
 RT: 21.515 min Scan# 3082
 Delta R.T. 0.000 min
 Lab File: BM037890.D
 Acq: 08 Dec 2022 17:13

Instrument :
 BNA_M
 ClientSampleId :
 SBLK468

Tgt Ion:149 Resp: 40625
 Ion Ratio Lower Upper
 149 100
 167 27.6 21.5 32.3
 279 4.9 3.2 4.8#

