

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037894.D
 Acq On : 08 Dec 2022 19:41
 Operator : CG/JU
 Sample : N5832-18 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXL3

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022
 Supervised By :mohammad ahmed 12/10/2022

Quant Time: Dec 08 22:41:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 08 01:49:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.086	152	299248	20.000	ng/u1	0.00
20) Naphthalene-d8	10.910	136	1166431	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.715	164	601906	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.456	188	1109369	20.000	ng/u1	0.00
79) Chrysene-d12	21.621	240	914218	20.000	ng/u1	0.00
88) Perylene-d12	24.109	264	1046721	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	3551	0.539	ng/uL	0.00
4) Pyridine-d5	3.887	84	16643m	0.851	ng/u1	0.02
7) Phenol-d5	7.239	99	56881	2.339	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	37653	2.543	ng/u1	0.00
11) 2-Chlorophenol-d4	7.610	132	48896	2.451	ng/u1	0.00
15) 4-Methylphenol-d8	8.792	113	42550	2.242	ng/u1	0.00
21) Nitrobenzene-d5	9.257	128	22263	2.411	ng/u1	0.00
24) 2-Nitrophenol-d4	9.980	143	22976	2.374	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	39644	2.157	ng/u1	0.00
31) 4-Chloroaniline-d4	11.045	131	32890	1.296	ng/u1	0.00
46) Dimethylphthalate-d6	14.121	166	106549	2.483	ng/u1	0.00
49) Acenaphthylene-d8	14.410	160	129552	2.470	ng/u1	0.00
54) 4-Nitrophenol-d4	14.915	143	8951m	1.224	ng/u1	0.00
60) Fluorene-d10	15.704	176	96466	2.523	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.815	200	7749m	1.306	ng/u1	0.00
73) Anthracene-d10	17.551	188	152192	2.939	ng/u1	0.00
81) Pyrene-d10	19.833	212	159212	2.899	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.944	264	148064	2.832	ng/u1	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.957	128	80264	1.275	ng/u1	97
50) Acenaphthylene	14.439	152	104239	1.808	ng/u1	99
72) Phenanthrene	17.498	178	207036	3.417	ng/u1	99
74) Anthracene	17.586	178	857379	13.926	ng/u1	100
80) Fluoranthene	19.503	202	435351	6.717	ng/u1	97
82) Pyrene	19.862	202	449937	6.670	ng/u1	99
85) Benzo(a)anthracene	21.603	228	289759	4.708	ng/u1	97
87) Chrysene	21.662	228	376992	6.528	ng/u1	99
90) Benzo(b)fluoranthene	23.344	252	902508	13.908	ng/u1	98
91) Benzo(k)fluoranthene	23.391	252	259465m	4.126	ng/u1	
93) Benzo(a)pyrene	23.997	252	390600	6.845	ng/u1	95
94) Indeno(1,2,3-cd)pyrene	26.697	276	361799	4.923	ng/u1	98
95) Dibenzo(a,h)anthracene	26.709	278	91053	1.470	ng/u1#	92
96) Benzo(g,h,i)perylene	27.503	276	286618	4.885	ng/u1	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037894.D
Acq On : 08 Dec 2022 19:41
Operator : CG/JU
Sample : N5832-18 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBXL3

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

Quant Time: Dec 08 22:41:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 08 01:49:06 2022
Response via : Initial Calibration

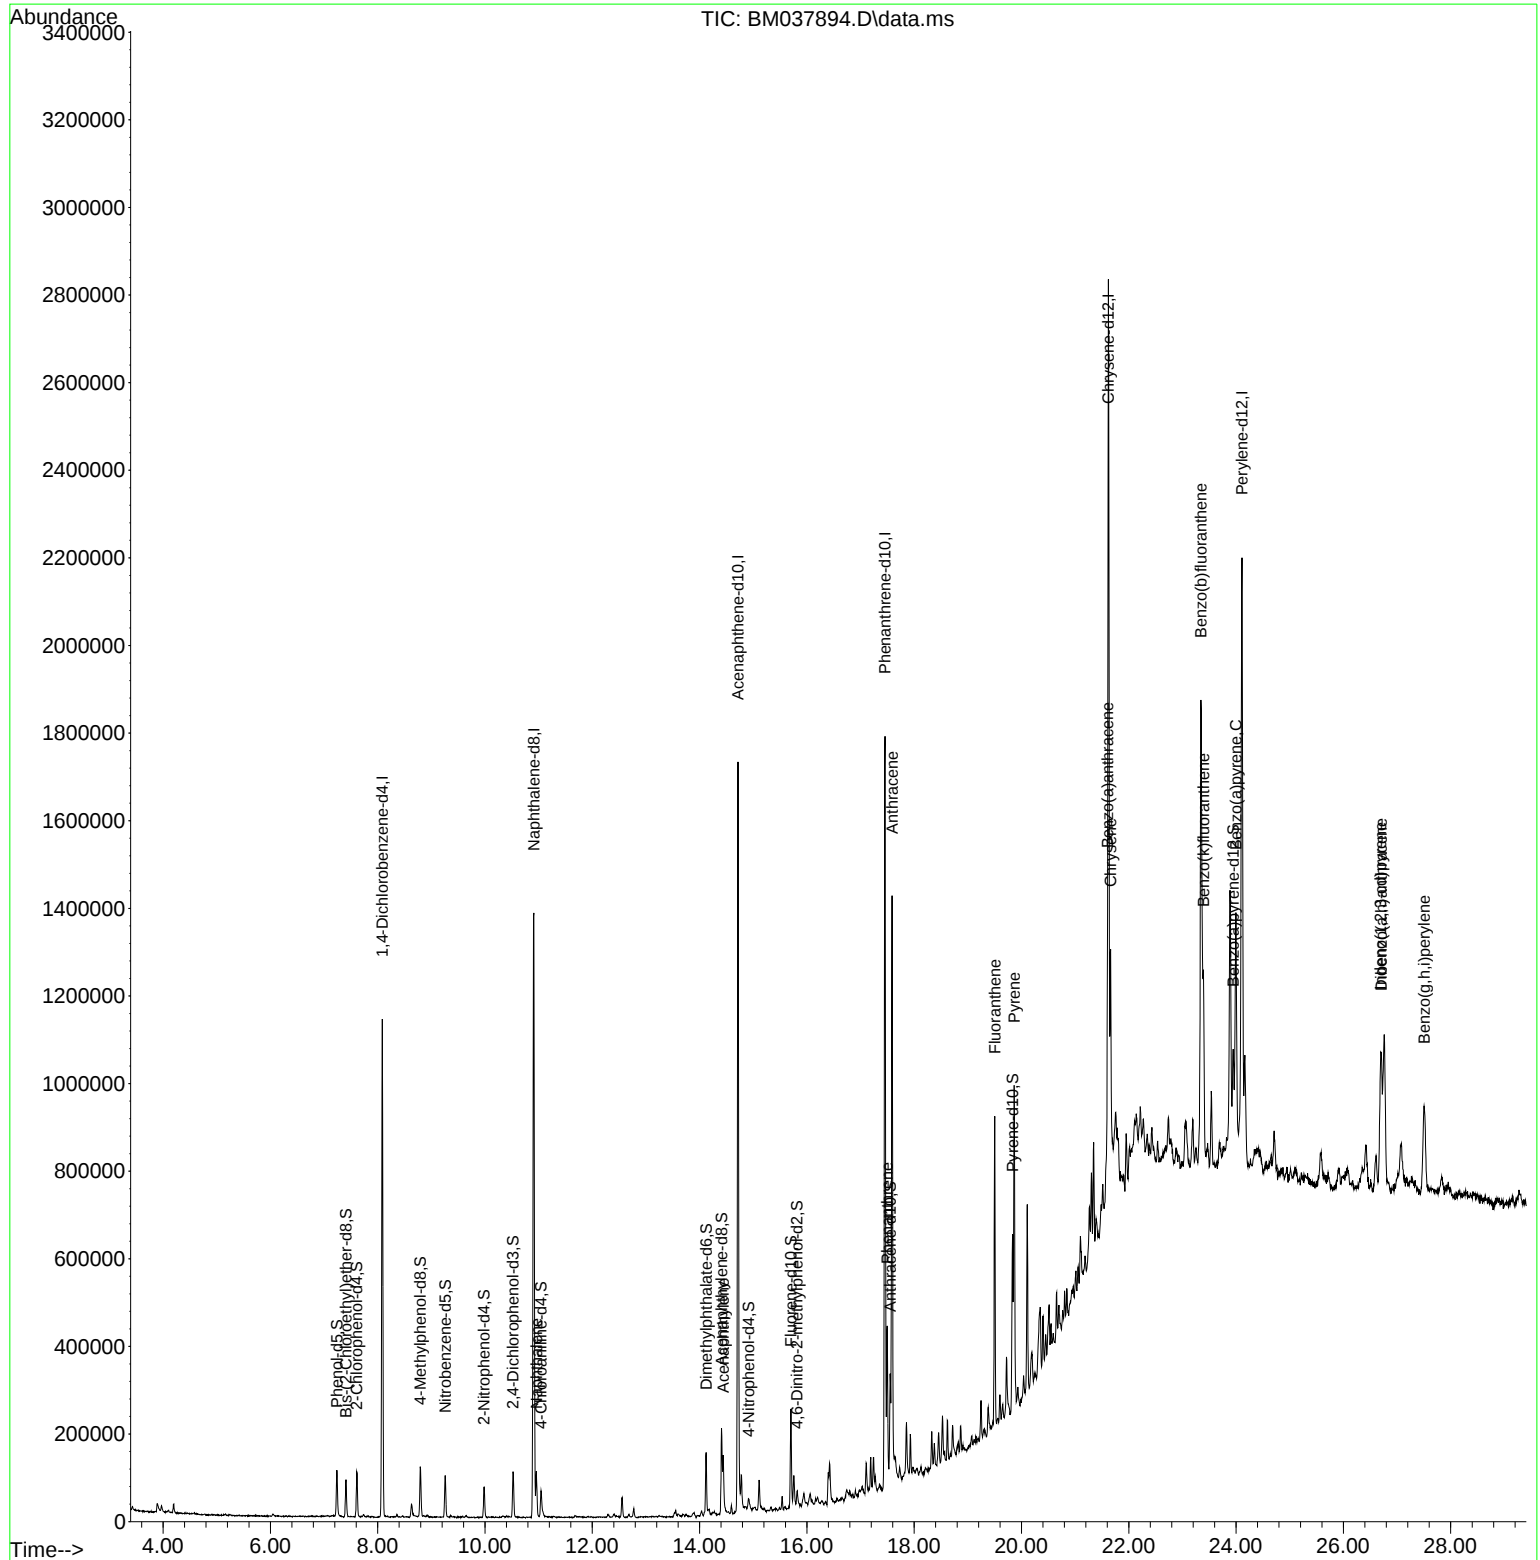







#30
Naphthalene
Concen: 1.275 ng/ul
RT: 10.957 min Scan# 1287
Delta R.T. -0.006 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41

Instrument :
BNA_M
ClientSampleId :
DBXL3

Tgt Ion:128 Resp: 80264
Ion Ratio Lower Upper
128 100
129 11.9 9.0 13.4
127 11.2 10.4 15.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

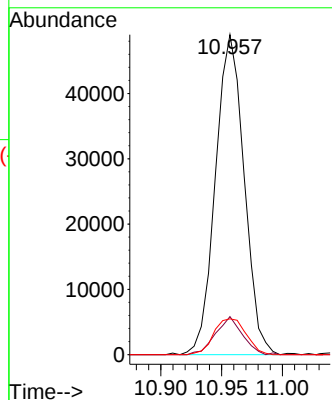

#50
Acenaphthylene
Concen: 1.808 ng/ul
RT: 14.439 min Scan# 1879
Delta R.T. -0.006 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41


Tgt Ion:152 Resp: 104239
Ion Ratio Lower Upper
152 100
151 18.3 15.3 22.9
153 13.1 10.2 15.4

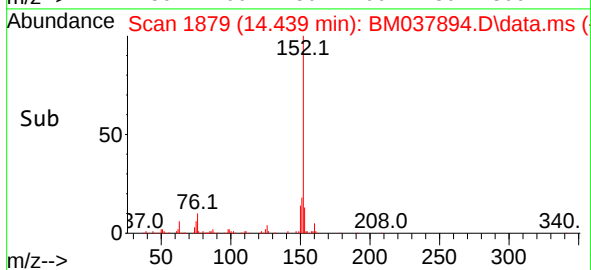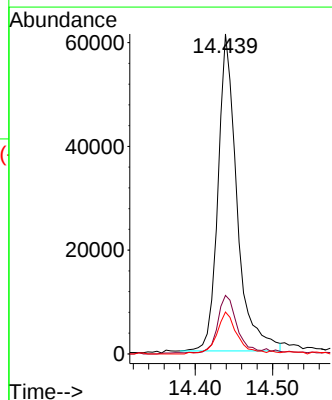



#72
Phenanthrene
Concen: 3.417 ng/ul
RT: 17.498 min Scan# 2399
Delta R.T. -0.000 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41




Instrument :
BNA_M
ClientSampleId :
DBXL3

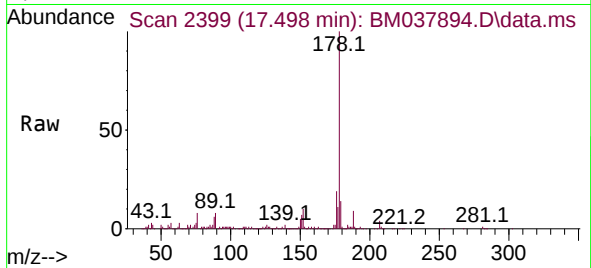

Tgt Ion:178 Resp: 207036
Ion Ratio Lower Upper
178 100
179 14.4 12.2 18.2
176 19.1 15.4 23.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

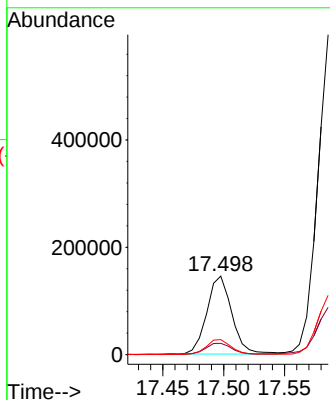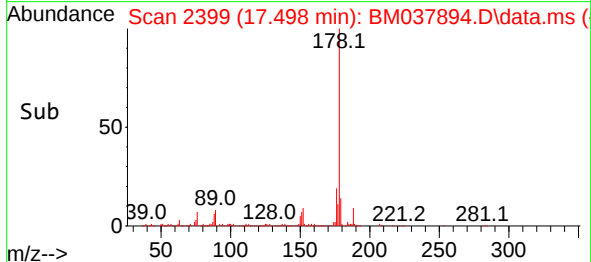

#74
Anthracene
Concen: 13.926 ng/ul
RT: 17.586 min Scan# 2414
Delta R.T. -0.006 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41


Tgt Ion:178 Resp: 857379
Ion Ratio Lower Upper
178 100
179 14.8 11.8 17.8
176 18.6 15.0 22.6

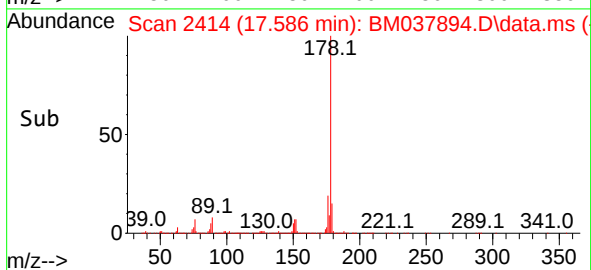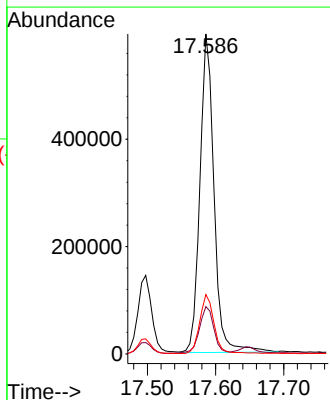



#80
Fluoranthene
Concen: 6.717 ng/ul
RT: 19.503 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41




Instrument :
BNA_M
ClientSampleId :
DBXL3

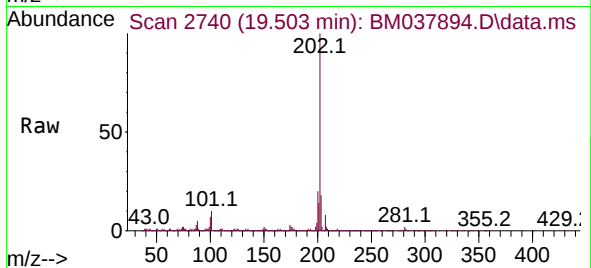


Tgt Ion:202 Resp: 43535
Ion Ratio Lower Upper
202 100
101 9.9 8.6 13.0
100 7.2 6.6 10.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

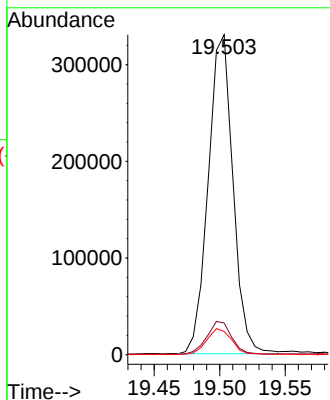


#82
Pyrene
Concen: 6.670 ng/ul
RT: 19.862 min Scan# 2801
Delta R.T. -0.006 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41




Tgt Ion:202 Resp: 449937
Ion Ratio Lower Upper
202 100
101 12.7 10.0 15.0
100 10.3 7.9 11.9

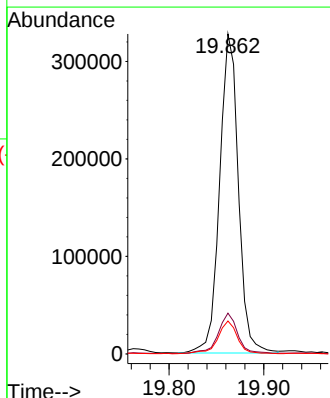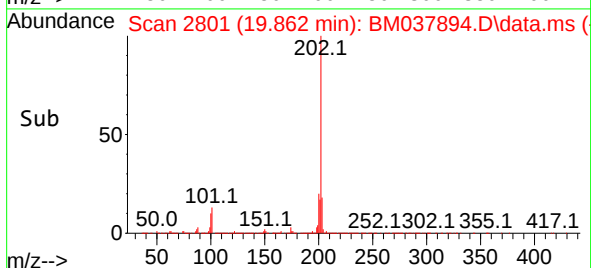



#85
Benzo(a)anthracene
Concen: 4.708 ng/u1
RT: 21.603 min Scan# 3097
Delta R.T. -0.006 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41




Instrument :
BNA_M
ClientSampleId :
DBXL3



Tgt Ion:228 Resp: 289759
Ion Ratio Lower Upper
228 100
229 22.2 15.5 23.3
226 27.5 21.8 32.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

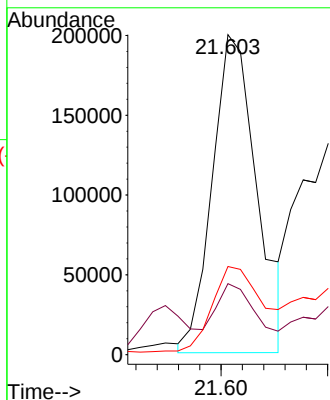

#87
Chrysene
Concen: 6.528 ng/u1
RT: 21.662 min Scan# 3107
Delta R.T. -0.000 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41

Tgt Ion:228 Resp: 376992
Ion Ratio Lower Upper
228 100
226 30.1 24.3 36.5
229 20.6 15.6 23.4

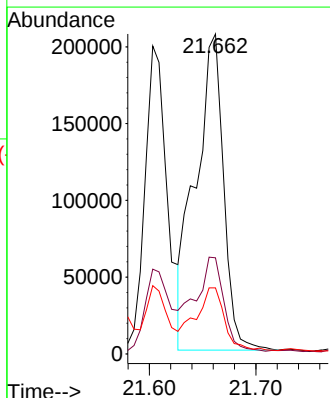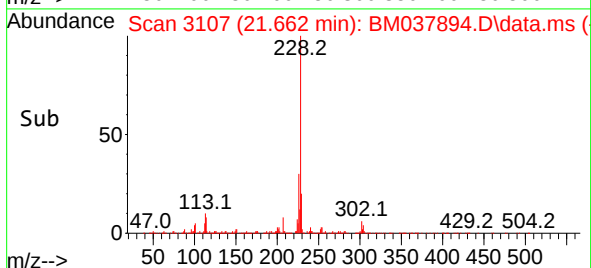







#90
Benzo(b)fluoranthene
Concen: 13.908 ng/ul
RT: 23.344 min Scan# 3393
Delta R.T. -0.000 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41

Instrument :
BNA_M
ClientSampleId :
DBXL3

Tgt Ion:252 Resp: 902508
Ion Ratio Lower Upper
252 100
253 23.0 17.6 26.4
125 10.3 8.0 12.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

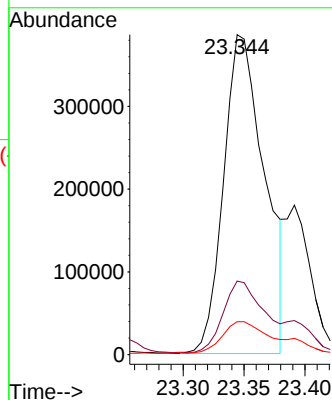

#91
Benzo(k)fluoranthene
Concen: 4.126 ng/ul m
RT: 23.391 min Scan# 3401
Delta R.T. -0.006 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41


Tgt Ion:252 Resp: 259465
Ion Ratio Lower Upper
252 100
253 22.7 17.4 26.2
125 10.9 8.1 12.1

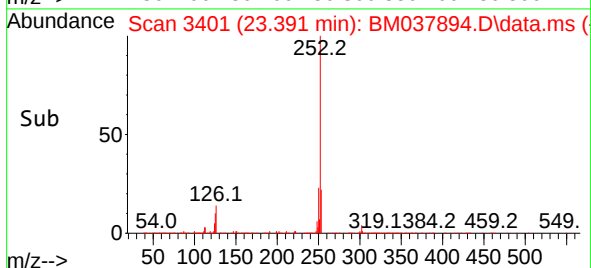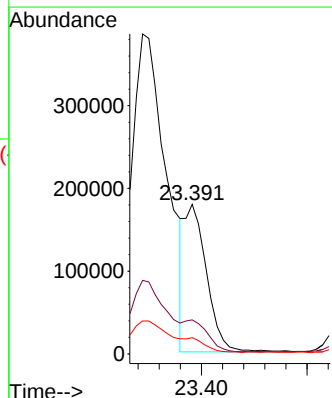



#93
Benzo(a)pyrene
Concen: 6.845 ng/ul
RT: 23.997 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41




Instrument :
BNA_M
ClientSampleId :
DBXL3

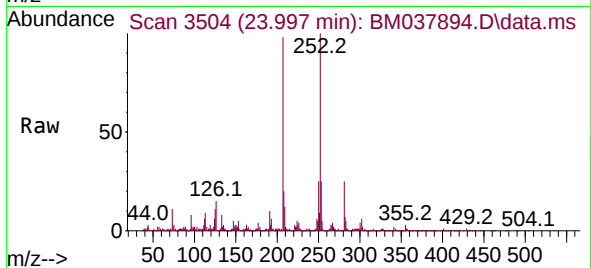


Tgt Ion:252 Resp: 390600
Ion Ratio Lower Upper
252 100
253 24.7 17.4 26.0
125 11.0 9.4 14.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

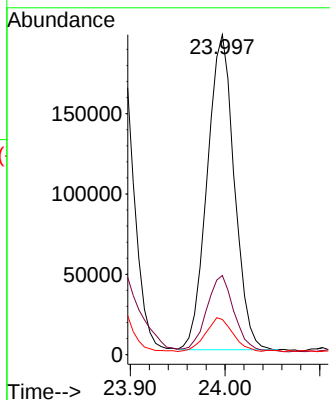


#94
Indeno(1,2,3-cd)pyrene
Concen: 4.923 ng/ul
RT: 26.697 min Scan# 3963
Delta R.T. -0.012 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41



Tgt Ion:276 Resp: 361799
Ion Ratio Lower Upper
276 100
138 23.4 19.3 28.9
277 23.7 19.8 29.8

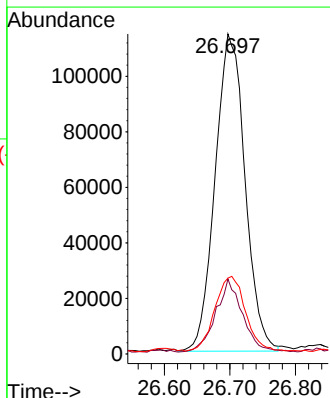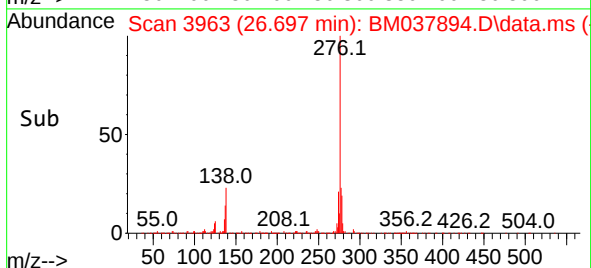

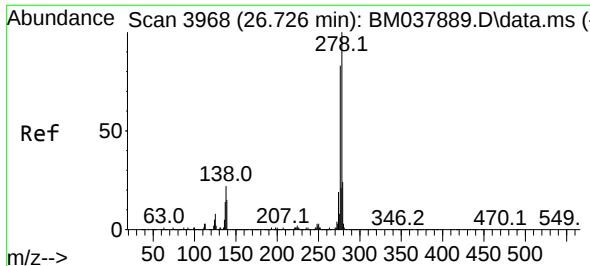





#95
Dibenzo(a,h)anthracene
Concen: 1.470 ng/ul
RT: 26.709 min Scan# 3968
Delta R.T. -0.018 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41

Instrument :
BNA_M
ClientSampleId :
DBXL3

Tgt Ion:278 Resp: 91053
Ion Ratio Lower Upper
278 100
139 20.4 12.4 18.6
279 27.9 19.8 29.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

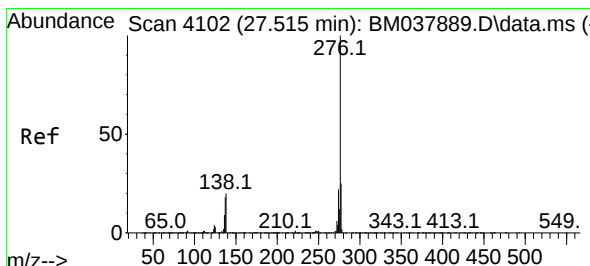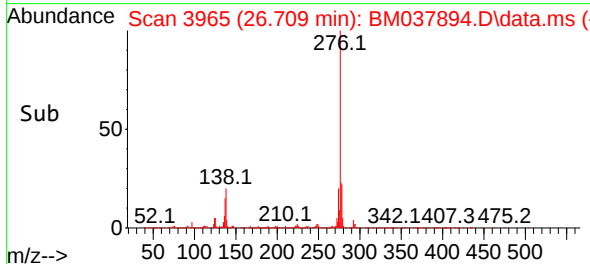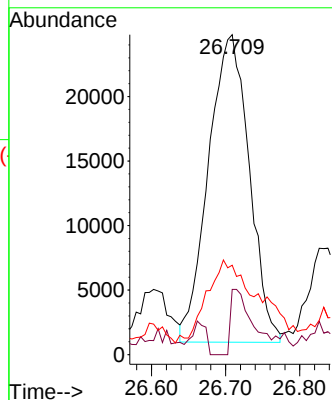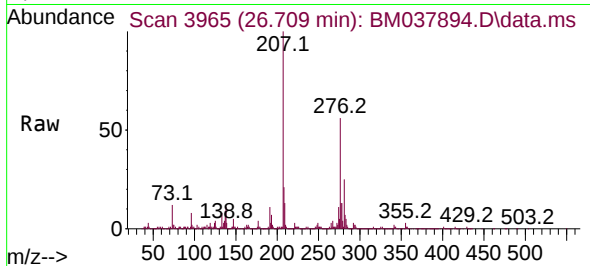

#96
Benzo(g,h,i)perylene
Concen: 4.885 ng/ul
RT: 27.503 min Scan# 4100
Delta R.T. -0.012 min
Lab File: BM037894.D
Acq: 08 Dec 2022 19:41

Tgt Ion:276 Resp: 286618
Ion Ratio Lower Upper
276 100
138 18.8 17.1 25.7
277 25.5 18.2 27.4

