

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037895.D
 Acq On : 08 Dec 2022 20:17
 Operator : CG/JU
 Sample : N5832-19 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXL4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022
 Supervised By :mohammad ahmed 12/10/2022

Quant Time: Dec 08 22:41:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 08 01:49:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.086	152	301256	20.000	ng/u1	0.00
20) Naphthalene-d8	10.910	136	1186850	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.715	164	661602	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.456	188	1245743	20.000	ng/u1	0.00
79) Chrysene-d12	21.621	240	908726	20.000	ng/u1	0.00
88) Perylene-d12	24.109	264	1042693	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	3271	0.493	ng/uL	0.00
4) Pyridine-d5	3.887	84	18550m	0.942	ng/u1	0.02
7) Phenol-d5	7.239	99	52635	2.150	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.410	67	32549	2.184	ng/u1	0.00
11) 2-Chlorophenol-d4	7.616	132	44229	2.202	ng/u1	0.00
15) 4-Methylphenol-d8	8.792	113	39423	2.063	ng/u1	0.00
21) Nitrobenzene-d5	9.257	128	20747	2.208	ng/u1	0.00
24) 2-Nitrophenol-d4	9.986	143	20609	2.093	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.522	165	37290	1.994	ng/u1	0.00
31) 4-Chloroaniline-d4	11.045	131	29009	1.124	ng/u1	0.00
46) Dimethylphthalate-d6	14.121	166	112334	2.382	ng/u1	0.00
49) Acenaphthylene-d8	14.410	160	132744	2.303	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	8613	1.071	ng/u1	0.00
60) Fluorene-d10	15.704	176	103777	2.470	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.815	200	7582	1.138	ng/u1	0.00
73) Anthracene-d10	17.556	188	154079	2.650	ng/u1	0.00
81) Pyrene-d10	19.833	212	147839	2.708	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.944	264	134325	2.579	ng/u1	0.00
Target Compounds					Qvalue	
30) Naphthalene	10.957	128	177960	2.779	ng/u1	100
36) 2-Methylnaphthalene	12.557	142	134207	3.231	ng/u1	96
50) Acenaphthylene	14.439	152	146827	2.316	ng/u1	99
52) Acenaphthene	14.780	153	65507	1.494	ng/u1	95
61) Fluorene	15.757	166	661231	13.545	ng/u1	99
72) Phenanthrene	17.498	178	2053561	30.186	ng/u1	100
74) Anthracene	17.598	178	12381867	179.095	ng/u1	97
80) Fluoranthene	19.503	202	2831818	43.956	ng/u1	99
82) Pyrene	19.868	202	3364598	50.182	ng/u1	99
85) Benzo(a)anthracene	21.609	228	888463	14.522	ng/u1	99
87) Chrysene	21.662	228	1245964	21.706	ng/u1	98
90) Benzo(b)fluoranthene	23.350	252	1633926	25.276	ng/u1	99
91) Benzo(k)fluoranthene	23.391	252	482564m	7.703	ng/u1	
93) Benzo(a)pyrene	23.997	252	700224	12.318	ng/u1	97
94) Indeno(1,2,3-cd)pyrene	26.697	276	460419	6.289	ng/u1	97
95) Dibenzo(a,h)anthracene	26.703	278	121417	1.967	ng/u1#	85
96) Benzo(g,h,i)perylene	27.503	276	358922	6.140	ng/u1	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037895.D
Acq On : 08 Dec 2022 20:17
Operator : CG/JU
Sample : N5832-19 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBXL4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022


Quant Time: Dec 08 22:41:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 08 01:49:06 2022
Response via : Initial Calibration

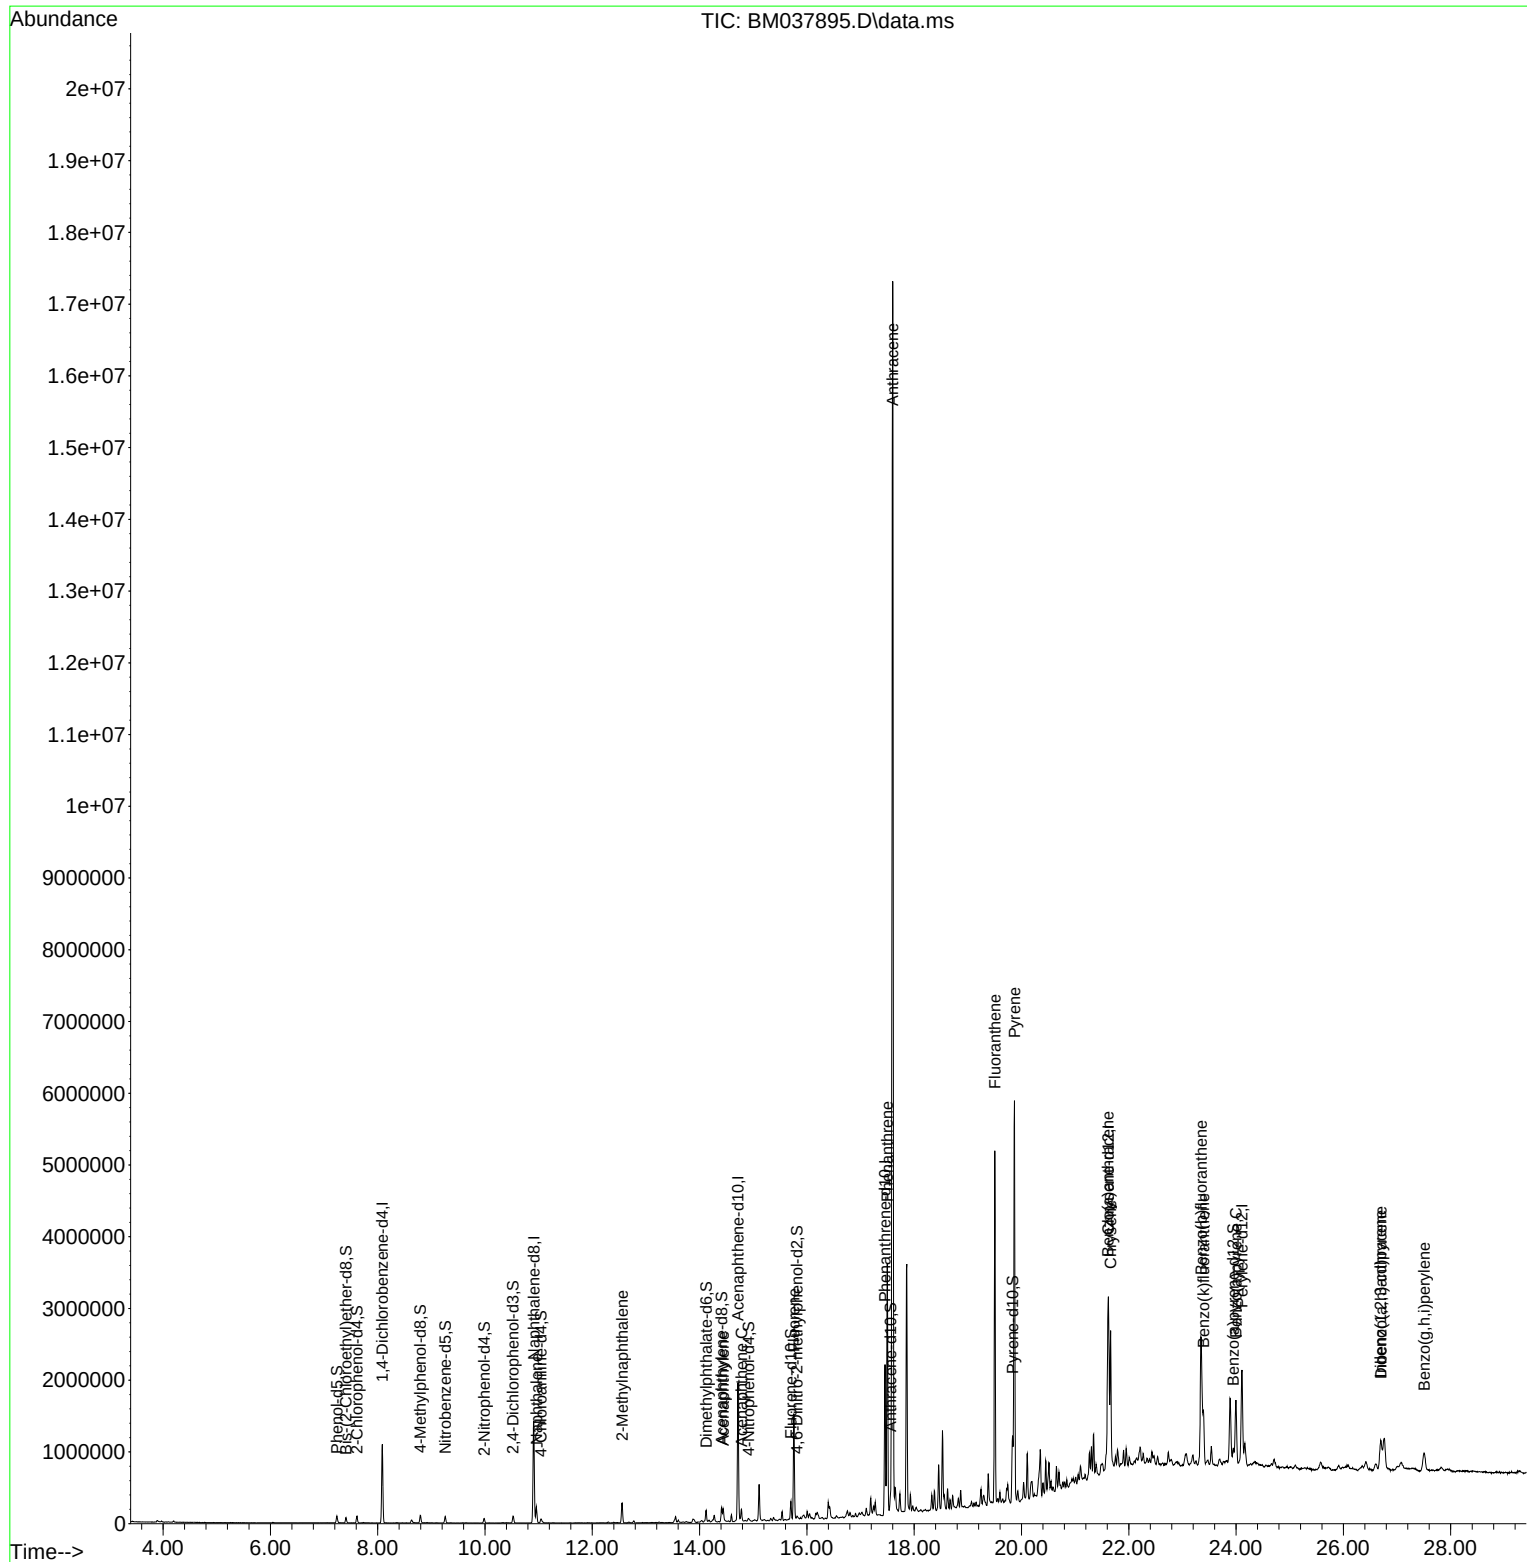



#30
Naphthalene
Concen: 2.779 ng/ul
RT: 10.957 min Scan# 1287
Delta R.T. -0.006 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17




Instrument :
BNA_M
ClientSampleId :
DBXL4



Tgt Ion:128 Resp: 177960
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.4
127 13.0 10.4 15.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

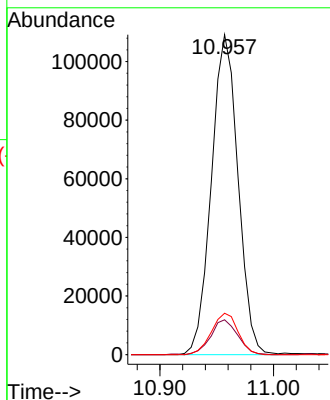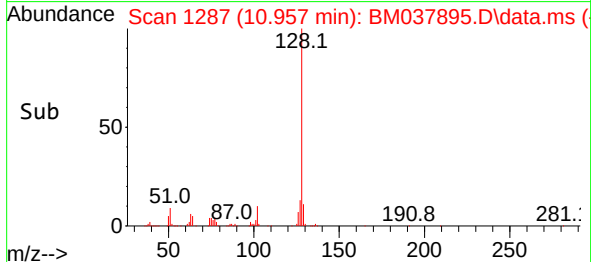

#36
2-Methylnaphthalene
Concen: 3.231 ng/ul
RT: 12.557 min Scan# 1559
Delta R.T. -0.000 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17


Tgt Ion:142 Resp: 134207
Ion Ratio Lower Upper
142 100
141 90.1 69.4 104.0

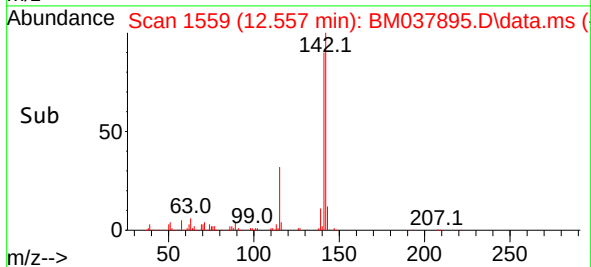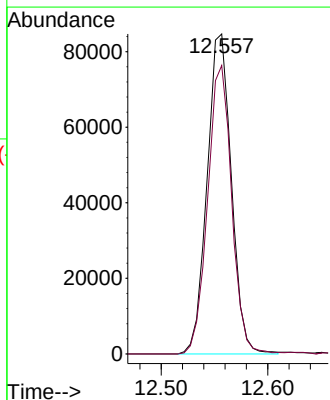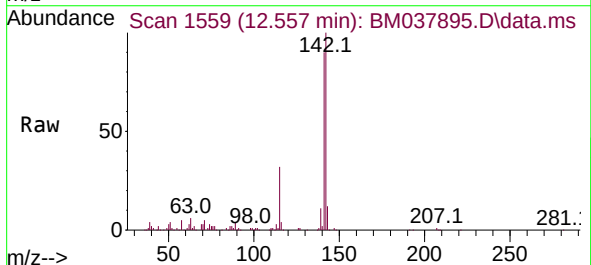

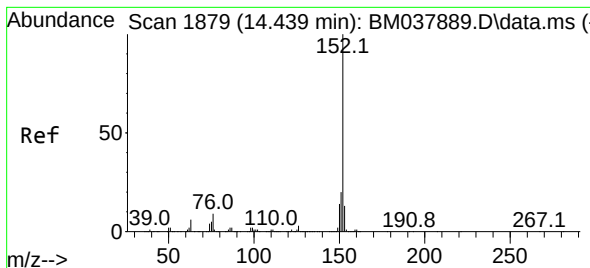

#50
Acenaphthylene
Concen: 2.316 ng/ul
RT: 14.439 min Scan# 1879
Delta R.T. -0.006 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17




Instrument :
BNA_M
ClientSampleId :
DBXL4

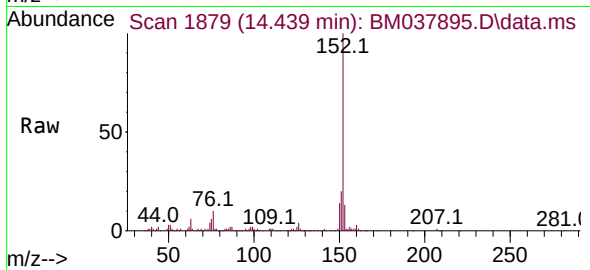


Tgt Ion:152 Resp: 146827
Ion Ratio Lower Upper
152 100
151 19.7 15.3 22.9
153 12.9 10.2 15.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

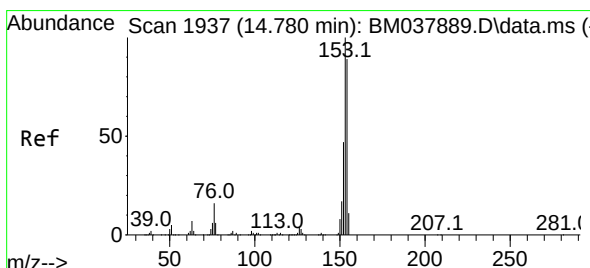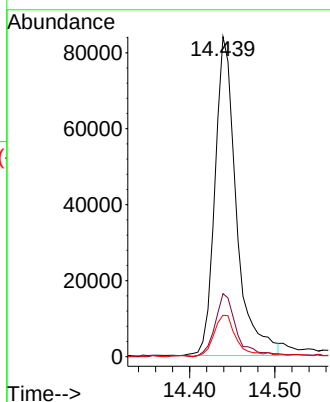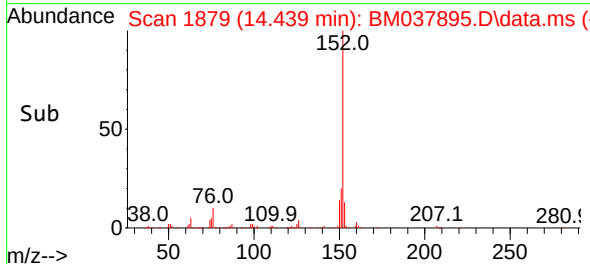


#52
Acenaphthene
Concen: 1.494 ng/ul
RT: 14.780 min Scan# 1937
Delta R.T. -0.000 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17

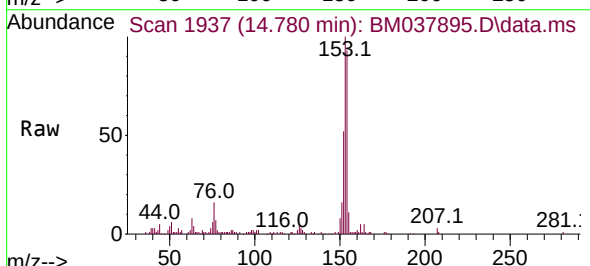

Tgt Ion:153 Resp: 65507
Ion Ratio Lower Upper
153 100
152 51.5 38.2 57.4
154 93.3 71.4 107.0

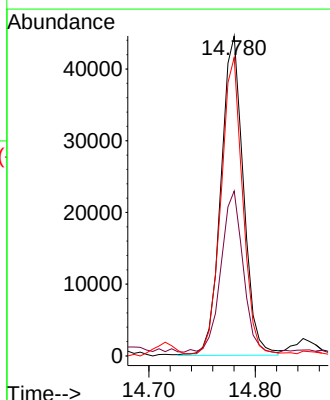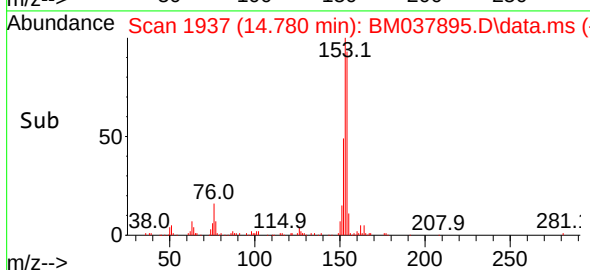



#61

Fluorene

Concen: 13.545 ng/ul

RT: 15.757 min Scan# 2104

Delta R.T. -0.006 min

Lab File: BM037895.D

Acq: 08 Dec 2022 20:17

Instrument :

BNA_M

ClientSampleId :

DBXL4

Tgt Ion:166 Resp: 661231

Ion Ratio Lower Upper

166 100





165 97.8 77.2 115.8

167 13.1 10.4 15.6

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

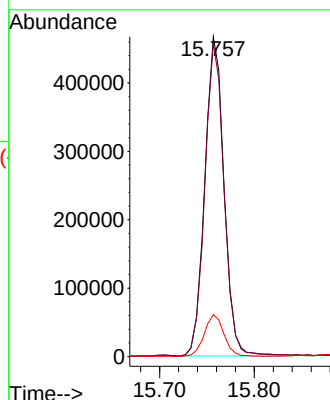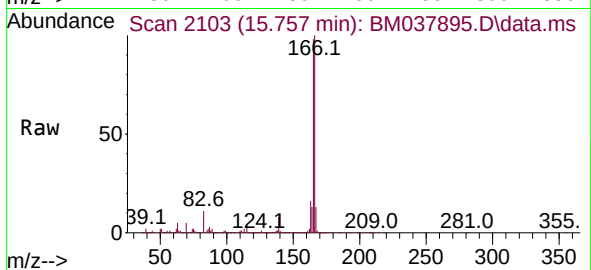

#72

Phenanthrene

Concen: 30.186 ng/ul

RT: 17.498 min Scan# 2399

Delta R.T. -0.000 min

Lab File: BM037895.D

Acq: 08 Dec 2022 20:17




Tgt Ion:178 Resp: 2053561


Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.2


176 19.1 15.4 23.0

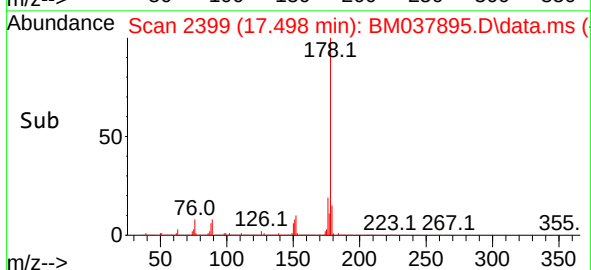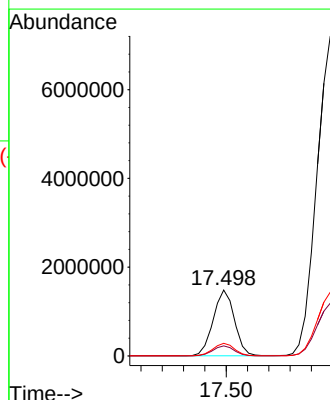



#74
 Anthracene
 Concen: 179.095 ng/u1
 RT: 17.598 min Scan# 2416
 Delta R.T. 0.006 min
 Lab File: BM037895.D
 Acq: 08 Dec 2022 20:17




Instrument :
 BNA_M
 ClientSampleId :
 DBXL4




Tgt Ion:178 Resp:1238186
 Ion Ratio Lower Upper
 178 100
 179 16.5 11.8 17.8
 176 19.9 15.0 22.6

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 12/09/2022
 Supervised By :mohammad ahmed 12/10/2022

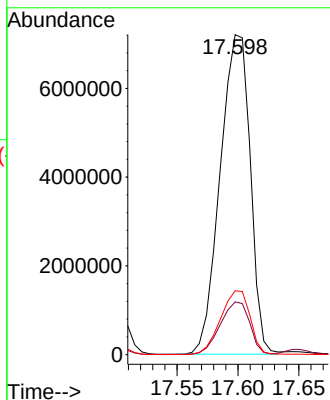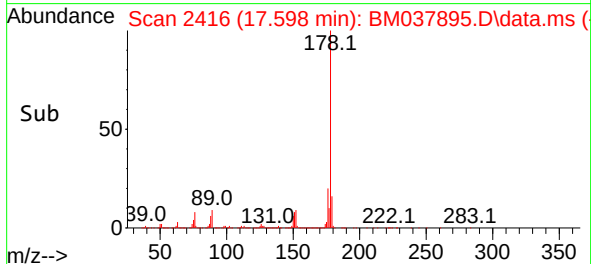


#80
 Fluoranthene
 Concen: 43.956 ng/u1
 RT: 19.503 min Scan# 2740
 Delta R.T. -0.000 min
 Lab File: BM037895.D
 Acq: 08 Dec 2022 20:17

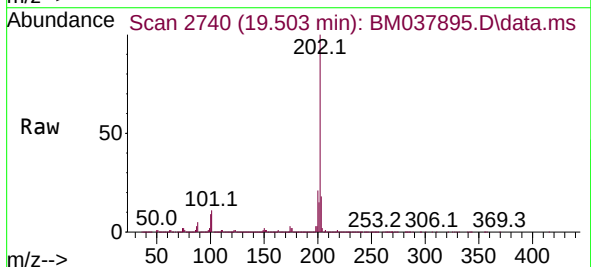


Tgt Ion:202 Resp: 2831818
 Ion Ratio Lower Upper
 202 100
 101 11.1 8.6 13.0
 100 8.6 6.6 10.0

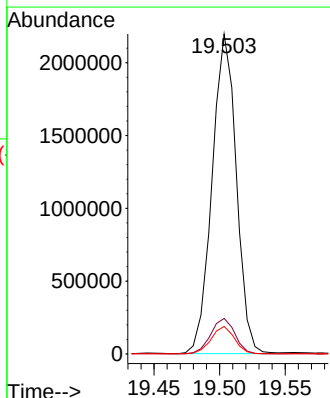



#82
Pyrene
Concen: 50.182 ng/ul
RT: 19.868 min Scan# 2802
Delta R.T. -0.000 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17




Instrument :
BNA_M
ClientSampleId :
DBXL4



Tgt Ion:202 Resp: 3364598
Ion Ratio Lower Upper
202 100
101 12.4 10.0 15.0
100 10.4 7.9 11.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

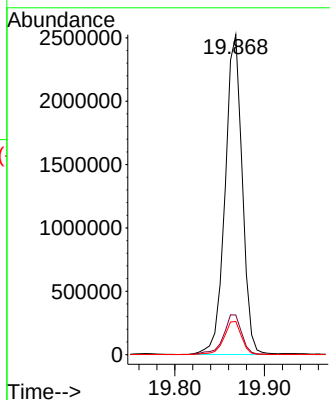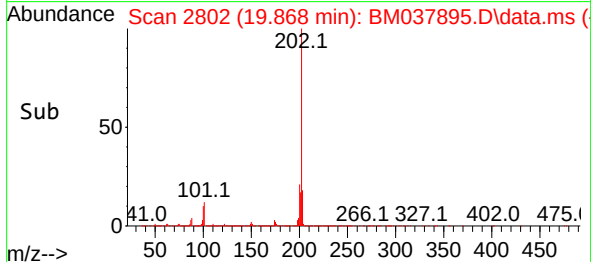

#85
Benzo(a)anthracene
Concen: 14.522 ng/ul
RT: 21.609 min Scan# 3098
Delta R.T. -0.000 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17


Tgt Ion:228 Resp: 888463
Ion Ratio Lower Upper
228 100
229 20.8 15.5 23.3
226 27.4 21.8 32.8

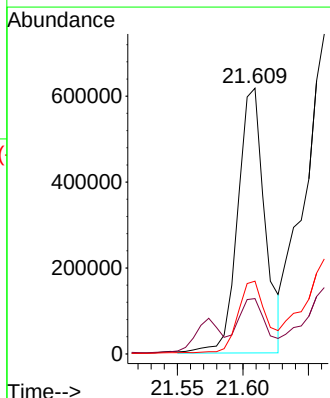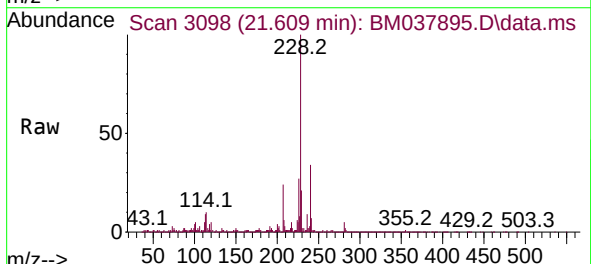



#87
Chrysene
Concen: 21.706 ng/ul
RT: 21.662 min Scan# 3107
Delta R.T. -0.000 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17




Instrument :
BNA_M
ClientSampleId :
DBXL4



Tgt Ion:228 Resp: 1245964
Ion Ratio Lower Upper
228 100
226 29.7 24.3 36.5
229 20.7 15.6 23.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

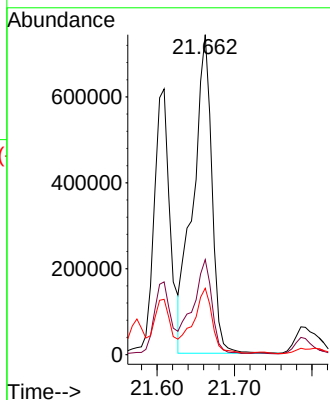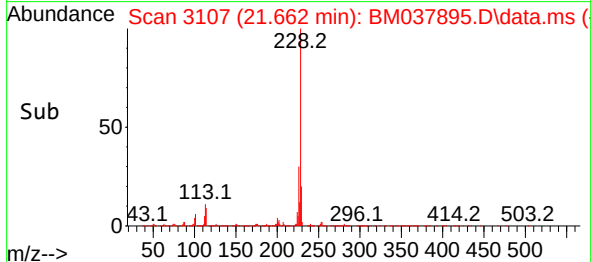

#90
Benzo(b)fluoranthene
Concen: 25.276 ng/ul
RT: 23.350 min Scan# 3394
Delta R.T. 0.006 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17

Tgt Ion:252 Resp: 1633926
Ion Ratio Lower Upper
252 100
253 22.6 17.6 26.4
125 10.4 8.0 12.0

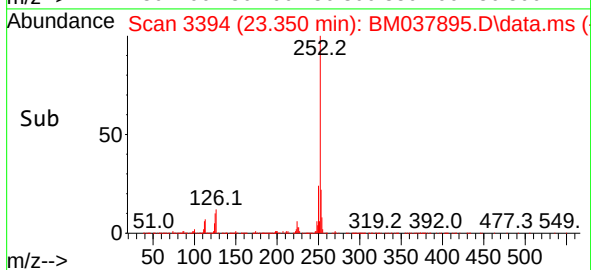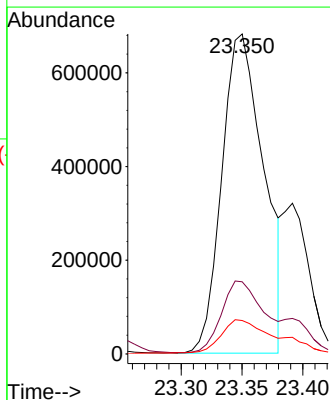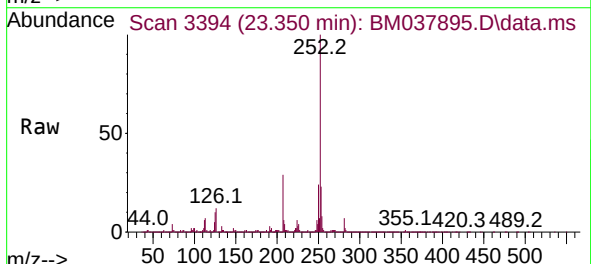







#91
Benzo(k)fluoranthene
Concen: 7.703 ng/ul m
RT: 23.391 min Scan# 3402
Delta R.T. -0.006 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17

Instrument :
BNA_M
ClientSampleId :
DBXL4

Tgt Ion:252 Resp: 482564
Ion Ratio Lower Upper
252 100
253 23.5 17.4 26.2
125 11.1 8.1 12.1




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

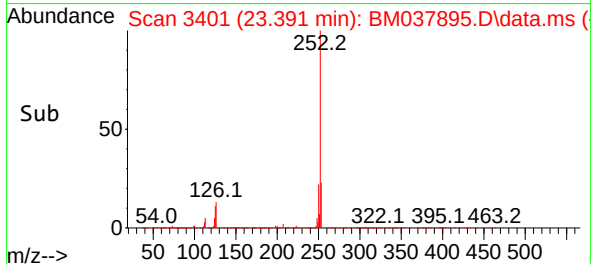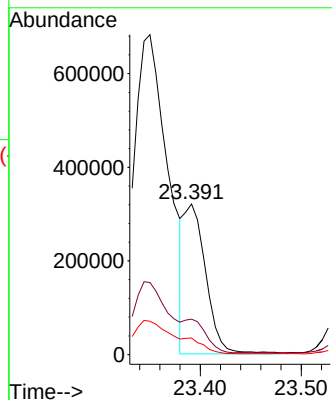

#93
Benzo(a)pyrene
Concen: 12.318 ng/ul
RT: 23.997 min Scan# 3504
Delta R.T. -0.000 min
Lab File: BM037895.D
Acq: 08 Dec 2022 20:17

Tgt Ion:252 Resp: 700224
Ion Ratio Lower Upper
252 100
253 23.5 17.4 26.0
125 10.9 9.4 14.0

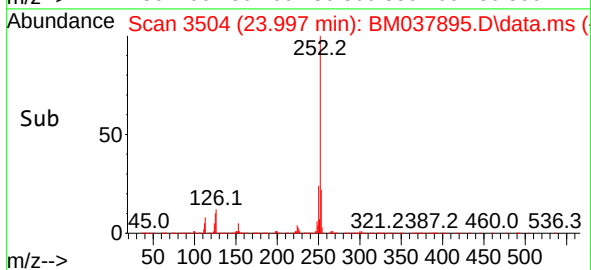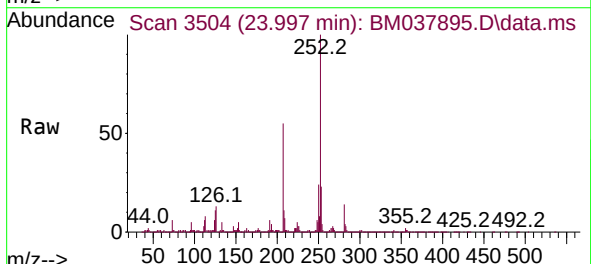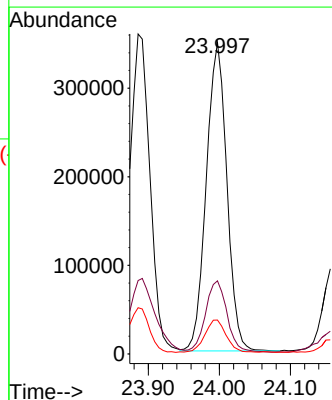



#94

Indeno(1,2,3-cd)pyrene

Concen: 6.289 ng/ul

RT: 26.697 min Scan# 3963

Delta R.T. -0.012 min

Lab File: BM037895.D

Acq: 08 Dec 2022 20:17

Instrument :

BNA_M

ClientSampleId :





DBXL4

Tgt Ion:	276	Resp:	460419
Ion Ratio	Lower	Upper	
276	100		
138	21.5	19.3	28.9
277	25.4	19.8	29.8

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022
Supervised By :mohammad ahmed 12/10/2022

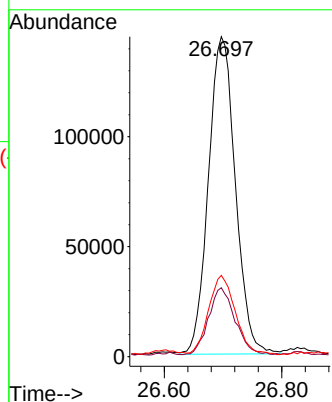

#95

Dibenzo(a,h)anthracene

Concen: 1.967 ng/ul




RT: 26.703 min Scan# 3964


Delta R.T. -0.024 min

Lab File: BM037895.D

Acq: 08 Dec 2022 20:17

Tgt Ion:	278	Resp:	121417
Ion Ratio	Lower	Upper	
278	100		
139	28.0	12.4	18.6#
279	27.9	19.8	29.6

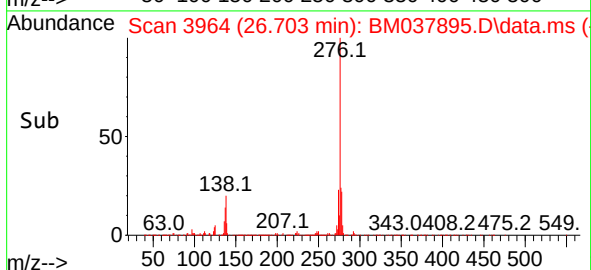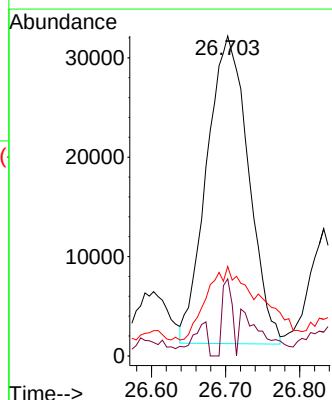



#96

Benzo(g,h,i)perylene

Concen: 6.140 ng/ul

RT: 27.503 min Scan# 41

Delta R.T. -0.012 min

Lab File: BM037895.D


Acq: 08 Dec 2022 20:17

Instrument :

BNA_M

ClientSampleId :

DBXL4



Tgt Ion:276 Resp: 35892

Ion Ratio Lower Upper

276 100

138 20.2 17.1 25.7

277 23.4 18.2 27.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/09/2022

Supervised By :mohammad ahmed 12/10/2022

