

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037877.D
 Acq On : 08 Dec 2022 09:08
 Operator : CG/JU
 Sample : PB149447BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037877.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	3	6	14	rVB	52119	74297	2.58%	0.201%
2	3.863	77	81	96	rBV	625130	994956	34.55%	2.695%
3	4.199	134	138	144	rVB5	15502	24857	0.86%	0.067%
4	5.257	316	318	322	rVB5	2634	3477	0.12%	0.009%
5	6.869	590	592	595	rBV3	2670	3039	0.11%	0.008%
6	7.240	648	655	664	rBV	766928	1166733	40.52%	3.161%
7	7.410	674	684	693	rBV	607367	934122	32.44%	2.531%
8	7.551	705	708	710	rBV4	2437	3016	0.10%	0.008%
9	7.610	712	718	728	rVV	762579	1190584	41.34%	3.225%
10	8.087	791	799	809	rVB	709702	1107423	38.46%	3.000%
11	8.210	814	820	824	rVB8	2346	5297	0.18%	0.014%
12	8.293	831	834	838	rVB5	2274	3471	0.12%	0.009%
13	8.793	913	919	935	rBV	881263	1391855	48.33%	3.771%
14	9.257	990	998	1007	rBV	718332	1140569	39.61%	3.090%
15	9.392	1020	1021	1025	rBV4	2704	3425	0.12%	0.009%
16	9.557	1044	1049	1050	rBV4	3082	4075	0.14%	0.011%
17	9.763	1083	1084	1087	rBV3	2919	3091	0.11%	0.008%
18	9.981	1114	1121	1130	rBV	536688	888505	30.85%	2.407%
19	10.039	1130	1131	1138	rVB6	4655	6212	0.22%	0.017%
20	10.522	1206	1213	1229	rBV	838166	1388022	48.20%	3.760%
21	10.622	1229	1230	1235	rVB5	2893	3312	0.12%	0.009%
22	10.904	1271	1278	1287	rVB	959637	1558962	54.14%	4.223%
23	11.045	1293	1302	1315	rBV	791698	1398436	48.56%	3.789%
24	11.875	1438	1443	1446	rBV6	1980	3858	0.13%	0.010%
25	12.157	1486	1491	1493	rVB6	2317	3392	0.12%	0.009%
26	12.481	1542	1546	1552	rVB3	16487	23857	0.83%	0.065%
27	13.275	1678	1681	1684	rBV4	2292	3446	0.12%	0.009%
28	14.122	1818	1825	1838	rBV	1252960	1730854	60.10%	4.689%
29	14.410	1868	1874	1890	rBV	1552142	2268346	78.77%	6.145%
30	14.716	1919	1926	1936	rBV	1272970	1844408	64.05%	4.997%
31	14.904	1952	1958	1979	rBV	308949	648561	22.52%	1.757%
32	15.127	1991	1996	1999	rVB7	4098	6277	0.22%	0.017%
33	15.463	2050	2053	2056	rBV5	2401	3304	0.11%	0.009%
34	15.498	2056	2059	2060	rVV3	3582	3074	0.11%	0.008%
35	15.527	2060	2064	2066	rVB5	2041	2885	0.10%	0.008%
36	15.704	2087	2094	2107	rBV	1838213	2651330	92.07%	7.183%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037877.D
 Acq On : 08 Dec 2022 09:08
 Operator : CG/JU
 Sample : PB149447BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	15.816	2107	2113	2126	rVV	327246	521606	18.11%	1.413%
38	15.898	2126	2127	2130	rVV3	6499	5899	0.20%	0.016%
39	15.939	2130	2134	2138	rVB6	8909	14690	0.51%	0.040%
40	16.092	2158	2160	2163	rVB3	4052	2987	0.10%	0.008%
41	16.139	2165	2168	2170	rBV4	2267	2978	0.10%	0.008%
42	16.233	2182	2184	2187	rBV3	3141	4417	0.15%	0.012%
43	16.480	2222	2226	2229	rBV5	2590	4074	0.14%	0.011%
44	16.910	2297	2299	2304	rVB4	5834	4381	0.15%	0.012%
45	17.227	2351	2353	2355	rBV3	2894	3167	0.11%	0.009%
46	17.451	2385	2391	2402	rBV	1271453	1847915	64.17%	5.006%
47	17.551	2402	2408	2420	rVV2	1799868	2587763	89.86%	7.011%
48	18.257	2526	2528	2529	rBV2	3702	3015	0.10%	0.008%
49	19.392	2719	2721	2726	rVB4	17848	24555	0.85%	0.067%
50	19.468	2731	2734	2740	rVV3	18032	27381	0.95%	0.074%
51	19.833	2790	2796	2808	rBV	2097448	2825260	98.11%	7.654%
52	20.804	2959	2961	2966	rBV2	38163	41261	1.43%	0.112%
53	21.621	3095	3100	3107	rBV	1366776	1777124	61.71%	4.814%
54	23.944	3488	3495	3507	rVB2	1365347	2879720	100.00%	7.802%
55	24.103	3516	3522	3532	rVB2	875795	1842609	63.99%	4.992%




Sum of corrected areas: 36912130

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037877.D
Acq On : 08 Dec 2022 09:08
Operator : CG/JU
Sample : PB149447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

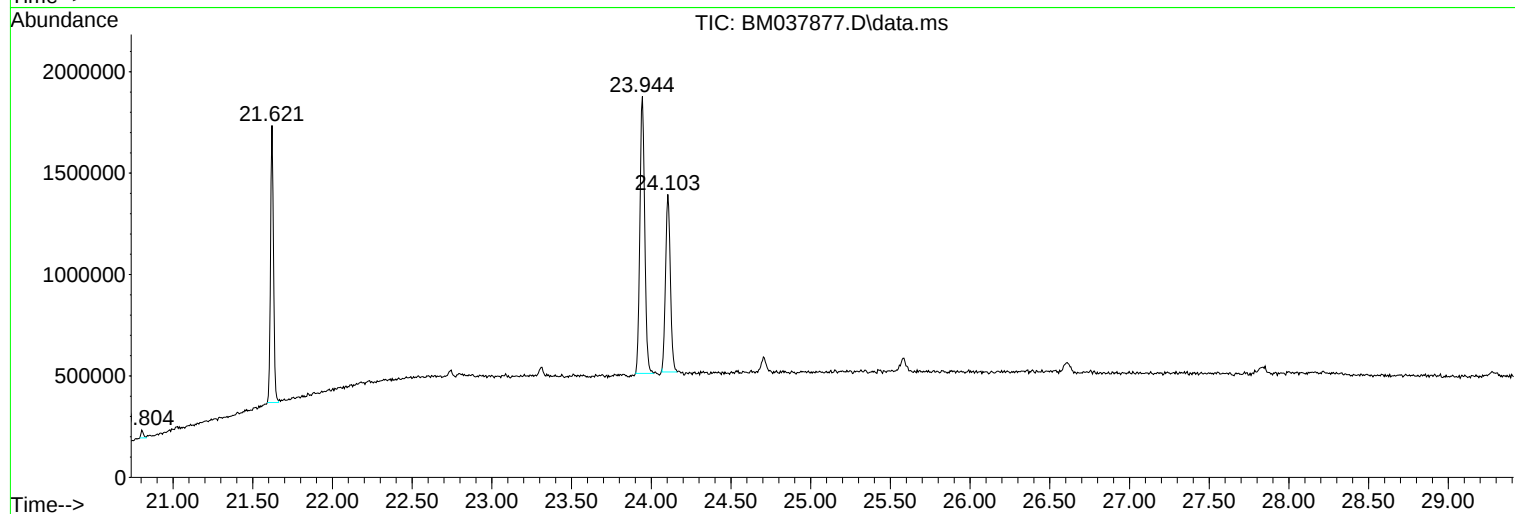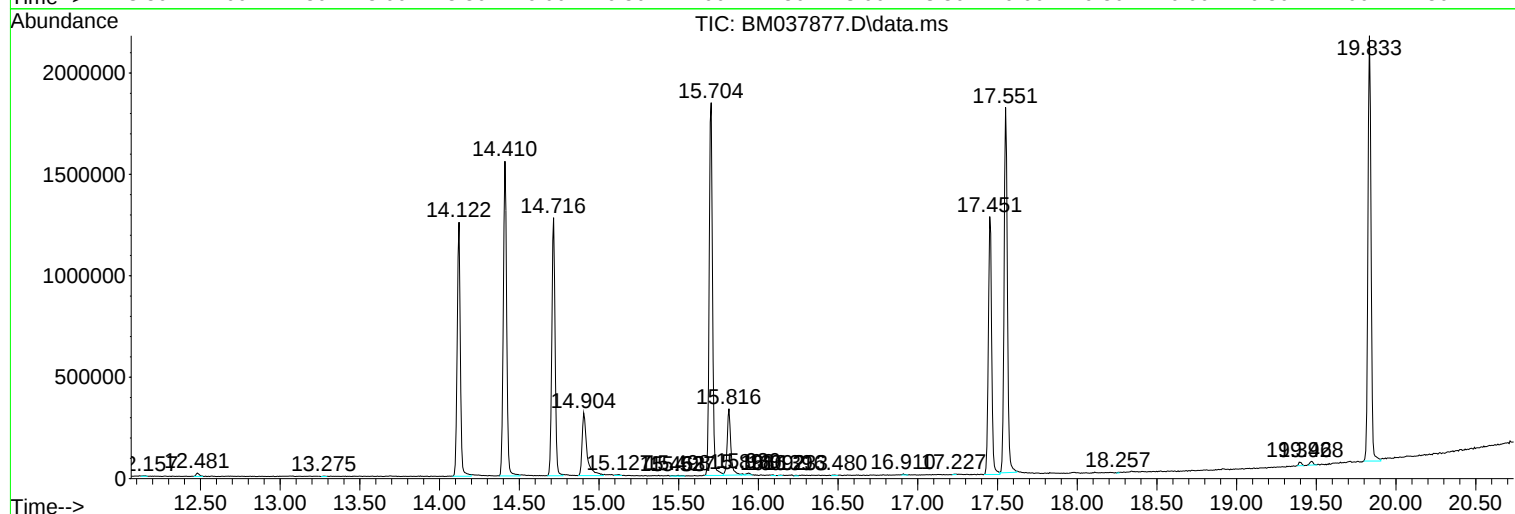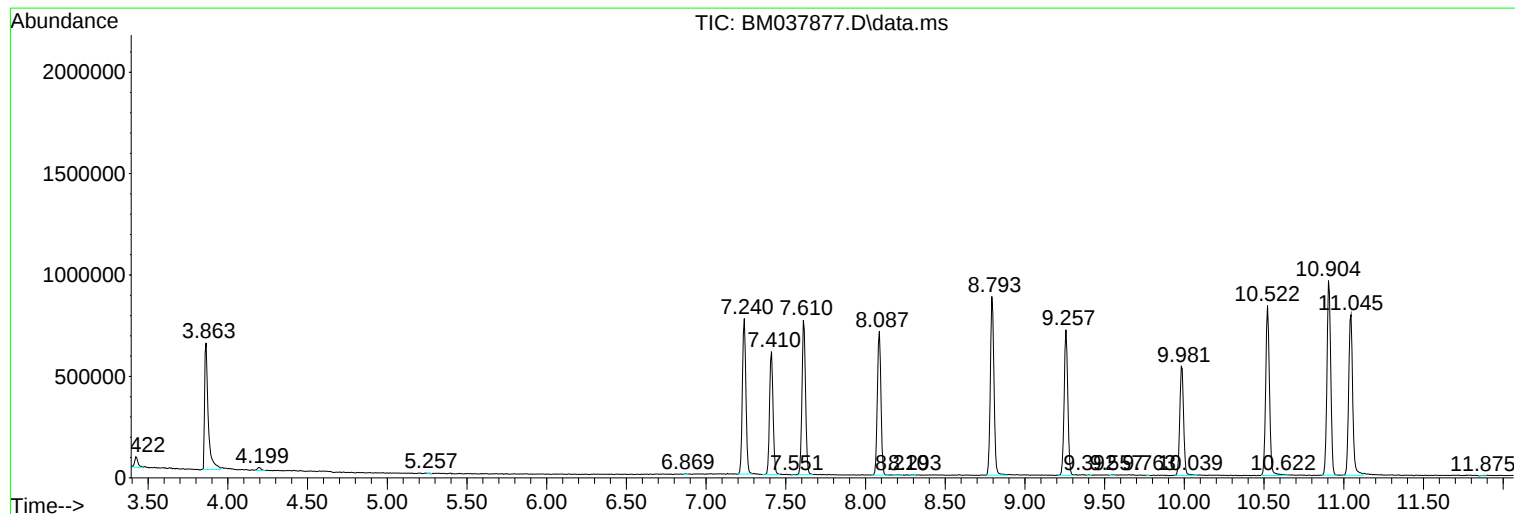

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037877.D
Acq On : 08 Dec 2022 09:08
Operator : CG/JU
Sample : PB149447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037877.D
Acq On : 08 Dec 2022 09:08
Operator : CG/JU
Sample : PB149447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc