

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037878.D
 Acq On : 08 Dec 2022 09:46
 Operator : CG/JU
 Sample : N5738-15MEDL2 150X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBNJ4MEDL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.199	134	138	142	rVB2	11042	15725	0.67%	0.140%
2	5.481	354	356	359	rVB4	2847	2465	0.10%	0.022%
3	5.599	373	376	377	rBV3	2477	2766	0.12%	0.025%
4	6.240	482	485	486	rBV3	2684	3311	0.14%	0.029%
5	6.581	541	543	547	rBV5	2203	3288	0.14%	0.029%
6	6.728	567	568	571	rBV3	2256	2495	0.11%	0.022%
7	7.240	652	655	658	rBV3	4100	3755	0.16%	0.033%
8	7.410	683	684	690	rVB4	4997	6177	0.26%	0.055%
9	7.616	716	719	725	rVB8	4671	7270	0.31%	0.065%
10	8.087	792	799	806	rBV	642464	1001281	42.35%	8.903%
11	8.245	824	826	830	rBV5	1559	2521	0.11%	0.022%
12	8.481	863	866	870	rVB5	2034	2504	0.11%	0.022%
13	8.645	891	894	897	rBV4	2505	3405	0.14%	0.030%
14	9.257	995	998	1001	rBV3	4066	4773	0.20%	0.042%
15	9.481	1034	1036	1040	rBV4	2543	2741	0.12%	0.024%
16	9.587	1052	1054	1057	rVB4	2897	2816	0.12%	0.025%
17	9.639	1060	1063	1064	rVV2	2727	3021	0.13%	0.027%
18	10.339	1179	1182	1183	rVB3	2809	2375	0.10%	0.021%
19	10.910	1272	1279	1289	rVV	751725	1281758	54.21%	11.397%
20	11.951	1453	1456	1461	rBV6	1787	2654	0.11%	0.024%
21	12.110	1480	1483	1485	rBV3	2313	2506	0.11%	0.022%
22	12.133	1485	1487	1491	rVB4	2346	2867	0.12%	0.025%
23	12.416	1532	1535	1538	rVV4	1932	2909	0.12%	0.026%
24	12.592	1563	1565	1570	rVB6	1813	2671	0.11%	0.024%
25	12.922	1618	1621	1624	rVB4	3224	4303	0.18%	0.038%
26	12.963	1624	1628	1629	rBV3	1979	2455	0.10%	0.022%
27	14.039	1809	1811	1816	rVB5	1691	2639	0.11%	0.023%
28	14.104	1820	1822	1823	rVV2	2631	2583	0.11%	0.023%
29	14.122	1823	1825	1828	rVV3	4616	5800	0.25%	0.052%
30	14.198	1835	1838	1841	rBV4	2420	2586	0.11%	0.023%
31	14.369	1864	1867	1869	rBV4	1909	2482	0.10%	0.022%
32	14.410	1869	1874	1880	rVB2	5471	9417	0.40%	0.084%
33	14.504	1887	1890	1892	rVB4	2345	2563	0.11%	0.023%
34	14.669	1914	1918	1919	rBV4	1831	2654	0.11%	0.024%
35	14.716	1919	1926	1954	rVV	775751	1329441	56.23%	11.820%
36	15.333	2025	2031	2038	rVV	41225	75927	3.21%	0.675%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037878.D
 Acq On : 08 Dec 2022 09:46
 Operator : CG/JU
 Sample : N5738-15MEDL2 150X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GBNJ4MEDL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	15.474	2053	2055	2058	rVB4	2582	2724	0.12%	0.024%
38	15.704	2090	2094	2100	rBV8	5221	9532	0.40%	0.085%
39	16.163	2170	2172	2175	rBV4	1789	2459	0.10%	0.022%
40	16.663	2254	2257	2261	rBV5	3394	4335	0.18%	0.039%
41	16.704	2261	2264	2267	rBV5	1724	2502	0.11%	0.022%
42	16.910	2295	2299	2300	rBV4	2655	3285	0.14%	0.029%
43	17.104	2326	2332	2350	rBV	1506453	2364224	100.00%	21.021%
44	17.457	2385	2392	2405	rBV	950263	1501797	63.52%	13.353%
45	17.751	2441	2442	2445	rBV2	2870	2536	0.11%	0.023%
46	17.980	2478	2481	2485	rBV6	4224	6200	0.26%	0.055%
47	18.015	2485	2487	2490	rVV3	3415	2779	0.12%	0.025%
48	18.057	2492	2494	2499	rVB5	4407	6678	0.28%	0.059%
49	18.127	2505	2506	2509	rBV3	3444	3881	0.16%	0.035%
50	21.621	3095	3100	3106	rBV	1232505	1704389	72.09%	15.154%
51	24.109	3516	3523	3535	rBV2	816238	1818713	76.93%	16.171%




Sum of corrected areas: 11246938

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037878.D
Acq On : 08 Dec 2022 09:46
Operator : CG/JU
Sample : N5738-15MEDL2 150X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBNJ4MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

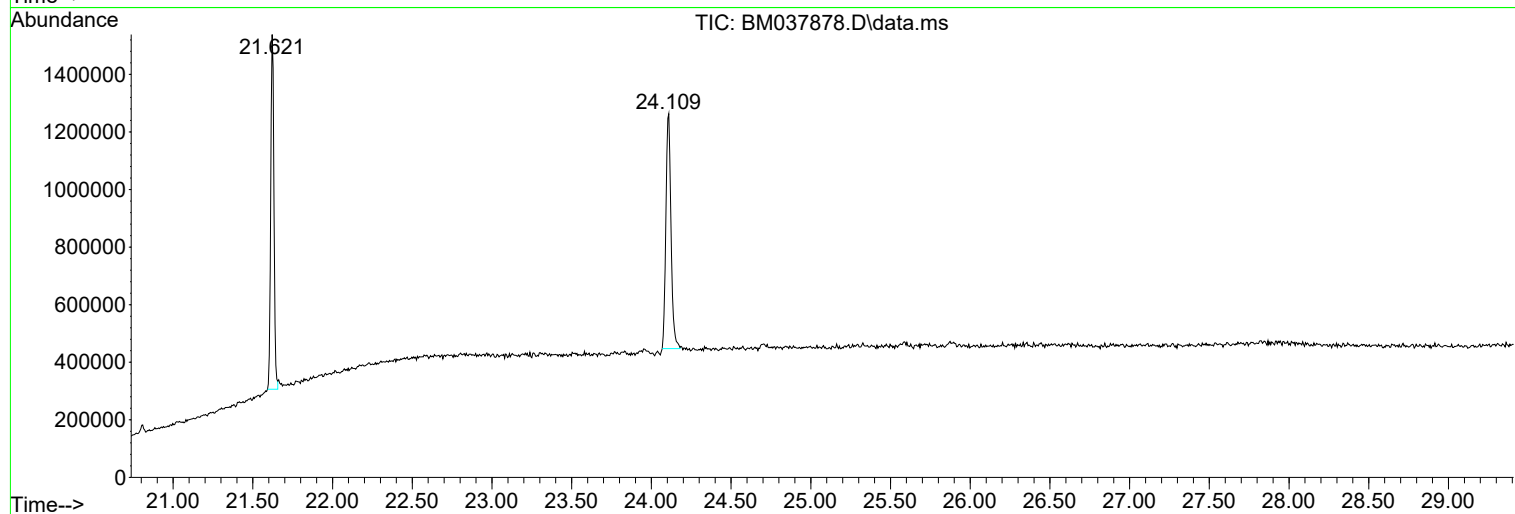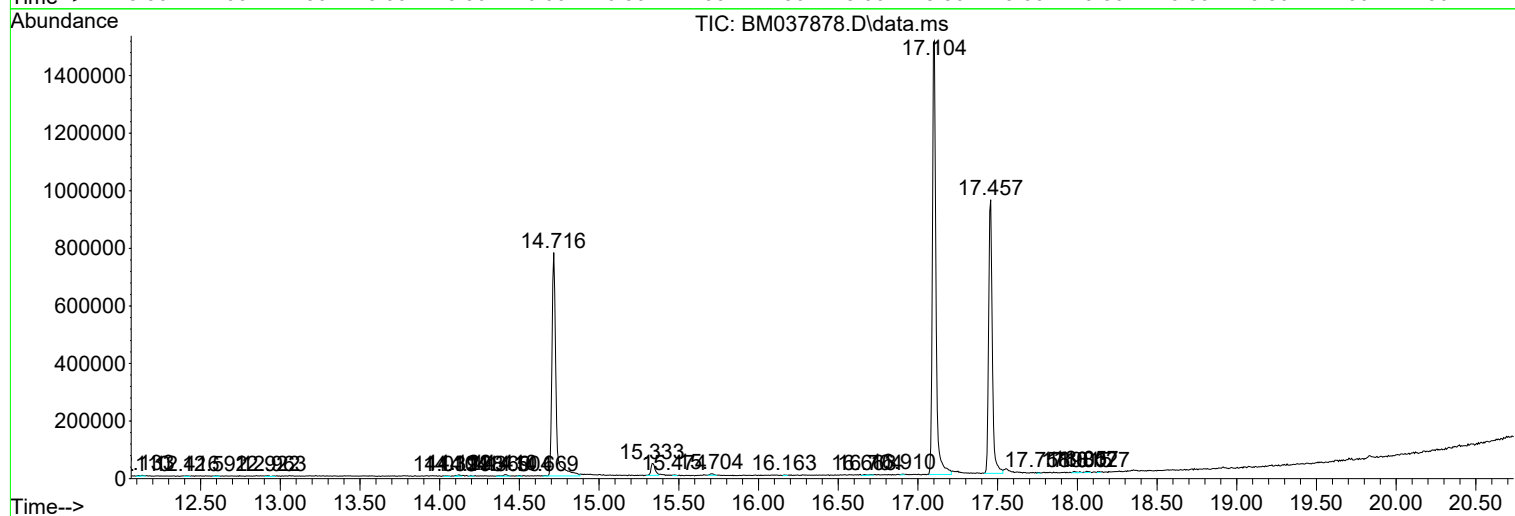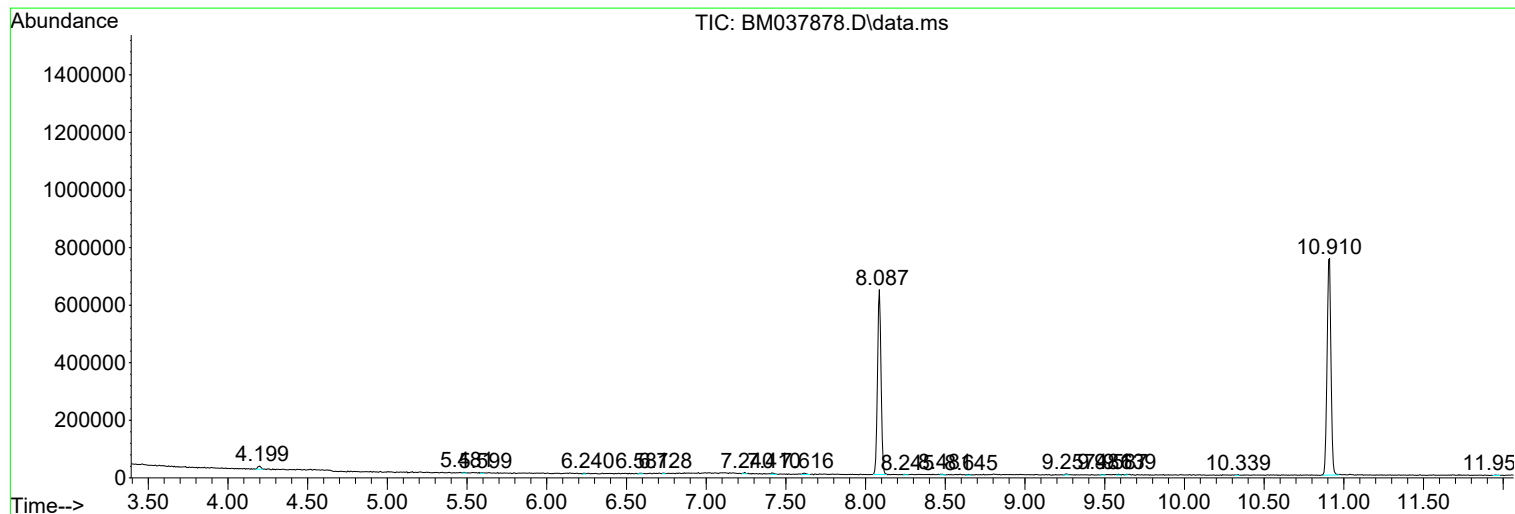

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037878.D
Acq On : 08 Dec 2022 09:46
Operator : CG/JU
Sample : N5738-15MEDL2 150X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBNJ4MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037878.D
Acq On : 08 Dec 2022 09:46
Operator : CG/JU
Sample : N5738-15MEDL2 150X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GBNJ4MEDL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------