

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037890.D
 Acq On : 08 Dec 2022 17:13
 Operator : CG/JU
 Sample : PB149468BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK468

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	3	7	12	rVB	58742	78745	2.32%	0.170%
2	3.499	18	19	22	rBV3	3912	4239	0.13%	0.009%
3	3.863	77	81	98	rBV	769438	1202971	35.51%	2.593%
4	4.199	134	138	142	rVB	21514	28020	0.83%	0.060%
5	4.428	175	177	183	rVB6	2637	3561	0.11%	0.008%
6	4.822	241	244	245	rVB3	4022	3435	0.10%	0.007%
7	5.616	375	379	383	rBV5	2566	4327	0.13%	0.009%
8	7.240	648	655	665	rBV	967010	1503015	44.37%	3.240%
9	7.410	676	684	695	rBV	788835	1186740	35.03%	2.558%
10	7.510	700	701	706	rVB5	2789	3480	0.10%	0.008%
11	7.557	706	709	712	rBV5	2570	4105	0.12%	0.009%
12	7.616	712	719	729	rBV	977345	1537650	45.39%	3.315%
13	8.087	791	799	808	rBV	1071534	1648196	48.66%	3.553%
14	8.669	894	898	900	rBV5	2537	4201	0.12%	0.009%
15	8.798	912	920	934	rBV	1105010	1765720	52.13%	3.806%
16	9.257	990	998	1008	rBV	876125	1439225	42.49%	3.103%
17	9.986	1110	1122	1129	rBV	696649	1152677	34.03%	2.485%
18	10.522	1206	1213	1223	rBV	1012869	1694273	50.02%	3.652%
19	10.910	1271	1279	1287	rBV	1353438	2229726	65.82%	4.807%
20	11.045	1294	1302	1319	rBV	993755	1731679	51.12%	3.733%
21	11.686	1406	1411	1415	rBV8	3590	6891	0.20%	0.015%
22	12.480	1539	1546	1553	rBV2	17853	35532	1.05%	0.077%
23	12.692	1579	1582	1585	rVB5	2860	4210	0.12%	0.009%
24	13.610	1733	1738	1742	rVV6	5666	8769	0.26%	0.019%
25	13.686	1750	1751	1755	rVB4	3112	3524	0.10%	0.008%
26	14.122	1819	1825	1838	rBV	1482504	1997781	58.98%	4.307%
27	14.233	1842	1844	1849	rVV5	4109	5752	0.17%	0.012%
28	14.410	1866	1874	1887	rBV	1805464	2700246	79.71%	5.821%
29	14.716	1919	1926	1935	rBV	1710092	2486698	73.41%	5.361%
30	14.910	1952	1959	1979	rBV	414143	837064	24.71%	1.804%
31	15.704	2087	2094	2108	rBV	2110108	3039346	89.73%	6.552%
32	15.816	2108	2113	2121	rVV	445093	619614	18.29%	1.336%
33	15.939	2129	2134	2142	rVB4	12818	25382	0.75%	0.055%
34	16.021	2147	2148	2152	rVB4	5740	4825	0.14%	0.010%
35	16.174	2172	2174	2179	rVB6	2802	4417	0.13%	0.010%
36	16.345	2200	2203	2206	rBV5	3141	3547	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
 Data File : BM037890.D
 Acq On : 08 Dec 2022 17:13
 Operator : CG/JU
 Sample : PB149468BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK468

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	16.433	2215	2218	2221	rBV5	3576	4844	0.14%	0.010%
38	16.904	2295	2298	2301	rBV5	3324	4154	0.12%	0.009%
39	17.104	2330	2332	2335	rBV4	3917	3553	0.10%	0.008%
40	17.227	2350	2353	2354	rVV3	4080	4274	0.13%	0.009%
41	17.245	2354	2356	2359	rVV3	5395	6812	0.20%	0.015%
42	17.268	2359	2360	2367	rVB6	5415	7022	0.21%	0.015%
43	17.457	2384	2392	2402	rBV	1735683	2508164	74.04%	5.407%
44	17.551	2402	2408	2423	rVB	2023501	3049371	90.02%	6.574%
45	17.715	2433	2436	2444	rVB10	8105	14809	0.44%	0.032%
46	17.862	2457	2461	2466	rBV4	8686	14774	0.44%	0.032%
47	18.333	2538	2541	2545	rVB5	10116	14938	0.44%	0.032%
48	18.409	2550	2554	2558	rBV	17107	22747	0.67%	0.049%
49	19.404	2719	2723	2727	rVB6	26158	36229	1.07%	0.078%
50	19.833	2790	2796	2809	rBV	2318198	3387392	100.00%	7.302%
51	20.803	2959	2961	2965	rBV2	58417	53510	1.58%	0.115%
52	21.621	3095	3100	3111	rBV2	1779652	2420482	71.46%	5.218%
53	23.944	3489	3495	3504	rVB2	1655481	3342716	98.68%	7.206%
54	24.109	3517	3523	3532	rVB2	1199247	2483449	73.31%	5.354%


Sum of corrected areas: 46388823

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037890.D
Acq On : 08 Dec 2022 17:13
Operator : CG/JU
Sample : PB149468BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK468

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

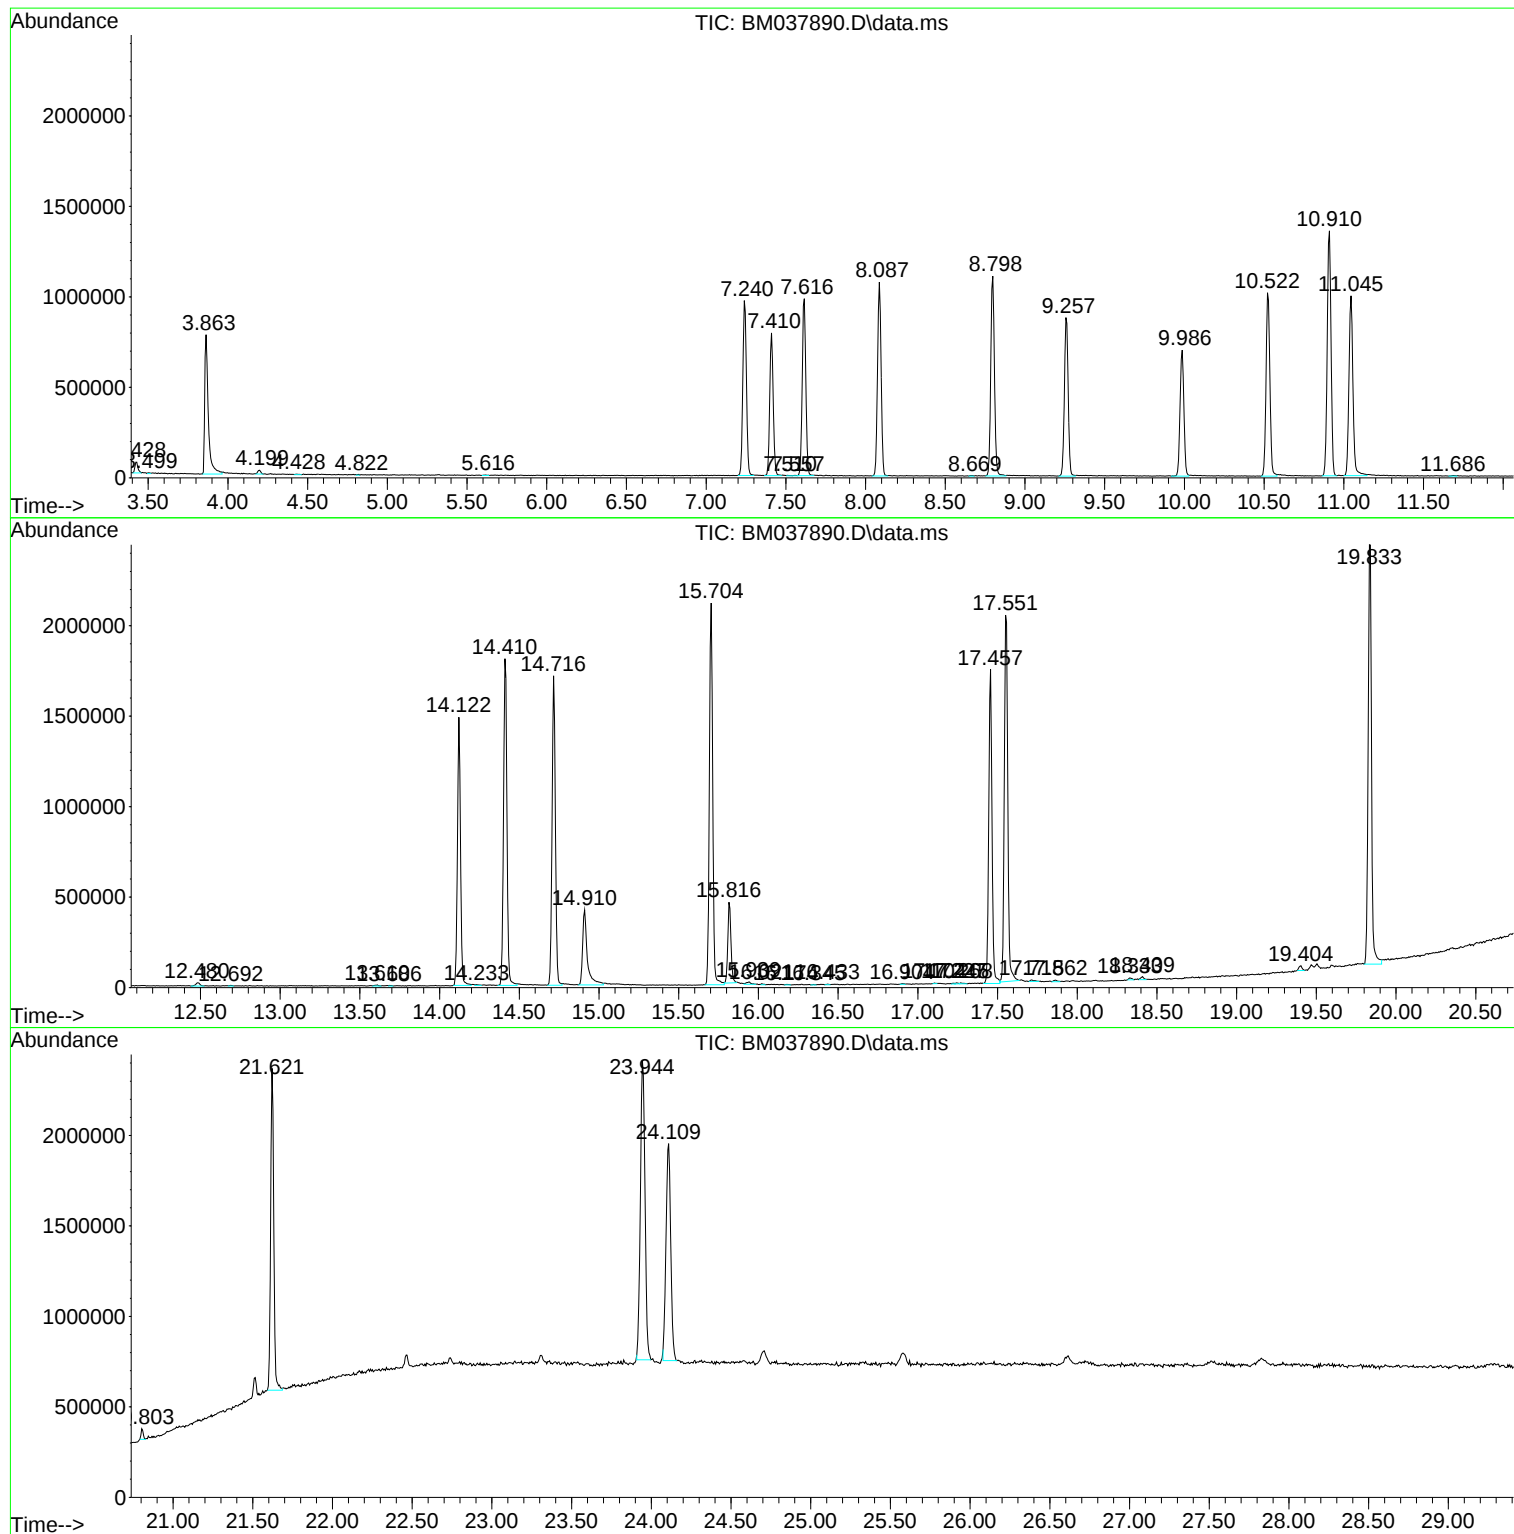

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037890.D
Acq On : 08 Dec 2022 17:13
Operator : CG/JU
Sample : PB149468BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK468

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120822\
Data File : BM037890.D
Acq On : 08 Dec 2022 17:13
Operator : CG/JU
Sample : PB149468BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK468

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc