

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120922\
 Data File : BM037915.D
 Acq On : 09 Dec 2022 14:02
 Operator : CG/JU
 Sample : N5896-03 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBXM1

Quant Time: Dec 09 21:48:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Dec 09 21:34:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.081	152	250886	20.000	ng/ul	0.00
20) Naphthalene-d8	10.904	136	1023203	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.710	164	579059	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.451	188	1195140	20.000	ng/ul	0.00
79) Chrysene-d12	21.621	240	923347	20.000	ng/ul	0.00
88) Perylene-d12	24.109	264	1020490	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	1532	0.277	ng/uL	0.00
4) Pyridine-d5	3.846	84	436	0.027	ng/ul	-0.01
7) Phenol-d5	7.234	99	37845	1.856	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.404	67	23654	1.905	ng/ul	0.00
11) 2-Chlorophenol-d4	7.610	132	32119	1.921	ng/ul	0.00
15) 4-Methylphenol-d8	8.792	113	28155	1.769	ng/ul	0.00
21) Nitrobenzene-d5	9.251	128	15474	1.910	ng/ul	0.00
24) 2-Nitrophenol-d4	9.981	143	14739	1.736	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.516	165	27659	1.715	ng/ul	0.00
31) 4-Chloroaniline-d4	11.045	131	26018	1.169	ng/ul	0.00
46) Dimethylphthalate-d6	14.116	166	80297	1.945	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	95303	1.889	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	6177	0.878	ng/ul	0.00
60) Fluorene-d10	15.698	176	76807	2.088	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.815	200	6108	0.956	ng/ul	0.00
73) Anthracene-d10	17.551	188	135485	2.429	ng/ul	0.00
81) Pyrene-d10	19.833	212	132919	2.396	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.944	264	109512	2.149	ng/ul	0.00
Target Compounds						Qvalue
30) Naphthalene	10.951	128	109971	1.992	ng/ul	99
50) Acenaphthylene	14.439	152	118578	2.137	ng/ul	97
52) Acenaphthene	14.774	153	93444	2.435	ng/ul	98
56) Dibenzofuran	15.104	168	119164	2.275	ng/ul	94
61) Fluorene	15.751	166	101421	2.374	ng/ul	97
72) Phenanthrene	17.492	178	618998	9.484	ng/ul	99
74) Anthracene	17.586	178	1096111	16.526	ng/ul	99
77) Carbazole	17.856	167	143367	2.495	ng/ul	98
80) Fluoranthene	19.498	202	835772	12.768	ng/ul	99
82) Pyrene	19.862	202	956694	14.043	ng/ul	99
85) Benzo(a)anthracene	21.662	228	248762	4.002	ng/ul	95
87) Chrysene	21.662	228	244626	4.194	ng/ul	97
90) Benzo(b)fluoranthene	23.344	252	1750054	27.662	ng/ul	99
91) Benzo(k)fluoranthene	23.344	252	1750054	28.542	ng/ul	98
93) Benzo(a)pyrene	23.997	252	643340	11.564	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	26.697	276	445661	6.220	ng/ul#	95
95) Dibenzo(a,h)anthracene	26.703	278	110897	1.836	ng/ul#	83
96) Benzo(g,h,i)perylene	27.503	276	341317	5.966	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120922\
Data File : BM037915.D
Acq On : 09 Dec 2022 14:02
Operator : CG/JU
Sample : N5896-03 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBXM1

Quant Time: Dec 09 21:48:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 09 21:34:57 2022
Response via : Initial Calibration




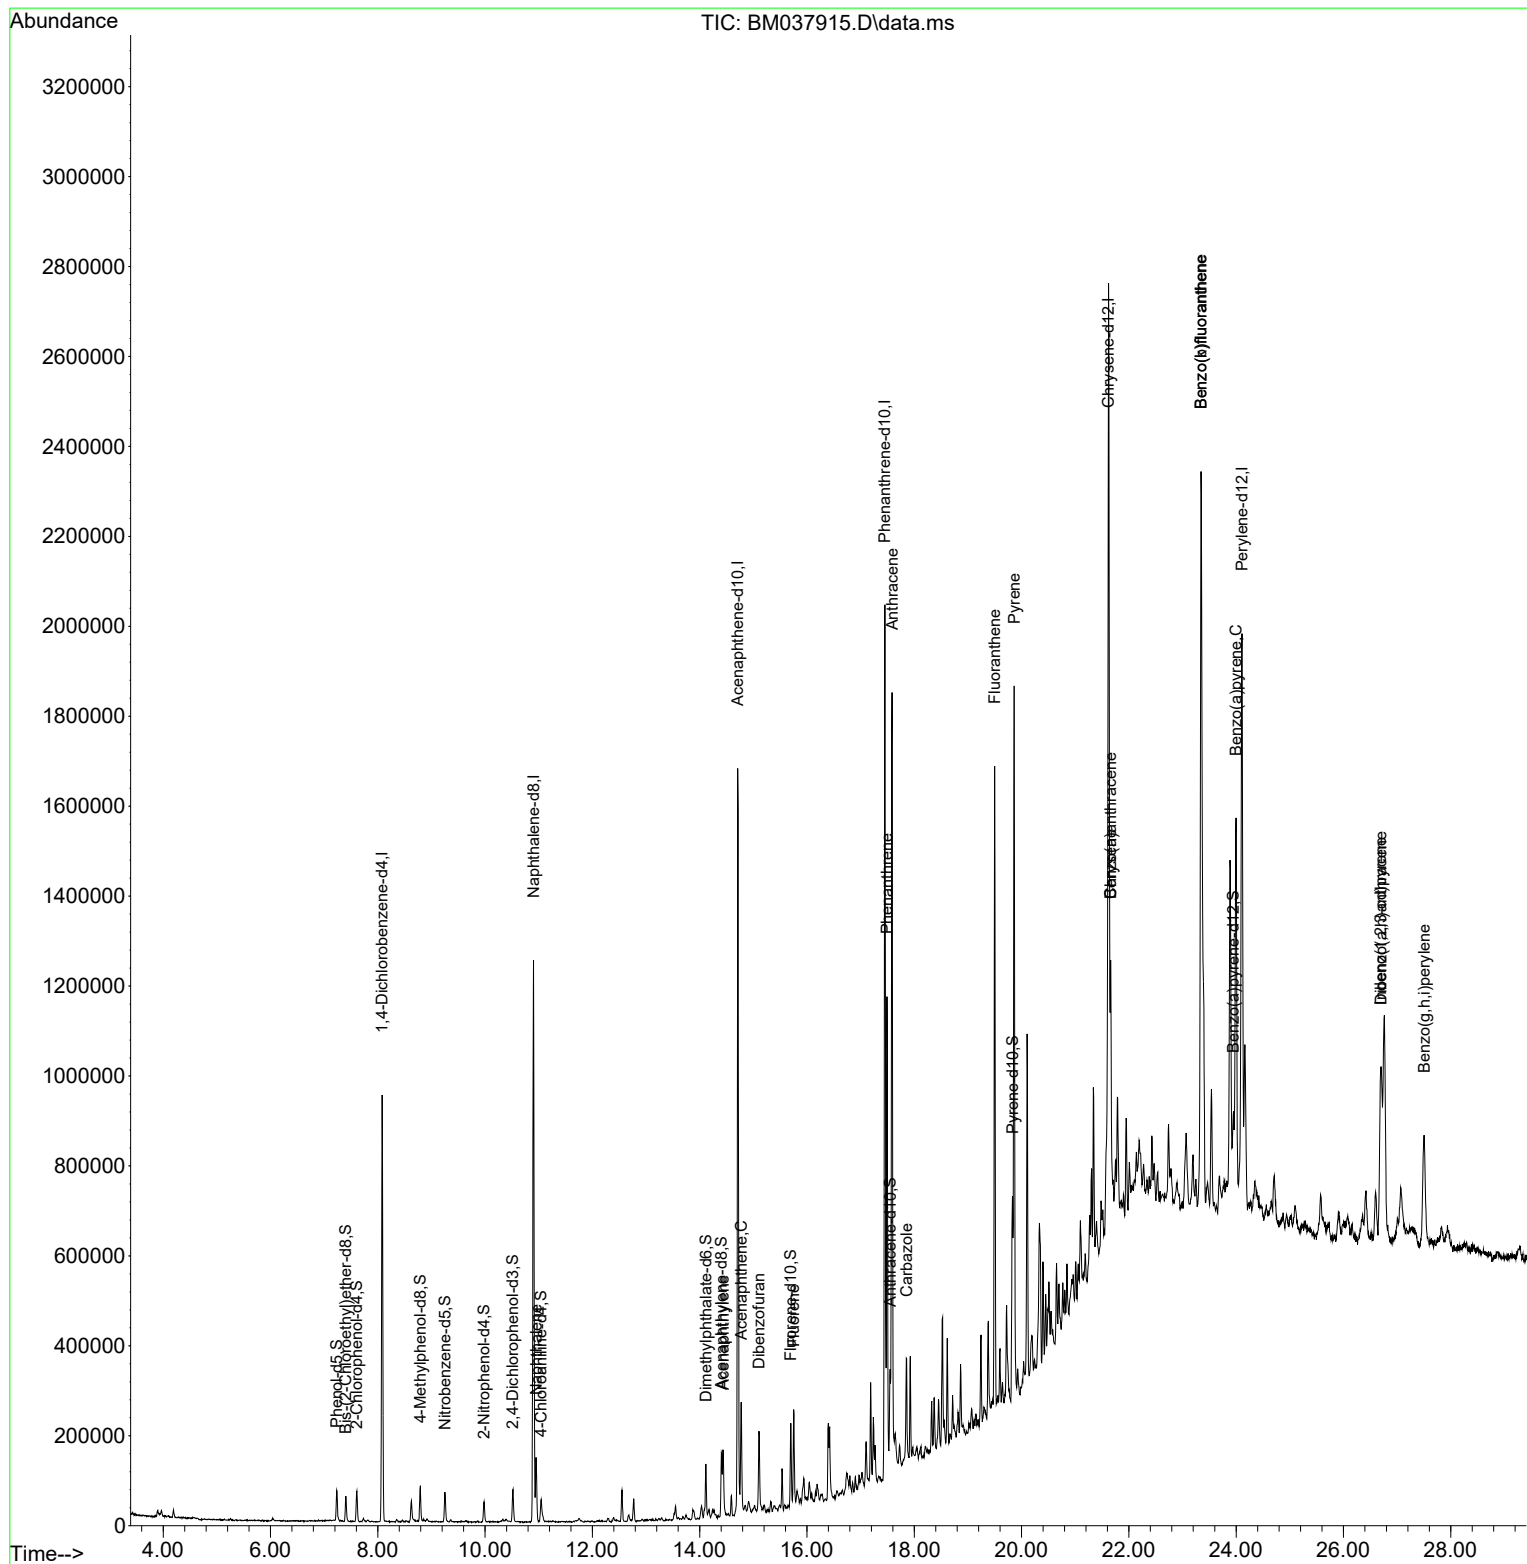




#30
Naphthalene
Concen: 1.992 ng/ul
RT: 10.951 min Scan# 1286
Delta R.T. -0.006 min
Lab File: BM037915.D
Acq: 09 Dec 2022 14:02




Instrument :
BNA_M
ClientSampleId :
DBXM1


Tgt Ion:128 Resp: 109971
Ion Ratio Lower Upper
128 100
129 10.9 9.0 13.4
127 12.3 10.4 15.6

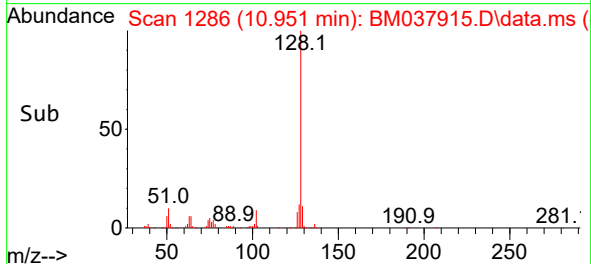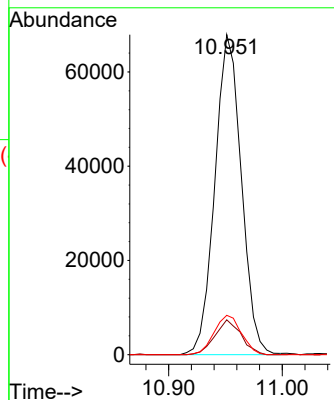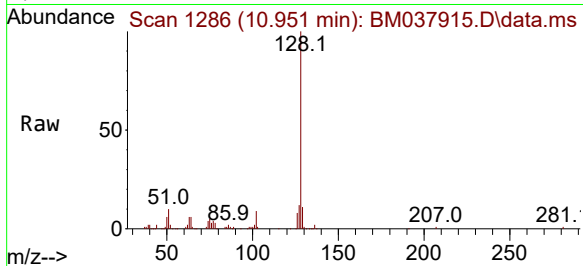

#50
Acenaphthylene
Concen: 2.137 ng/ul
RT: 14.439 min Scan# 1879
Delta R.T. -0.000 min
Lab File: BM037915.D
Acq: 09 Dec 2022 14:02

Tgt Ion:152 Resp: 118578
Ion Ratio Lower Upper
152 100
151 20.6 15.3 22.9
153 14.1 10.2 15.4


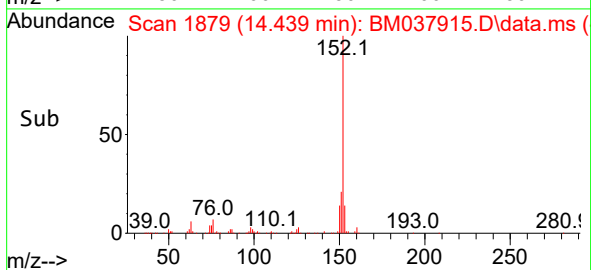
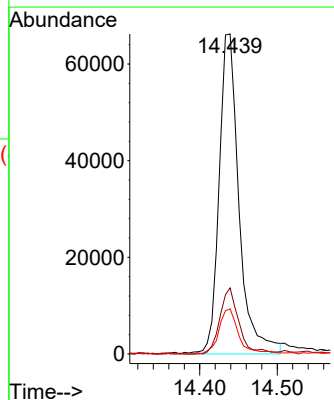
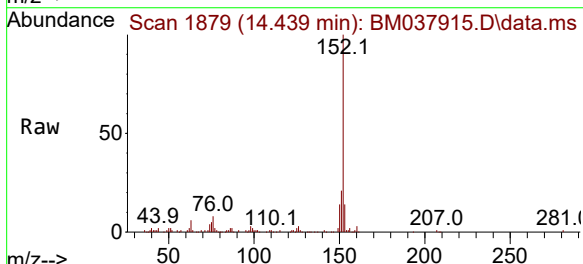




#52
Acenaphthene
Concen: 2.435 ng/ul
RT: 14.774 min Scan# 1936
Delta R.T. -0.000 min
Lab File: BM037915.D
Acq: 09 Dec 2022 14:02




Instrument :
BNA_M
ClientSampleId :
DBXM1


Tgt Ion:153 Resp: 93444
Ion Ratio Lower Upper
153 100
152 50.9 38.2 57.4
154 88.5 71.4 107.0

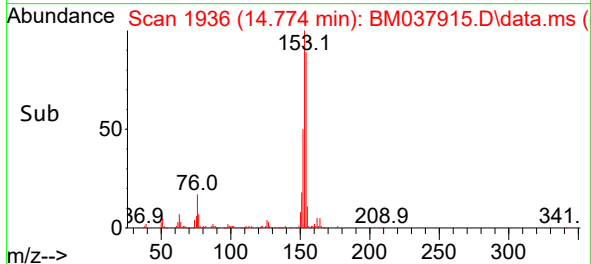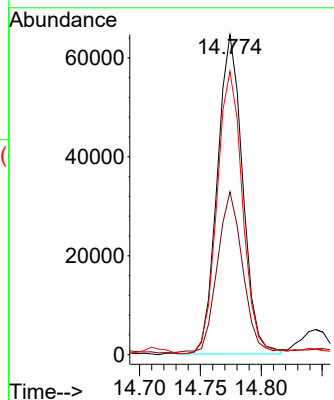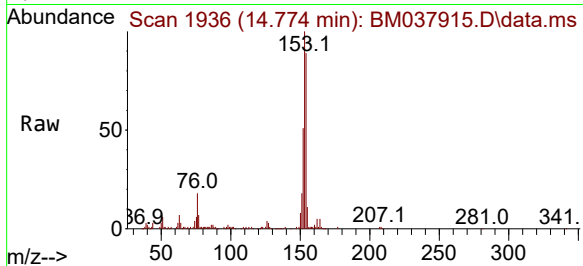

#56
Dibenzofuran
Concen: 2.275 ng/ul
RT: 15.104 min Scan# 1992
Delta R.T. -0.006 min
Lab File: BM037915.D
Acq: 09 Dec 2022 14:02

Tgt Ion:168 Resp: 119164
Ion Ratio Lower Upper
168 100
139 38.5 28.1 42.1

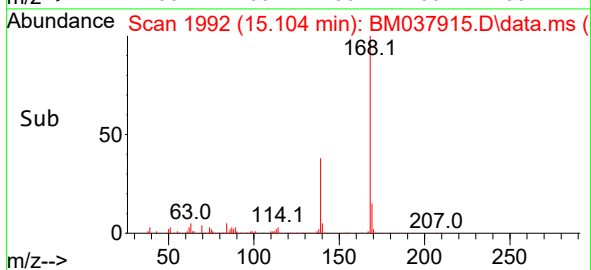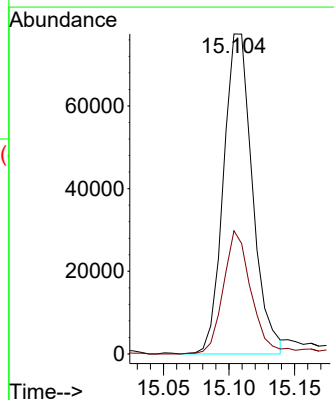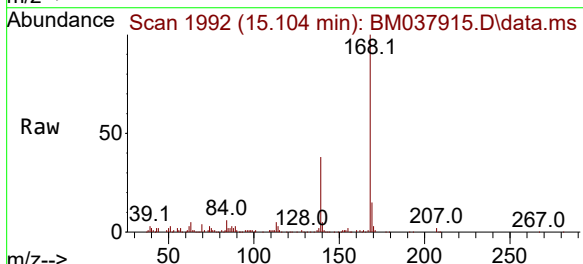



#61

Fluorene

Concen: 2.374 ng/ul

RT: 15.751 min Scan# 2103

Delta R.T. -0.006 min

Lab File: BM037915.D

Acq: 09 Dec 2022 14:02

Instrument :

BNA_M

ClientSampleId :

DBXM1





Tgt Ion:166 Resp: 101421

Ion Ratio Lower Upper

166 100

165 93.4 77.2 115.8

167 13.9 10.4 15.6

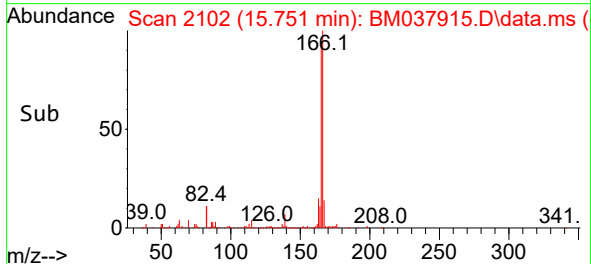

#72

Phenanthrene

Concen: 9.484 ng/ul

RT: 17.492 min Scan# 2398

Delta R.T. -0.000 min

Lab File: BM037915.D

Acq: 09 Dec 2022 14:02




Tgt Ion:178 Resp: 618998


Ion Ratio Lower Upper

178 100

179 15.6 12.2 18.2

176 18.9 15.4 23.0


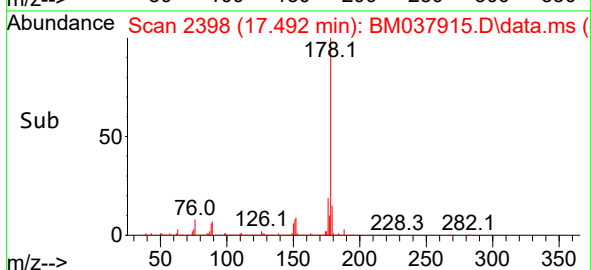






#74
 Anthracene
 Concen: 16.526 ng/ul
 RT: 17.586 min Scan# 2414
 Delta R.T. -0.000 min
 Lab File: BM037915.D
 Acq: 09 Dec 2022 14:02




Instrument :
 BNA_M
 ClientSampleId :
 DBXM1


Tgt Ion:178 Resp: 1096111
 Ion Ratio Lower Upper
 178 100
 179 15.2 11.8 17.8
 176 18.7 15.0 22.6

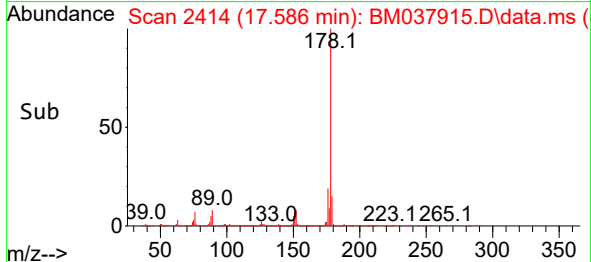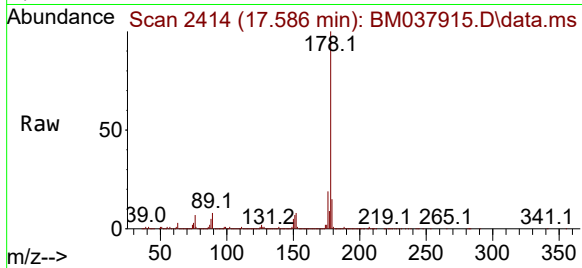

#77
 Carbazole
 Concen: 2.495 ng/ul
 RT: 17.856 min Scan# 2460
 Delta R.T. -0.000 min
 Lab File: BM037915.D
 Acq: 09 Dec 2022 14:02

Tgt Ion:167 Resp: 143367
 Ion Ratio Lower Upper
 167 100
 166 20.4 16.7 25.1
 139 13.3 9.8 14.6


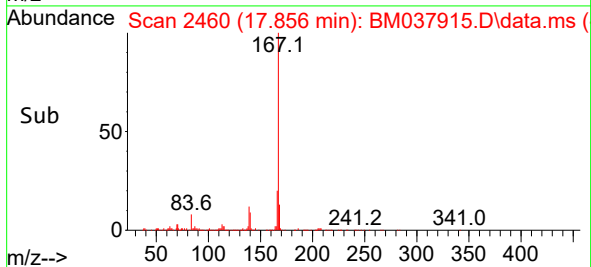

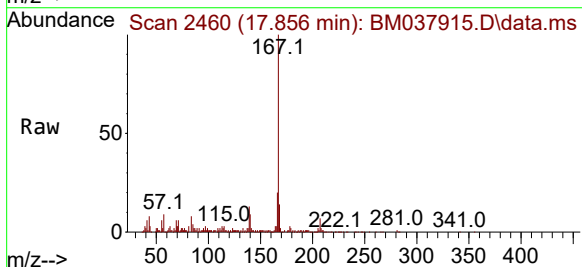




#80
Fluoranthene
Concen: 12.768 ng/ul
RT: 19.498 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM037915.D
Acq: 09 Dec 2022 14:02




Instrument :
BNA_M
ClientSampleId :
DBXM1


Tgt Ion:202 Resp: 835772
Ion Ratio Lower Upper
202 100
101 10.0 8.6 13.0
100 8.1 6.6 10.0

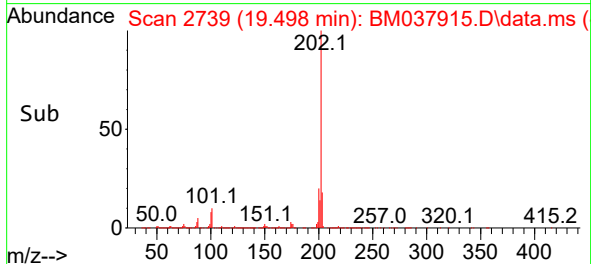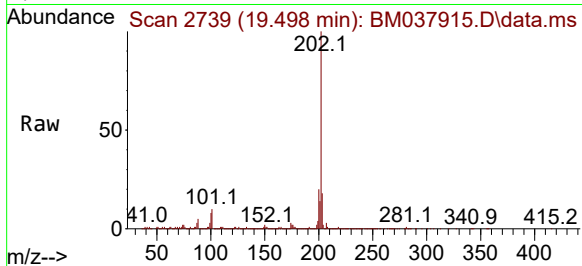

#82
Pyrene
Concen: 14.043 ng/ul
RT: 19.862 min Scan# 2801
Delta R.T. -0.000 min
Lab File: BM037915.D
Acq: 09 Dec 2022 14:02

Tgt Ion:202 Resp: 956694
Ion Ratio Lower Upper
202 100
101 11.7 10.0 15.0
100 9.9 7.9 11.9

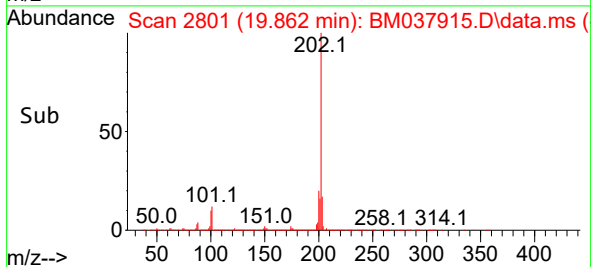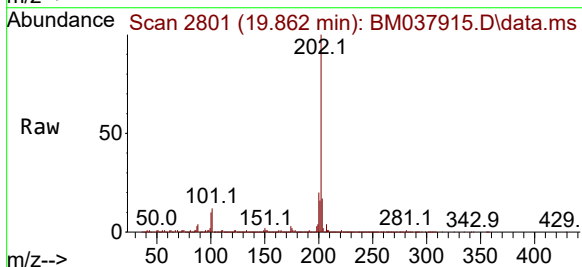



#85

Benzo(a)anthracene

Concen: 4.002 ng/ul

RT: 21.662 min Scan# 3107

Delta R.T. 0.059 min

Lab File: BM037915.D

Acq: 09 Dec 2022 14:02

Instrument :

BNA_M

ClientSampleId :

DBXM1





Tgt Ion:228 Resp: 248762

Ion Ratio Lower Upper

228 100

229 21.6 15.5 23.3

226 29.6 21.8 32.8

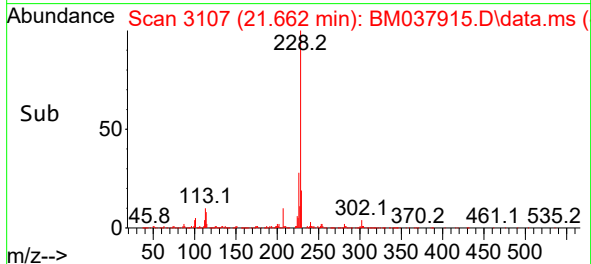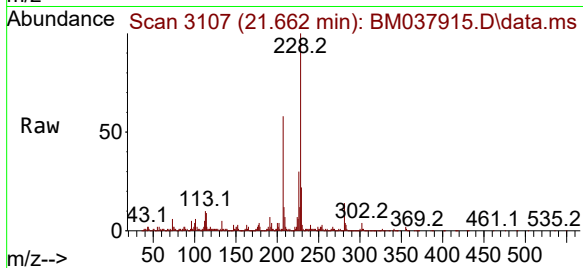

#87

Chrysene

Concen: 4.194 ng/ul

RT: 21.662 min Scan# 3107

Delta R.T. -0.000 min

Lab File: BM037915.D

Acq: 09 Dec 2022 14:02




Tgt Ion:228 Resp: 244626


Ion Ratio Lower Upper

228 100

226 29.6 24.3 36.5

229 21.6 15.6 23.4



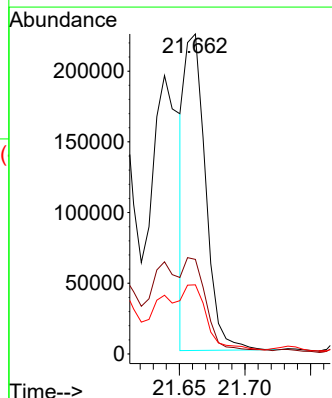
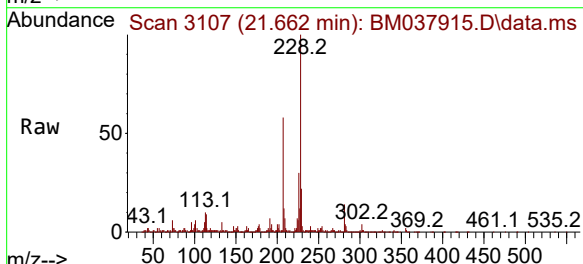




#90
Benzo(b)fluoranthene
Concen: 27.662 ng/ul
RT: 23.344 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM037915.D
Acq: 09 Dec 2022 14:02




Instrument :
BNA_M
ClientSampleId :
DBXM1


Tgt Ion:252 Resp: 1750054
Ion Ratio Lower Upper
252 100
253 22.9 17.6 26.4
125 10.1 8.0 12.0

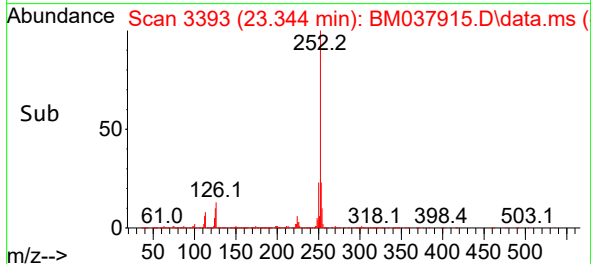

#91
Benzo(k)fluoranthene
Concen: 28.542 ng/ul
RT: 23.344 min Scan# 3393
Delta R.T. -0.047 min
Lab File: BM037915.D
Acq: 09 Dec 2022 14:02

Tgt Ion:252 Resp: 1750054
Ion Ratio Lower Upper
252 100
253 22.9 17.4 26.2
125 10.1 8.1 12.1

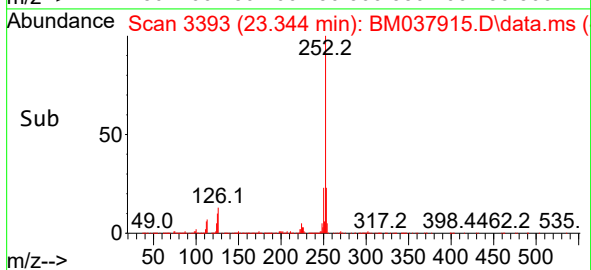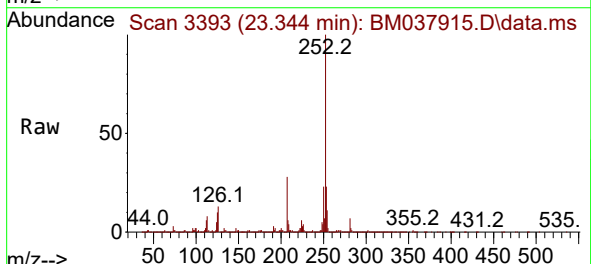



#93

Benzo(a)pyrene

Concen: 11.564 ng/ul

RT: 23.997 min Scan# 3

Delta R.T. 0.006 min

Lab File: BM037915.D

Acq: 09 Dec 2022 14:02

Instrument :

BNA_M

ClientSampleId :

DBXM1





Tgt Ion:252 Resp: 643340

Ion Ratio Lower Upper

252 100

253 23.4 17.4 26.0

125 10.8 9.4 14.0



#94

Indeno(1,2,3-cd)pyrene

Concen: 6.220 ng/ul

RT: 26.697 min Scan# 3963

Delta R.T. -0.006 min

Lab File: BM037915.D

Acq: 09 Dec 2022 14:02




Tgt Ion:276 Resp: 445661


Ion Ratio Lower Upper

276 100

138 18.9 19.3 28.9#

277 24.7 19.8 29.8

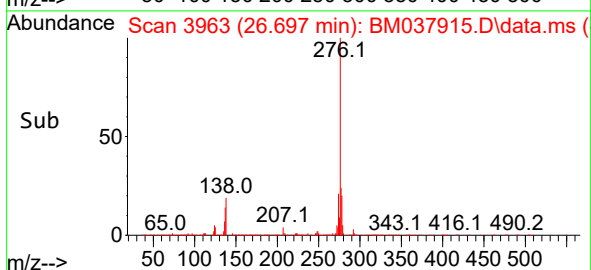



#95

Dibenzo(a,h)anthracene

Concen: 1.836 ng/ul

RT: 26.703 min Scan# 3964

Delta R.T. -0.012 min

Lab File: BM037915.D

Acq: 09 Dec 2022 14:02

Instrument :

BNA_M

ClientSampleId :

DBXM1





Tgt Ion:278 Resp: 110897

Ion Ratio Lower Upper

278 100

139 0.0 12.4 18.6#

279 27.4 19.8 29.6

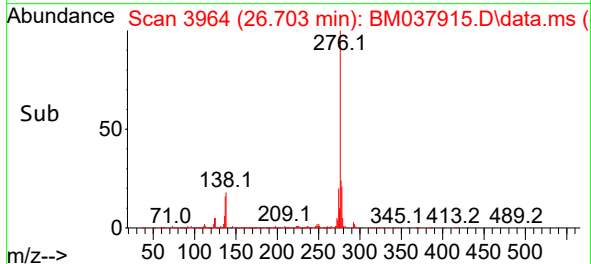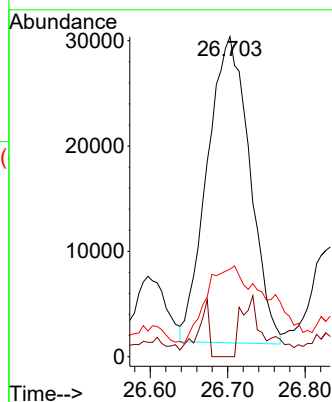

#96

Benzo(g,h,i)perylene

Concen: 5.966 ng/ul

RT: 27.503 min Scan# 4100

Delta R.T. -0.000 min

Lab File: BM037915.D

Acq: 09 Dec 2022 14:02

Tgt Ion:276 Resp: 341317

Ion Ratio Lower Upper

276 100

138 19.5 17.1 25.7

277 23.1 18.2 27.4

