

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120922\
 Data File : BM037909.D
 Acq On : 09 Dec 2022 10:22
 Operator : CG/JU
 Sample : PB149458BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK458

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

Signal : TIC: BM037909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	3	6	12	rVB	47133	61888	2.04%	0.148%
2	3.857	76	80	102	rBV	700892	1134008	37.42%	2.705%
3	4.193	133	137	144	rVB2	17385	25464	0.84%	0.061%
4	5.428	340	347	350	rBV8	1565	3332	0.11%	0.008%
5	6.345	500	503	507	rBV5	2326	3164	0.10%	0.008%
6	6.681	556	560	562	rBV5	3419	3841	0.13%	0.009%
7	7.234	648	654	663	rBV	886747	1390196	45.88%	3.316%
8	7.404	677	683	693	rVB	705752	1062349	35.06%	2.534%
9	7.610	709	718	728	rBV	912549	1406372	46.41%	3.355%
10	8.081	791	798	808	rVB	884744	1358824	44.84%	3.241%
11	8.281	829	832	838	rBV8	2286	4623	0.15%	0.011%
12	8.792	912	919	931	rBV	1030531	1634365	53.94%	3.899%
13	9.257	990	998	1010	rBV	827462	1352868	44.65%	3.227%
14	9.980	1112	1121	1132	rBV	660454	1067351	35.22%	2.546%
15	10.522	1203	1213	1229	rBV	949538	1622233	53.54%	3.870%
16	10.904	1269	1278	1287	rBV	1180579	1906417	62.92%	4.548%
17	11.039	1294	1301	1319	rBV	942116	1644809	54.28%	3.923%
18	11.880	1443	1444	1448	rBV4	2550	3112	0.10%	0.007%
19	12.480	1541	1546	1552	rBV	17229	28203	0.93%	0.067%
20	13.598	1734	1736	1741	rVB5	3235	4123	0.14%	0.010%
21	14.121	1817	1825	1836	rBV	1370455	1982661	65.43%	4.729%
22	14.410	1867	1874	1884	rBV	1779274	2575791	85.01%	6.144%
23	14.480	1884	1886	1890	rVB4	5047	6001	0.20%	0.014%
24	14.710	1918	1925	1937	rBV	1488571	2197430	72.52%	5.242%
25	14.904	1952	1958	1973	rBV	348646	692723	22.86%	1.652%
26	15.062	1983	1985	1990	rVB6	4098	4993	0.16%	0.012%
27	15.115	1990	1994	1995	rBV4	3931	4508	0.15%	0.011%
28	15.333	2029	2031	2035	rBV4	2672	4568	0.15%	0.011%
29	15.698	2087	2093	2105	rBV	2091786	2970611	98.04%	7.086%
30	15.815	2107	2113	2126	rVB	361507	525927	17.36%	1.255%
31	15.939	2131	2134	2138	rVB4	10157	16016	0.53%	0.038%
32	16.480	2223	2226	2229	rVB5	4028	4082	0.13%	0.010%
33	16.898	2291	2297	2302	rBV9	3948	7598	0.25%	0.018%
34	17.103	2329	2332	2333	rBV3	2921	3395	0.11%	0.008%
35	17.233	2352	2354	2357	rBV3	4868	5821	0.19%	0.014%
36	17.262	2357	2359	2362	rVB4	3119	3130	0.10%	0.007%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120922\
 Data File : BM037909.D
 Acq On : 09 Dec 2022 10:22
 Operator : CG/JU
 Sample : PB149458BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK458

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
 Title : SVOA CALIBRATION

37	17.451	2385	2391	2402	rBV	1509293	2173030	71.71%	5.183%
38	17.551	2402	2408	2421	rVV	2071302	2868850	94.68%	6.843%
39	17.974	2478	2480	2483	rBV4	4245	4753	0.16%	0.011%
40	18.403	2551	2553	2559	rVB2	9713	12873	0.42%	0.031%
41	19.397	2719	2722	2725	rVB3	27289	27326	0.90%	0.065%
42	19.833	2790	2796	2804	rBV	2276936	3021261	99.71%	7.207%
43	21.509	3078	3081	3084	rBV	132242	154347	5.09%	0.368%
44	21.621	3095	3100	3108	rBV	1481676	1937209	63.93%	4.621%
45	23.944	3488	3495	3504	rVB2	1478238	3030104	100.00%	7.228%
46	24.103	3516	3522	3530	rVB2	948493	1969664	65.00%	4.698%




Sum of corrected areas: 41922214

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120922\
Data File : BM037909.D
Acq On : 09 Dec 2022 10:22
Operator : CG/JU
Sample : PB149458BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK458

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

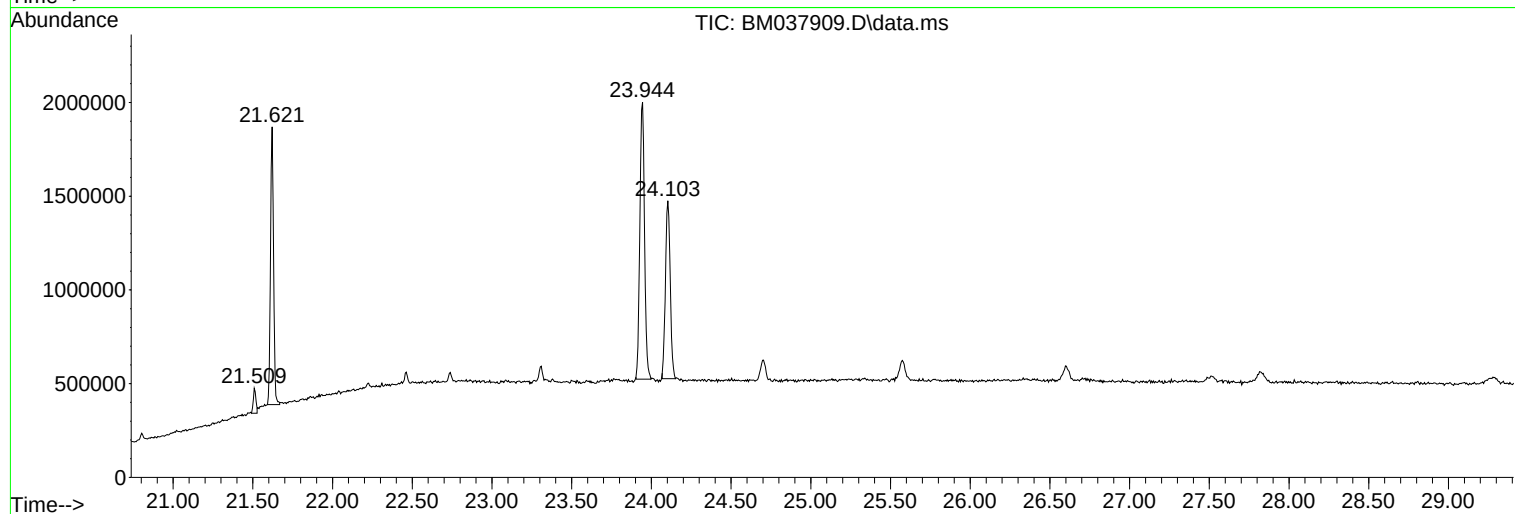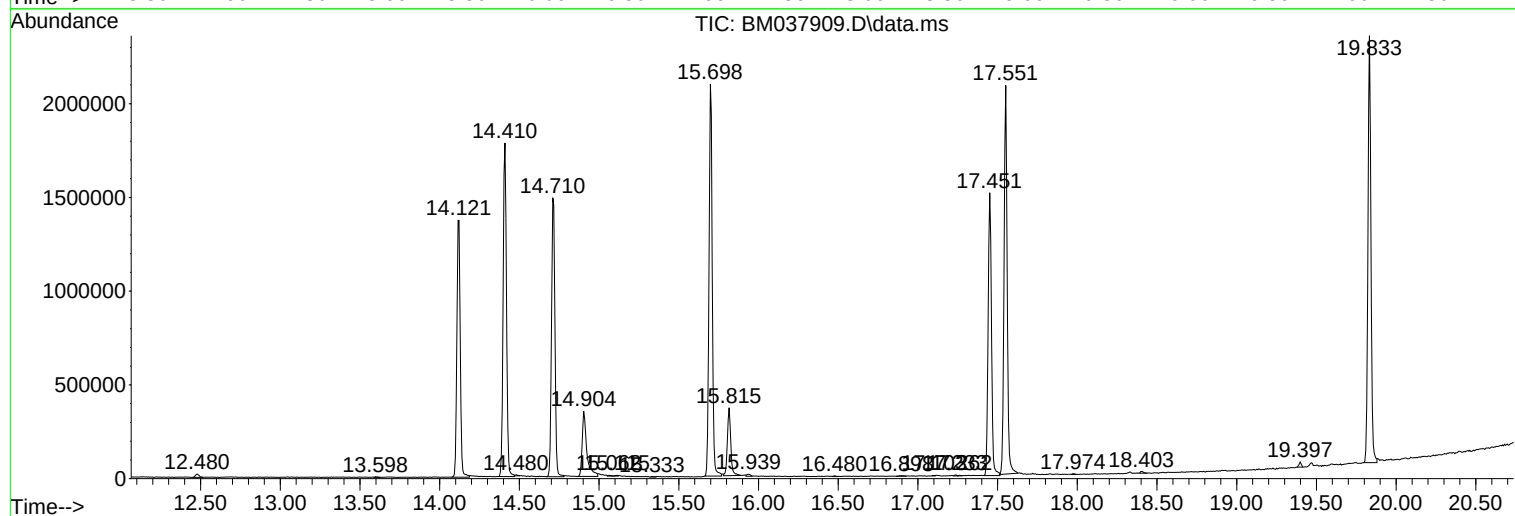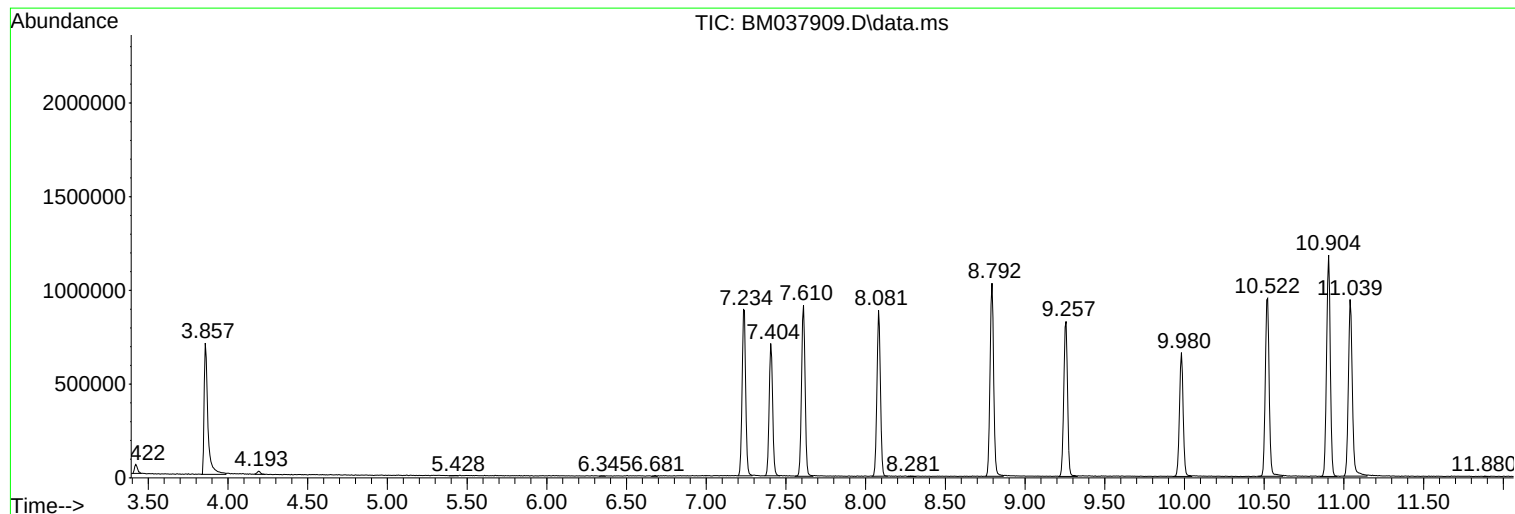

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120922\
Data File : BM037909.D
Acq On : 09 Dec 2022 10:22
Operator : CG/JU
Sample : PB149458BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK458

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM120922\
Data File : BM037909.D
Acq On : 09 Dec 2022 10:22
Operator : CG/JU
Sample : PB149458BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK458

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM120722.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc