
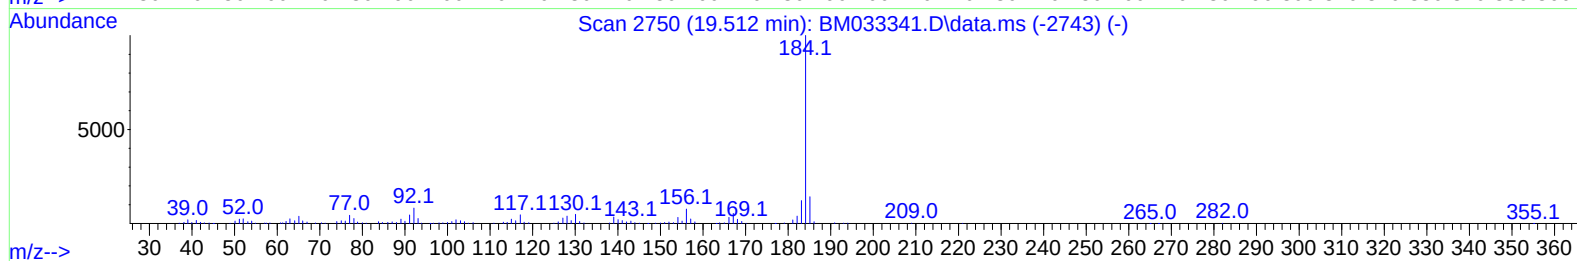
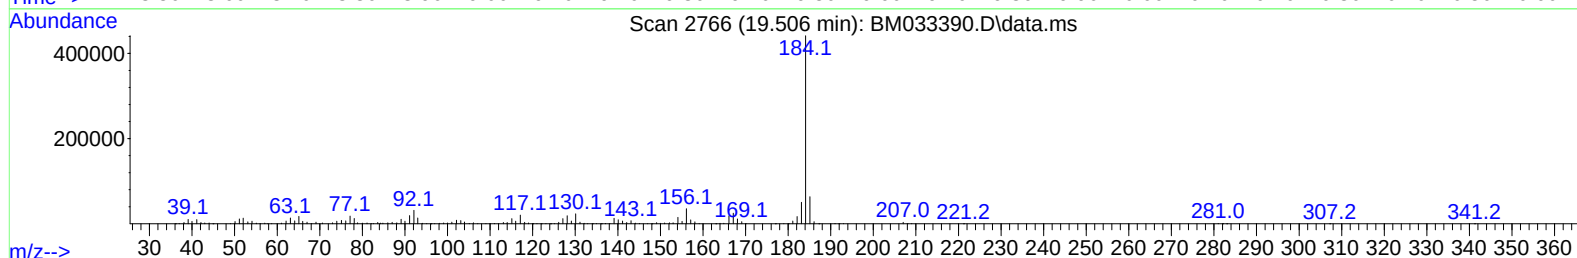


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121021\
Data File : BM033390.D
Acq On : 10 Dec 2021 12:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 02:22:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 07:11:07 2021
Response via : Initial Calibration

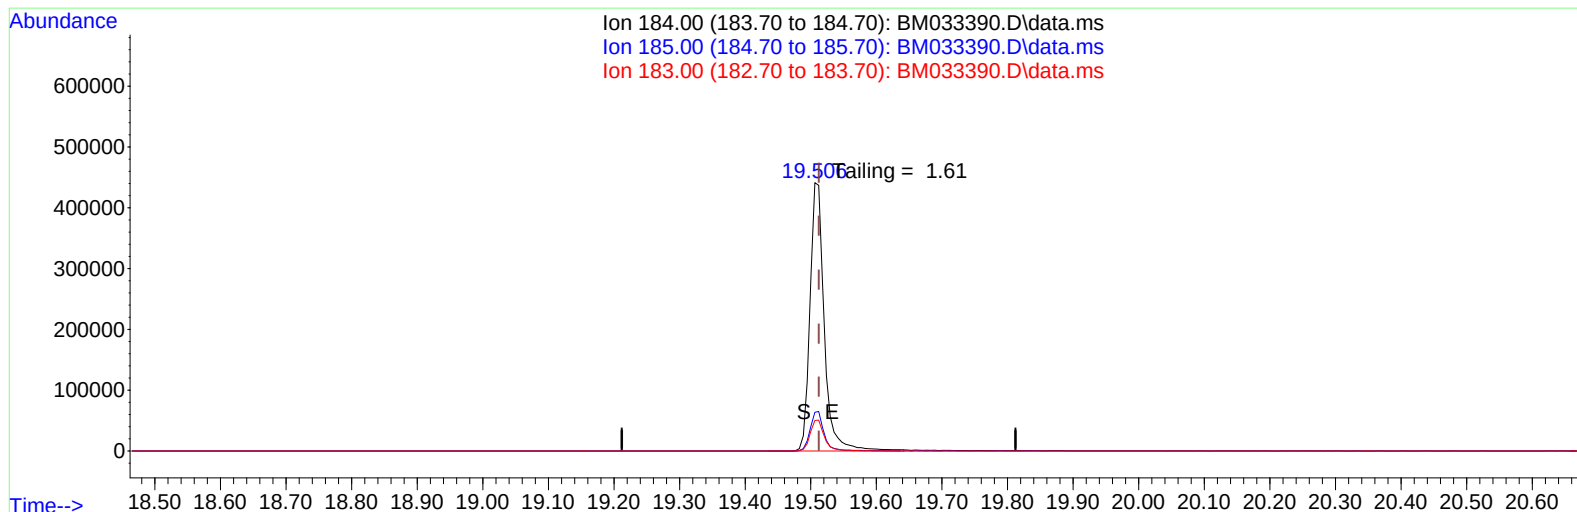

TIC: BM033390.D\data.ms

(77) Benzidine




19.506min (-0.006) 0.00 ng

response 675221

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.43
183.00	12.10	11.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121021\
Data File : BM033390.D
Acq On : 10 Dec 2021 12:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 02:22:13 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 09 07:11:07 2021
Response via : Initial Calibration

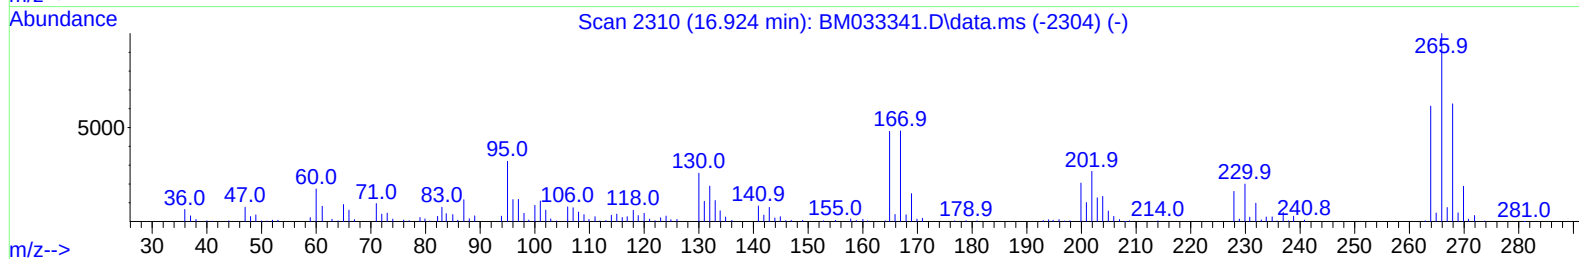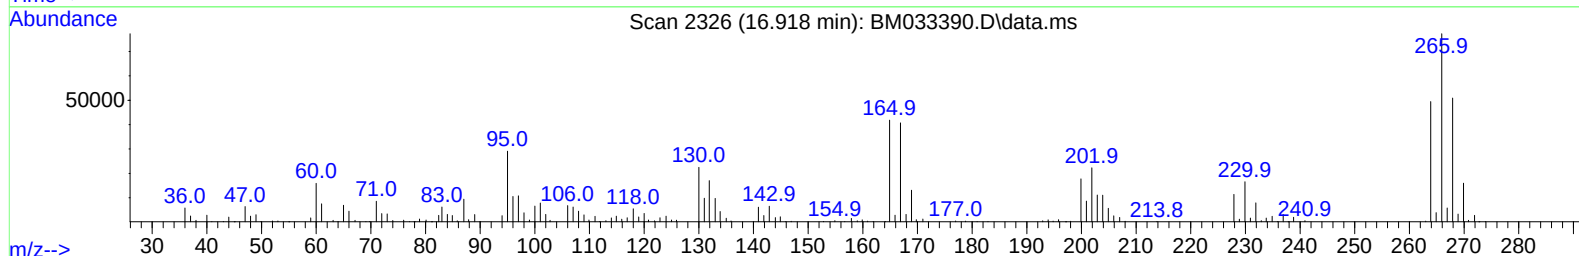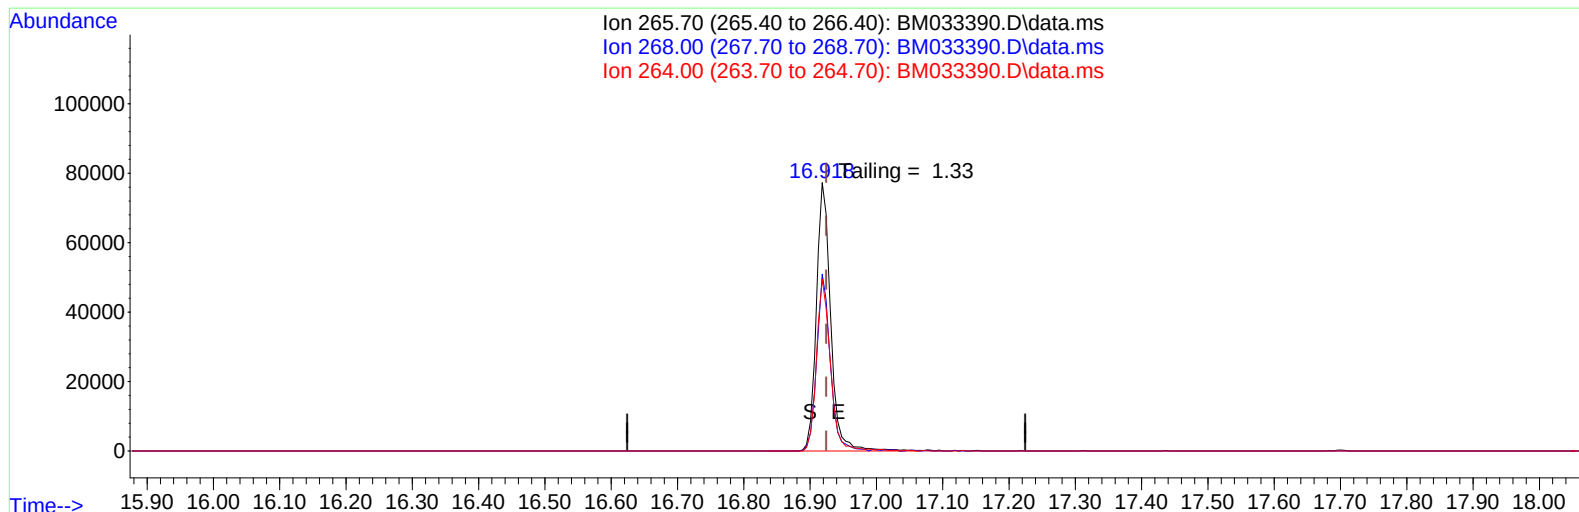

TIC: BM033390.D\data.ms

(70) Pentachlorophenol (C)

16.918min (-0.006) 0.00 ng

response 116548

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	65.88
264.00	61.40	64.01
0.00	0.00	0.00