

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121021\
 Data File : BM033409.D
 Acq On : 11 Dec 2021 00:02
 Operator : CG/JU
 Sample : M4927-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PH1-BOT-13

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM033409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.490	379	383	389	rVB	444013	634289	11.71%	2.850%
2	7.078	648	653	662	rVB	882749	1399538	25.85%	6.288%
3	7.901	789	793	800	rVB	281441	452814	8.36%	2.034%
4	9.066	985	991	1004	rVB	1088154	1852947	34.22%	8.325%
5	10.695	1262	1268	1276	rVB	493381	809087	14.94%	3.635%
6	13.154	1678	1686	1696	rBV	2770096	4051194	74.82%	18.202%
7	14.530	1913	1920	1929	rVB	729731	1105004	20.41%	4.965%
8	16.013	2160	2172	2186	rBV	1526623	2343216	43.27%	10.528%
9	17.265	2379	2385	2392	rBV	821069	1206919	22.29%	5.423%
10	17.924	2493	2497	2503	rVB	71775	87982	1.62%	0.395%
11	18.148	2531	2535	2541	rBV2	42499	62649	1.16%	0.281%
12	19.001	2676	2680	2685	rBV5	33999	62864	1.16%	0.282%
13	19.877	2824	2829	2848	rVB	4162754	5414717	100.00%	24.328%
14	21.124	3038	3041	3050	rBV	178917	251777	4.65%	1.131%
15	21.430	3088	3093	3103	rBV	883028	1164567	21.51%	5.232%
16	22.624	3292	3296	3302	rVB	223645	292126	5.40%	1.313%
17	23.747	3481	3487	3499	rVB2	511487	1065343	19.67%	4.787%




Sum of corrected areas: 22257033

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121021\
Data File : BM033409.D
Acq On : 11 Dec 2021 00:02
Operator : CG/JU
Sample : M4927-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PH1-BOT-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

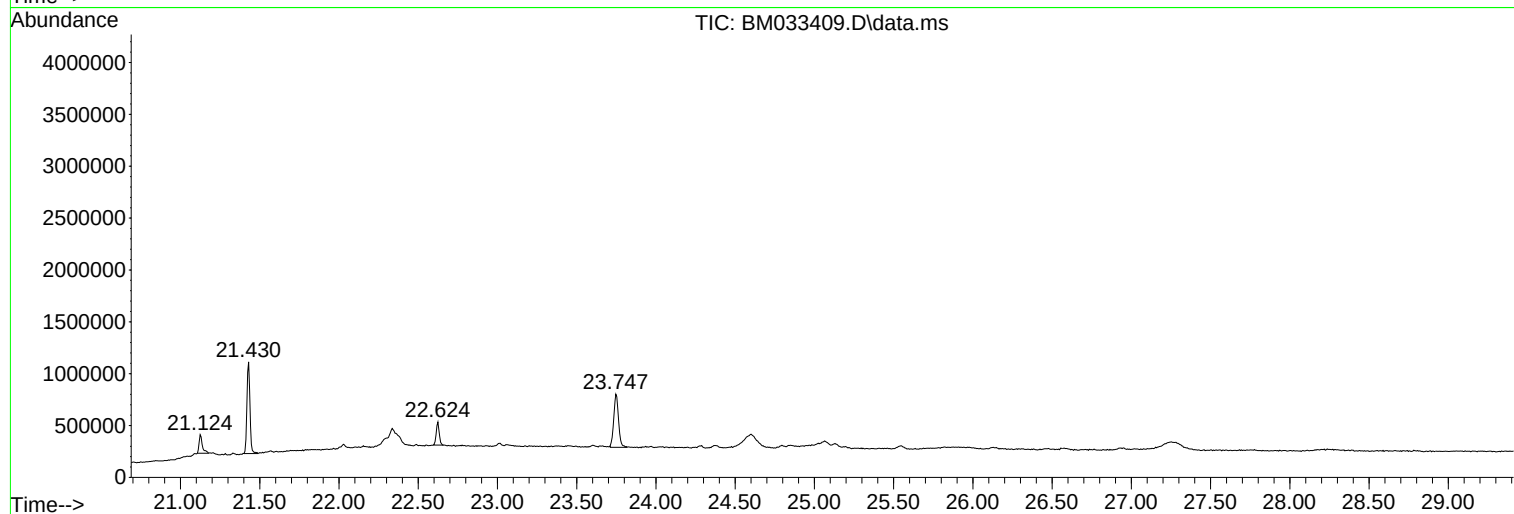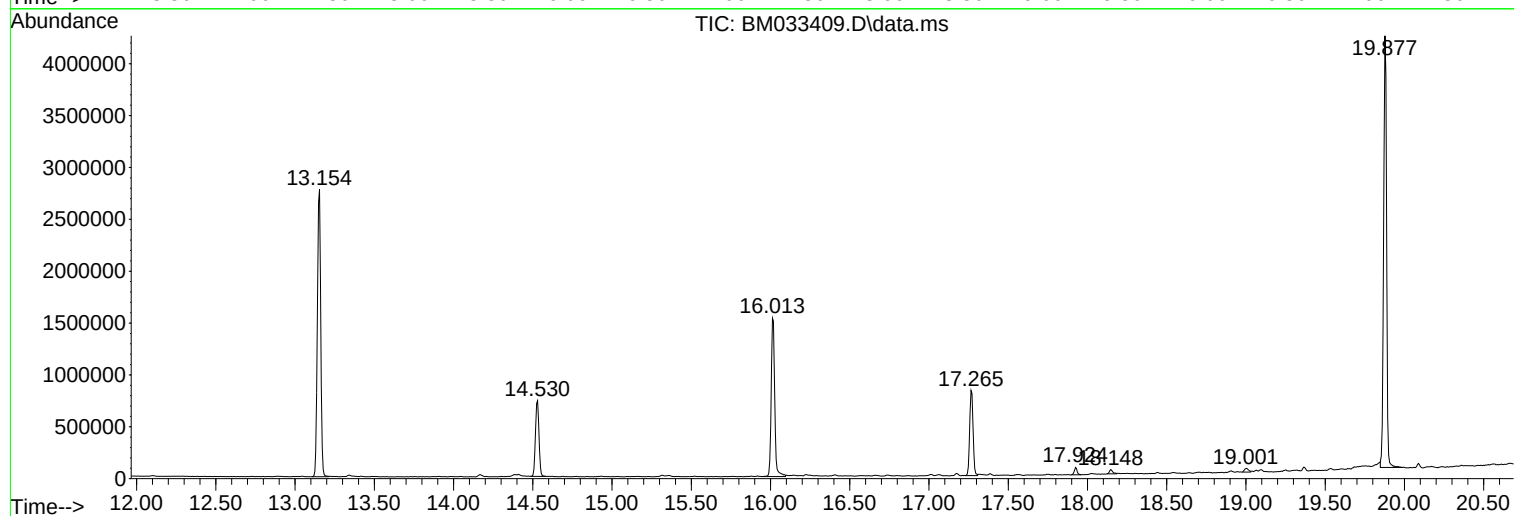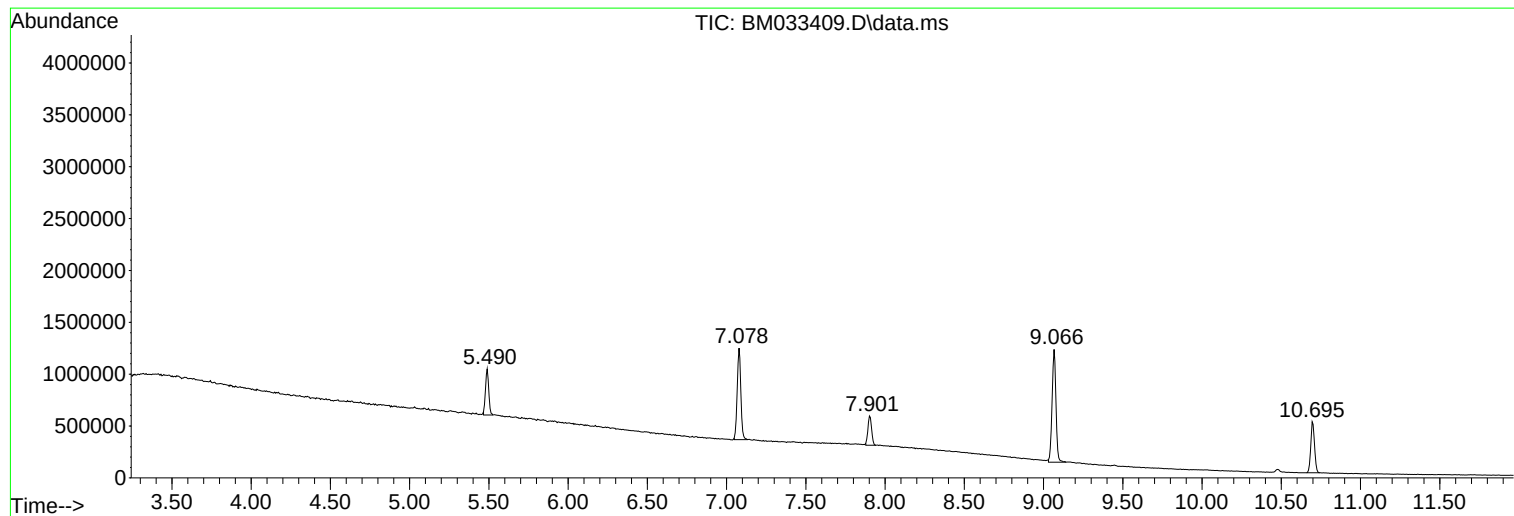

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121021\
Data File : BM033409.D
Acq On : 11 Dec 2021 00:02
Operator : CG/JU
Sample : M4927-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PH1-BOT-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM121021\
Data File : BM033409.D
Acq On : 11 Dec 2021 00:02
Operator : CG/JU
Sample : M4927-12
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PH1-BOT-13

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM120821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------