


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121021\  
 Data File : BM033390.D  
 Acq On : 10 Dec 2021 12:18  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM120821.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sun Dec 12 00:15:00 2021

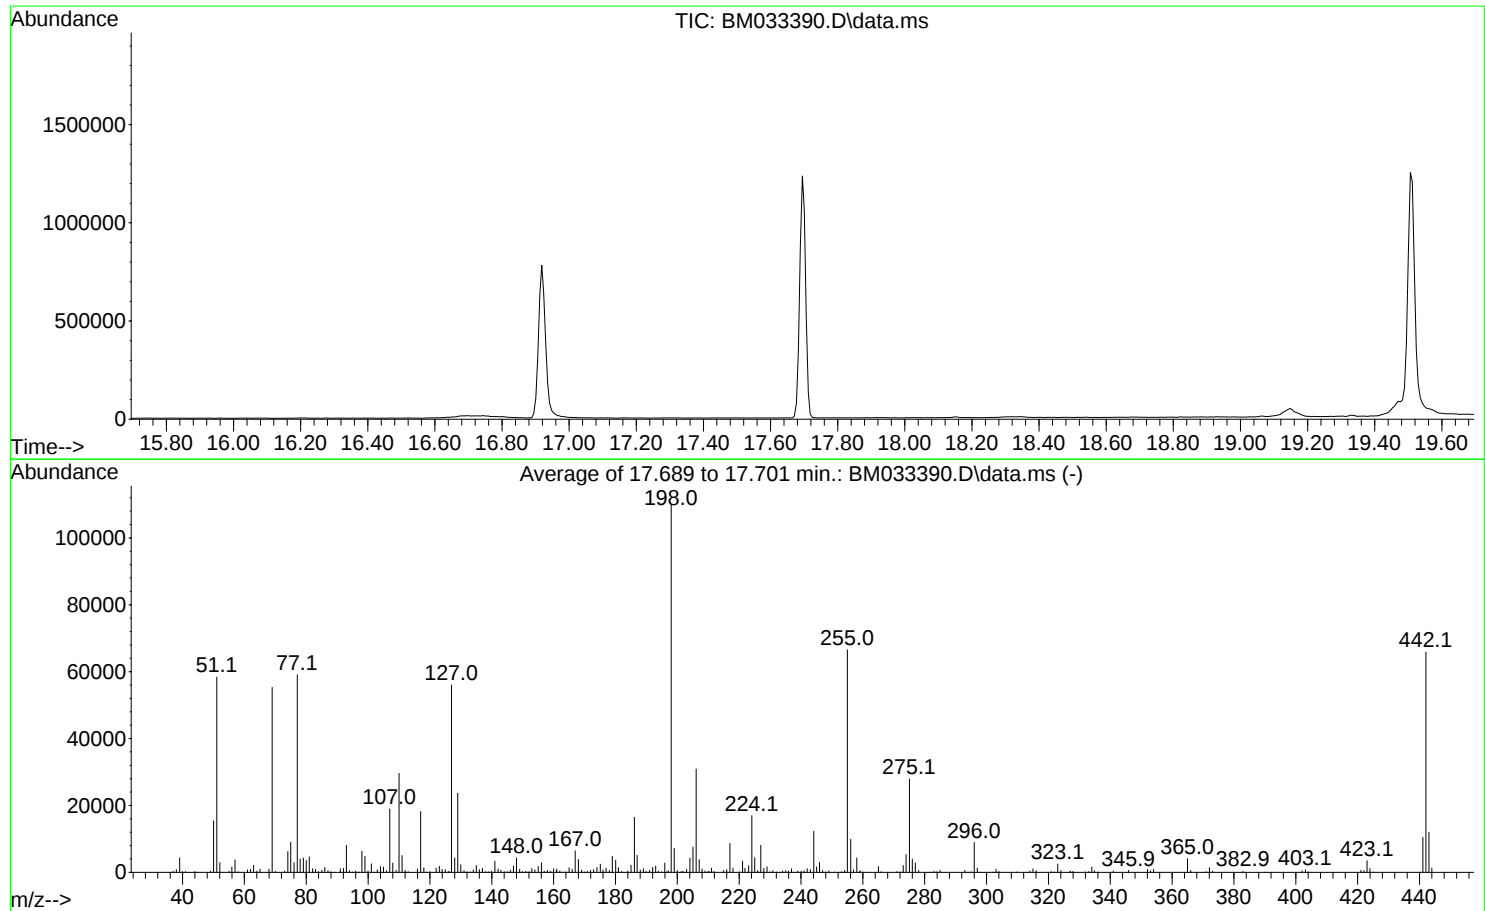




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2451

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 53.1         | 58363      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 940        | PASS                |
| 69             | 198             | 0.00            | 100             | 50.3         | 55312      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 292        | PASS                |
| 127            | 198             | 10              | 80              | 50.9         | 55997      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 461        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 109981     | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 7168       | PASS                |
| 275            | 198             | 10              | 60              | 25.4         | 27896      | PASS                |
| 365            | 198             | 1               | 100             | 3.7          | 4062       | PASS                |
| 441            | 198             | 0.01            | 100             | 9.5          | 10461      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 65883      | PASS                |
| 443            | 442             | 15              | 24              | 18.2         | 11988      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121021\  
Data File : BM033390.D  
Acq On : 10 Dec 2021 12:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Dec 11 02:22:13 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM120821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 09 07:11:07 2021  
Response via : Initial Calibration

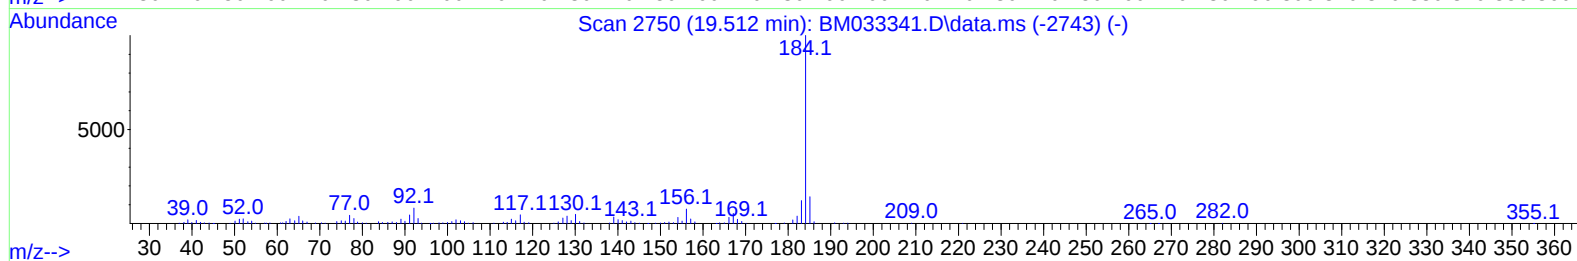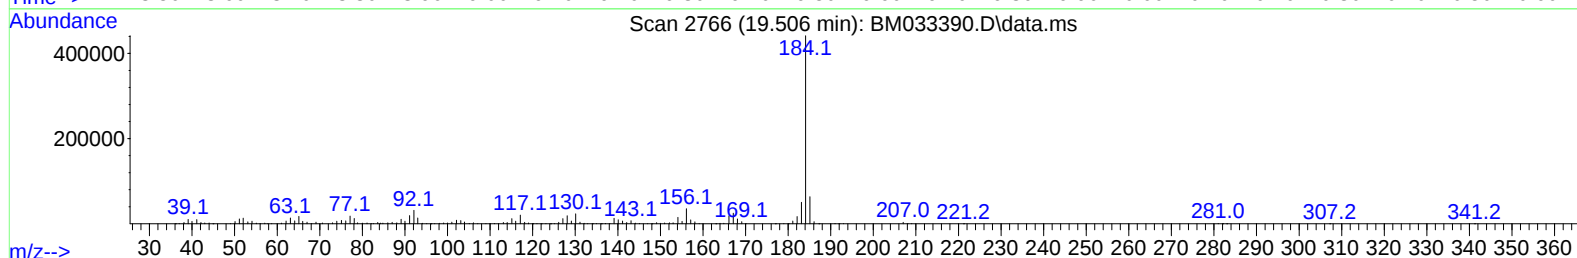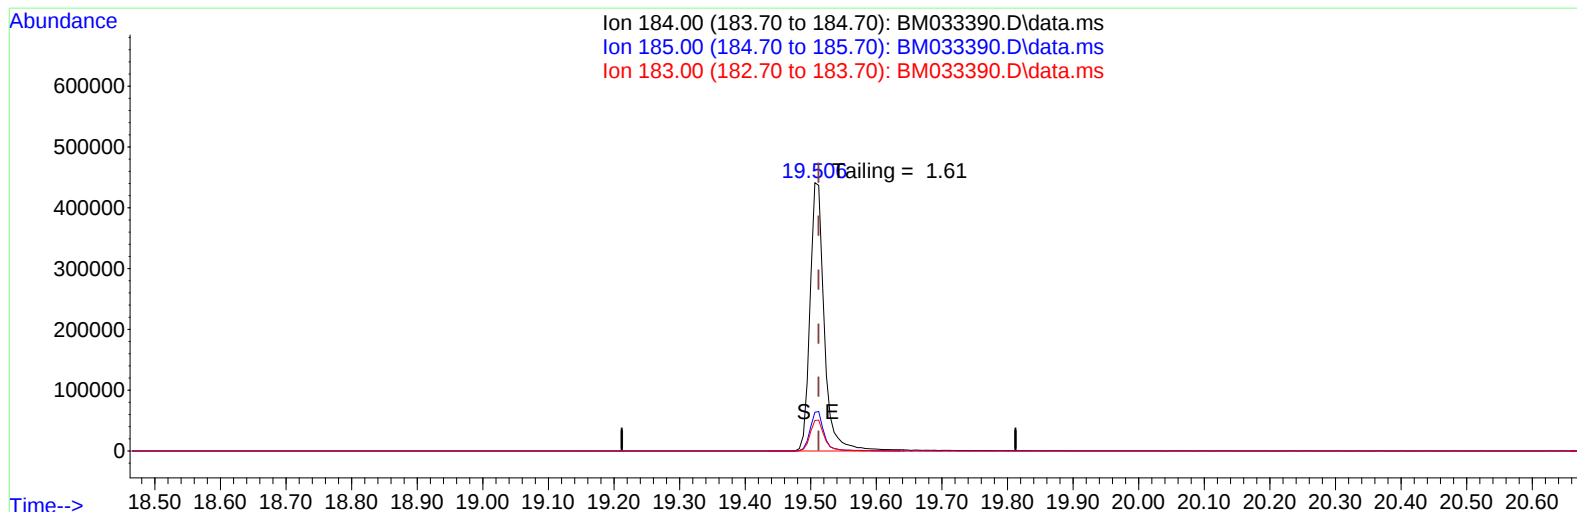

TIC: BM033390.D\data.ms

(77) Benzidine

19.506min (-0.006) 0.00 ng




response 675221

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.43  |
| 183.00 | 12.10  | 11.43  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM121021\  
Data File : BM033390.D  
Acq On : 10 Dec 2021 12:18  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Dec 11 02:22:13 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM120821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Dec 09 07:11:07 2021  
Response via : Initial Calibration

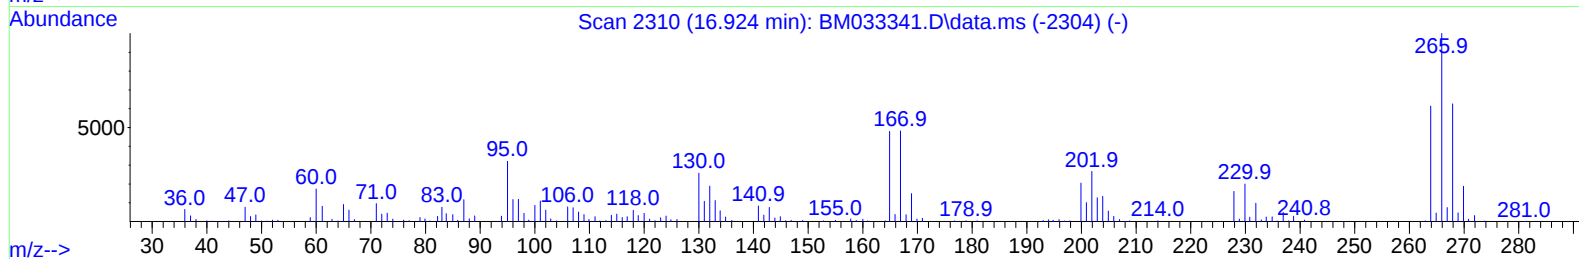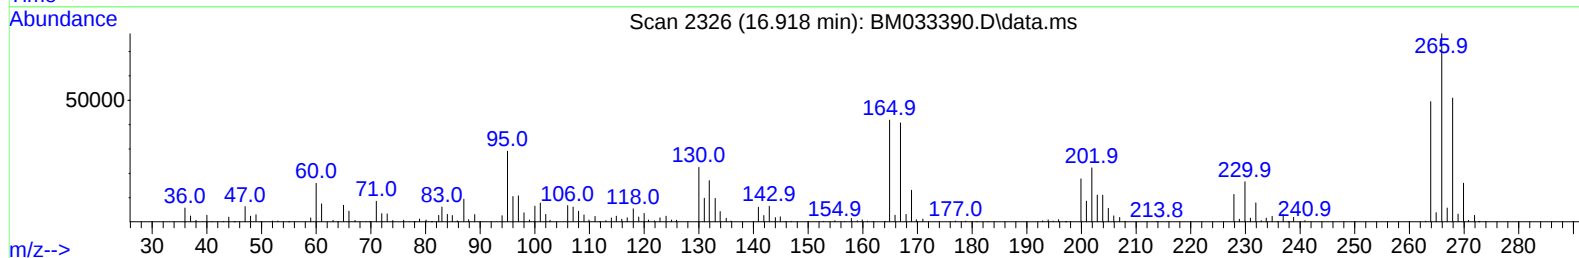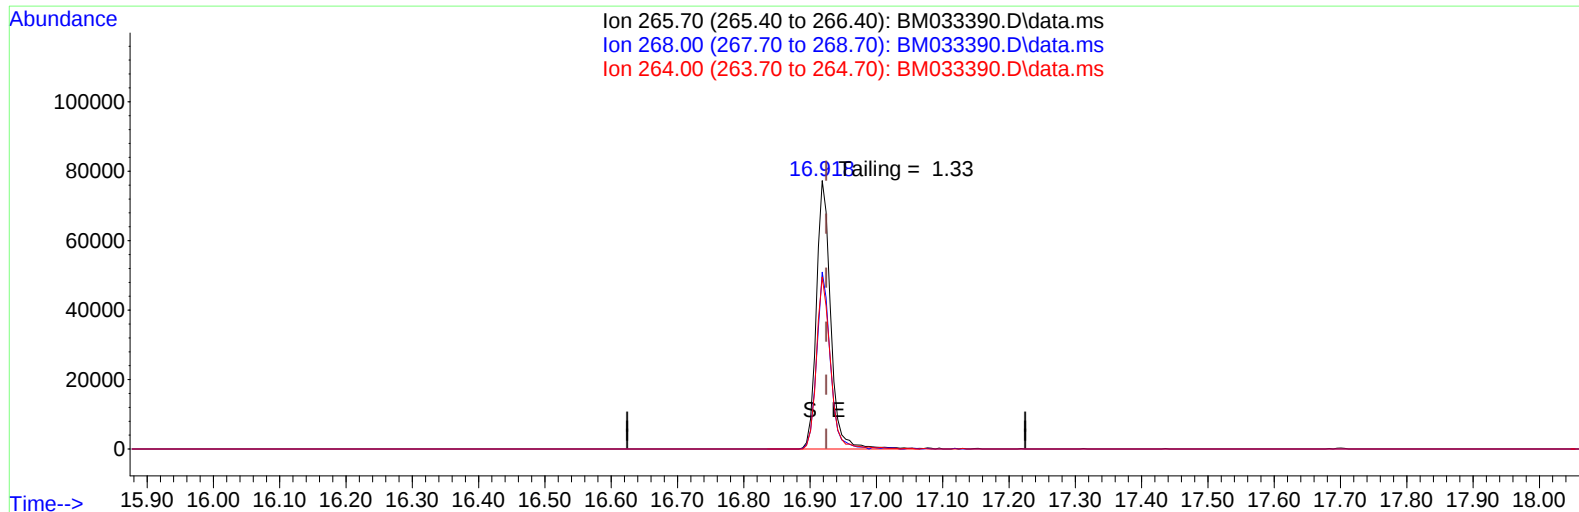

TIC: BM033390.D\data.ms

**(70) Pentachlorophenol (C)**

16.918min (-0.006) 0.00 ng

response 116548

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 65.88  |
| 264.00 | 61.40  | 64.01  |
| 0.00   | 0.00   | 0.00   |

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 12/10/2021    | BNA_M            | <u>BM033390.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 359784           | 20.73              |
| DDD           | 823              | 20.29              |
| DDE           | 0                | 19.9               |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 823           | 360607           | 0.23               |
|               |                  |                    |