

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM121115\  
 Data File : BM003499.D  
 Acq On : 12 Dec 2015 01:30  
 Operator : UM/IZ  
 Sample : G4734-17  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 A4KX8

Quant Time: Dec 12 02:19:01 2015  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM02.2-EPA-BM120115.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Sat Dec 12 00:54:45 2015  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.72  | 152  | 1831     | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.51 | 136  | 9487     | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.37 | 164  | 5280     | 20.00 | ng/ul | 0.00     |
| 62) Phenanthrene-d10      | 17.12 | 188  | 9847     | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.31 | 240  | 9026     | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.56 | 264  | 8443     | 20.00 | ng/ul | -0.01    |

## System Monitoring Compounds

|                                |       |     |        |         |       |      |
|--------------------------------|-------|-----|--------|---------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.18  | 96  | 1897   | 51.48   | ng/uL | 0.00 |
| 5) Phenol-d5                   | 6.89  | 99  | 40041  | 273.92  | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 7.05  | 67  | 109421 | 1356.89 | ng/ul | 0.00 |
| 9) 2-Chlorophenol-d4           | 7.25  | 132 | 132833 | 1099.07 | ng/ul | 0.00 |
| 13) 4-Methylphenol-d8          | 8.42  | 113 | 82680  | 674.22  | ng/ul | 0.00 |
| 19) Nitrobenzene-d5            | 8.87  | 128 | 82983  | 1282.36 | ng/ul | 0.00 |
| 22) 2-Nitrophenol-d4           | 9.60  | 143 | 89412  | 1321.67 | ng/ul | 0.00 |
| 26) 2,4-Dichlorophenol-d3      | 10.13 | 165 | 154377 | 1150.80 | ng/ul | 0.00 |
| 29) 4-Chloroaniline-d4         | 10.65 | 131 | 8483   | 55.89   | ng/ul | 0.00 |
| 44) Dimethylphthalate-d6       | 13.78 | 166 | 510011 | 1284.81 | ng/ul | 0.00 |
| 47) Acenaphthylene-d8          | 14.06 | 160 | 621018 | 1272.77 | ng/ul | 0.00 |
| 52) 4-Nitrophenol-d4           | 14.57 | 143 | 9687   | 136.15  | ng/ul | 0.00 |
| 58) Fluorene-d10               | 15.36 | 176 | 436840 | 1278.87 | ng/ul | 0.00 |
| 63) 4,6-Dinitro-2-methylphenol | 15.49 | 200 | 53442  | 1060.78 | ng/ul | 0.00 |
| 71) Anthracene-d10             | 17.22 | 188 | 603230 | 1378.85 | ng/ul | 0.00 |
| 79) Pyrene-d10                 | 19.52 | 212 | 615437 | 1392.82 | ng/ul | 0.00 |
| 90) Benzo(a)pyrene-d12         | 23.42 | 264 | 557863 | 1369.47 | ng/ul | 0.00 |

## Target Compounds

|                                |       |     |         |               | Qvalue |
|--------------------------------|-------|-----|---------|---------------|--------|
| 6) Phenol                      | 6.92  | 94  | 14995   | 97.16 ng/ul   | 98     |
| 8) Bis(2-Chloroethyl)ether     | 7.15  | 93  | 522     | 4.39 ng/ul#   | 71     |
| 12) 2,2'-oxybis(1-Chloropropan | 8.42  | 45  | 249     | 2.10 ng/ul#   | 60     |
| 15) N-Nitroso-di-n-propylamine | 8.42  | 70  | 1727    | 19.48 ng/ul#  | 1      |
| 16) 4-Methylphenol             | 8.48  | 108 | 982     | 7.38 ng/ul    | 94     |
| 20) Nitrobenzene               | 8.87  | 77  | 375     | 2.51 ng/ul#   | 37     |
| 21) Isophorone                 | 9.60  | 82  | 6860    | 24.57 ng/ul#  | 66     |
| 28) Naphthalene                | 10.56 | 128 | 2577501 | 5380.64 ng/ul | 99     |
| 34) 2-Methylnaphthalene        | 12.18 | 142 | 4042    | 11.55 ng/ul   | 93     |
| 35) 1-Methylnaphthalene        | 12.40 | 142 | 1692    | 5.12 ng/ul#   | 94     |
| 39) 2,4,6-Trichlorophenol      | 12.87 | 196 | 253     | 2.44 ng/ul#   | 12     |
| 40) 2,4,5-Trichlorophenol      | 12.87 | 196 | 253     | 2.21 ng/ul#   | 11     |
| 46) 2,6-Dinitrotoluene         | 13.78 | 165 | 2985    | 39.84 ng/ul#  | 35     |
| 50) Acenaphthene               | 14.43 | 153 | 1553    | 4.36 ng/ul    | 89     |
| 54) Dibenzofuran               | 14.77 | 168 | 1974    | 3.91 ng/ul    | 94     |
| 59) Fluorene                   | 15.42 | 166 | 2781    | 7.11 ng/ul#   | 85     |
| 65) N-Nitrosodiphenylamine     | 15.49 | 169 | 387     | 1.29 ng/ul#   | 24     |
| 70) Phenanthrene               | 17.16 | 178 | 7919    | 14.61 ng/ul   | 100    |
| 72) Anthracene                 | 17.16 | 178 | 7919    | 14.49 ng/ul   | 99     |
| 75) Carbazole                  | 17.52 | 167 | 2430    | 5.14 ng/ul#   | 87     |
| 77) Fluoranthene               | 19.18 | 202 | 1117    | 2.04 ng/ul#   | 73     |
| 80) Pyrene                     | 19.54 | 202 | 725     | 1.24 ng/ul#   | 69     |
| 84) Bis(2-ethylhexyl)phthalate | 21.23 | 149 | 2894    | 10.93 ng/ul#  | 96     |

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM121115\  
Data File : BM003499.D  
Acq On : 12 Dec 2015 01:30  
Operator : UM/IZ  
Sample : G4734-17  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
A4KX8

Quant Time: Dec 12 02:19:01 2015  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM02.2-EPA-BM120115.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Dec 12 00:54:45 2015  
Response via : Initial Calibration


| Internal Standards | R.T.  | QIon | Response | Conc | Units  | Dev(Min) |
|--------------------|-------|------|----------|------|--------|----------|
| 91) Benzo(a)pyrene | 23.42 | 252  | 1569     | 3.28 | ng/ul# | 61       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_M\DATA\BM121115\  
Data File : BM003499.D  
Acq On : 12 Dec 2015 01:30  
Operator : UM/IZ  
Sample : G4734-17  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
A4KX8

Quant Time: Dec 12 02:19:01 2015  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\SOM02.2-EPA-BM120115.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Sat Dec 12 00:54:45 2015  
Response via : Initial Calibration

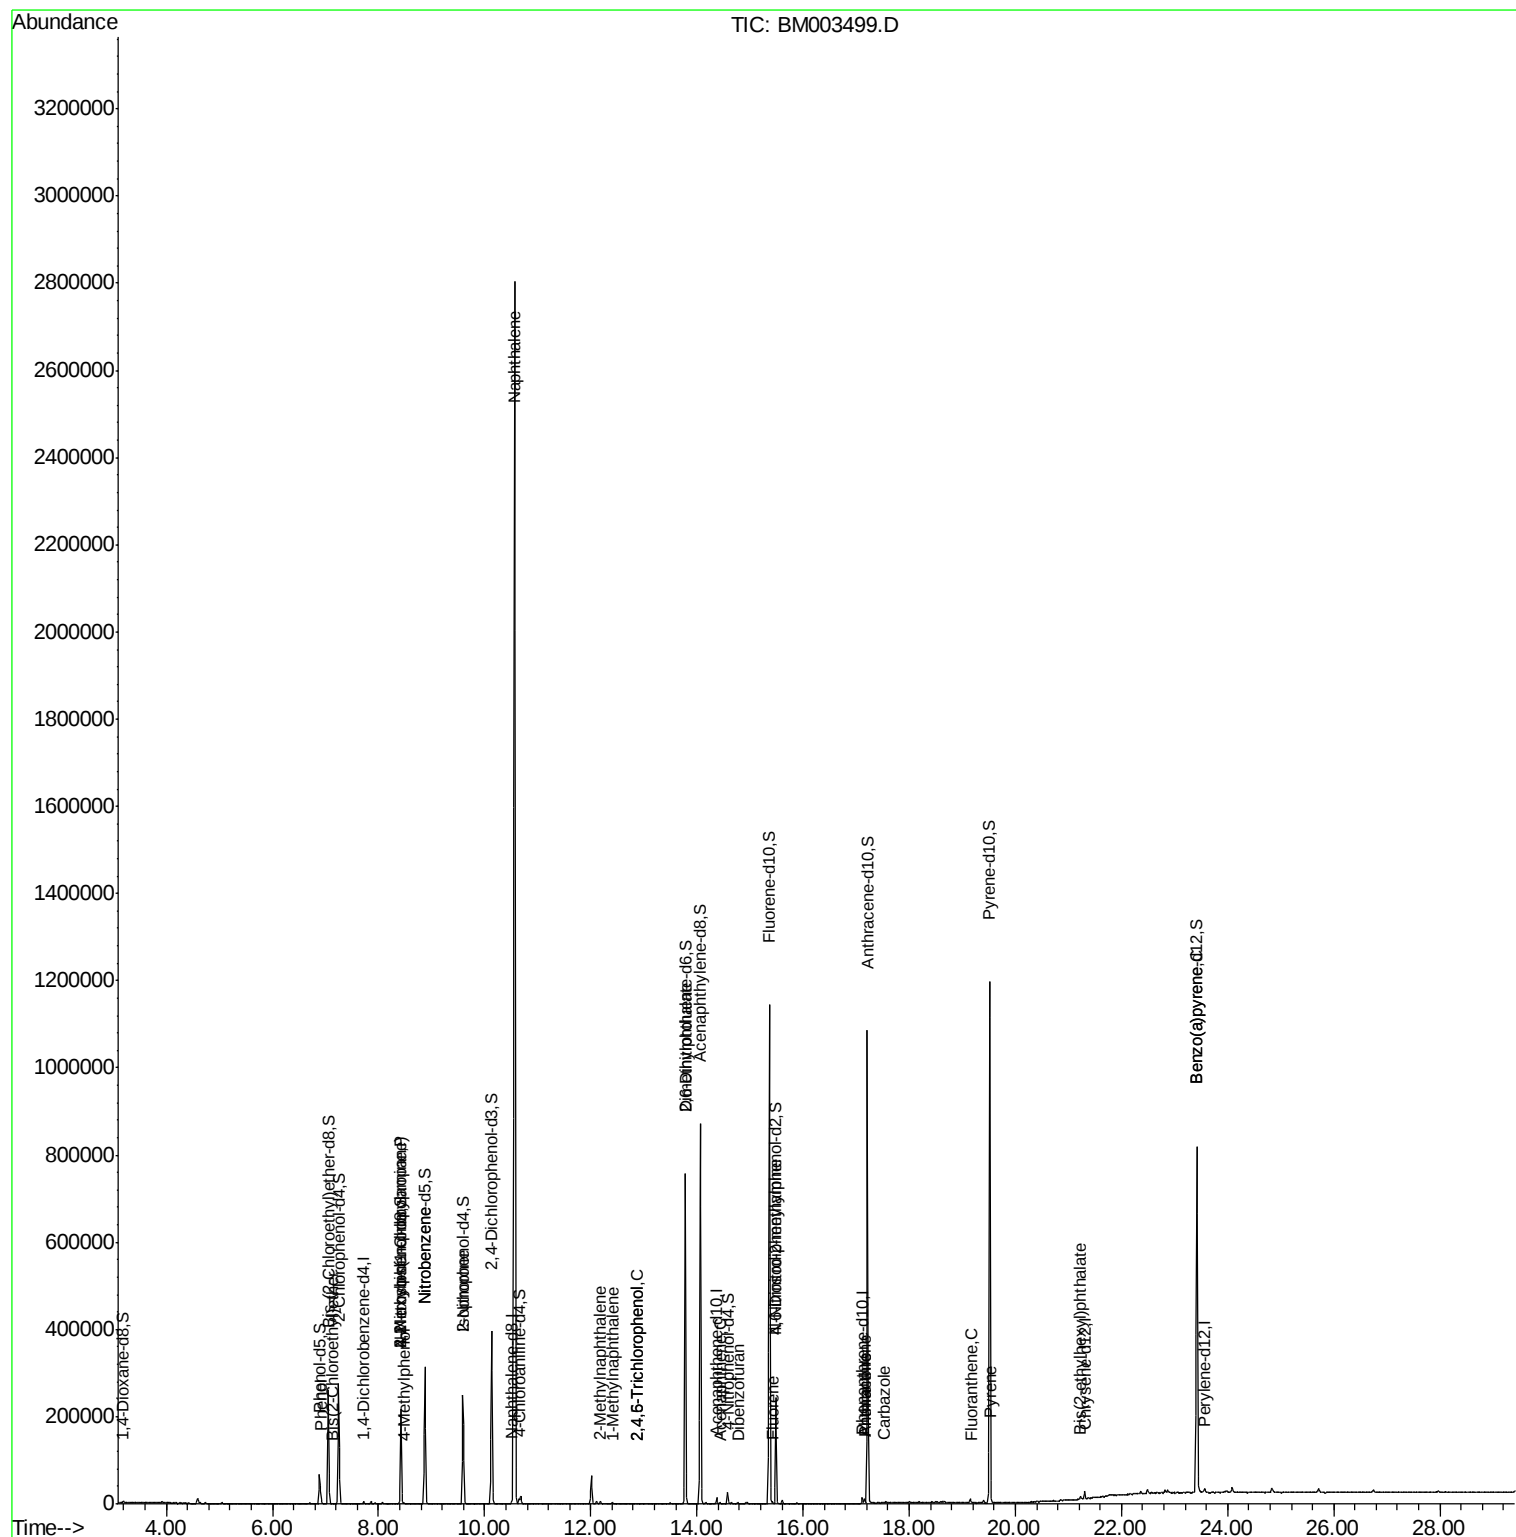



#6

Phenol

Concen: 97.16 ng/ul

RT: 6.92 min Scan# 651

Delta R.T. -0.00 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30

Instrument :

BNA\_M

ClientSampleId :

A4KX8


Tgt Ion: 94 Resp: 14995

Ion Ratio Lower Upper

94 100

65 25.0 20.6 30.8




66 35.8 27.4 41.0

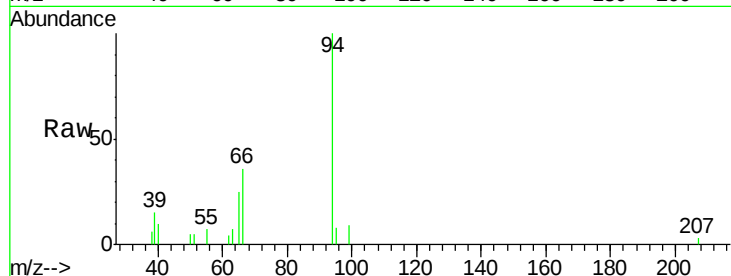

Abundance Ion 94.00 (93.70 to 94.70): BM003485.D (-645) (-)

Ion 65.00 (64.70 to 65.70): BM003485.D (-645) (-)

Ion 66.00 (65.70 to 66.70): BM003485.D (-645) (-)

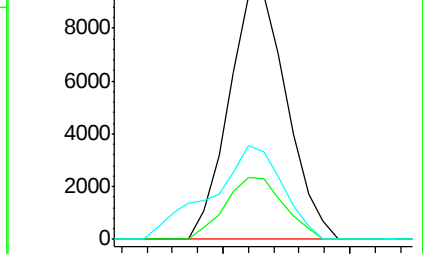

#8

Bis(2-Chloroethyl)ether

Concen: 4.39 ng/ul

RT: 7.15 min Scan# 690

Delta R.T. -0.00 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30


Tgt Ion: 93 Resp: 522

Ion Ratio Lower Upper

93 100

63 54.4 52.9 79.3



95 0.0 26.1 39.1#




Abundance Ion 93.00 (92.70 to 93.70): BM003485.D (-684) (-)

Ion 63.00 (62.70 to 63.70): BM003485.D (-684) (-)

Ion 95.00 (94.70 to 95.70): BM003485.D (-684) (-)

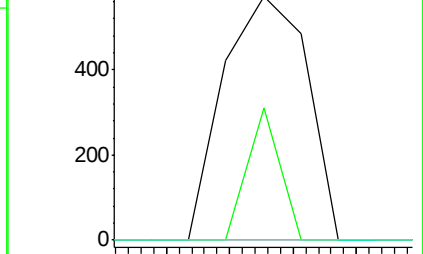


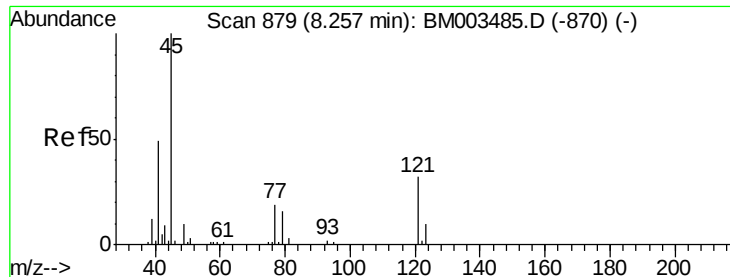




#12  
 2,2'-oxybis(1-Chloropropane)  
 Concen: 2.10 ng/ul  
 RT: 8.42 min Scan# 907  
 Delta R.T. 0.16 min  
 Lab File: BM003499.D  
 Acq: 12 Dec 2015 01:30

Instrument :  
 BNA\_M  
 ClientSampleId :  
 A4KX8

Tgt Ion: 45 Resp: 249  
 Ion Ratio Lower Upper  
 45 100  
 77 0.0 15.2 22.8#  
 79 0.0 12.3 18.5#

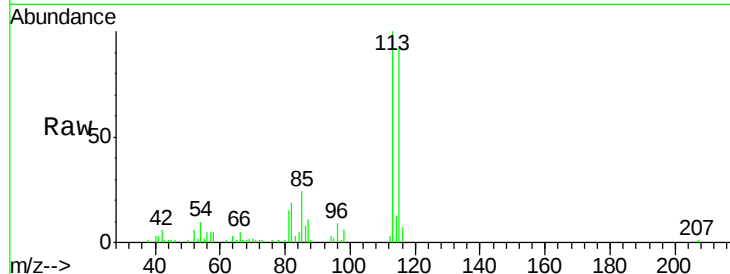


Abundance Ion 45.00 (44.70 to 45.70): BM0  
 Ion 77.00 (76.70 to 77.70): BM0  
 Ion 79.00 (78.70 to 79.70): BM0

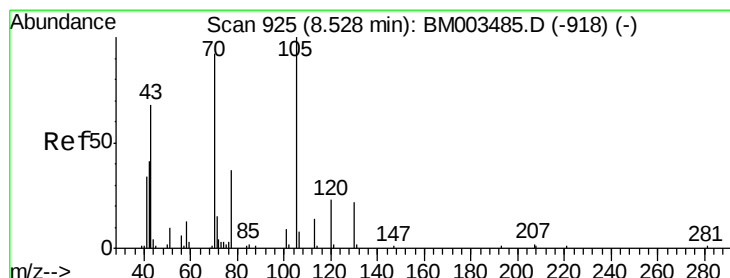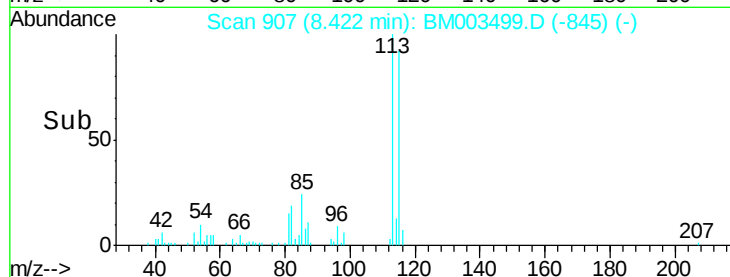
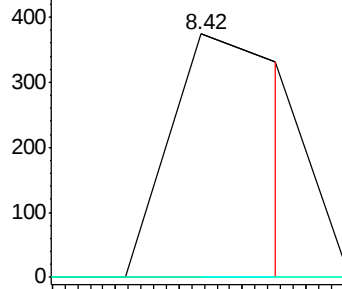



#15  
 N-Nitroso-di-n-propylamine  
 Concen: 19.48 ng/ul  
 RT: 8.42 min Scan# 907  
 Delta R.T. -0.11 min  
 Lab File: BM003499.D  
 Acq: 12 Dec 2015 01:30

Tgt Ion: 70 Resp: 1727  
 Ion Ratio Lower Upper  
 70 100  
 42 283.1 35.0 52.6#  
 101 0.0 8.6 13.0#  
 130 0.0 18.6 27.8#

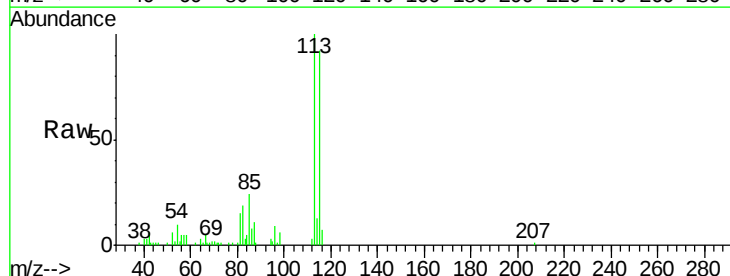

Abundance Ion 70.00 (69.70 to 70.70): BM0  
 Ion 42.00 (41.70 to 42.70): BM0  
 Ion 101.00 (100.70 to 101.70): E  
 Ion 130.00 (129.70 to 130.70): E

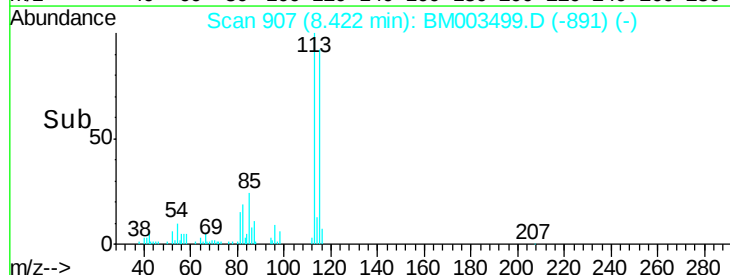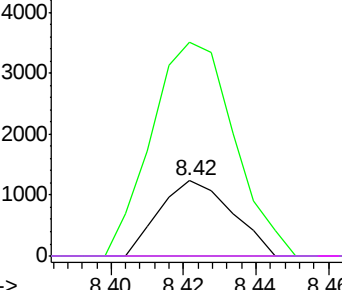

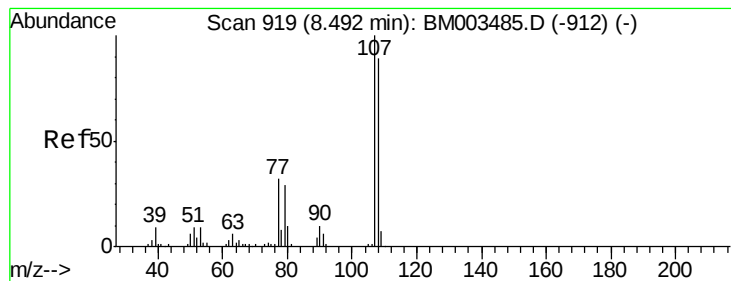

#16

4-Methylphenol

Concen: 7.38 ng/ul

RT: 8.48 min Scan# 917

Delta R.T. -0.01 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30

Instrument :

BNA\_M

ClientSampleId :


A4KX8

Tgt Ion: 108 Resp: 982

Ion Ratio Lower Upper




108 100

107 116.7 88.2 132.4



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

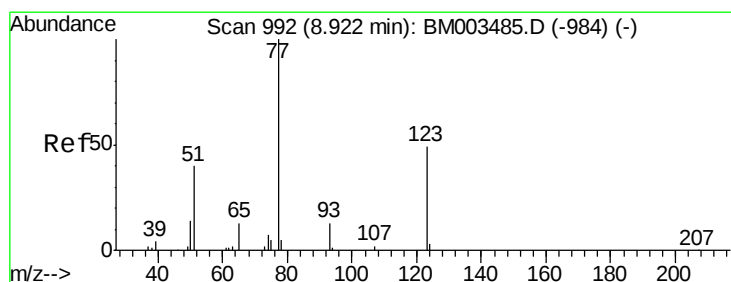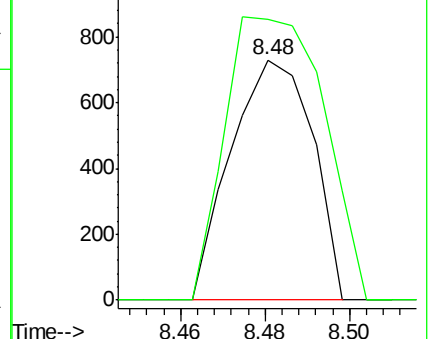

#20

Nitrobenzene

Concen: 2.51 ng/ul

RT: 8.87 min Scan# 984

Delta R.T. -0.05 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30


Tgt Ion: 77 Resp: 375

Ion Ratio Lower Upper

77 100

123 0.0 37.8 56.8#



65 0.0 9.8 14.8#

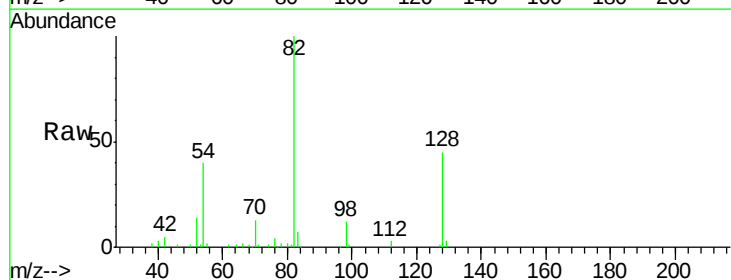


Abundance Ion 77.00 (76.70 to 77.70): BM0

Ion 123.00 (122.70 to 123.70): E

Ion 65.00 (64.70 to 65.70): BM0




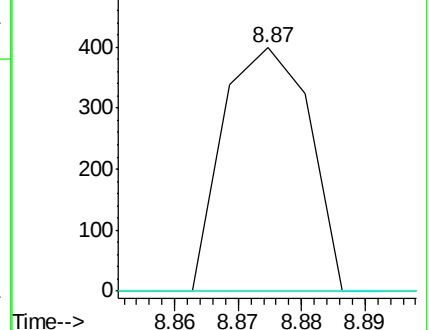




#21  
Isophorone  
Concen: 24.57 ng/ul  
RT: 9.60 min Scan# 1107  
Delta R.T. 0.16 min  
Lab File: BM003499.D  
Acq: 12 Dec 2015 01:30




Instrument :  
BNA\_M  
ClientSampleId :  
A4KX8


Tgt Ion: 82 Resp: 6860  
Ion Ratio Lower Upper  
82 100  
95 11.0 5.8 8.8#  
138 0.0 15.5 23.3#

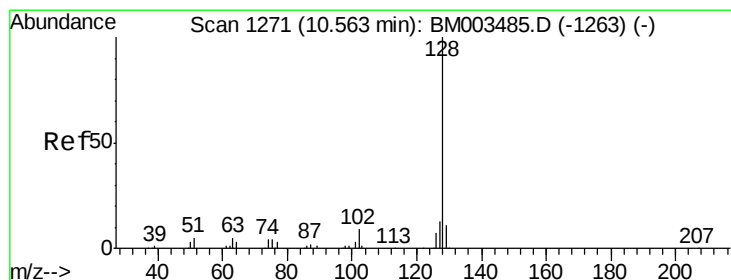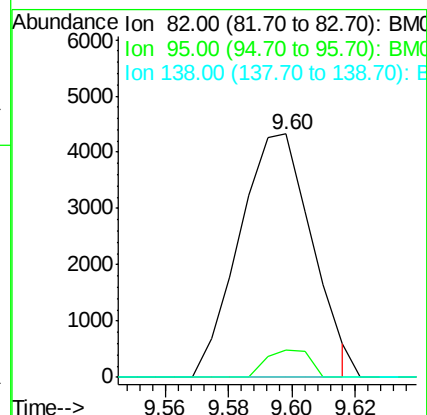

#28  
Naphthalene  
Concen: 5380.64 ng/ul  
RT: 10.56 min Scan# 1271  
Delta R.T. -0.00 min  
Lab File: BM003499.D  
Acq: 12 Dec 2015 01:30

Tgt Ion: 128 Resp: 2577501  
Ion Ratio Lower Upper  
128 100  
129 11.2 8.6 12.8  
127 13.3 10.3 15.5



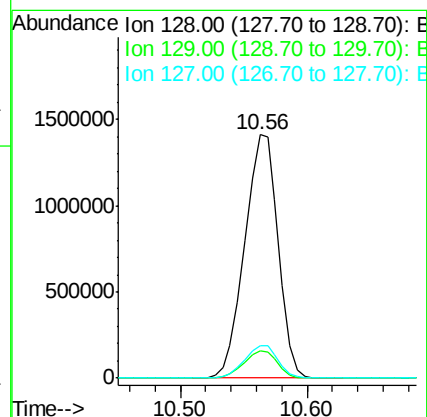
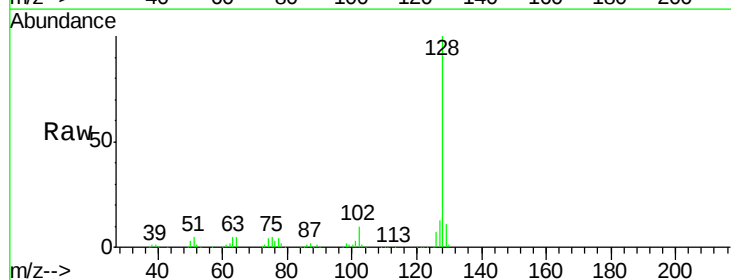


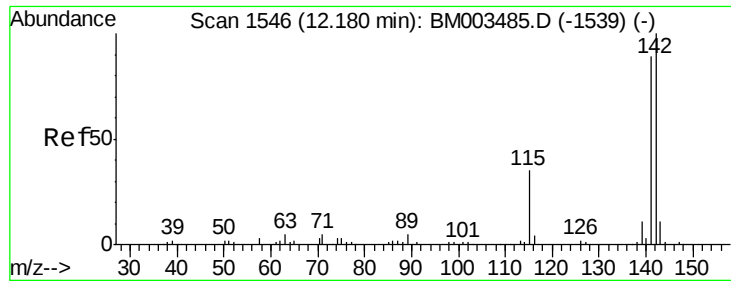

#34  
 2-Methylnaphthalene  
 Concen: 11.55 ng/ul  
 RT: 12.18 min Scan# 1546  
 Delta R.T. -0.00 min  
 Lab File: BM003499.D  
 Acq: 12 Dec 2015 01:30




Instrument :  
 BNA\_M  
 ClientSampleId :  
 A4KX8


Tgt Ion:142 Resp: 4042  
 Ion Ratio Lower Upper  
 142 100  
 141 81.3 70.5 105.7

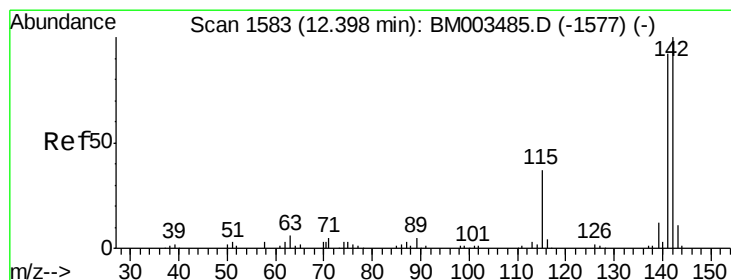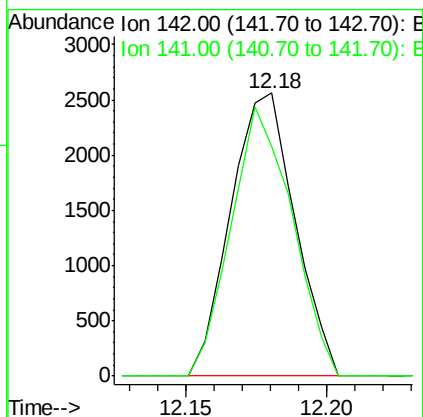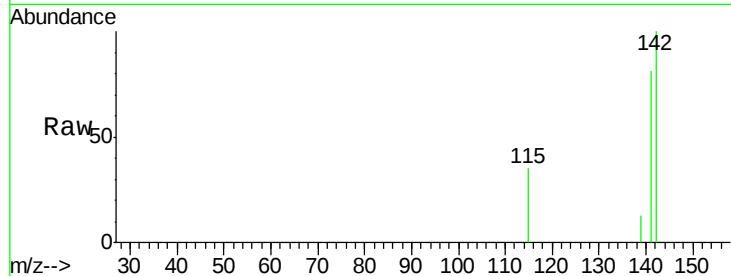

#35  
 1-Methylnaphthalene  
 Concen: 5.12 ng/ul  
 RT: 12.40 min Scan# 1583  
 Delta R.T. -0.00 min  
 Lab File: BM003499.D  
 Acq: 12 Dec 2015 01:30

Tgt Ion:142 Resp: 1692  
 Ion Ratio Lower Upper  
 142 100  
 141 96.8 73.2 109.8  
 116 0.0 3.0 4.6#



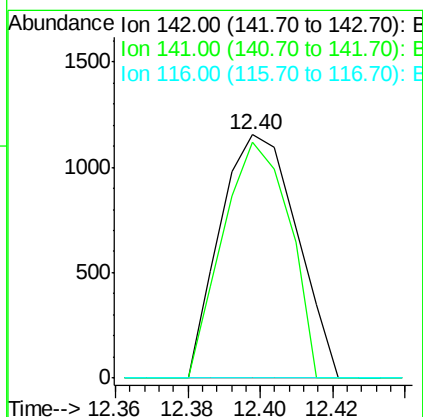
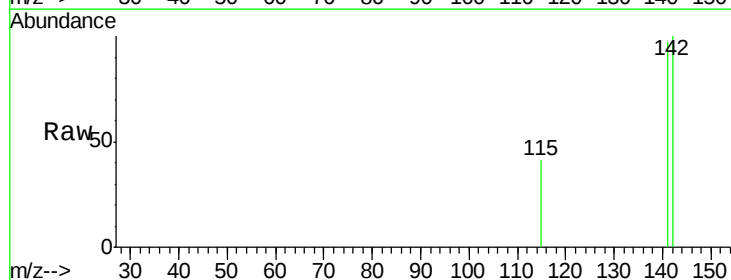




#39  
 2,4,6-Trichlorophenol  
 Concen: 2.44 ng/ul  
 RT: 12.87 min Scan# 1663  
 Delta R.T. 0.07 min  
 Lab File: BM003499.D  
 Acq: 12 Dec 2015 01:30




Instrument :  
 BNA\_M  
 ClientSampleId :  
 A4KX8


Tgt Ion:196 Resp: 253  
 Ion Ratio Lower Upper  
 196 100  
 198 0.0 76.1 114.1#  
 200 0.0 24.3 36.5#

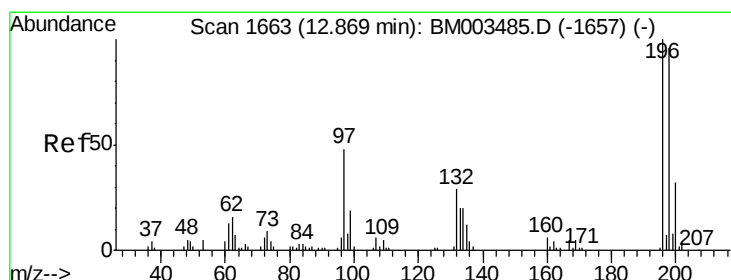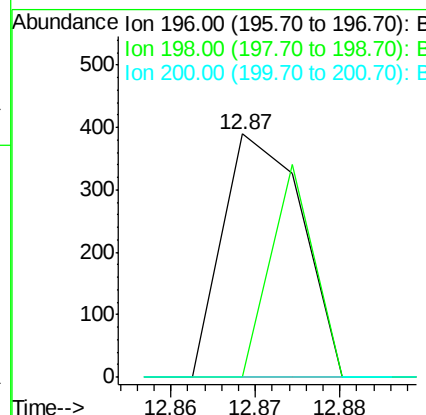

#40  
 2,4,5-Trichlorophenol  
 Concen: 2.21 ng/ul  
 RT: 12.87 min Scan# 1663  
 Delta R.T. -0.00 min  
 Lab File: BM003499.D  
 Acq: 12 Dec 2015 01:30

Tgt Ion:196 Resp: 253  
 Ion Ratio Lower Upper  
 196 100  
 198 0.0 77.8 116.8#  
 200 0.0 24.8 37.2#

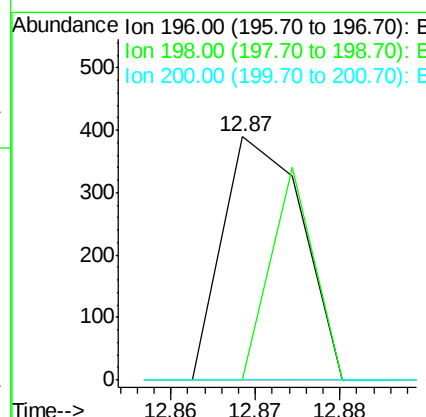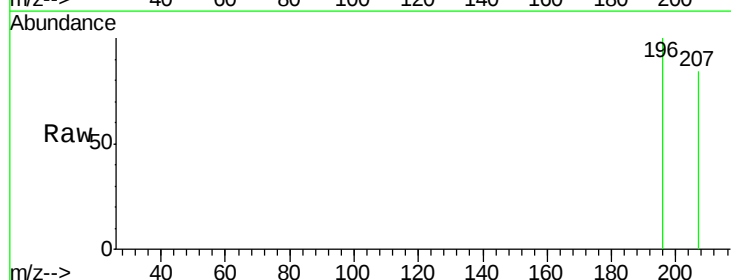



#46

2,6-Dinitrotoluene

Concen: 39.84 ng/ul

RT: 13.78 min Scan# 1818

Delta R.T. -0.17 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30

Instrument :

BNA\_M

ClientSampleId :

A4KX8


Tgt Ion:165 Resp: 2985

Ion Ratio Lower Upper

165 100

89 0.0 42.0 63.0#




121 40.7 16.6 24.8#

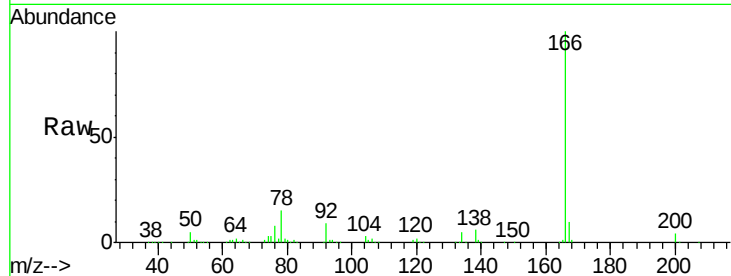

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

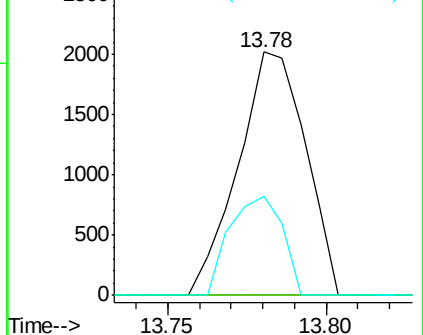

#50

Acenaphthene

Concen: 4.36 ng/ul

RT: 14.43 min Scan# 1929

Delta R.T. -0.00 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30


Tgt Ion:153 Resp: 1553

Ion Ratio Lower Upper

153 100

152 42.9 37.8 56.6



154 76.6 70.8 106.2




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

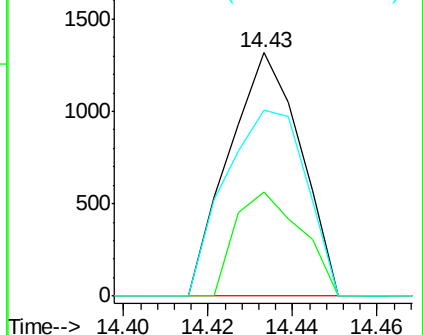



#54

Dibenzenofuran

Concen: 3.91 ng/ul

RT: 14.77 min Scan# 1986

Delta R.T. -0.00 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30

Instrument :

BNA\_M

ClientSampleId :





A4KX8

Tgt Ion:168 Resp: 1974

Ion Ratio Lower Upper

168 100

139 41.6 30.6 45.8

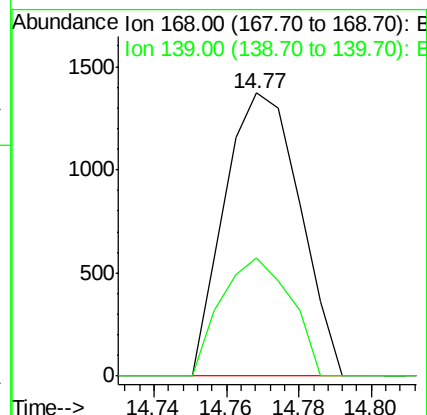

#59

Fluorene

Concen: 7.11 ng/ul

RT: 15.42 min Scan# 2097

Delta R.T. -0.00 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30




Tgt Ion:166 Resp: 2781


Ion Ratio Lower Upper

166 100

165 110.8 78.8 118.2

167 0.0 10.8 16.2#

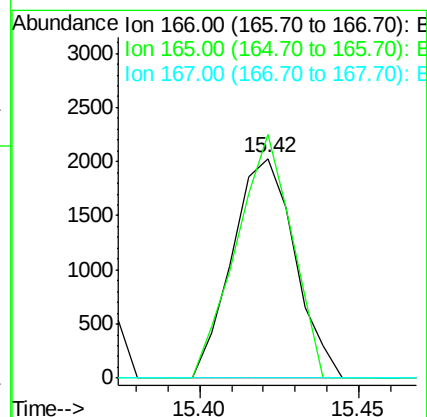



#65

N-Nitrosodiphenylamine

Concen: 1.29 ng/ul

RT: 15.49 min Scan# 2109

Delta R.T. -0.14 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30

Instrument :

BNA\_M

ClientSampleId :

A4KX8


Tgt Ion:169 Resp: 387

Ion Ratio Lower Upper

169 100

168 0.0 53.4 80.0#




167 0.0 29.0 43.4#

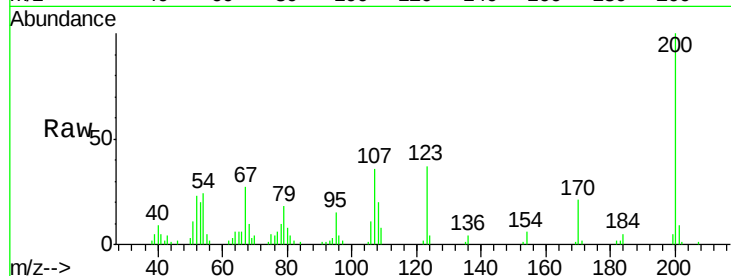

Abundance Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

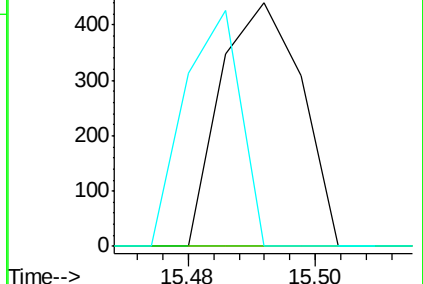

#70

Phenanthrene

Concen: 14.61 ng/ul

RT: 17.16 min Scan# 2392

Delta R.T. -0.01 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30


Tgt Ion:178 Resp: 7919

Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.2



176 19.3 15.6 23.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

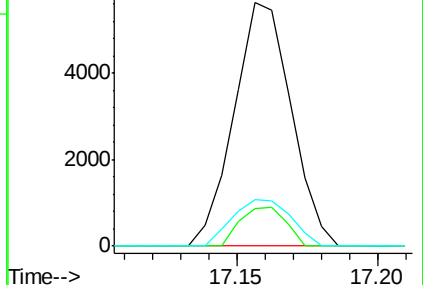

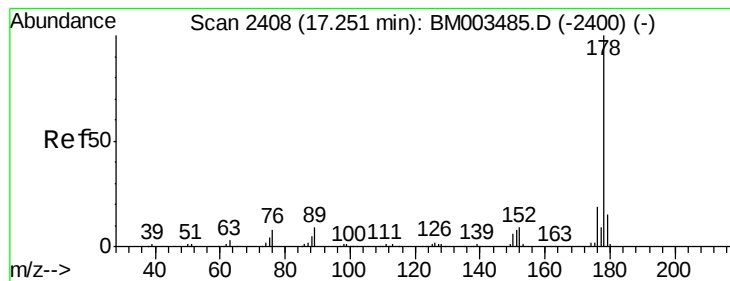

#72

Anthracene

Concen: 14.49 ng/ul

RT: 17.16 min Scan# 2392

Delta R.T. -0.09 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30

Instrument :

BNA\_M

ClientSampleId :

A4KX8


Tgt Ion:178 Resp: 7919

Ion Ratio Lower Upper

178 100

179 15.3 12.2 18.4




176 19.3 14.9 22.3

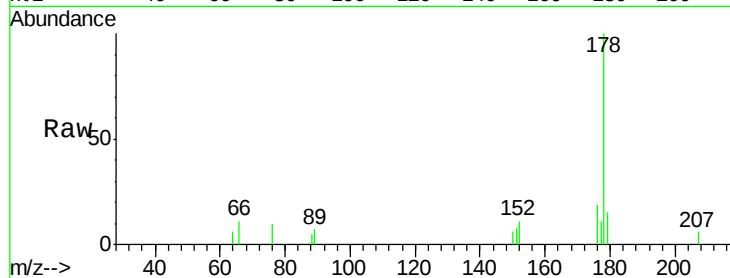

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

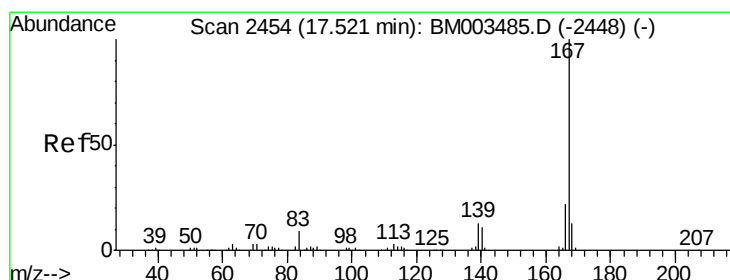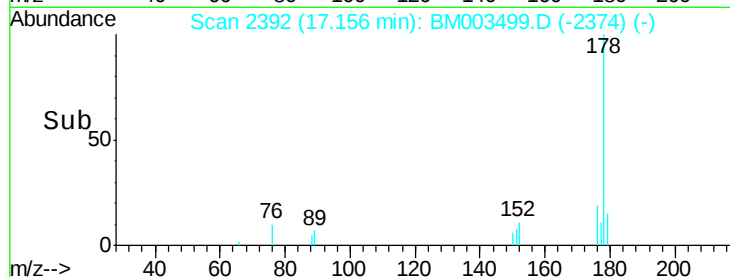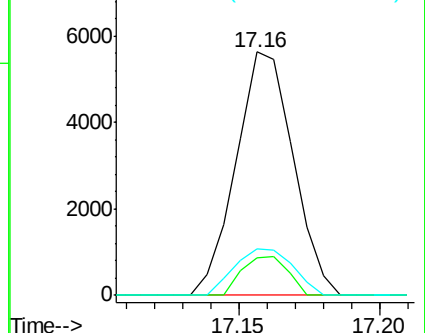

#75

Carbazole

Concen: 5.14 ng/ul

RT: 17.52 min Scan# 2454

Delta R.T. -0.00 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30


Tgt Ion:167 Resp: 2430

Ion Ratio Lower Upper

167 100

166 20.7 16.8 25.2



139 0.0 10.6 16.0#

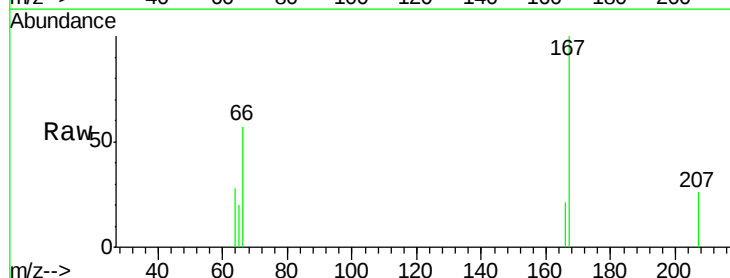


Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

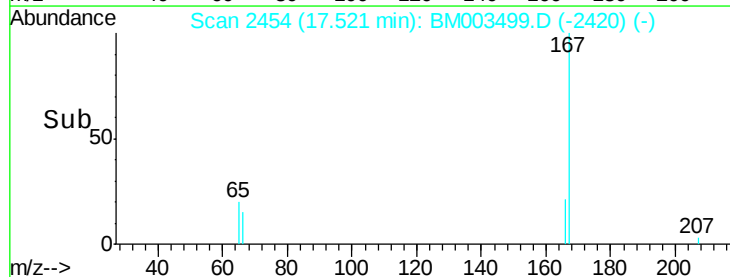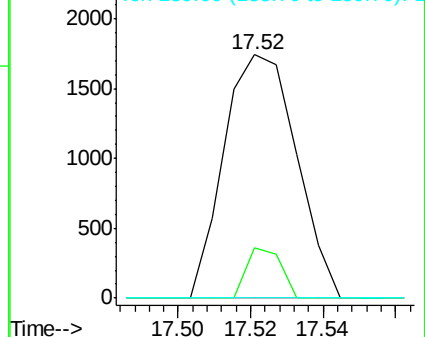


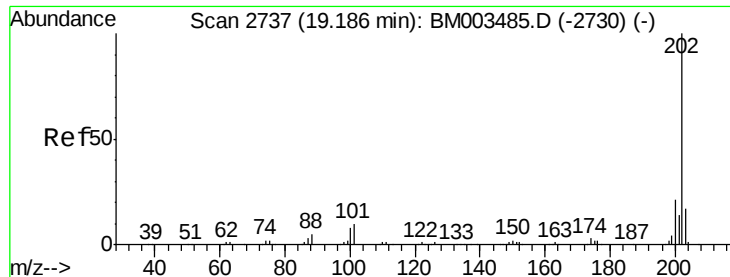




#77  
**Fluoranthene**  
 Concen: 2.04 ng/ul  
 RT: 19.18 min Scan# 2736  
 Delta R.T. -0.01 min  
 Lab File: BM003499.D  
 Acq: 12 Dec 2015 01:30

Instrument :  
 BNA\_M  
 ClientSampleId :  
 A4KX8

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 202     | 100   |       |       |
| 101     | 0.0   | 9.2   | 13.8# |
| 100     | 0.0   | 7.0   | 10.4# |

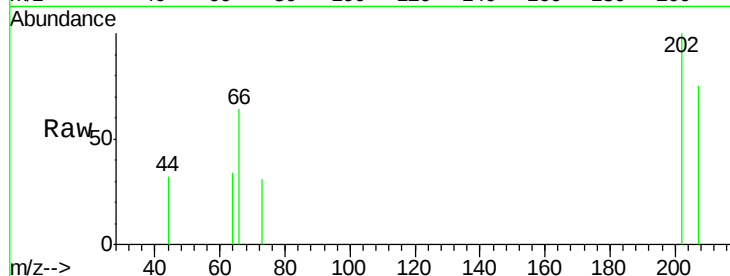


Abundance Ion 202.00 (201.70 to 202.70): E  
 Ion 101.00 (100.70 to 101.70): E  
 Ion 100.00 (99.70 to 100.70): B

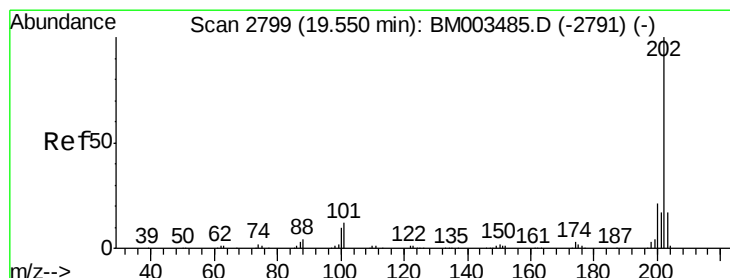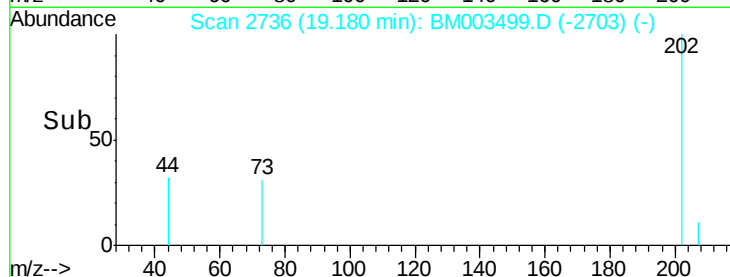
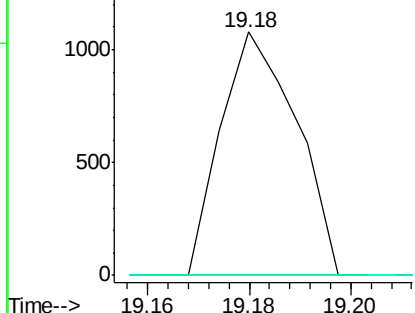



#80  
**Pyrene**  
 Concen: 1.24 ng/ul  
 RT: 19.54 min Scan# 2798  
 Delta R.T. -0.01 min  
 Lab File: BM003499.D  
 Acq: 12 Dec 2015 01:30

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 202     | 100   |       |       |
| 101     | 0.0   | 10.6  | 16.0# |
| 100     | 0.0   | 8.5   | 12.7# |

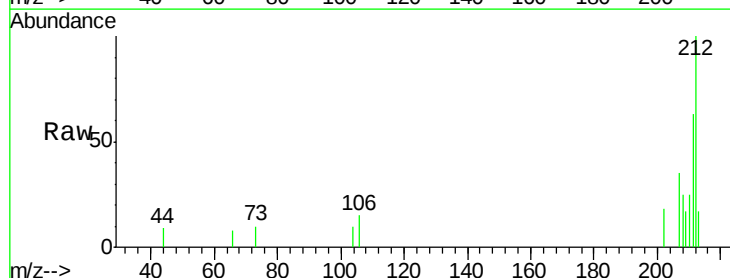

Abundance Ion 202.00 (201.70 to 202.70): E  
 Ion 101.00 (100.70 to 101.70): E  
 Ion 100.00 (99.70 to 100.70): B

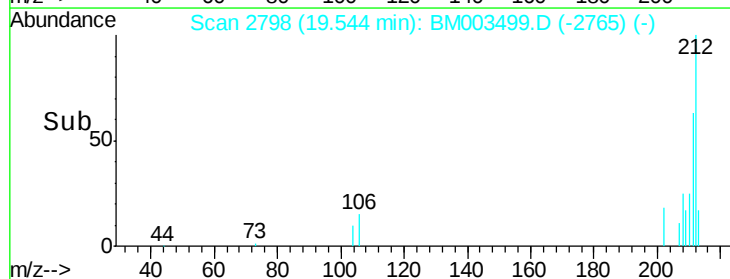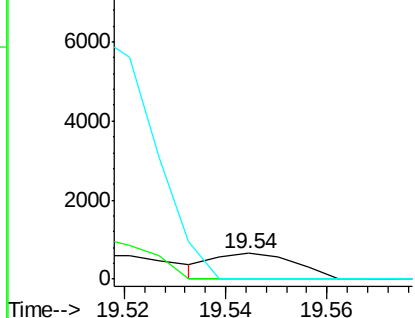



#84

Bis(2-ethylhexyl)phthalate

Concen: 10.93 ng/ul

RT: 21.23 min Scan# 3084

Delta R.T. -0.01 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30

Instrument :

BNA\_M

ClientSampleId :

A4KX8


Tgt Ion:149 Resp: 2894

Ion Ratio Lower Upper

149 100

167 25.4 21.6 32.4




279 0.0 2.9 4.3#



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

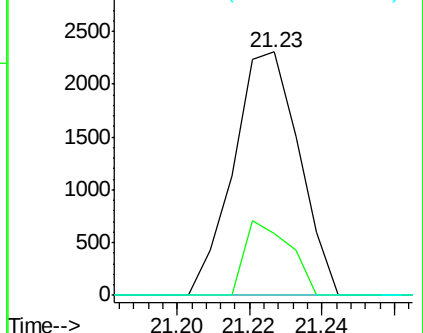

#91

Benzo(a)pyrene

Concen: 3.28 ng/ul

RT: 23.42 min Scan# 3457

Delta R.T. -0.05 min

Lab File: BM003499.D

Acq: 12 Dec 2015 01:30


Tgt Ion:252 Resp: 1569

Ion Ratio Lower Upper

252 100

253 42.2 17.4 26.2#

125 0.0 9.8 14.8#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

