

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121115\
 Data File : BM003483.D
 Acq On : 11 Dec 2015 15:17
 Operator : UM/IZ
 Sample : PB87218BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK18

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	20	rVB	2657	3276	0.18%	0.020%
2	6.887	638	646	654	rVB	61838	90624	5.03%	0.544%
3	7.051	668	674	685	rVB	206274	314732	17.46%	1.891%
4	7.251	701	708	718	rVB	225659	348838	19.35%	2.096%
5	7.722	781	788	796	rVB	256949	408695	22.67%	2.455%
6	8.422	902	907	915	rBV	178344	275900	15.30%	1.657%
7	8.540	923	927	934	rVB	6832	10313	0.57%	0.062%
8	8.875	978	984	993	rBV	258675	406550	22.55%	2.442%
9	9.598	1100	1107	1113	rVB	211802	336045	18.64%	2.019%
10	10.134	1191	1198	1211	rBV	338508	551702	30.60%	3.314%
11	10.510	1254	1262	1271	rBV	416129	690338	38.29%	4.147%
12	12.104	1528	1533	1538	rBV	4316	6554	0.36%	0.039%
13	13.780	1812	1818	1829	rBV	735928	995569	55.22%	5.981%
14	14.063	1859	1866	1880	rBV	816302	1170852	64.95%	7.034%
15	14.375	1912	1919	1930	rVB2	658165	987303	54.77%	5.931%
16	14.575	1948	1953	1964	rVB	28193	46505	2.58%	0.279%
17	15.369	2081	2088	2099	rBV	1105877	1591675	88.29%	9.562%
18	15.486	2103	2108	2116	rVV	205211	261000	14.48%	1.568%
19	15.604	2125	2128	2133	rVB	9185	11460	0.64%	0.069%
20	16.269	2236	2241	2244	rVB	3149	3753	0.21%	0.023%
21	16.910	2346	2350	2353	rBV	1673	2454	0.14%	0.015%
22	17.121	2379	2386	2393	rBV	809319	1126222	62.47%	6.766%
23	17.221	2396	2403	2418	rVV	1223000	1732226	96.09%	10.406%
24	18.086	2546	2550	2554	rVB	2278	2852	0.16%	0.017%
25	19.151	2726	2731	2736	rBV	9237	12391	0.69%	0.074%
26	19.410	2771	2775	2779	rBV	7899	9533	0.53%	0.057%
27	19.521	2788	2794	2807	rVB	1347252	1802764	100.00%	10.830%
28	19.757	2831	2834	2838	rBV3	1977	2825	0.16%	0.017%
29	20.868	3021	3023	3027	rBV2	2299	1904	0.11%	0.011%
30	21.051	3050	3054	3057	rBV2	2456	3209	0.18%	0.019%
31	21.098	3058	3062	3067	rVB	9938	11440	0.63%	0.069%
32	21.321	3094	3100	3107	rBV	824405	1014175	56.26%	6.093%
33	21.909	3197	3200	3202	rBV2	3805	4221	0.23%	0.025%
34	22.833	3354	3357	3361	rBV3	7262	10944	0.61%	0.066%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121115\
Data File : BM003483.D
Acq On : 11 Dec 2015 15:17
Operator : UM/IZ
Sample : PB87218BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK18

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION

35	22.880	3362	3365	3371	rVB3	8342	11641	0.65%	0.070%
36	23.433	3451	3459	3473	rBV	776435	1446671	80.25%	8.691%
37	23.574	3476	3483	3493	rVB2	487959	920896	51.08%	5.532%
38	24.103	3569	3573	3577	rVB3	11367	18083	1.00%	0.109%


Sum of corrected areas: 16646135

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121115\
Data File : BM003483.D
Acq On : 11 Dec 2015 15:17
Operator : UM/IZ
Sample : PB87218BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK18

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

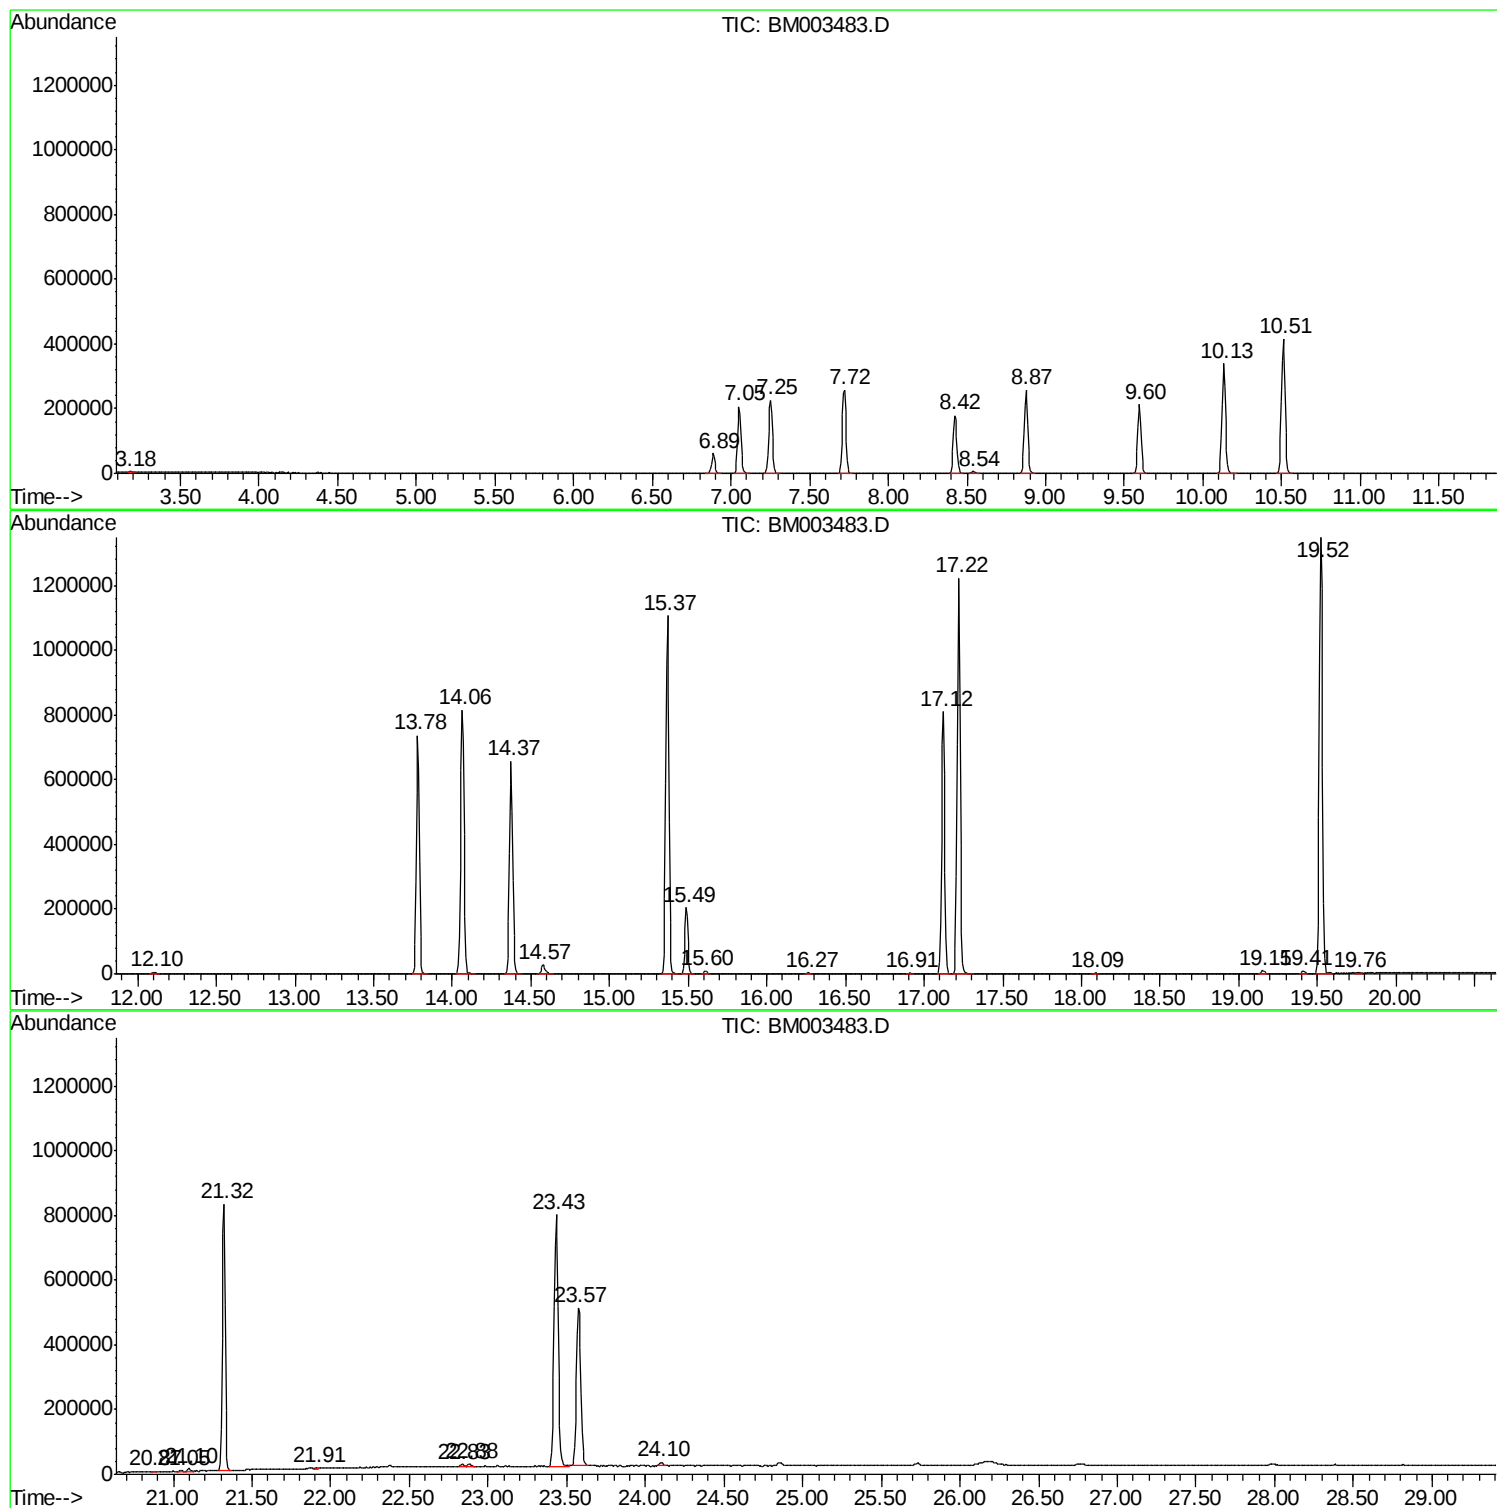

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121115\
Data File : BM003483.D
Acq On : 11 Dec 2015 15:17
Operator : UM/IZ
Sample : PB87218BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK18

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121115\
Data File : BM003483.D
Acq On : 11 Dec 2015 15:17
Operator : UM/IZ
Sample : PB87218BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK18

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc