

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121115\
 Data File : BM003487.D
 Acq On : 11 Dec 2015 18:18
 Operator : UM/IZ
 Sample : G4718-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	13	16	21	rVB	3026	4158	0.29%	0.029%
2	6.887	639	646	654	rVB	61303	89603	6.18%	0.616%
3	7.051	668	674	684	rVB	213653	323685	22.33%	2.226%
4	7.251	702	708	719	rVB	232856	354847	24.48%	2.440%
5	7.722	781	788	795	rBV	295204	455852	31.45%	3.134%
6	8.422	902	907	917	rBV	179336	276582	19.08%	1.902%
7	8.875	978	984	994	rBV	245761	384224	26.51%	2.642%
8	9.598	1101	1107	1115	rBV	191836	309532	21.36%	2.128%
9	10.134	1191	1198	1211	rBV	291679	483114	33.33%	3.322%
10	10.510	1255	1262	1273	rBV	420390	690607	47.65%	4.749%
11	10.651	1282	1286	1292	rVB	1288	1769	0.12%	0.012%
12	12.104	1530	1533	1538	rVB	3834	5502	0.38%	0.038%
13	13.780	1812	1818	1831	rBV	550065	743706	51.31%	5.114%
14	14.063	1859	1866	1879	rBV	656791	933097	64.38%	6.416%
15	14.374	1912	1919	1931	rVB2	543565	847420	58.47%	5.827%
16	14.580	1948	1954	1965	rBV	22127	37653	2.60%	0.259%
17	15.368	2081	2088	2101	rBV	841529	1192791	82.30%	8.202%
18	15.486	2103	2108	2115	rBV	161888	203885	14.07%	1.402%
19	15.604	2125	2128	2133	rBB	6301	7651	0.53%	0.053%
20	16.904	2345	2349	2354	rBV	1476	2084	0.14%	0.014%
21	17.121	2379	2386	2396	rBV	627447	901050	62.17%	6.196%
22	17.215	2396	2402	2417	rVV2	910502	1307229	90.19%	8.988%
23	19.151	2727	2731	2735	rBV	7326	8347	0.58%	0.057%
24	19.404	2770	2774	2779	rBV	5270	7251	0.50%	0.050%
25	19.521	2787	2794	2806	rBV	1053395	1449347	100.00%	9.966%
26	19.756	2829	2834	2839	rBV	3008	4033	0.28%	0.028%
27	21.045	3051	3053	3057	rVB3	2417	2793	0.19%	0.019%
28	21.092	3057	3061	3066	rBV	9169	12056	0.83%	0.083%
29	21.315	3094	3099	3107	rBV	820633	1023096	70.59%	7.035%
30	23.427	3451	3458	3472	rBV	768887	1436676	99.13%	9.879%
31	23.574	3475	3483	3495	rVB	544153	1024822	70.71%	7.047%
32	24.103	3569	3573	3578	rVB2	8308	14491	1.00%	0.100%
33	24.838	3696	3698	3699	rBV2	5787	4489	0.31%	0.031%

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121115\
Data File : BM003487.D
Acq On : 11 Dec 2015 18:18
Operator : UM/IZ
Sample : G4718-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Title : SVOA CALIBRATION


Sum of corrected areas: 14543442

Data Path : Z:\HPCHEM1\BNA M\DATA\BM121115\
Data File : BM003487.D
Acq On : 11 Dec 2015 18:18
Operator : UM/IZ
Sample : G4718-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

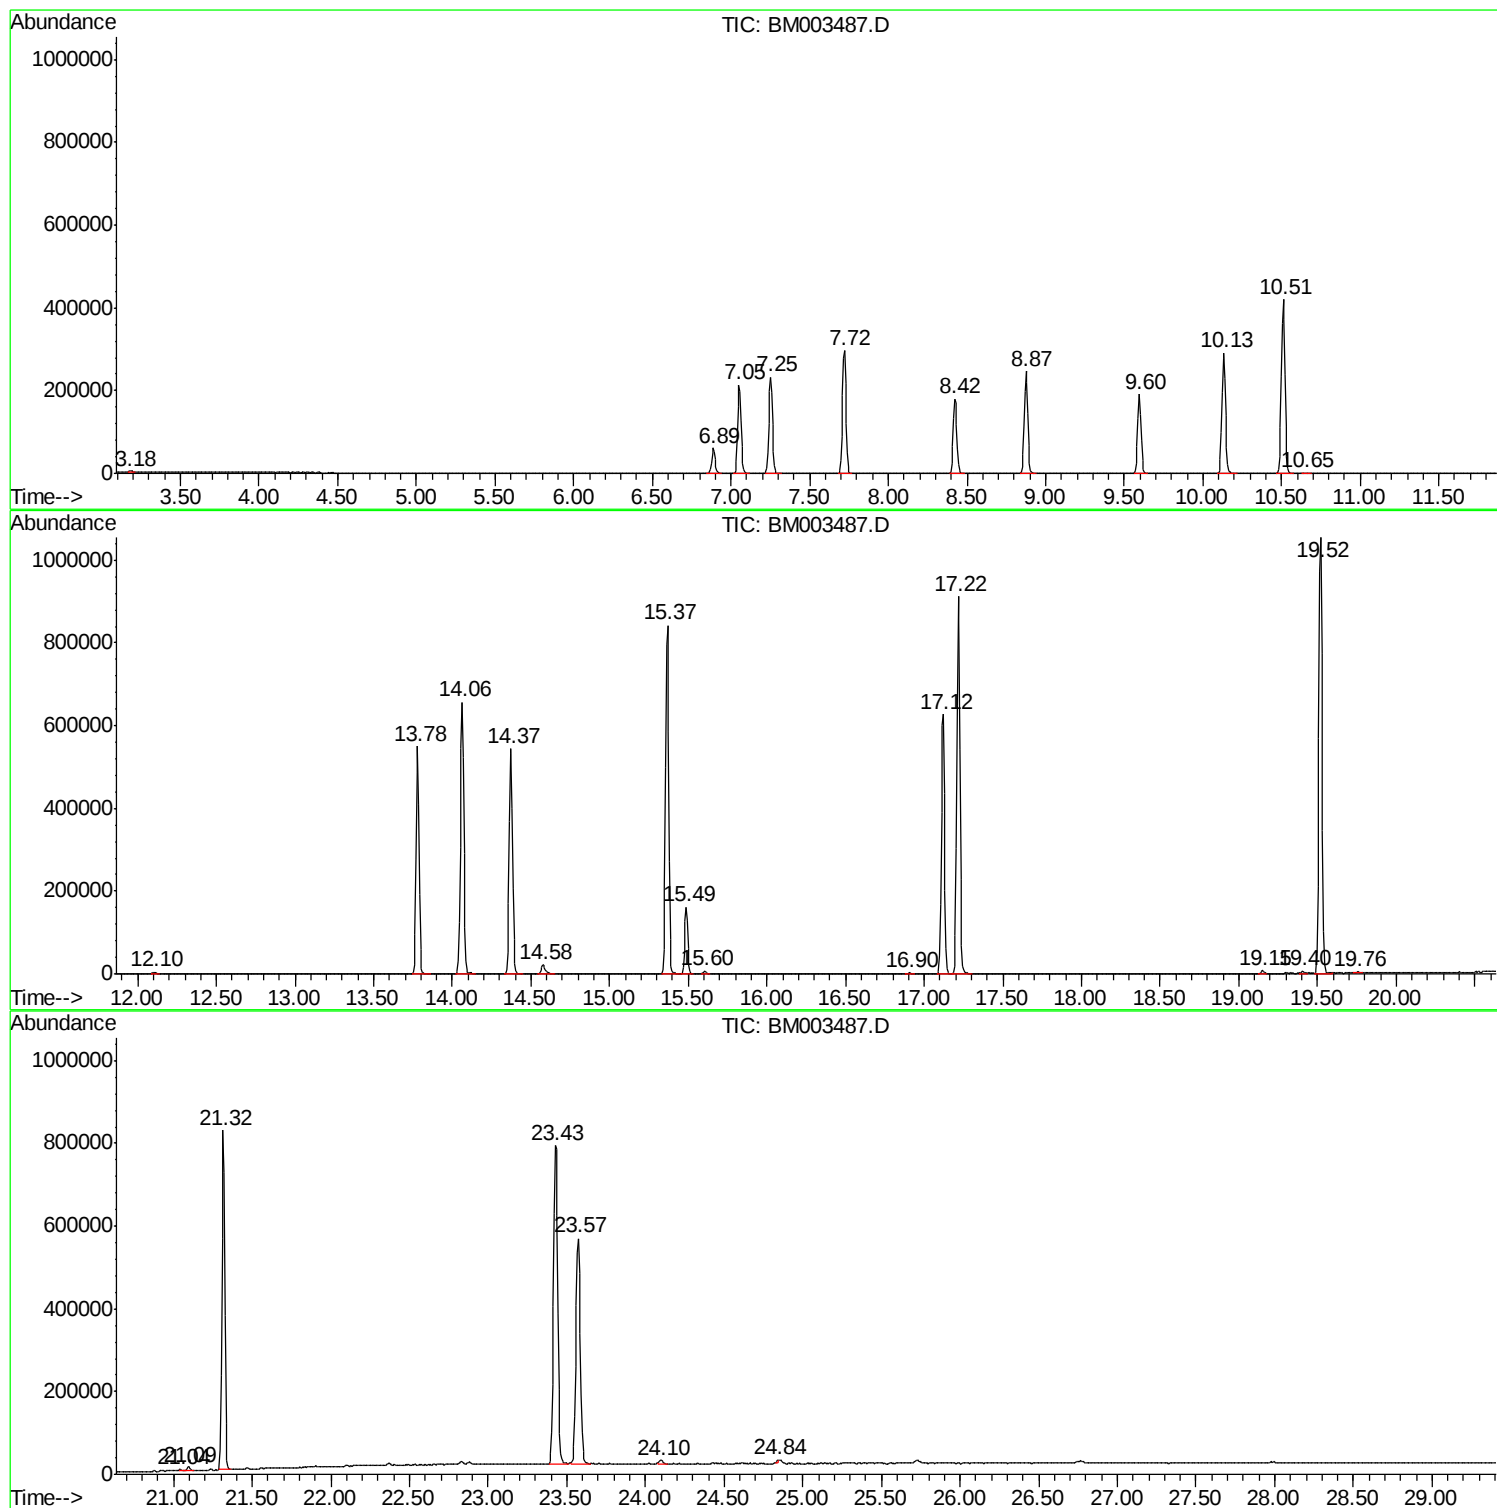

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121115\
Data File : BM003487.D
Acq On : 11 Dec 2015 18:18
Operator : UM/IZ
Sample : G4718-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM121115\
Data File : BM003487.D
Acq On : 11 Dec 2015 18:18
Operator : UM/IZ
Sample : G4718-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD2

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc