


Data Path : Z:\HPCHEM1\BNA M\Data\BM121115\
 Data File : BM003481.D
 Acq On : 11 Dec 2015 09:38
 Operator : UM/IZ
 Sample : DFTPP55
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP55

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM120115.M
 Title : SVOA CALIBRATION
 Last Update : Mon Dec 14 04:23:11 2015

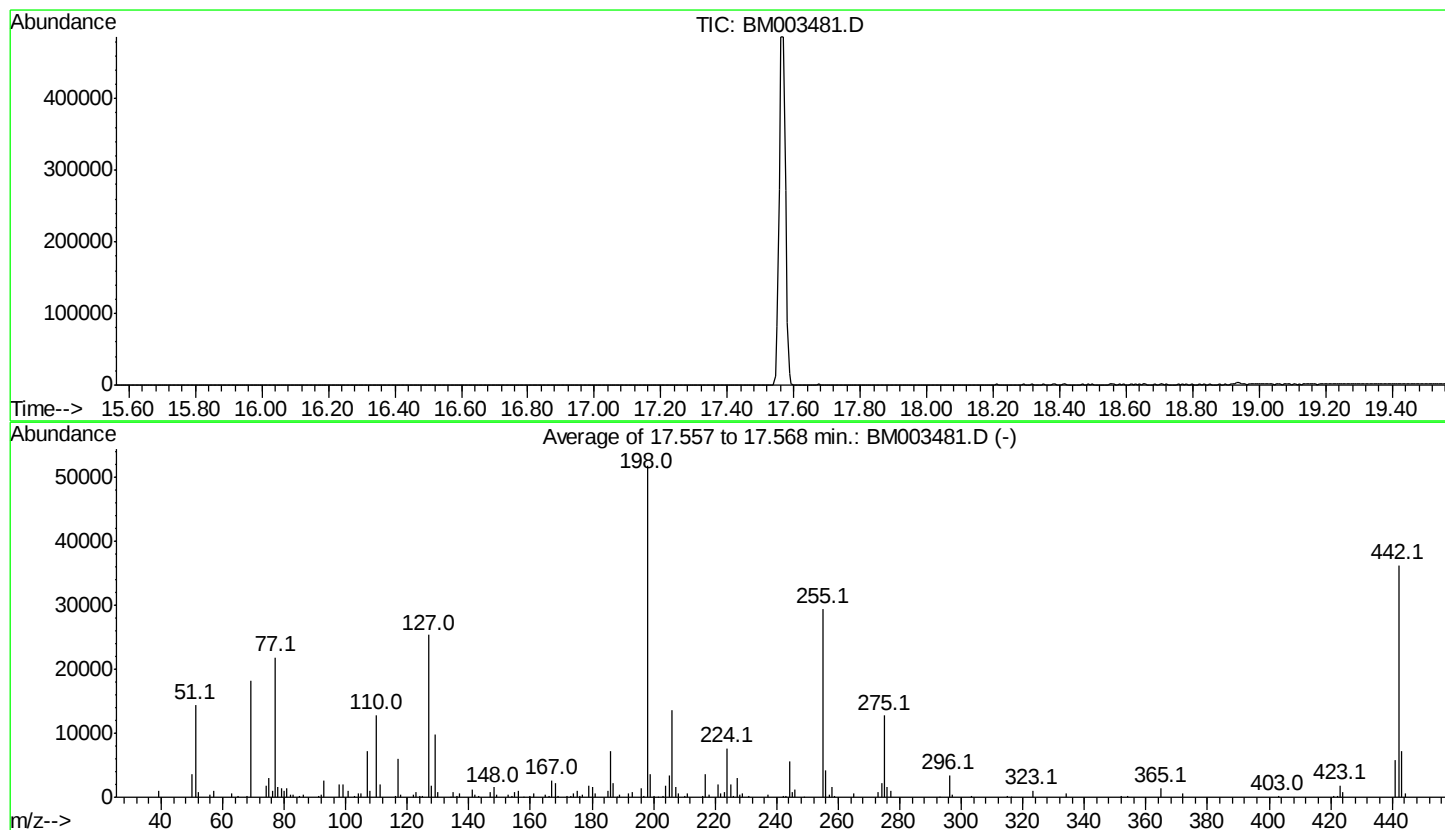

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	14472	PASS
68	69	0.00	2	1.2	218	PASS
69	198	0.00	100	35.3	18239	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	25362	PASS
197	198	0.00	2	0.3	132	PASS
198	198	100	100	100.0	51733	PASS
199	198	5	9	7.1	3672	PASS
275	198	10	60	24.6	12739	PASS
365	198	1	100	2.8	1428	PASS
441	443	0.01	100	80.4	5739	PASS
442	198	50	100	69.9	36152	PASS
443	442	15	24	19.7	7140	PASS

m/z	Abundance
207.10	577.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

m/z	Abundance
39.00	840.0
50.00	2836.0
51.10	11314.0
52.00	608.0
56.00	319.0
57.00	834.0
63.00	515.0
69.00	14254.0
74.00	1470.0
75.00	2454.0
76.10	706.0
77.10	17272.0
78.10	1159.0
79.00	987.0
80.00	778.0
81.00	1226.0
82.00	320.0
83.00	304.0
86.00	320.0
93.00	1999.0
98.00	1375.0
99.00	1652.0
101.00	645.0
104.00	390.0
104.90	444.0
107.00	5428.0
108.00	925.0
110.00	9736.0
111.00	1580.0
117.00	4562.0
118.00	347.0
122.00	353.0
123.00	549.0
127.00	18592.0
128.00	1428.0
129.00	7155.0
130.00	658.0
135.00	565.0
137.00	412.0
141.00	930.0
141.90	309.0
147.00	564.0
148.00	1123.0
148.90	335.0
153.00	305.0
155.00	476.0
156.00	802.0
161.00	392.0
165.00	323.0
167.00	1801.0
168.00	1926.0
174.00	437.0
175.00	678.0
177.00	307.0
178.90	1370.0
180.00	1101.0
181.00	453.0
185.00	613.0
186.10	5007.0
187.00	1699.0
192.00	365.0
193.10	518.0
196.10	992.0
198.00	34360.0
199.00	2571.0
204.00	1133.0
205.00	2184.0
206.10	9158.0
207.10	1678.0
208.00	410.0
211.20	374.0
217.00	2324.0
218.00	336.0
221.10	1255.0
221.90	338.0
223.10	484.0
224.00	4806.0
225.10	1290.0
227.00	2030.0
229.00	488.0
237.00	316.0
244.10	3539.0
245.00	464.0
246.10	751.0
255.10	18024.0
256.00	2741.0
258.00	997.0
265.00	478.0
273.00	459.0
274.00	1281.0
275.10	7520.0
276.00	1123.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

277.00	639.0
296.00	2150.0
323.10	744.0
334.10	376.0
365.00	877.0
372.10	348.0
423.10	1002.0
424.10	437.0
441.10	2739.0
442.10	17560.0
443.10	3648.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

m/z	Abundance
39.10	1286.0
50.10	4115.0
51.10	17096.0
52.10	853.0
56.00	428.0
57.00	1204.0
63.00	866.0
65.00	384.0
68.00	355.0
69.00	21584.0
74.00	2244.0
75.00	3649.0
76.10	1176.0
77.10	25496.0
78.00	2035.0
79.00	1778.0
80.00	1267.0
81.00	1697.0
82.00	470.0
83.00	374.0
85.00	370.0
86.00	518.0
91.00	408.0
92.00	537.0
93.00	3037.0
98.00	2394.0
99.00	2316.0
100.90	1096.0
103.00	314.0
104.00	657.0
105.00	553.0
107.00	8304.0
108.00	1239.0
110.00	15216.0
111.00	2210.0
116.00	385.0
117.00	6856.0
118.00	540.0
122.00	506.0
123.00	809.0
124.00	410.0
125.00	346.0
127.00	30056.0
128.00	2246.0
129.00	11680.0
130.00	960.0
135.00	937.0
136.00	479.0
137.00	625.0
141.00	1506.0
142.00	593.0
143.00	341.0
147.00	802.0
148.00	1721.0
148.90	442.0
152.90	481.0
153.90	337.0
155.00	862.0
156.00	1152.0
157.90	320.0
160.00	472.0
161.00	741.0
164.90	623.0
166.10	436.0
167.00	3191.0
168.00	2466.0
169.10	382.0
172.00	336.0
173.00	335.0
174.00	671.0
175.00	1175.0
177.00	493.0
178.90	2012.0
180.00	1676.0
181.00	732.0
185.00	1063.0
186.10	8535.0
187.00	2474.0
189.00	588.0
192.00	752.0
193.00	886.0
196.00	1550.0
196.80	396.0
198.00	60424.0
199.00	4315.0
199.90	353.0
203.00	431.0
204.00	2217.0
205.00	3947.0
206.10	15694.0
207.10	2502.0
208.00	746.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

210.20	340.0
211.00	651.0
216.00	300.0
217.00	4075.0
218.00	527.0
221.10	2426.0
221.80	600.0
223.00	966.0
224.10	9149.0
225.10	2479.0
226.00	307.0
227.00	3583.0
228.00	606.0
229.00	742.0
231.10	301.0
237.10	493.0
242.10	439.0
243.00	367.0
244.10	6910.0
245.10	875.0
246.00	1337.0
255.10	34520.0
256.10	4801.0
257.10	454.0
258.00	1730.0
259.00	335.0
265.00	779.0
273.10	960.0
274.10	2699.0
275.10	14839.0
276.10	2007.0
277.00	1116.0
296.00	3891.0
297.10	551.0
303.10	412.0
315.00	371.0
316.00	304.0
323.10	1236.0
334.10	759.0
352.10	366.0
354.10	338.0
365.10	1628.0
372.10	545.0
403.00	378.0
422.10	348.0
423.10	2000.0
424.10	923.0
441.10	6428.0
442.10	39792.0
443.10	7777.0
444.10	806.0

Instrument :

BNA_M

ClientSampleId :

DFTPP55

m/z	Abundance
39.00	1156.0
50.10	3735.0
51.10	15007.0
52.00	658.0
56.00	492.0
57.00	1116.0
63.00	624.0
65.10	316.0
68.10	300.0
69.00	18880.0
74.00	1944.0
75.00	3094.0
76.00	1059.0
77.10	22600.0
78.00	1626.0
79.00	1471.0
80.00	1036.0
81.00	1535.0
82.00	402.0
83.00	344.0
86.00	528.0
91.00	339.0
92.00	434.0
93.00	2680.0
98.00	2012.0
99.00	1899.0
101.00	1028.0
103.00	374.0
104.00	622.0
105.00	599.0
107.00	7657.0
108.00	1140.0
110.00	13623.0
111.00	2112.0
116.10	328.0
117.00	6605.0
118.00	501.0
122.00	459.0
123.00	769.0
124.00	424.0
125.00	354.0
127.00	27440.0
128.00	1951.0
129.00	10493.0
130.00	836.0
133.90	310.0
135.00	846.0
135.90	353.0
137.00	543.0
141.00	1430.0
142.10	487.0
147.00	836.0
148.00	1675.0
149.00	495.0
153.00	451.0
154.00	399.0
155.00	784.0
156.00	1325.0
160.00	415.0
161.00	734.0
165.00	513.0
166.00	414.0
167.00	2961.0
168.00	2196.0
169.00	322.0
173.00	308.0
174.00	659.0
175.00	1280.0
176.00	358.0
177.00	562.0
179.00	2066.0
180.00	1881.0
181.00	714.0
185.00	1060.0
186.10	8298.0
187.00	2279.0
188.00	318.0
189.00	484.0
192.00	748.0
193.00	903.0
196.00	1733.0
198.00	60416.0
199.00	4132.0
200.00	323.0
201.60	308.0
203.00	473.0
204.00	2160.0
205.00	3815.0
206.10	16080.0
207.00	2521.0
208.00	617.0
211.00	630.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55

216.00	332.0
217.00	4421.0
217.90	503.0
221.00	2460.0
221.90	659.0
223.00	943.0
224.10	8907.0
225.00	2383.0
226.00	380.0
227.10	3602.0
228.00	567.0
229.00	735.0
231.00	321.0
237.00	487.0
241.90	451.0
243.00	507.0
244.10	6626.0
245.10	807.0
246.00	1290.0
248.90	301.0
255.10	35616.0
256.10	5126.0
257.00	473.0
258.00	2108.0
259.00	323.0
265.10	815.0
273.00	1062.0
274.10	2824.0
275.10	15859.0
276.10	1913.0
277.00	1521.0
293.00	319.0
296.10	4456.0
297.00	651.0
303.10	499.0
315.00	504.0
323.10	1279.0
334.10	849.0
352.00	407.0
354.10	445.0
365.10	1780.0
372.10	718.0
403.00	451.0
421.00	372.0
422.10	368.0
423.10	2574.0
424.10	882.0
441.10	8050.0
442.10	51104.0
443.10	9995.0
444.10	965.0

Instrument :
BNA_M
ClientSampleId :
DFTPP55