

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121118\
Data File : BM018053.D Quantitation Report (QT Reviewed)

Acq On : 11 Dec 2018 12:31

Operator : JU/SJ

Sample : J6155-16

Misc :

ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 12 00:38:10 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Dec 12 00:24:38 2018

Response via : Initial Calibration

Instrument :

BNA_M


Client Sampled :

A4150

Manual Integrations
APPROVED

Sohil

12/12/2018 5:42:24 PM

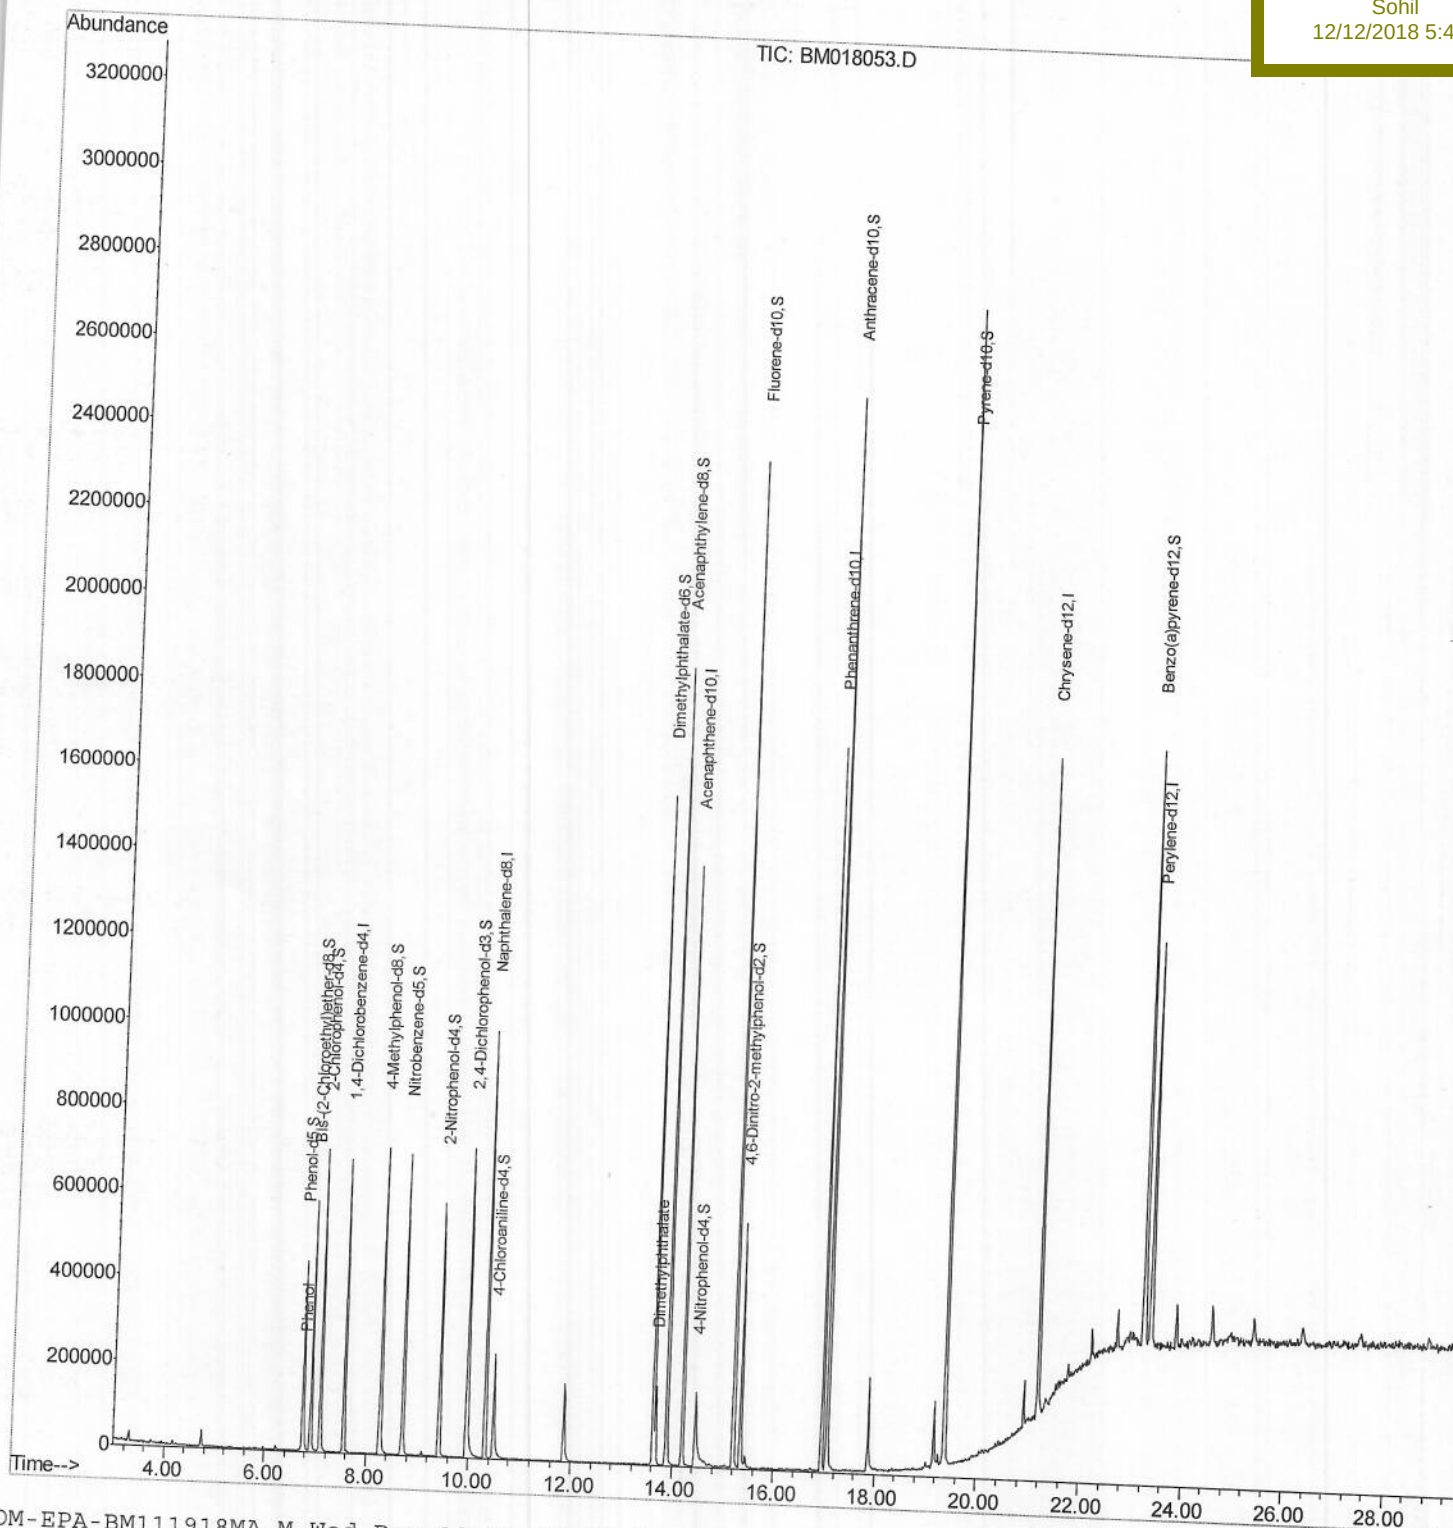

SOM-EPA-BM111918MA.M Wed Dec 12 00:37:13 2018

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121118\
Quantitation Report (Qedit)




Data File : BM018053.D
Acq On : 11 Dec 2018 12:31
Operator : JU/SJ
Sample : J6155-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Quant Time: Dec 12 00:27:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 12 00:24:38 2018
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
A4150

Manual Integrations
APPROVED

Sohil
12/12/2018 5:42:24 PM

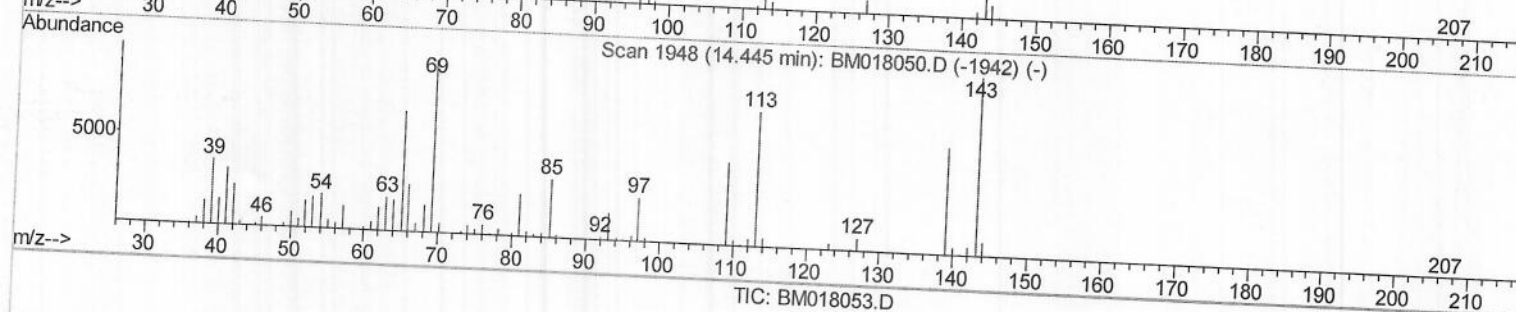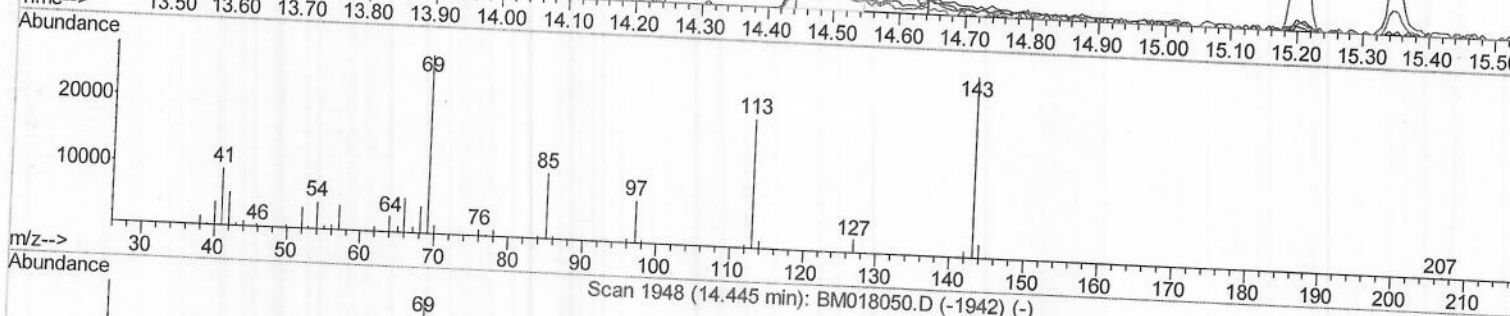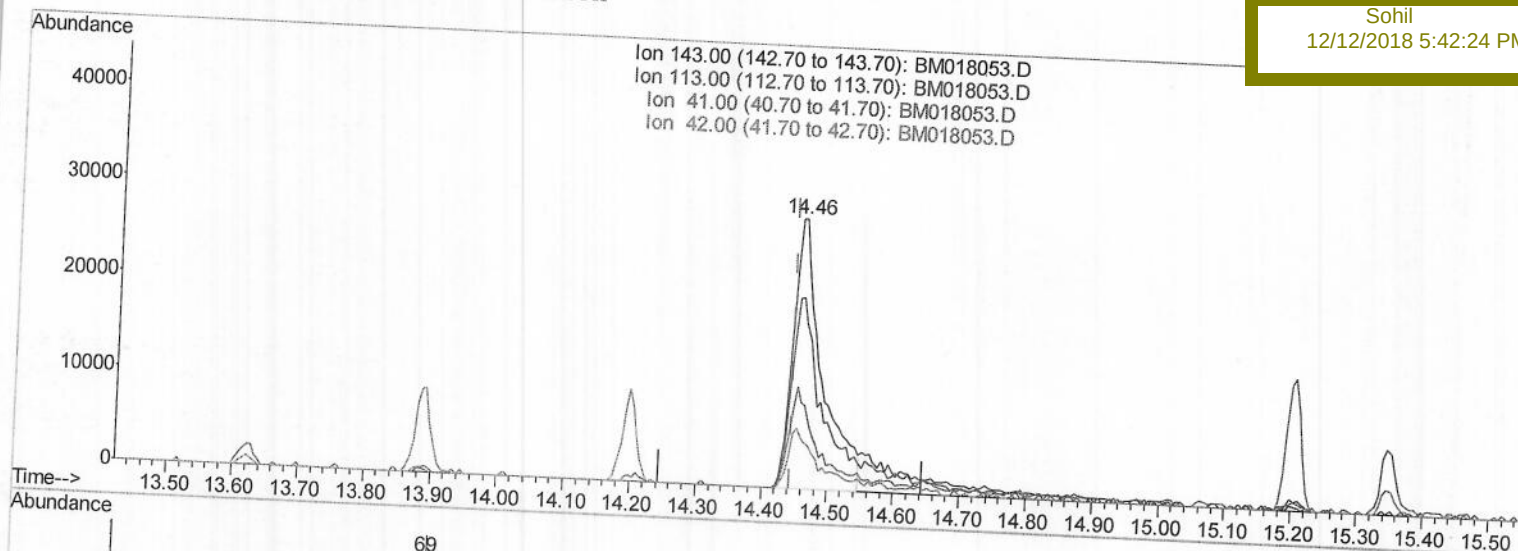

(51) 4-Nitrophenol-d4 (S)

14.457min (+0.012) 11.98ng/ul

response 87865

Ion	Exp%	Act%
143.00	100	100
113.00	79.10	71.55
41.00	40.10	32.39
42.00	26.80	19.62#

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121118\
Quantitation Report (Qedit)




Data File : BM018053.D
Acq On : 11 Dec 2018 12:31
Operator : JU/SJ
Sample : J6155-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4150

Quant Time: Dec 12 00:27:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 12 00:24:38 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/12/2018 5:42:24 PM

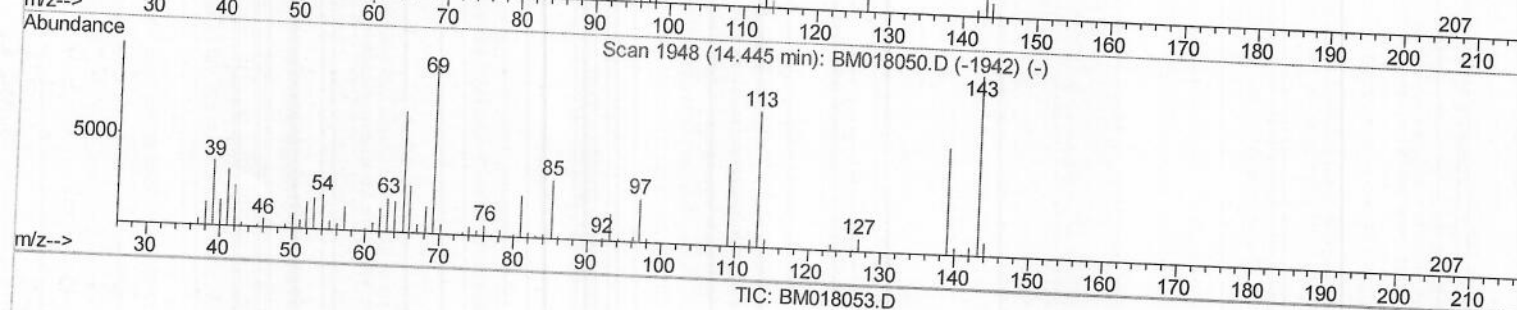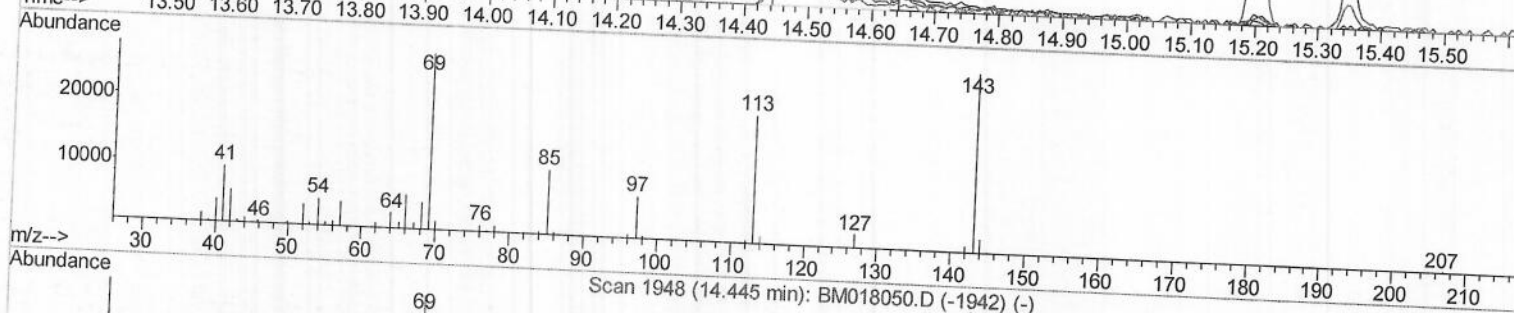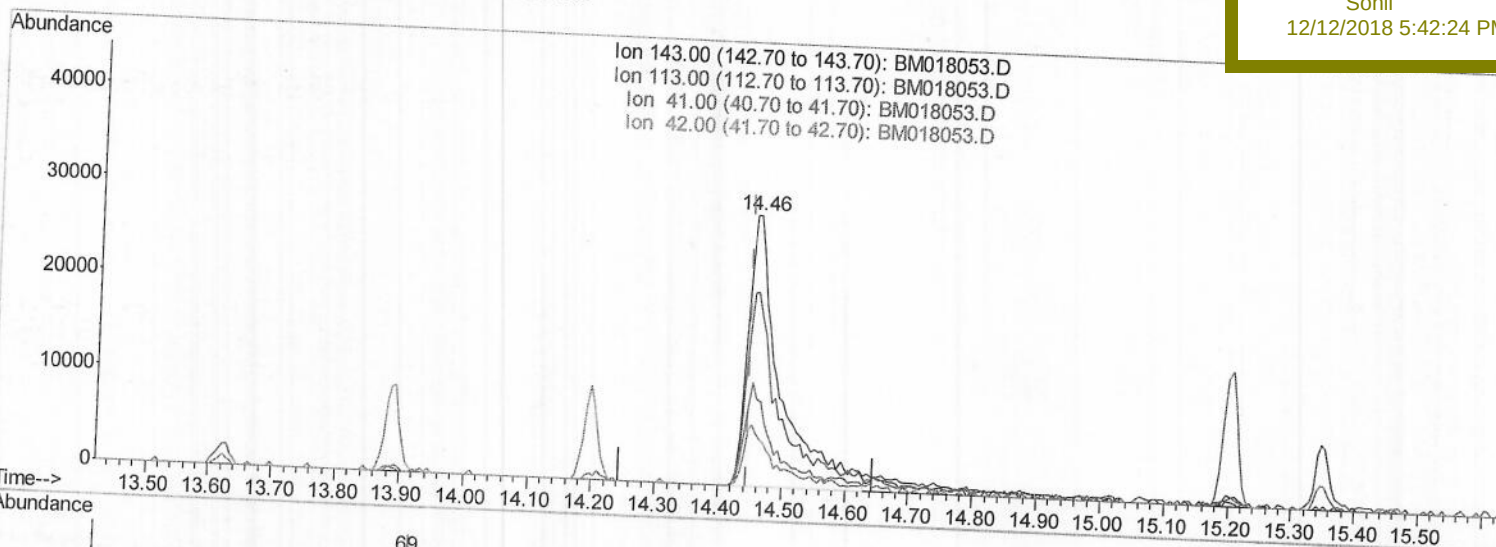

(51) 4-Nitrophenol-d4 (S)

14.457min (+0.012) 13.81ng/ul m

response 101302

Ion	Exp%	Act%
143.00	100	100
113.00	79.10	71.55
41.00	40.10	32.39
42.00	26.80	19.62#

SJ 12/12/18

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM121118\
Quantitation Report (QT Reviewed)

Data File : BM018053.D
Acq On : 11 Dec 2018 12:31
Operator : JU/SJ
Sample : J6155-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
Client Sample Id :
A4150

Quant Time: Dec 12 00:38:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 12 00:24:38 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/12/2018 5:42:24 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	191253	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	823075	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	465014	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	1008243	20.00	ng/ul	0.00
77) Chrysene-d12	21.17	240	773875	20.00	ng/ul	0.00
85) Perylene-d12	23.34	264	667189	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.16	96	2476	0.59	ng/uL	0.00
5) Phenol-d5	6.75	99	297021	17.00	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	6.90	67	249200	23.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	342656	25.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	297252	20.83	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	177382	28.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	203757	28.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	333188	24.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.48	131	196723	16.62	ng/ul	0.00
43) Dimethylphthalate-d6	13.62	166	1092869	27.09	ng/ul	0.00
46) Acenaphthylene-d8	13.89	160	1377955	28.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.46	143	101302m	13.81	ng/ul	0.01
57) Fluorene-d10	15.20	176	926044	26.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	138985	19.28	ng/ul	0.00
70) Anthracene-d10	17.06	188	1399494	27.88	ng/ul	0.00
78) Pyrene-d10	19.37	212	1445069	38.59	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.21	264	965334	26.68	ng/ul	0.00
Target Compounds						
6) Phenol	6.78	94	45254	2.596	ng/ul	95
44) Dimethylphthalate	13.67	163	120616	3.086	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed