

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121118\
 Data File : BM018066.D
 Acq On : 11 Dec 2018 20:24
 Operator : JU/SJ
 Sample : J6170-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F9M04

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:42:50 PM

Quant Time: Dec 12 01:30:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 12 00:58:41 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	176365	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	769080	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.20	164	418750	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.96	188	858063	20.00	ng/ul	0.00
77) Chrysene-d12	21.17	240	670333	20.00	ng/ul	0.00
85) Perylene-d12	23.35	264	632281	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.16	96	5190	1.35	ng/uL	0.00
5) Phenol-d5	6.74	99	94607	5.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	254429	26.20	ng/ul	0.00
9) 2-Chlorophenol-d4	7.09	132	307715	24.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	175481	13.33	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	186906	31.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	211559	31.25	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	329417	25.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.49	131	13727	1.24	ng/ul	0.02
43) Dimethylphthalate-d6	13.62	166	1173560	32.30	ng/ul	0.00
46) Acenaphthylene-d8	13.89	160	1427479	32.46	ng/ul	0.00
51) 4-Nitrophenol-d4	14.47	143	23459m	3.55	ng/ul	0.03
57) Fluorene-d10	15.20	176	1011276	32.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.34	200	160877	26.23	ng/ul	0.00
70) Anthracene-d10	17.06	188	1506961	35.27	ng/ul	0.00
78) Pyrene-d10	19.36	212	1424657	43.92	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.21	264	1224407	35.71	ng/ul	0.00

Target Compounds

					Ovalue	
28) Naphthalene	10.38	128	17861404	445.749	ng/ul#	95
34) 2-Methylnaphthalene	11.99	142	1182648	39.536	ng/ul	99
40) 1,1'-Biphenyl	13.02	154	150164	4.356	ng/ul	99
58) Fluorene	15.26	166	41868	1.199	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM121118\
Data File : BM018066.D
Acq On : 11 Dec 2018 20:24
Operator : JU/SJ
Sample : J6170-11
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
F9M04

Quant Time: Dec 12 01:30:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM11918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 12 00:58:41 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/12/2018 5:42:50 PM

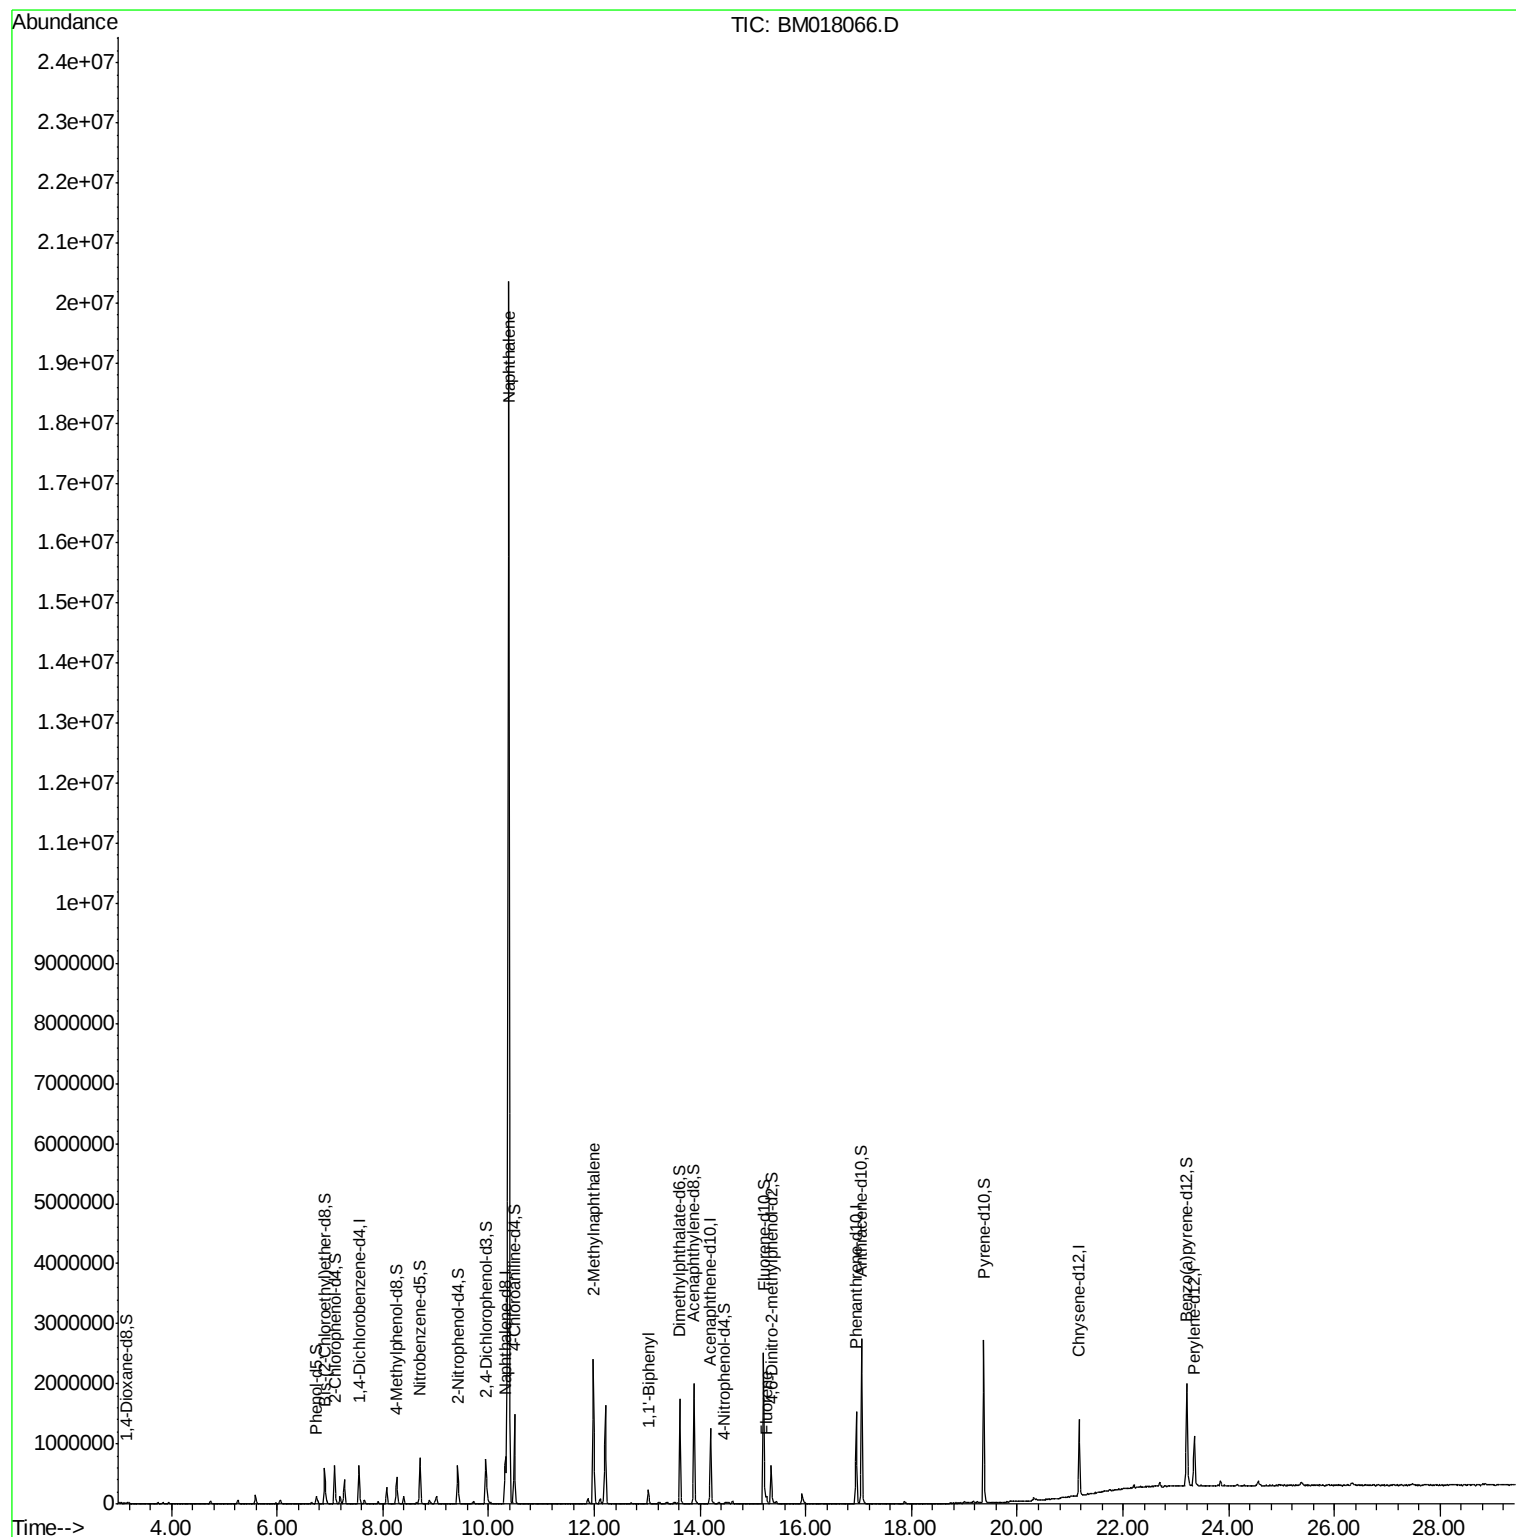

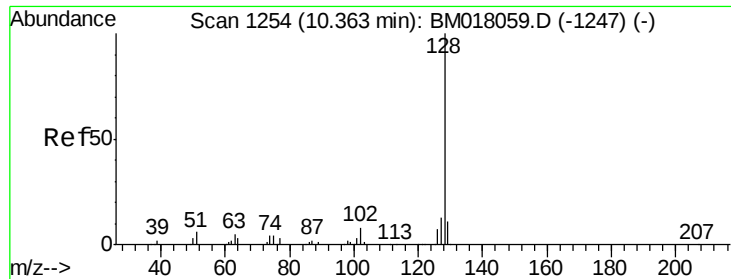

#28

Naphthalene

Concen: 445.749 ng/ul

RT: 10.38 min Scan# 1257

Delta R.T. 0.02 min

Lab File: BM018066.D

Acq: 11 Dec 2018 20:24

Instrument :

BNA_M

ClientSampleId :

F9M04

Tot Ion:128 Resp:17861404

Ion Ratio Lower Upper


128 100

129 12.8 8.6 12.8#




127 15.4 10.8 16.2

Manual Integrations
APPROVED

Sohil
12/12/2018 5:42:50 PM

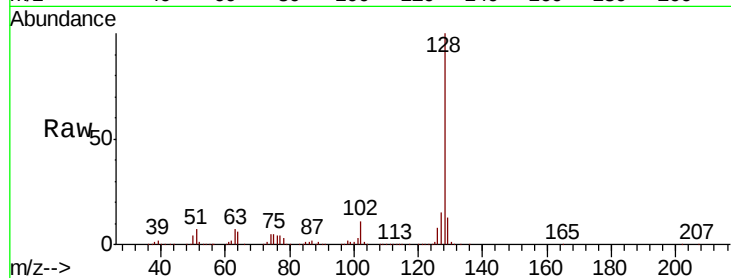

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

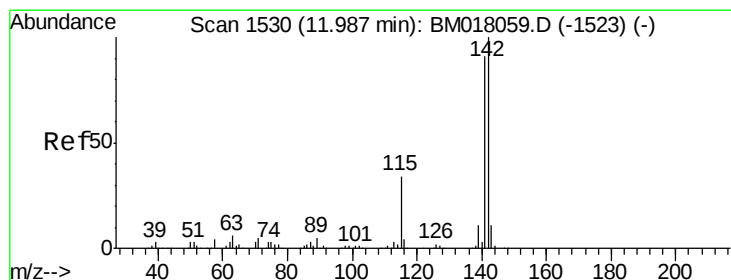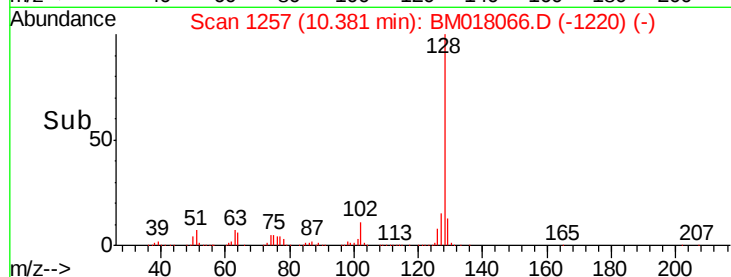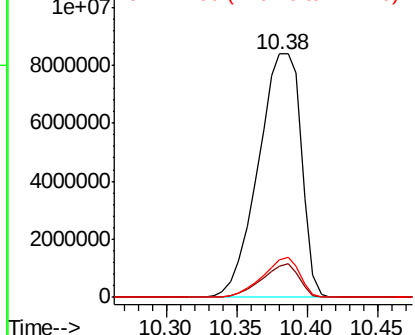

#34

2-Methylnaphthalene

Concen: 39.536 ng/ul

RT: 11.99 min Scan# 1530

Delta R.T. -0.00 min

Lab File: BM018066.D


Acq: 11 Dec 2018 20:24

Tgt Ion:142 Resp: 1182648



Ion Ratio Lower Upper


142 100

141 89.5 72.6 108.8

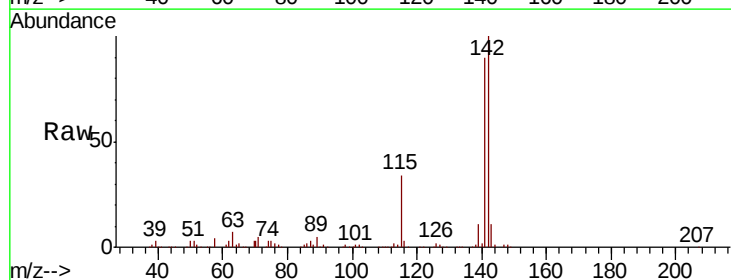

Abundance Ion 142.00 (141.70 to 142.70): E
Ion 141.00 (140.70 to 141.70): E

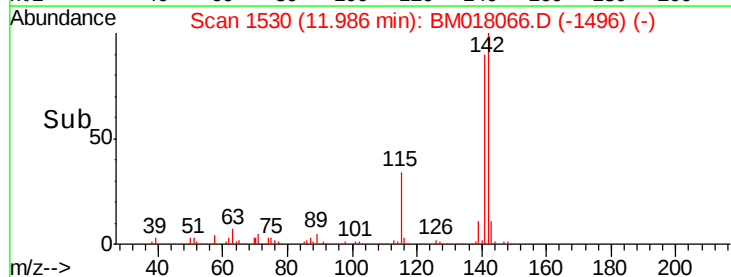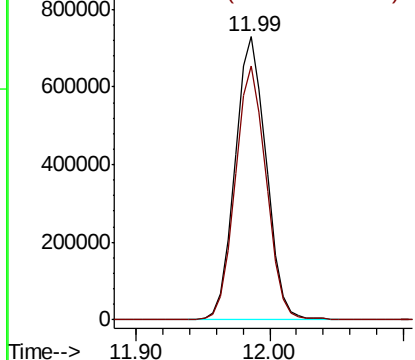

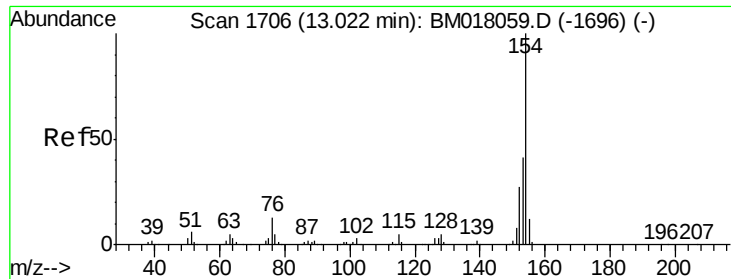





#40
 1,1'-Biphenyl
 Concen: 4.356 ng/ul
 RT: 13.02 min Scan# 1706
 Delta R.T. -0.00 min
 Lab File: BM018066.D
 Acq: 11 Dec 2018 20:24

Instrument :
 BNA_M
 ClientSampled :
 F9M04

Tot Ion:	154	Resp:	150164
Ion Ratio	Lower	Upper	
154	100		
153	39.9	32.5	48.7
76	13.8	10.6	15.8

Manual Integrations
 APPROVED

Sohil
 12/12/2018 5:42:50 PM

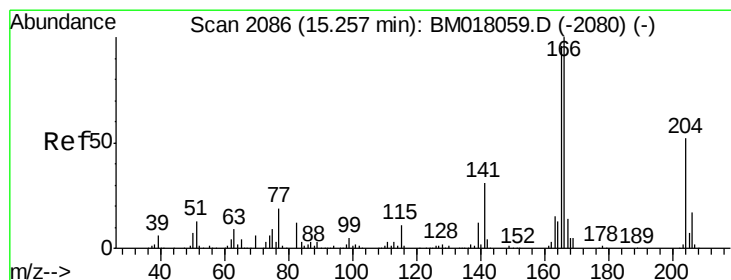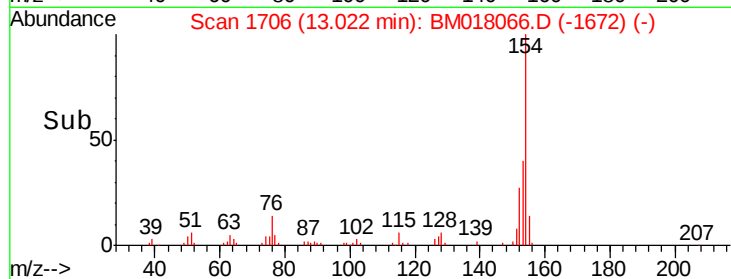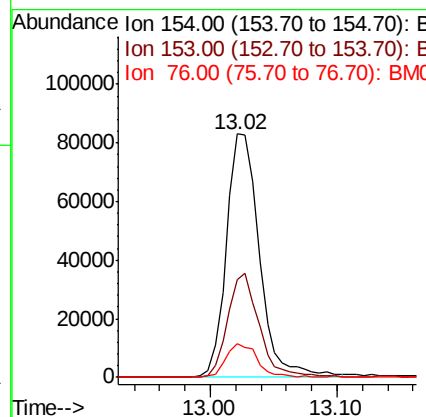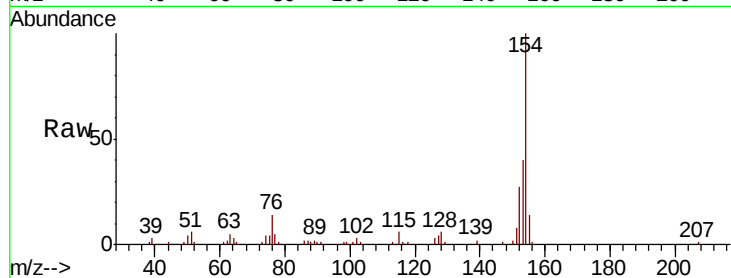

#58
 Fluorene
 Concen: 1.199 ng/ul
 RT: 15.26 min Scan# 2086
 Delta R.T. -0.00 min
 Lab File: BM018066.D
 Acq: 11 Dec 2018 20:24

Tgt Ion:	166	Resp:	41868
Ion Ratio	Lower	Upper	
166	100		
165	93.7	78.0	117.0
167	11.0	10.8	16.2

