

Data File : BM018115.D
Acq On : 13 Dec 2018 04:43
Operator : JU/SJ
Sample : J6227-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9F35

Quant Time: Dec 13 06:43:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 13 03:40:23 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	152554	20.00	ng/ul	0.00
18) Naphthalene-d8	10.31	136	669638	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.19	164	415958	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	915047	20.00	ng/ul	0.00
77) Chrysene-d12	21.16	240	1021952	20.00	ng/ul	0.00
85) Perylene-d12	23.34	264	901991	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.15	96	9593	2.88	ng/uL	0.00
5) Phenol-d5	6.73	99	235517	16.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.89	67	140928	16.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.08	132	191819	17.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	179494	15.77	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	105144	20.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.41	143	119949	20.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	196576	17.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.47	131	158881	16.50	ng/ul	0.00
43) Dimethylphthalate-d6	13.62	166	690489	19.13	ng/ul	0.00
46) Acenaphthylene-d8	13.88	160	801217	18.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	81851	12.47	ng/ul	0.02
57) Fluorene-d10	15.20	176	543536	17.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.34	200	52018	7.95	ng/ul	0.00
70) Anthracene-d10	17.05	188	788857	17.32	ng/ul	0.00
78) Pyrene-d10	19.36	212	969642	19.61	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.20	264	885158	18.09	ng/ul	0.00


Target Compounds						Qvalue
6) Phenol	6.76	94	64264	4.621	ng/ul	98
44) Dimethylphthalate	13.66	163	240593	6.881	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM018115.D
Acq On : 13 Dec 2018 04:43
Operator : JU/SJ
Sample : J6227-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F9F35

Quant Time: Dec 13 06:43:34 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM111918MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 13 03:40:23 2018
Response via : Initial Calibration

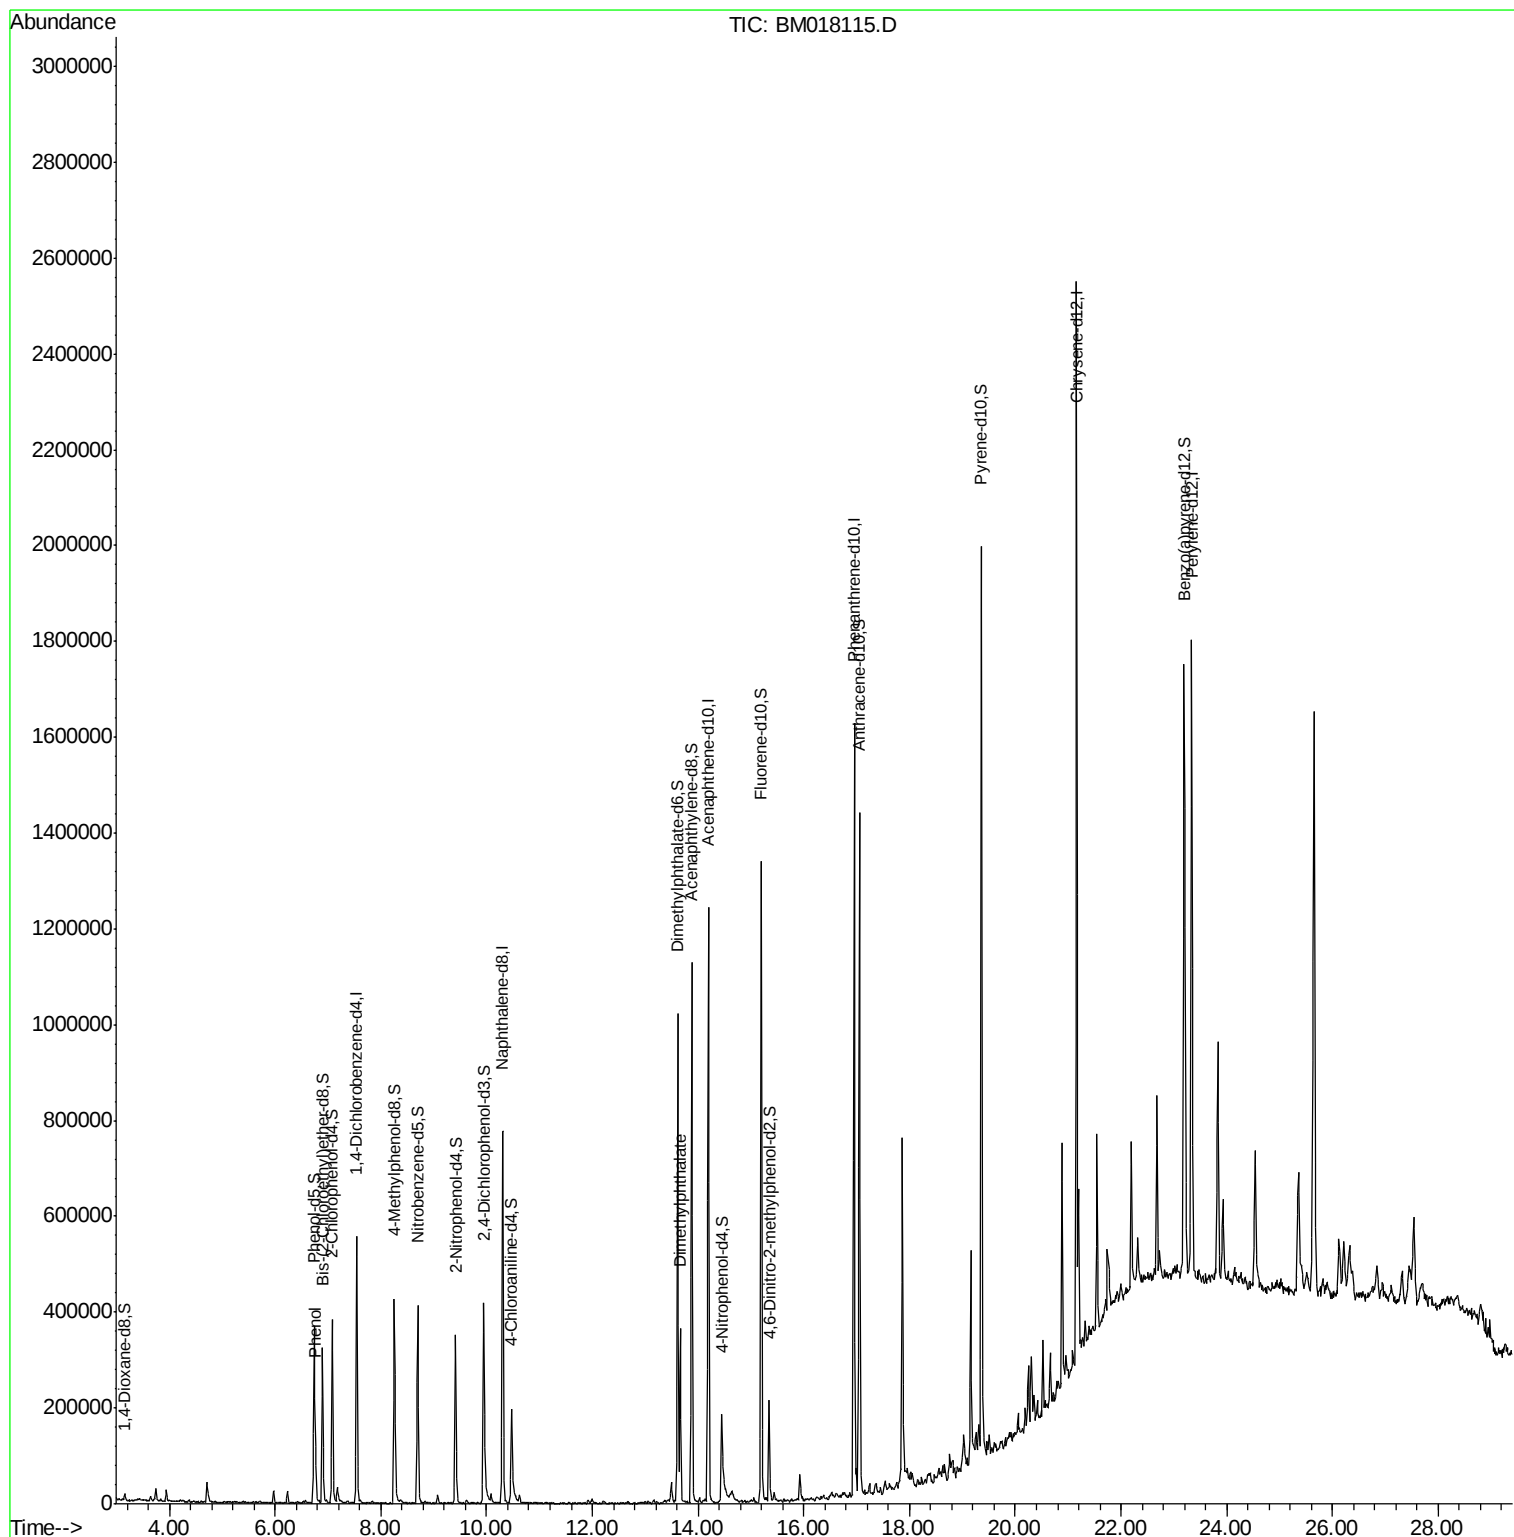

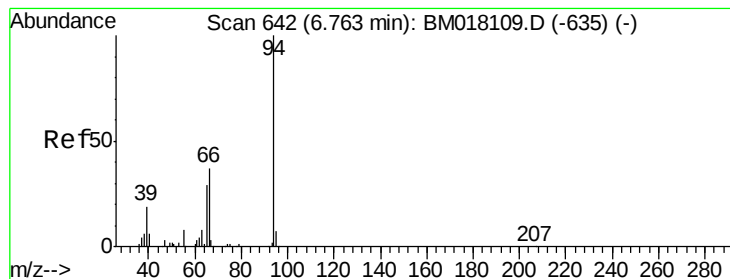

#6

Phenol

Concen: 4.621 ng/ul

RT: 6.76 min Scan# 642

Delta R.T. 0.00 min

Lab File: BM018115.D

Acq: 13 Dec 2018 04:43

Instrument :

BNA_M

ClientSampleId :

F9F35


Tgt Ion: 94 Resp: 64264

Ion Ratio Lower Upper

94 100

65 32.0 24.7 37.1




66 42.4 34.6 51.8

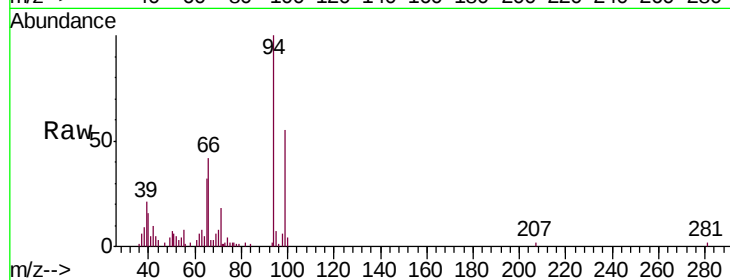

Abundance Ion 94.00 (93.70 to 94.70): BM018109.D (-635) (-)

Ion 65.00 (64.70 to 65.70): BM018109.D (-635) (-)

Ion 66.00 (65.70 to 66.70): BM018109.D (-635) (-)

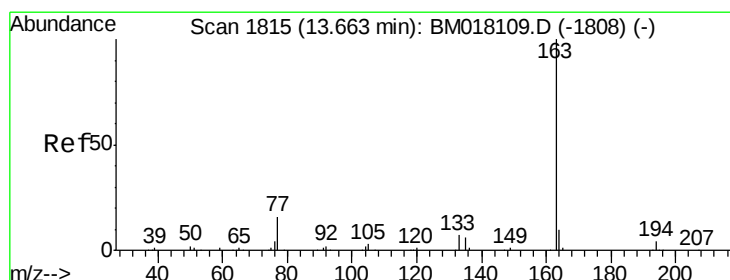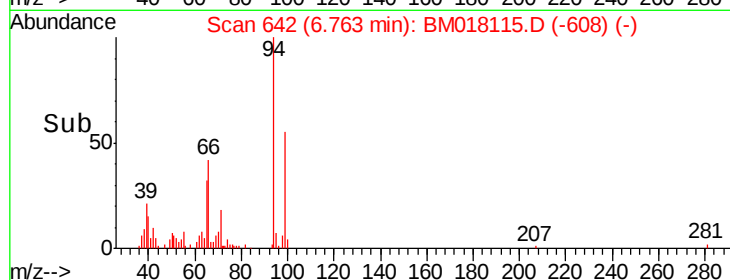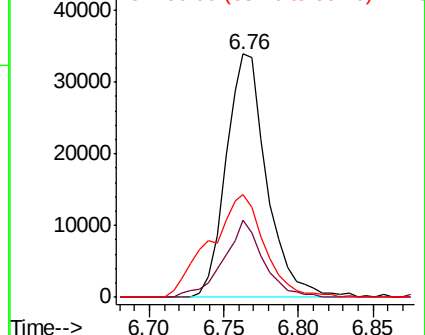

#44

Dimethylphthalate

Concen: 6.881 ng/ul

RT: 13.66 min Scan# 1815

Delta R.T. 0.00 min

Lab File: BM018115.D

Acq: 13 Dec 2018 04:43


Tgt Ion: 163 Resp: 240593

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 10.6 8.1 12.1

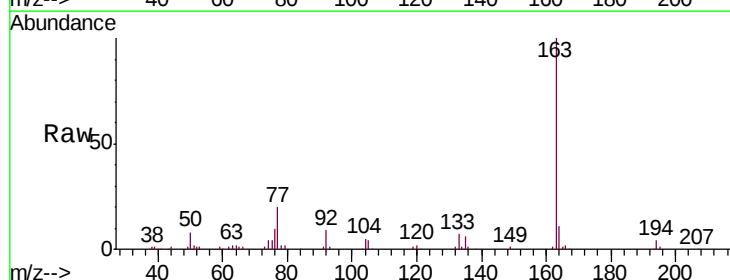

Abundance Ion 163.00 (162.70 to 163.70): BM018109.D (-1808) (-)

Ion 194.00 (193.70 to 194.70): BM018109.D (-1808) (-)

Ion 164.00 (163.70 to 164.70): BM018109.D (-1808) (-)

